

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060921\
 Data File : VX022606.D
 Acq On : 09 Jun 2021 12:08
 Operator : JC/MD
 Sample : VX0609WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0609WBL01

Quant Time: Jun 10 05:39:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 07 14:27:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	59540	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	122173	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	108396	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	41354	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	50069	47.303	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.600%
35) Dibromofluoromethane	5.397	113	35971	47.058	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.120%
50) Toluene-d8	8.653	98	149659	49.069	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.140%
62) 4-Bromofluorobenzene	11.085	95	51121	45.093	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060921\
Data File : VX022606.D
Acq On : 09 Jun 2021 12:08
Operator : JC/MD
Sample : VX0609WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0609WBL01

Quant Time: Jun 10 05:39:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060721W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 07 14:27:50 2021
Response via : Initial Calibration




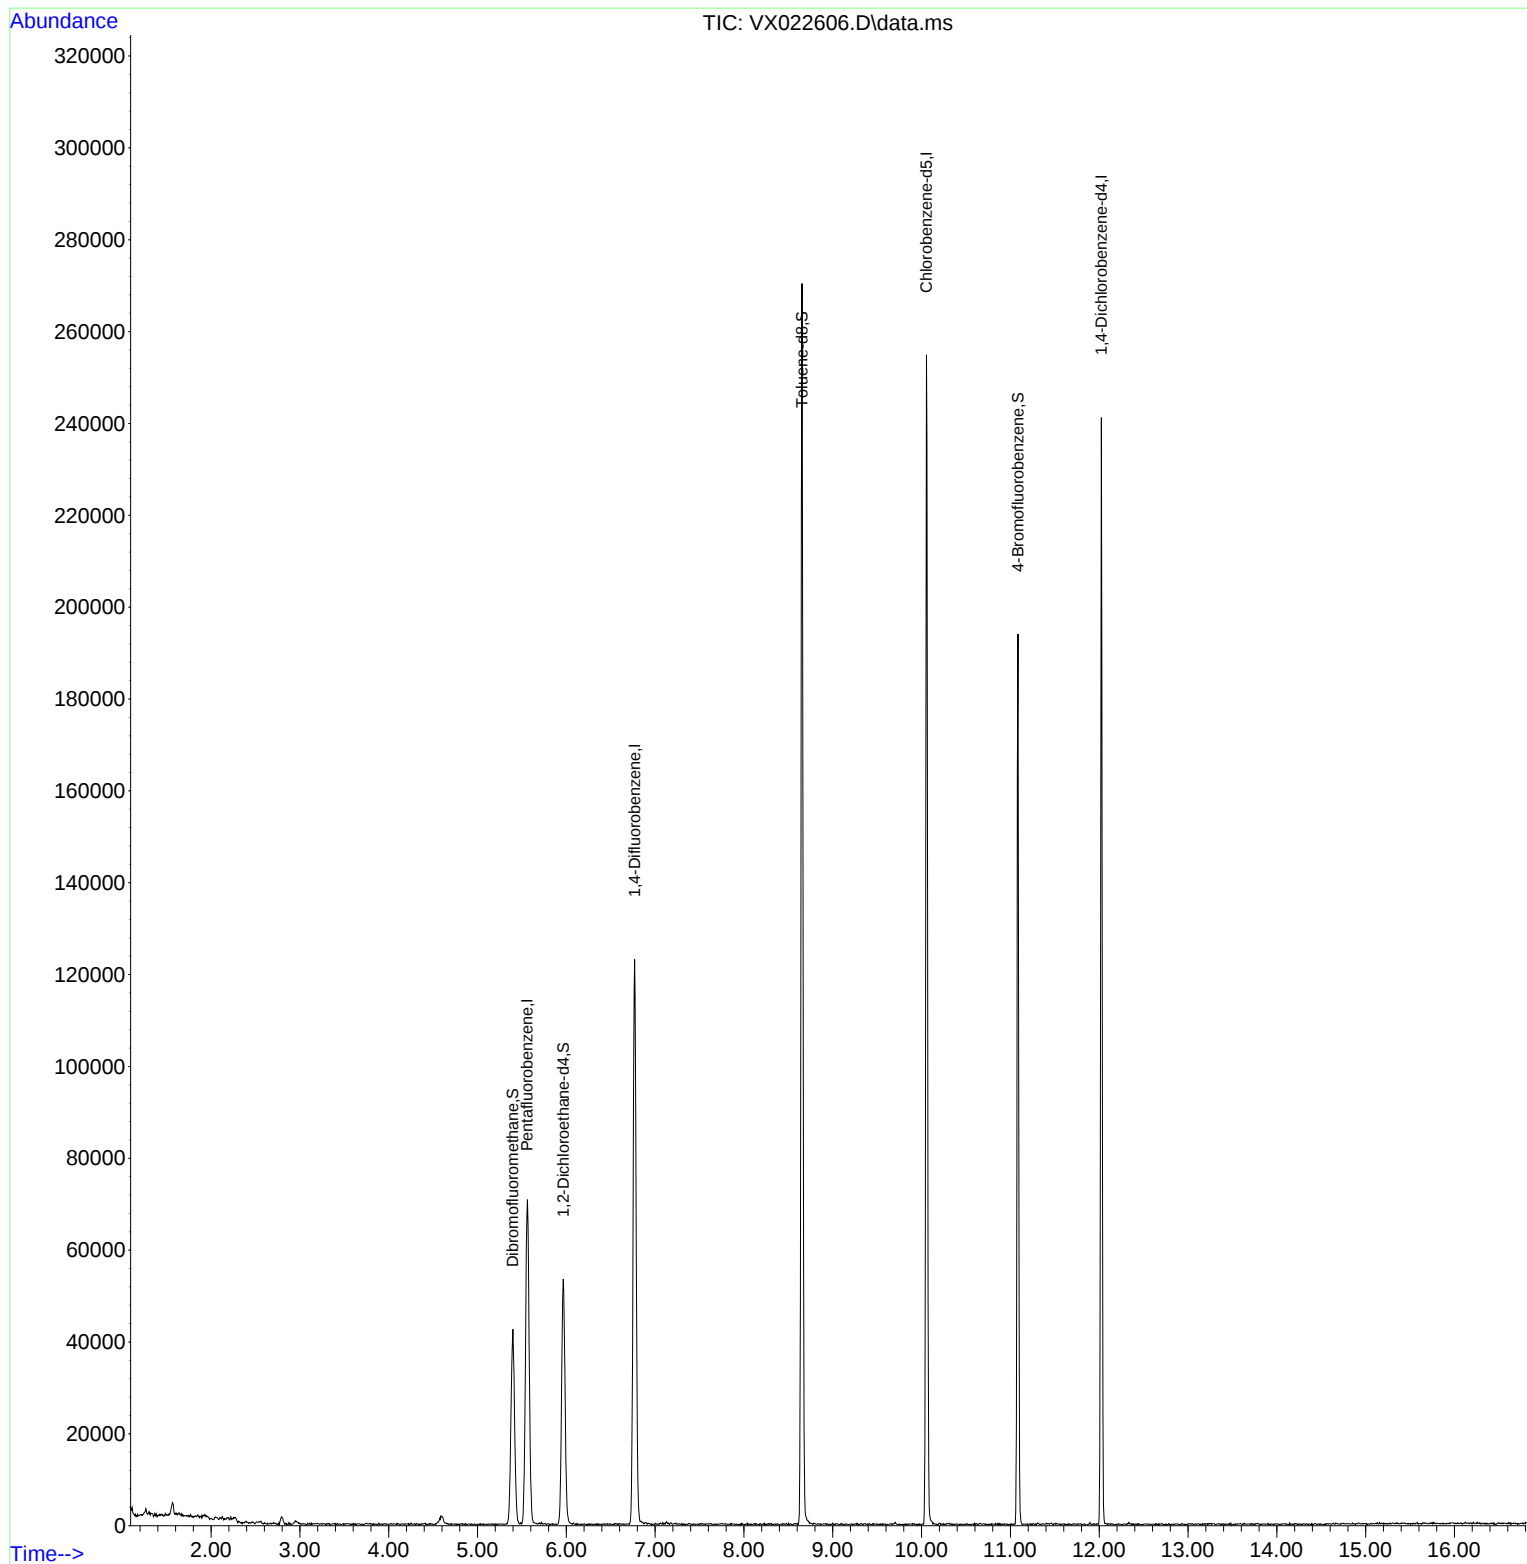


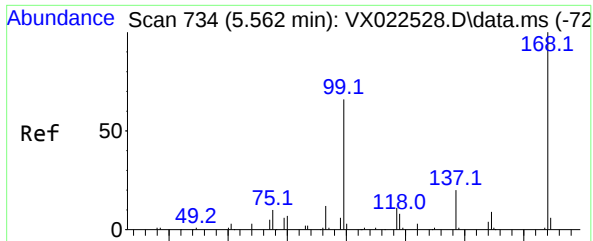

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.006 min
Lab File: VX022606.D
Acq: 09 Jun 2021 12:08




Instrument :
MSVOA_X
ClientSampleId :
VX0609WBL01


Tgt Ion:168 Resp: 59540
Ion Ratio Lower Upper
168 100
99 67.6 45.8 68.6

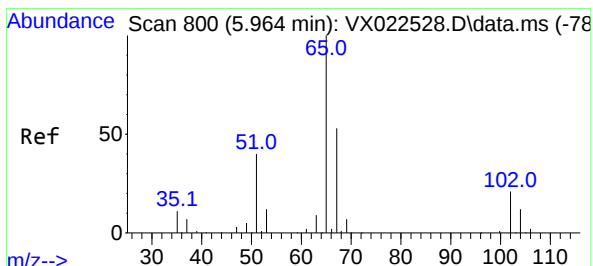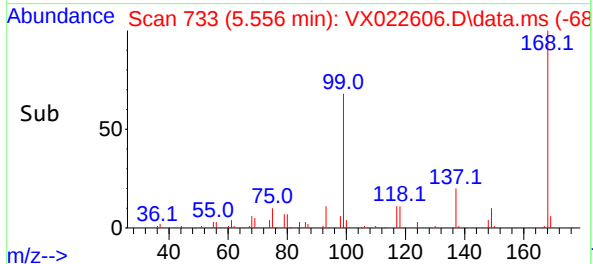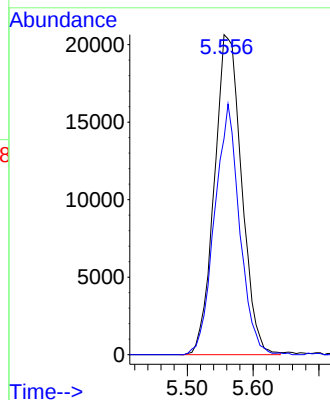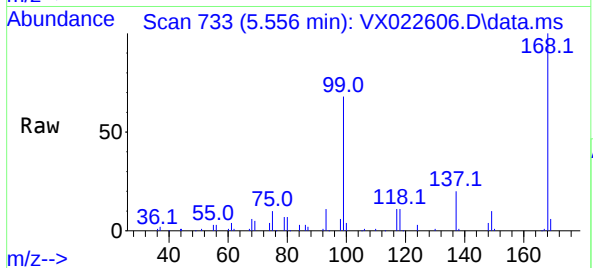

#33
1,2-Dichloroethane-d4
Concen: 47.303 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022606.D
Acq: 09 Jun 2021 12:08

Tgt Ion: 65 Resp: 50069
Ion Ratio Lower Upper
65 100
67 52.7 0.0 105.4


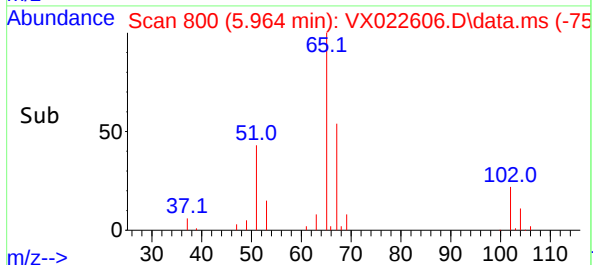
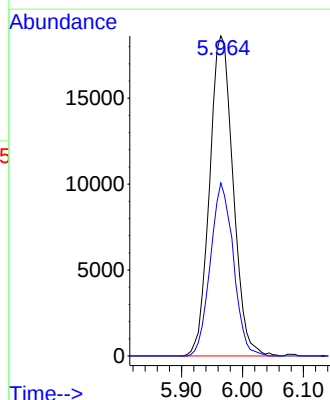
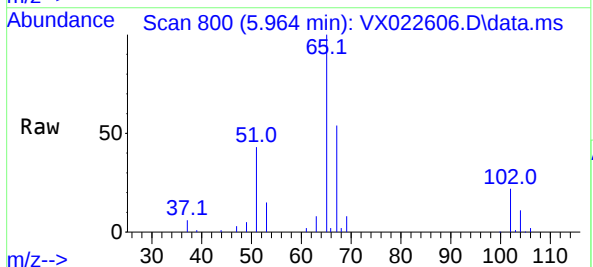


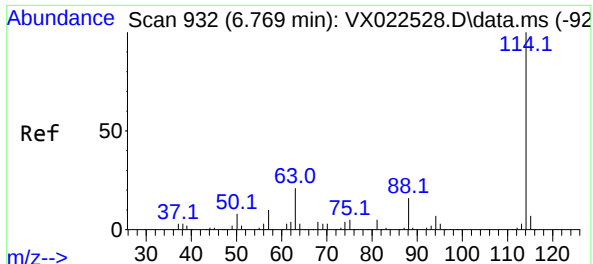

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022606.D
Acq: 09 Jun 2021 12:08




Instrument :
MSVOA_X
ClientSampleId :
VX0609WBL01


Tgt Ion:114 Resp: 122173
Ion Ratio Lower Upper
114 100
63 21.6 0.0 40.8
88 16.3 0.0 32.8

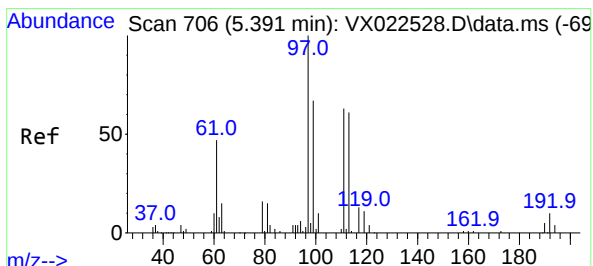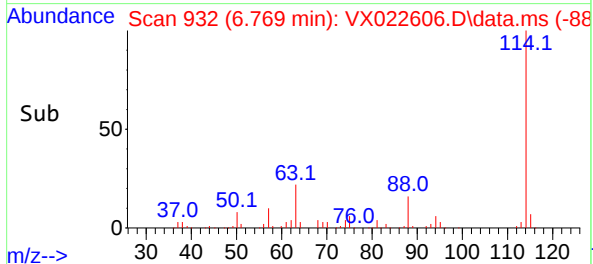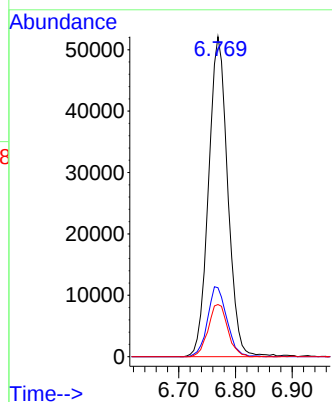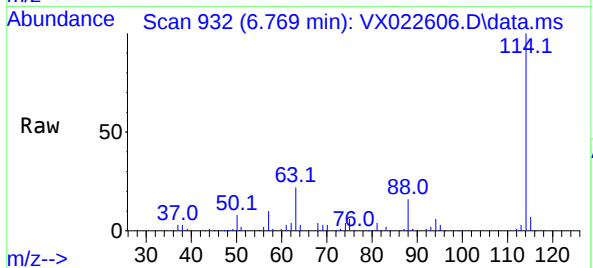

#35
Dibromofluoromethane
Concen: 47.058 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022606.D
Acq: 09 Jun 2021 12:08

Tgt Ion:113 Resp: 35971
Ion Ratio Lower Upper
113 100
111 102.4 81.9 122.9
192 15.7 16.7 25.1#


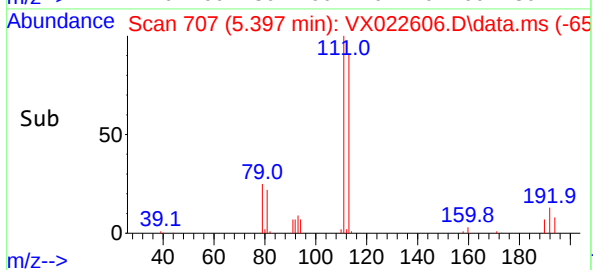
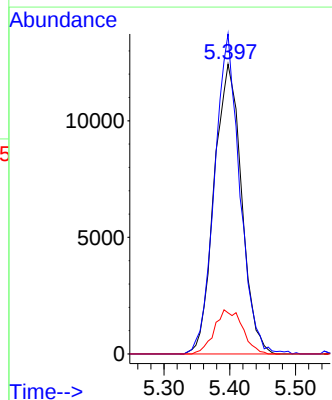
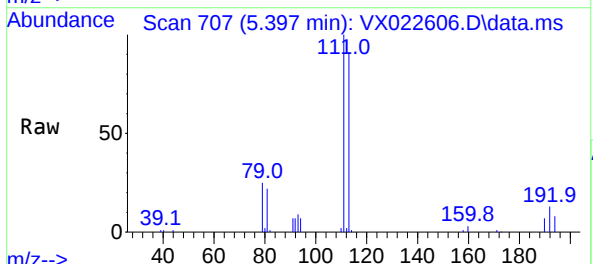


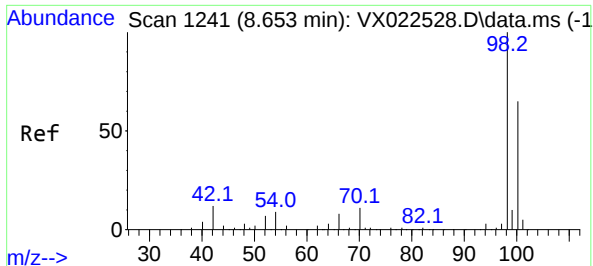

#50
Toluene-d8
Concen: 49.069 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022606.D
Acq: 09 Jun 2021 12:08




Instrument :
MSVOA_X
ClientSampleId :
VX0609WBL01


Tgt Ion: 98 Resp: 149659
Ion Ratio Lower Upper
98 100
100 65.0 51.9 77.9

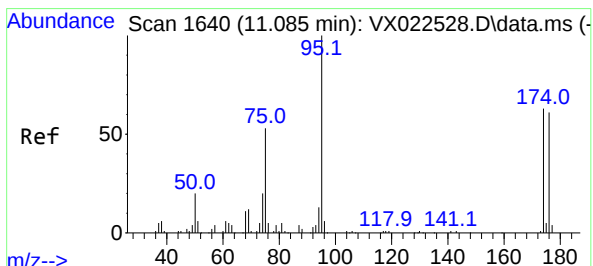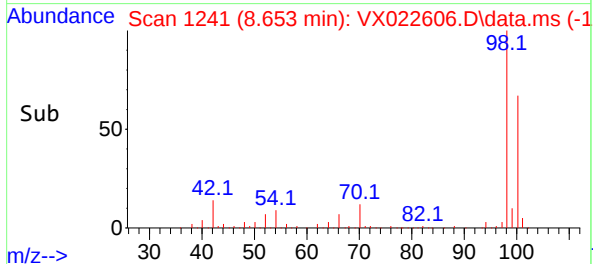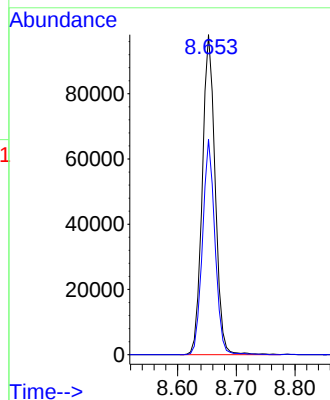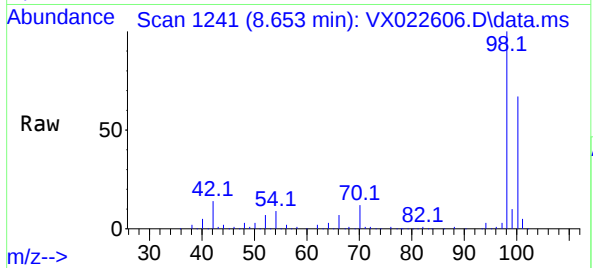

#62
4-Bromofluorobenzene
Concen: 45.093 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022606.D
Acq: 09 Jun 2021 12:08

Tgt Ion: 95 Resp: 51121
Ion Ratio Lower Upper
95 100
174 62.0 0.0 154.6
176 61.4 0.0 155.8


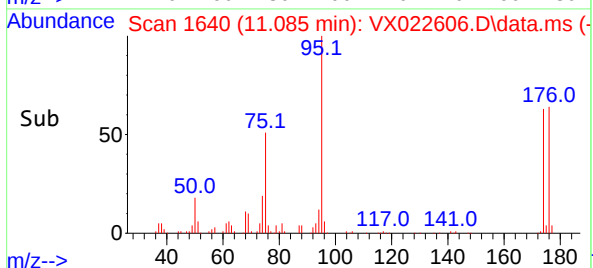
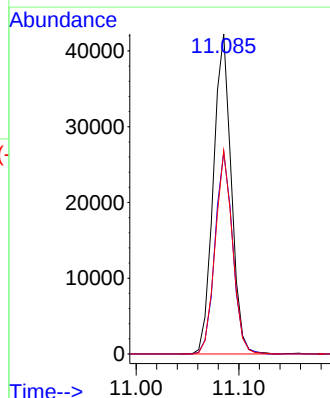
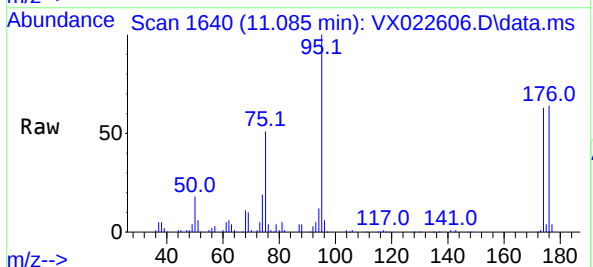


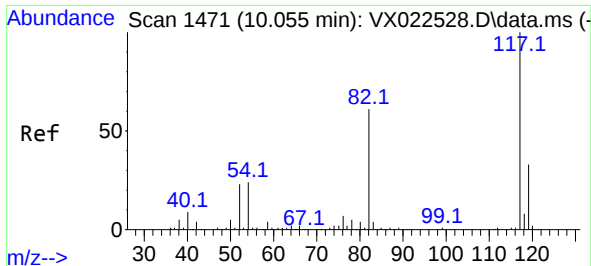

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX022606.D
Acq: 09 Jun 2021 12:08

Instrument :
MSVOA_X
ClientSampleId :
VX0609WBL01

Tgt Ion:117 Resp: 108396
Ion Ratio Lower Upper
117 100
82 60.6 47.4 71.2
119 30.3 26.6 39.8

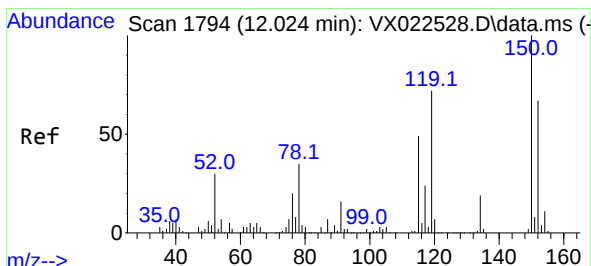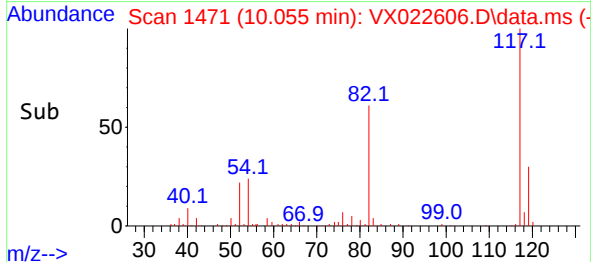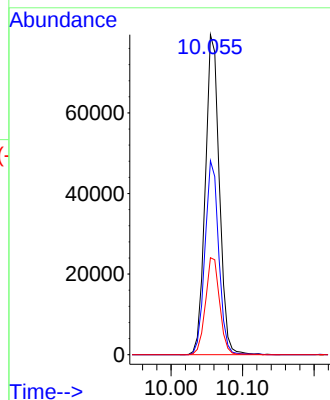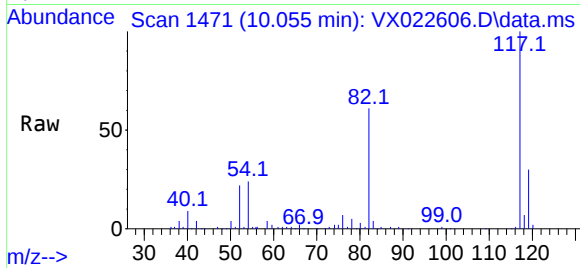

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX022606.D
Acq: 09 Jun 2021 12:08

Tgt Ion:152 Resp: 41354
Ion Ratio Lower Upper
152 100
115 69.2 41.1 123.3
150 158.4 0.0 349.0

