
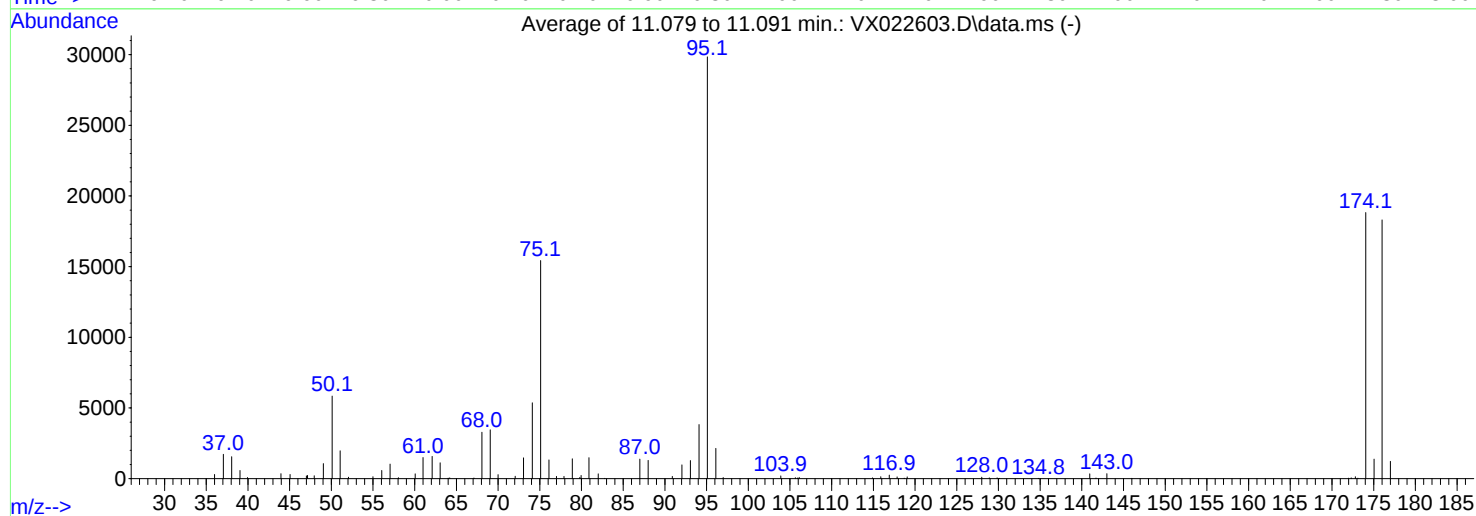


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060921\
 Data File : VX022603.D
 Acq On : 09 Jun 2021 09:18
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060721W.M
 Title : SW846 8260
 Last Update : Mon Jun 07 14:27:50 2021

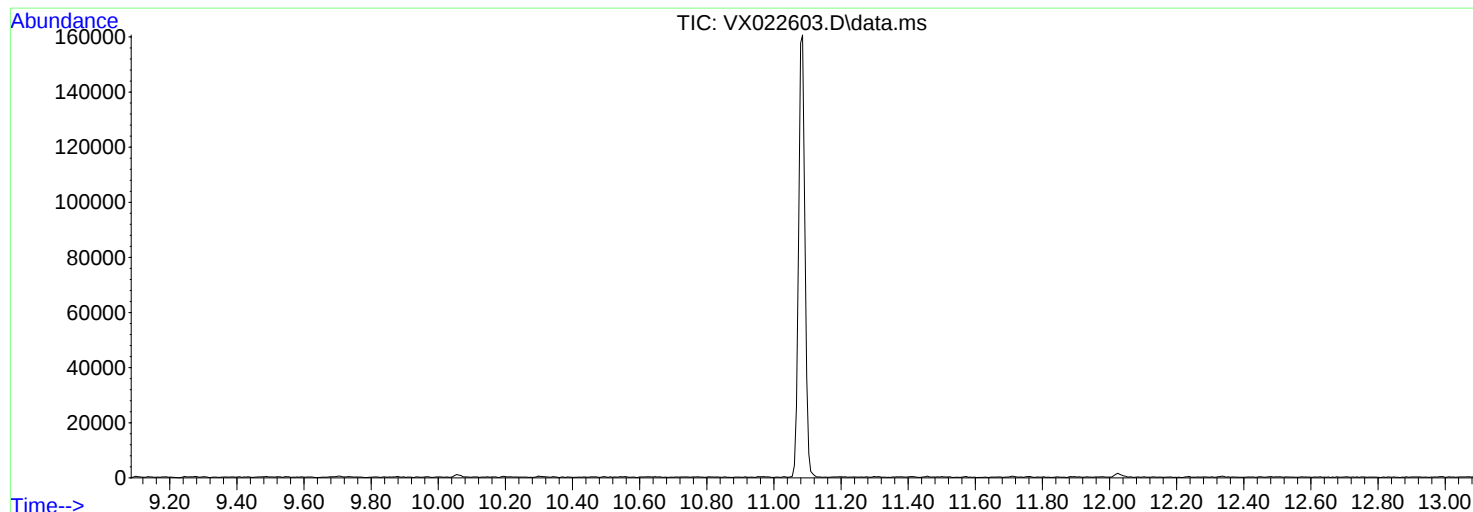

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	5846	PASS
75	95	30	60	51.7	15433	PASS
95	95	100	100	100.0	29843	PASS
96	95	5	9	7.2	2141	PASS
173	174	0.00	2	0.7	131	PASS
174	95	50	100	63.1	18825	PASS
175	174	5	9	7.3	1377	PASS
176	174	95	101	97.2	18300	PASS
177	176	5	9	6.7	1228	PASS