

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060922\
 Data File : VX029355.D
 Acq On : 09 Jun 2022 19:08
 Operator : JC/MD
 Sample : N3237-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TB-20220607

Quant Time: Jun 10 08:10:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 08 03:00:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	209179	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	350075	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	327870	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	177944	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	184926	58.370	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 116.740%	
35) Dibromofluoromethane	5.391	113	163041	54.783	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 109.560%	
50) Toluene-d8	8.653	98	503081	47.795	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 95.600%	
62) 4-Bromofluorobenzene	11.085	95	239068	58.039	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 116.080%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060922\
Data File : VX029355.D
Acq On : 09 Jun 2022 19:08
Operator : JC/MD
Sample : N3237-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220607

Quant Time: Jun 10 08:10:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 08 03:00:38 2022
Response via : Initial Calibration




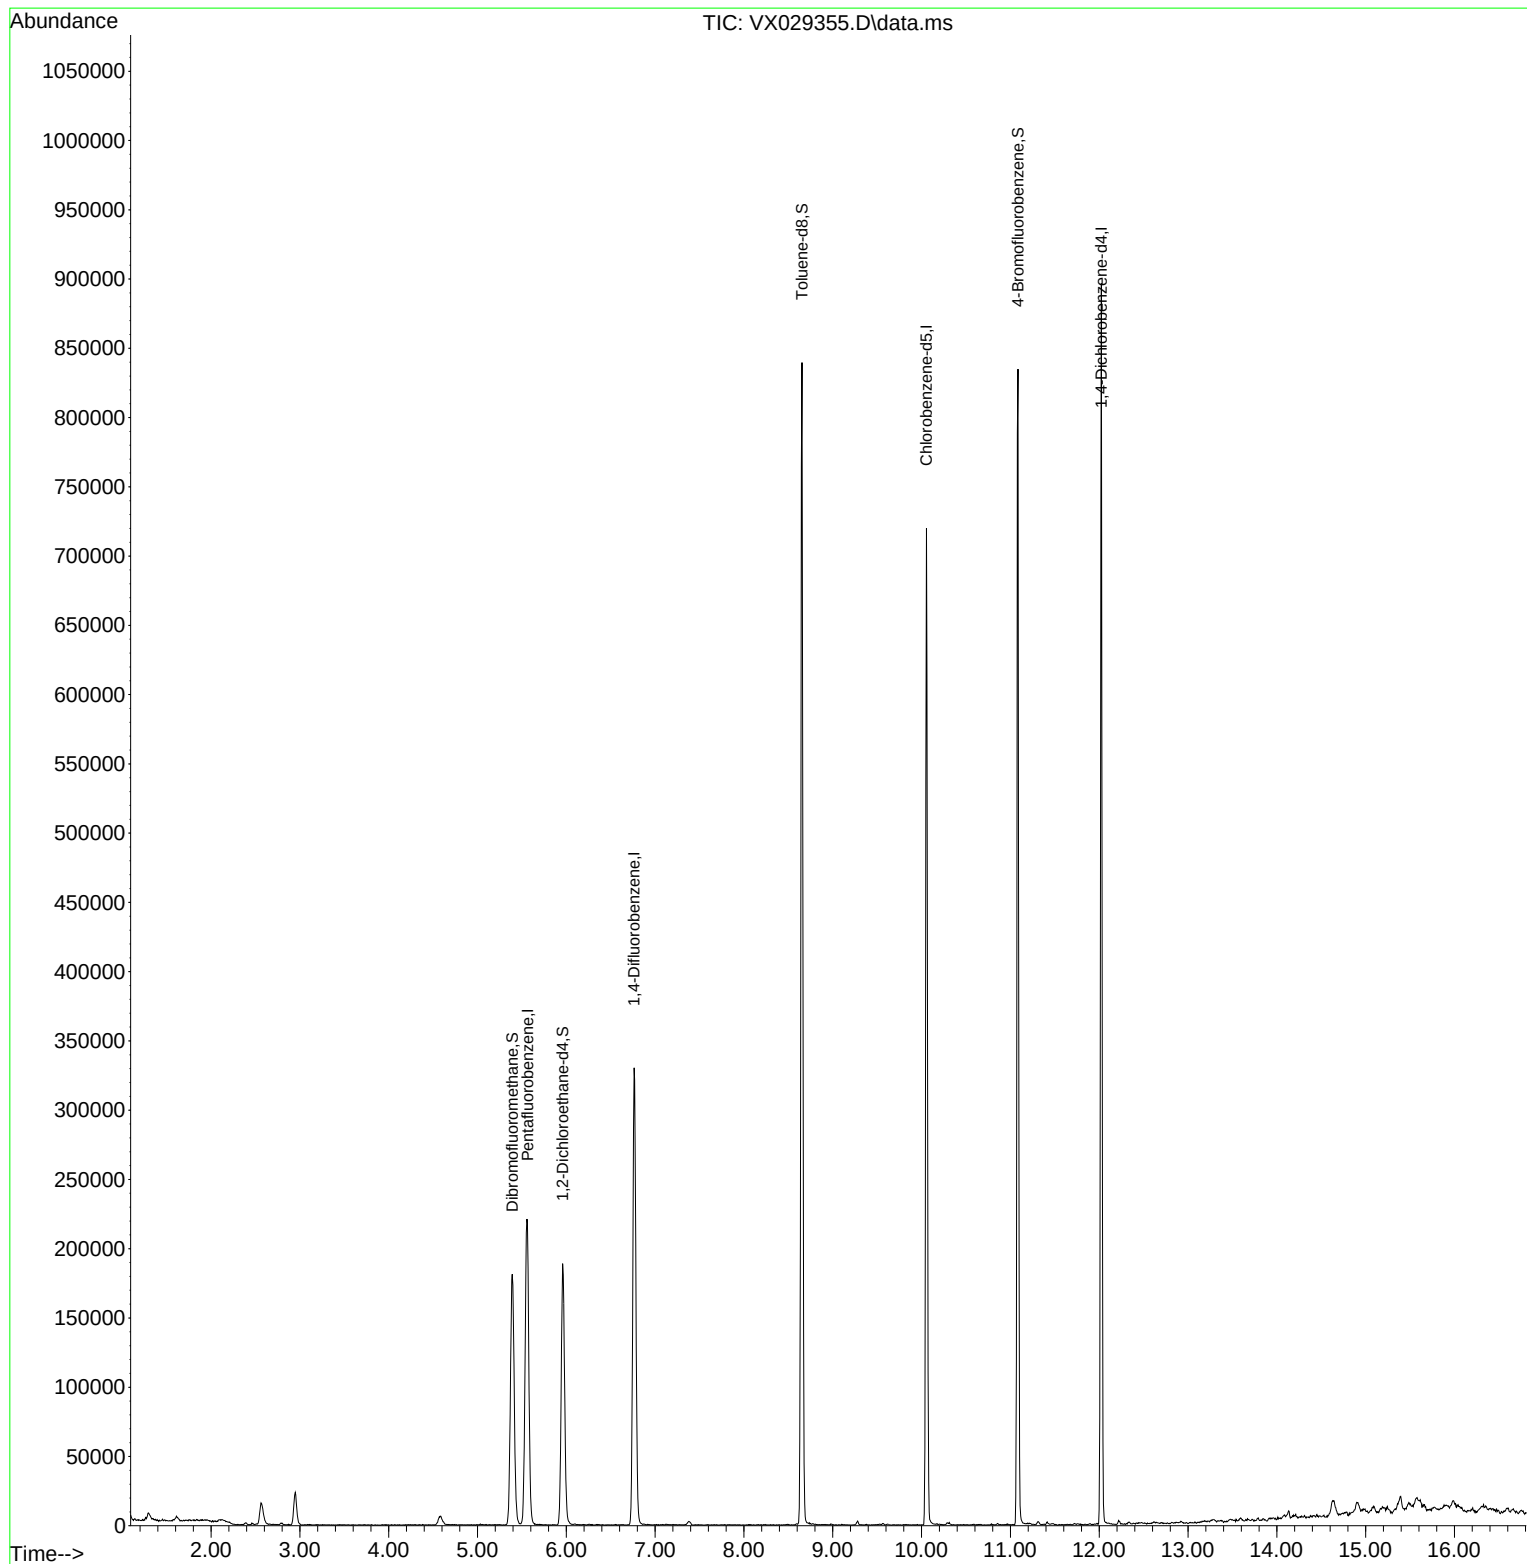


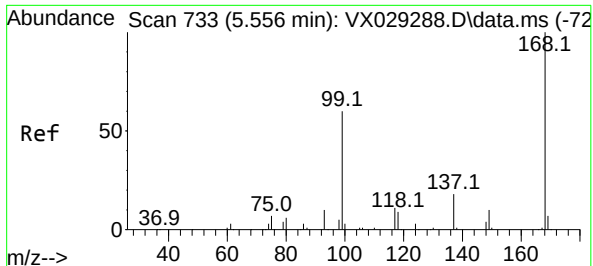

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX029355.D
Acq: 09 Jun 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220607


Tgt Ion:168 Resp: 209179
Ion Ratio Lower Upper
168 100
99 62.8 41.7 62.5#

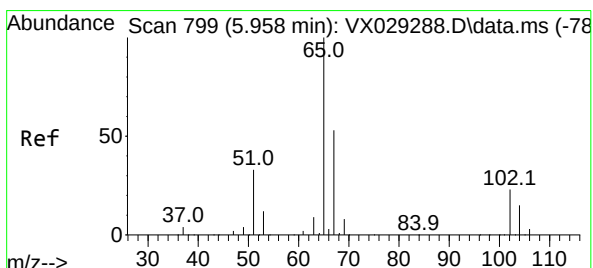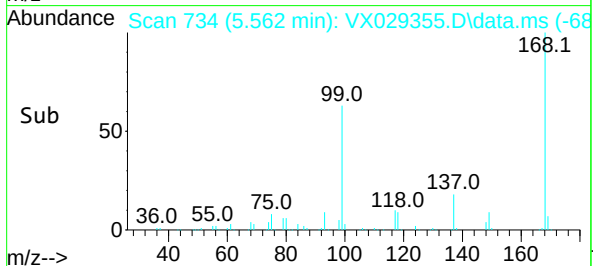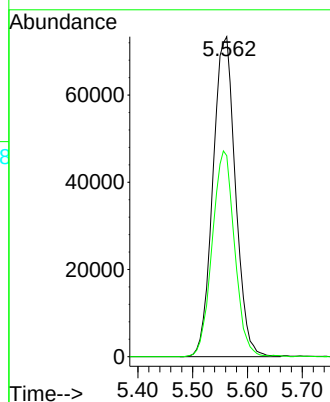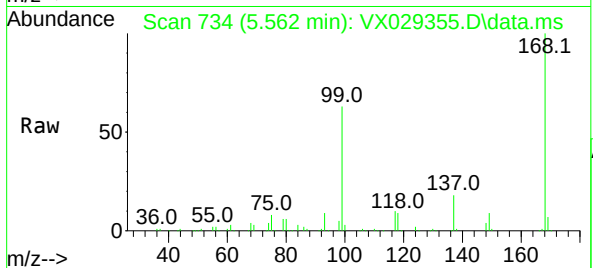

#33
1,2-Dichloroethane-d4
Concen: 58.370 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX029355.D
Acq: 09 Jun 2022 19:08

Tgt Ion: 65 Resp: 184926
Ion Ratio Lower Upper
65 100
67 52.0 0.0 107.4


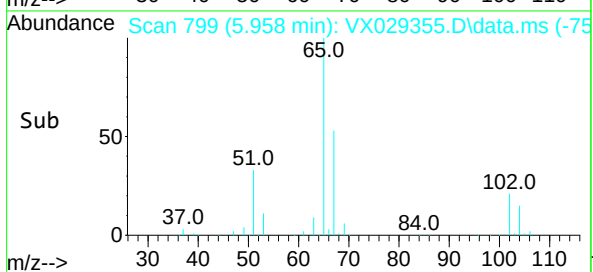
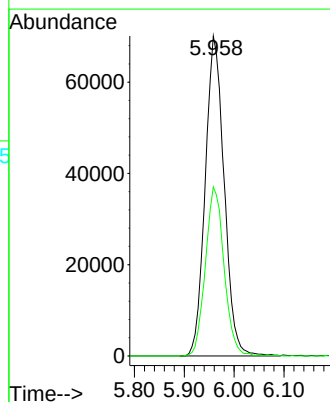
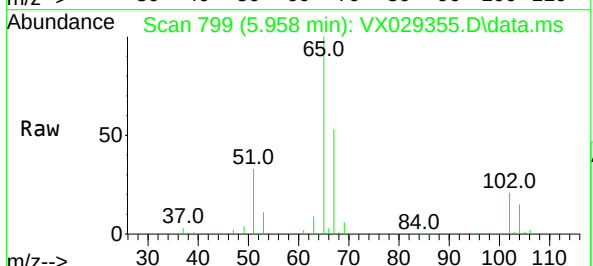


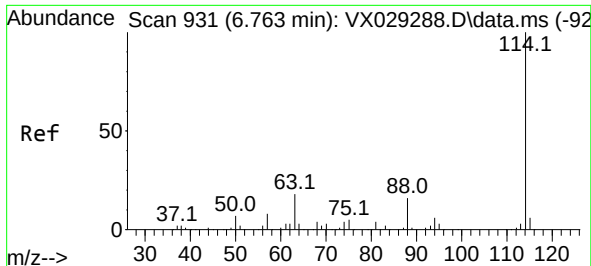

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX029355.D
Acq: 09 Jun 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220607


Tgt Ion:114 Resp: 350075
Ion Ratio Lower Upper
114 100
63 20.7 0.0 36.8
88 16.7 0.0 32.4

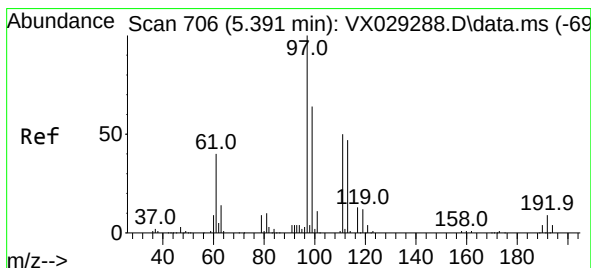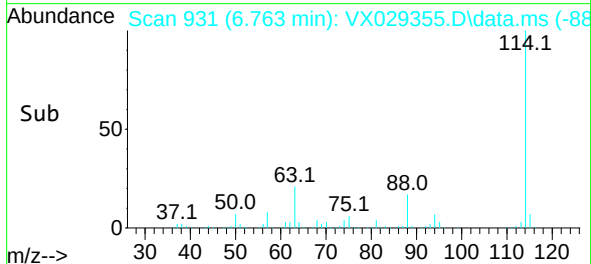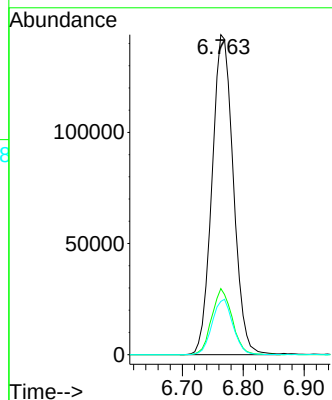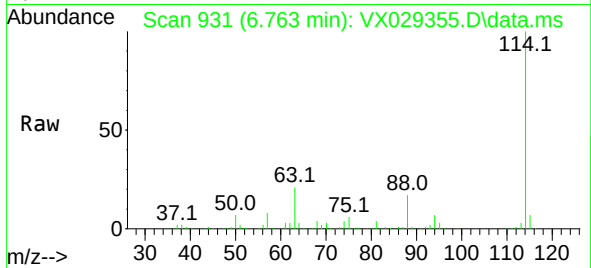

#35
Dibromofluoromethane
Concen: 54.783 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX029355.D
Acq: 09 Jun 2022 19:08

Tgt Ion:113 Resp: 163041
Ion Ratio Lower Upper
113 100
111 102.1 82.8 124.2
192 18.0 16.9 25.3


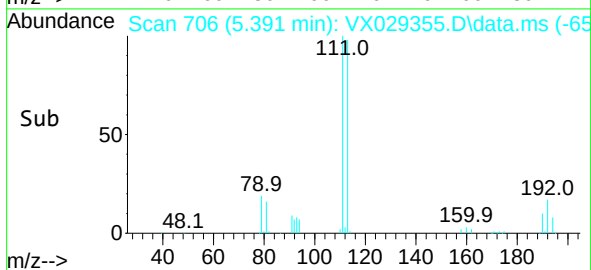
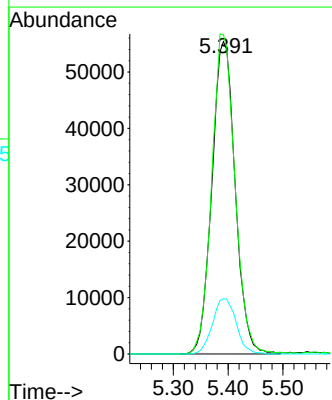
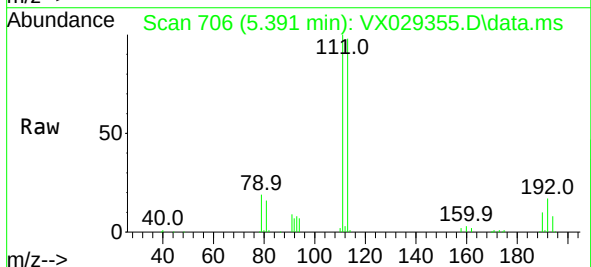


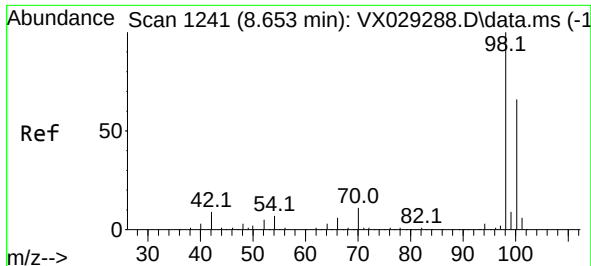

#50
Toluene-d8
Concen: 47.795 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029355.D
Acq: 09 Jun 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220607


Tgt Ion: 98 Resp: 503081
Ion Ratio Lower Upper
98 100
100 65.9 52.6 78.8

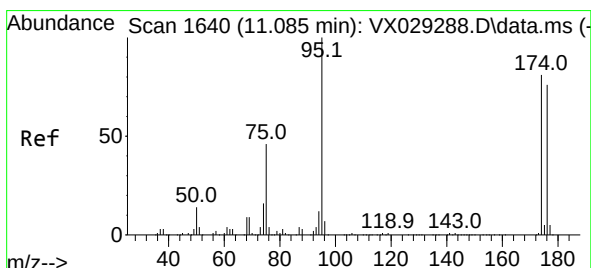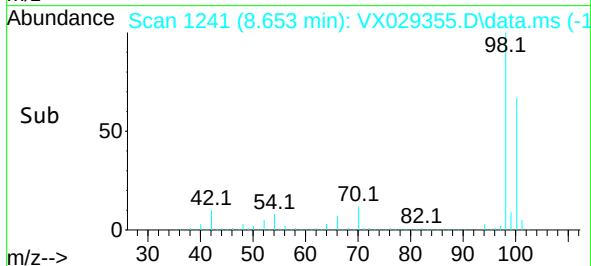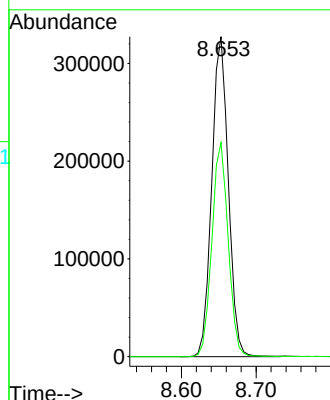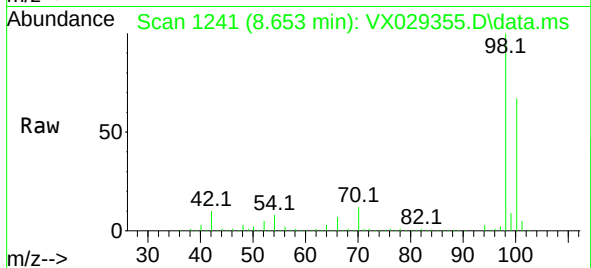

#62
4-Bromofluorobenzene
Concen: 58.039 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.000 min
Lab File: VX029355.D
Acq: 09 Jun 2022 19:08

Tgt Ion: 95 Resp: 239068
Ion Ratio Lower Upper
95 100
174 71.6 0.0 163.0
176 69.2 0.0 155.0


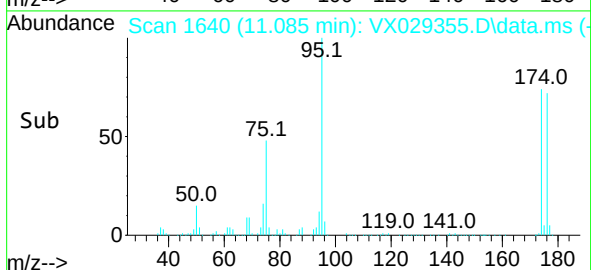
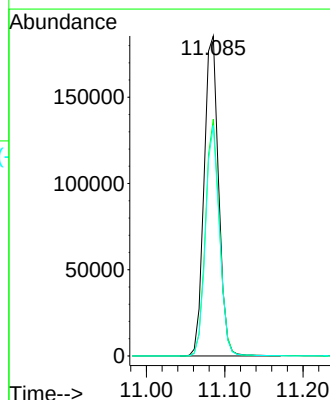
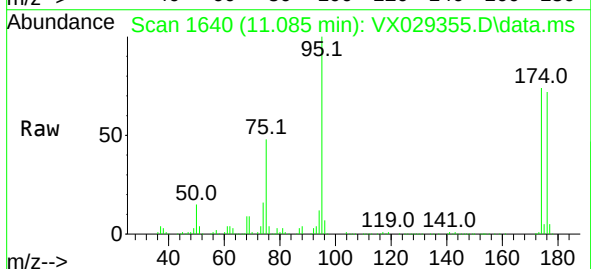


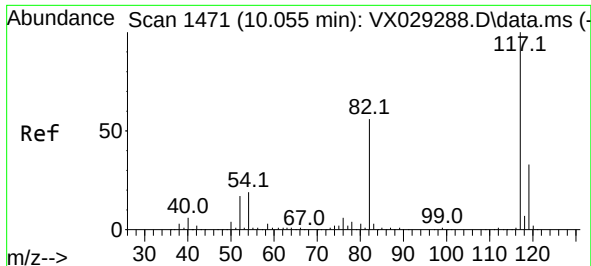

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029355.D
Acq: 09 Jun 2022 19:08

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220607

Tgt Ion:117 Resp: 327870
Ion Ratio Lower Upper
117 100
82 58.0 41.8 62.8
119 32.5 24.8 37.2

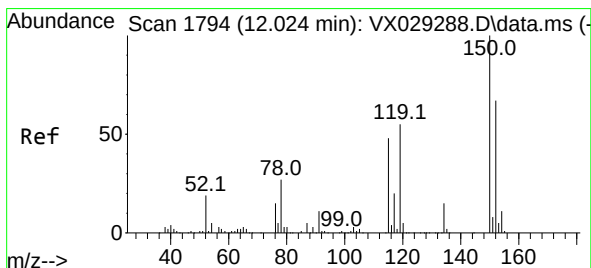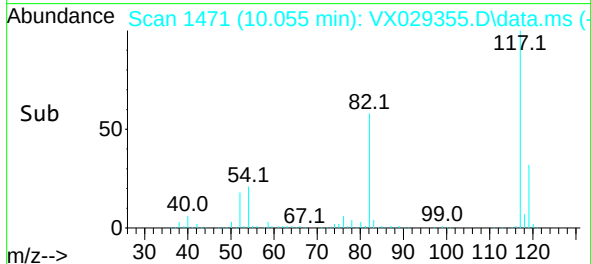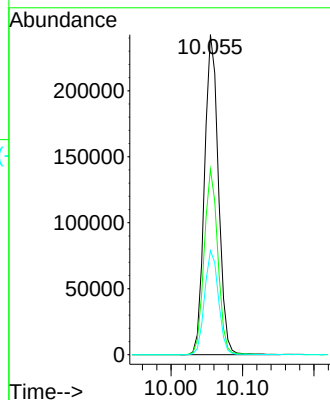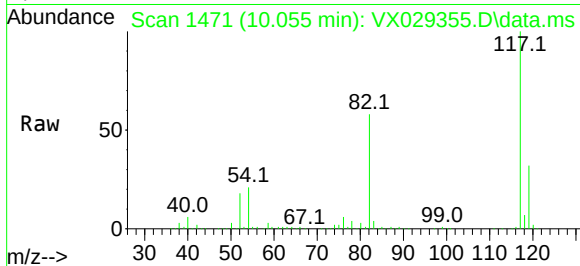

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX029355.D
Acq: 09 Jun 2022 19:08

Tgt Ion:152 Resp: 177944
Ion Ratio Lower Upper
152 100
115 64.3 37.5 112.7
150 155.5 0.0 338.2

