

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036104.D
 Acq On : 09 Jun 2023 13:32
 Operator : JC/MD
 Sample : 03107-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ6

Quant Time: Jun 10 00:14:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 10 00:08:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	217485	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	196853	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	87697	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	62351	42.197	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.400%
7) Chloroethane-d5	1.672	69	52083	45.960	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.920%
11) 1,1-Dichloroethene-d2	2.306	65	33494	44.707	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.420%
21) 2-Butanone-d5	4.458	46	142910	117.994	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	117.990%
24) Chloroform-d	5.050	84	135027	43.823	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.640%
26) 1,2-Dichloroethane-d4	5.952	65	110186	49.008	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.020%
32) Benzene-d6	5.970	84	275014	46.441	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.880%
36) 1,2-Dichloropropane-d6	7.299	67	87541	47.560	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.120%
41) Toluene-d8	8.647	98	244219	44.808	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.620%
43) trans-1,3-Dichloroprop...	8.945	79	35474	40.150	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.300%
47) 2-Hexanone-d5	9.384	63	92769	113.187	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	113.190%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	123038	48.939	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.880%
66) 1,2-Dichlorobenzene-d4	12.317	152	78755	46.254	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.500%
Target Compounds						
					Qvalue	
13) Acetone	2.392	43	5434	4.246	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036104.D
Acq On : 09 Jun 2023 13:32
Operator : JC/MD
Sample : 03107-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ6

Quant Time: Jun 10 00:14:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 10 00:08:47 2023
Response via : Initial Calibration

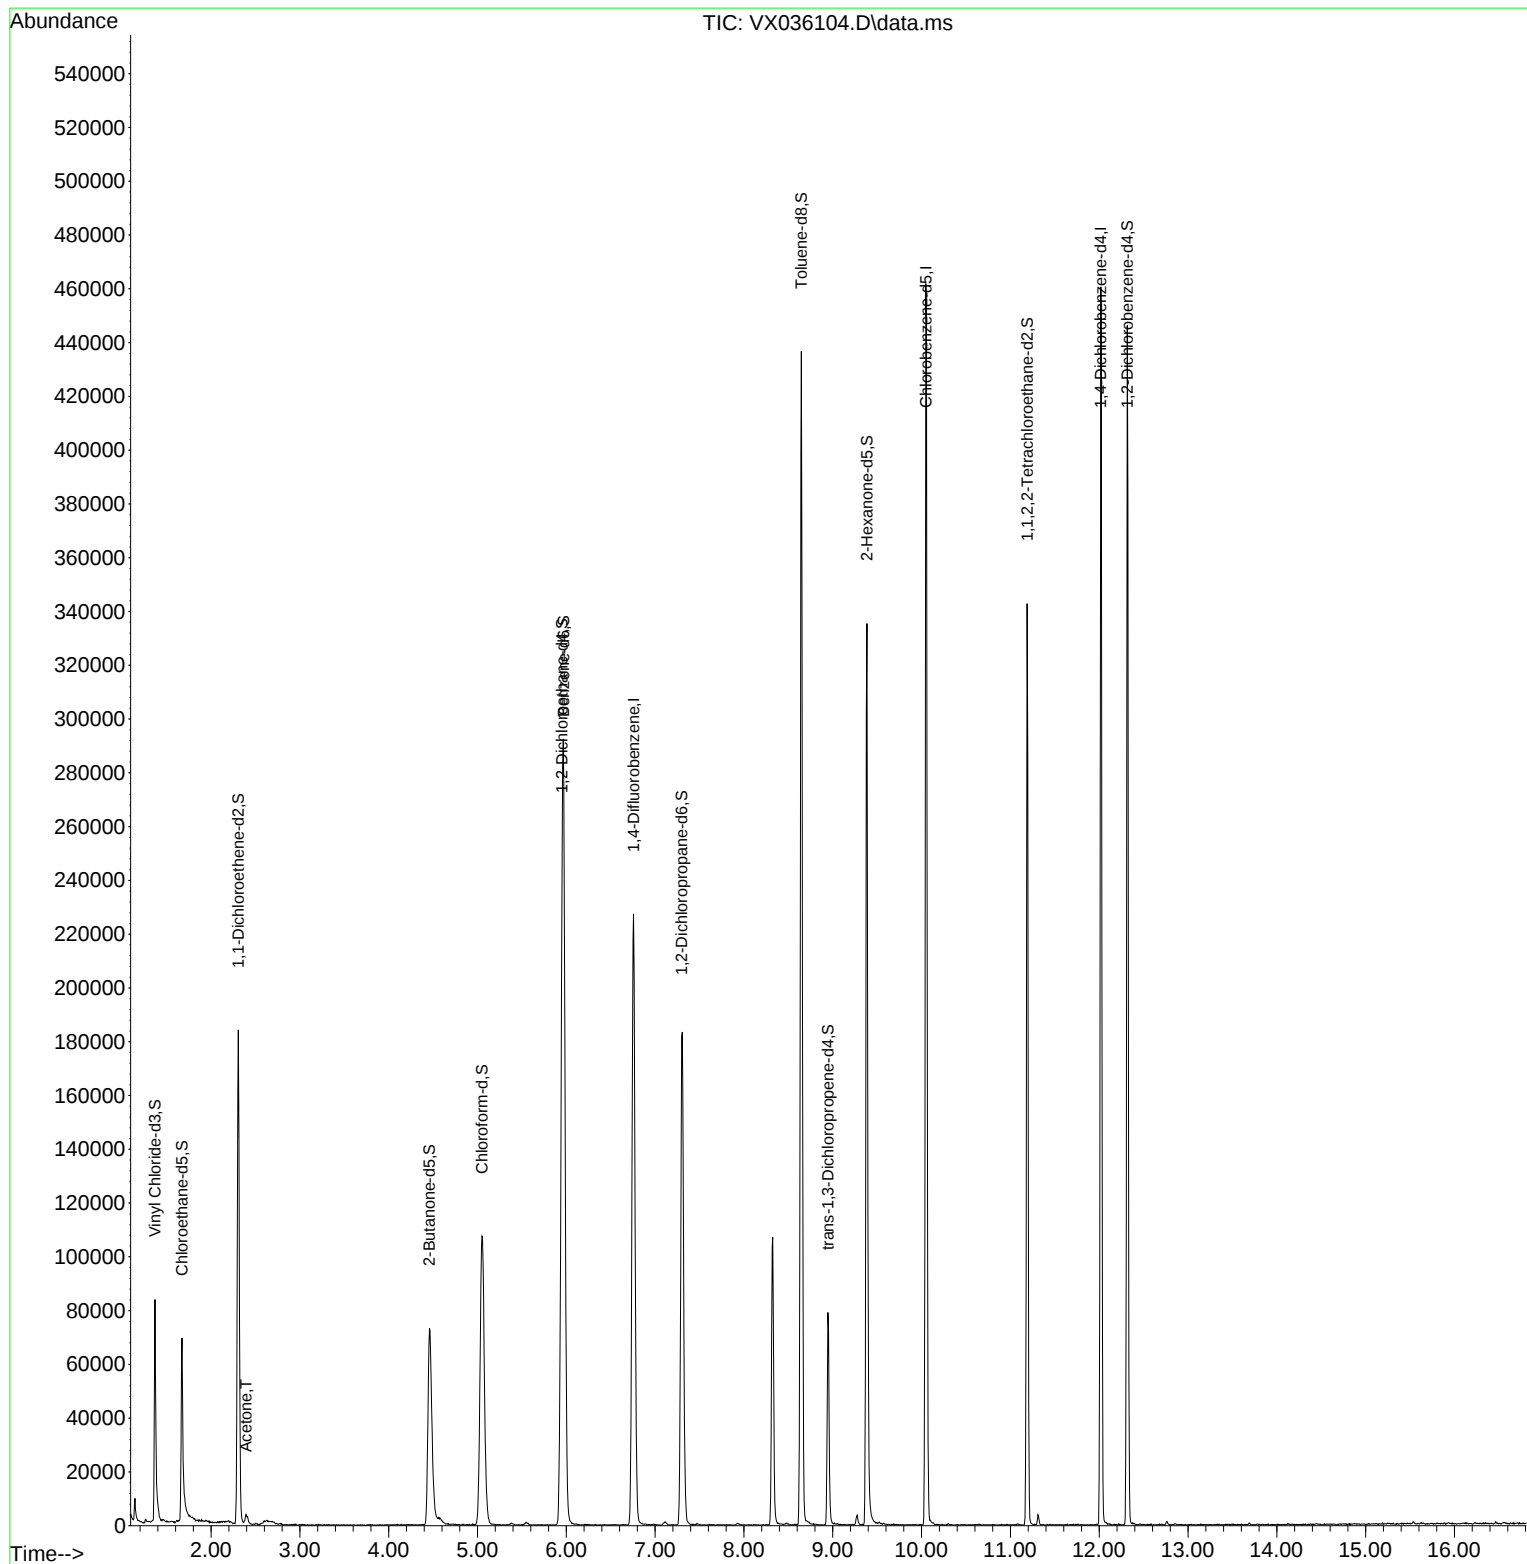

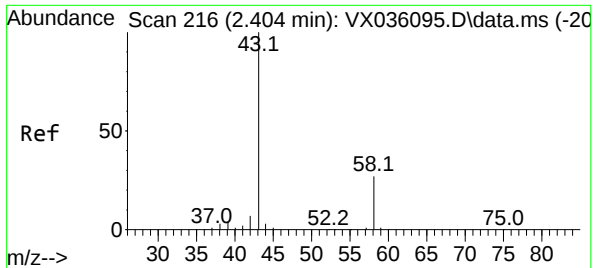

#13
 Acetone
 Concen: 4.246 ug/L
 RT: 2.392 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: VX036104.D
 Acq: 09 Jun 2023 13:32

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ6

Tgt Ion: 43 Resp: 5434
 Ion Ratio Lower Upper
 43 100
 58 28.9 0.0 55.4

