

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036106.D
 Acq On : 09 Jun 2023 14:19
 Operator : JC/MD
 Sample : 03107-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ9

Quant Time: Jun 10 00:14:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 10 00:08:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	279822	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	255614	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	116814	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	85608	45.030	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.060%
7) Chloroethane-d5	1.672	69	71378	48.954	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.900%
11) 1,1-Dichloroethene-d2	2.306	65	45957	47.677	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.360%
21) 2-Butanone-d5	4.477	46	157582	101.124	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.120%
24) Chloroform-d	5.056	84	189662	47.842	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.680%
26) 1,2-Dichloroethane-d4	5.958	65	147455	50.973	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.940%
32) Benzene-d6	5.970	84	375929	48.889	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.780%
36) 1,2-Dichloropropane-d6	7.306	67	119967	50.194	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.380%
41) Toluene-d8	8.647	98	339305	47.943	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.880%
43) trans-1,3-Dichloroprop...	8.952	79	49943	43.532	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.060%
47) 2-Hexanone-d5	9.384	63	107765	101.258	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	101.260%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	158687	48.608	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.220%
66) 1,2-Dichlorobenzene-d4	12.317	152	115824	51.070	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.140%
Target Compounds						
					Qvalue	
13) Acetone	2.410	43	5048	3.066	ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036106.D
Acq On : 09 Jun 2023 14:19
Operator : JC/MD
Sample : 03107-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ9

Quant Time: Jun 10 00:14:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 10 00:08:47 2023
Response via : Initial Calibration

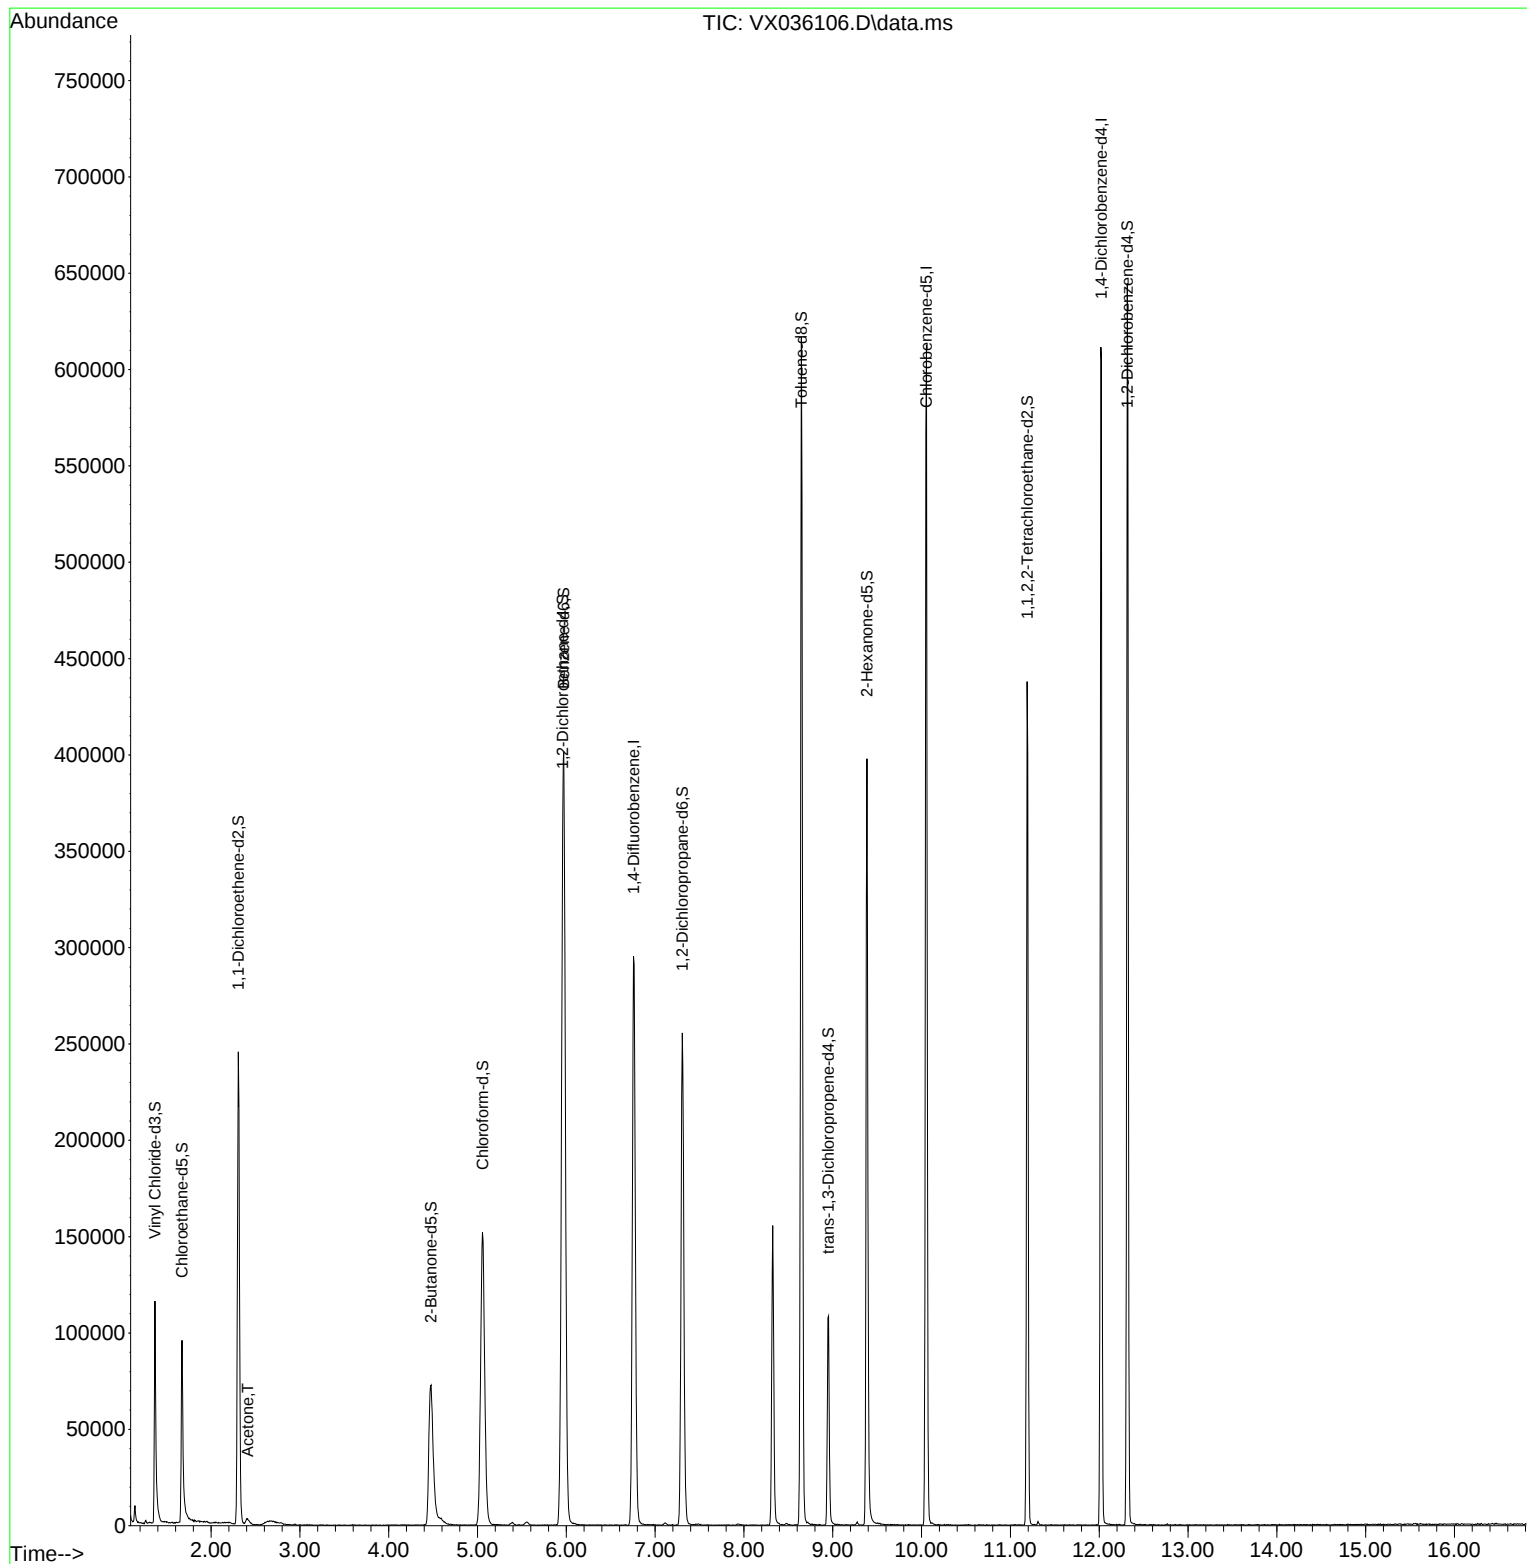

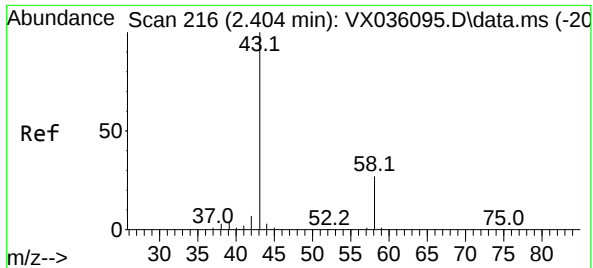

#13
 Acetone
 Concen: 3.066 ug/L
 RT: 2.410 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX036106.D
 Acq: 09 Jun 2023 14:19

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ9

Tgt Ion: 43 Resp: 5048
 Ion Ratio Lower Upper
 43 100
 58 14.1 0.0 55.4

