

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036108.D
 Acq On : 09 Jun 2023 15:05
 Operator : JC/MD
 Sample : 03107-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK2

Quant Time: Jun 10 00:15:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 10 00:08:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	294022	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	271571	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	123385	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	85682	42.892	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.780%
7) Chloroethane-d5	1.672	69	74350	48.530	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.060%
11) 1,1-Dichloroethene-d2	2.306	65	46625	46.034	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.060%
21) 2-Butanone-d5	4.471	46	162076	98.984	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.980%
24) Chloroform-d	5.056	84	195971	47.046	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.100%
26) 1,2-Dichloroethane-d4	5.958	65	156491	51.484	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.960%
32) Benzene-d6	5.976	84	392913	48.095	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.200%
36) 1,2-Dichloropropane-d6	7.305	67	127020	50.022	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.040%
41) Toluene-d8	8.647	98	352736	46.912	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.820%
43) trans-1,3-Dichloroprop...	8.952	79	52763	43.287	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.580%
47) 2-Hexanone-d5	9.384	63	112314	99.331	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.330%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	168081	48.461	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.920%
66) 1,2-Dichlorobenzene-d4	12.317	152	121133	50.566	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.140%
Target Compounds						
12) 1,1-Dichloroethene	2.319	96	4834	2.474	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036108.D
Acq On : 09 Jun 2023 15:05
Operator : JC/MD
Sample : 03107-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK2

Quant Time: Jun 10 00:15:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM060623WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 10 00:08:47 2023
Response via : Initial Calibration

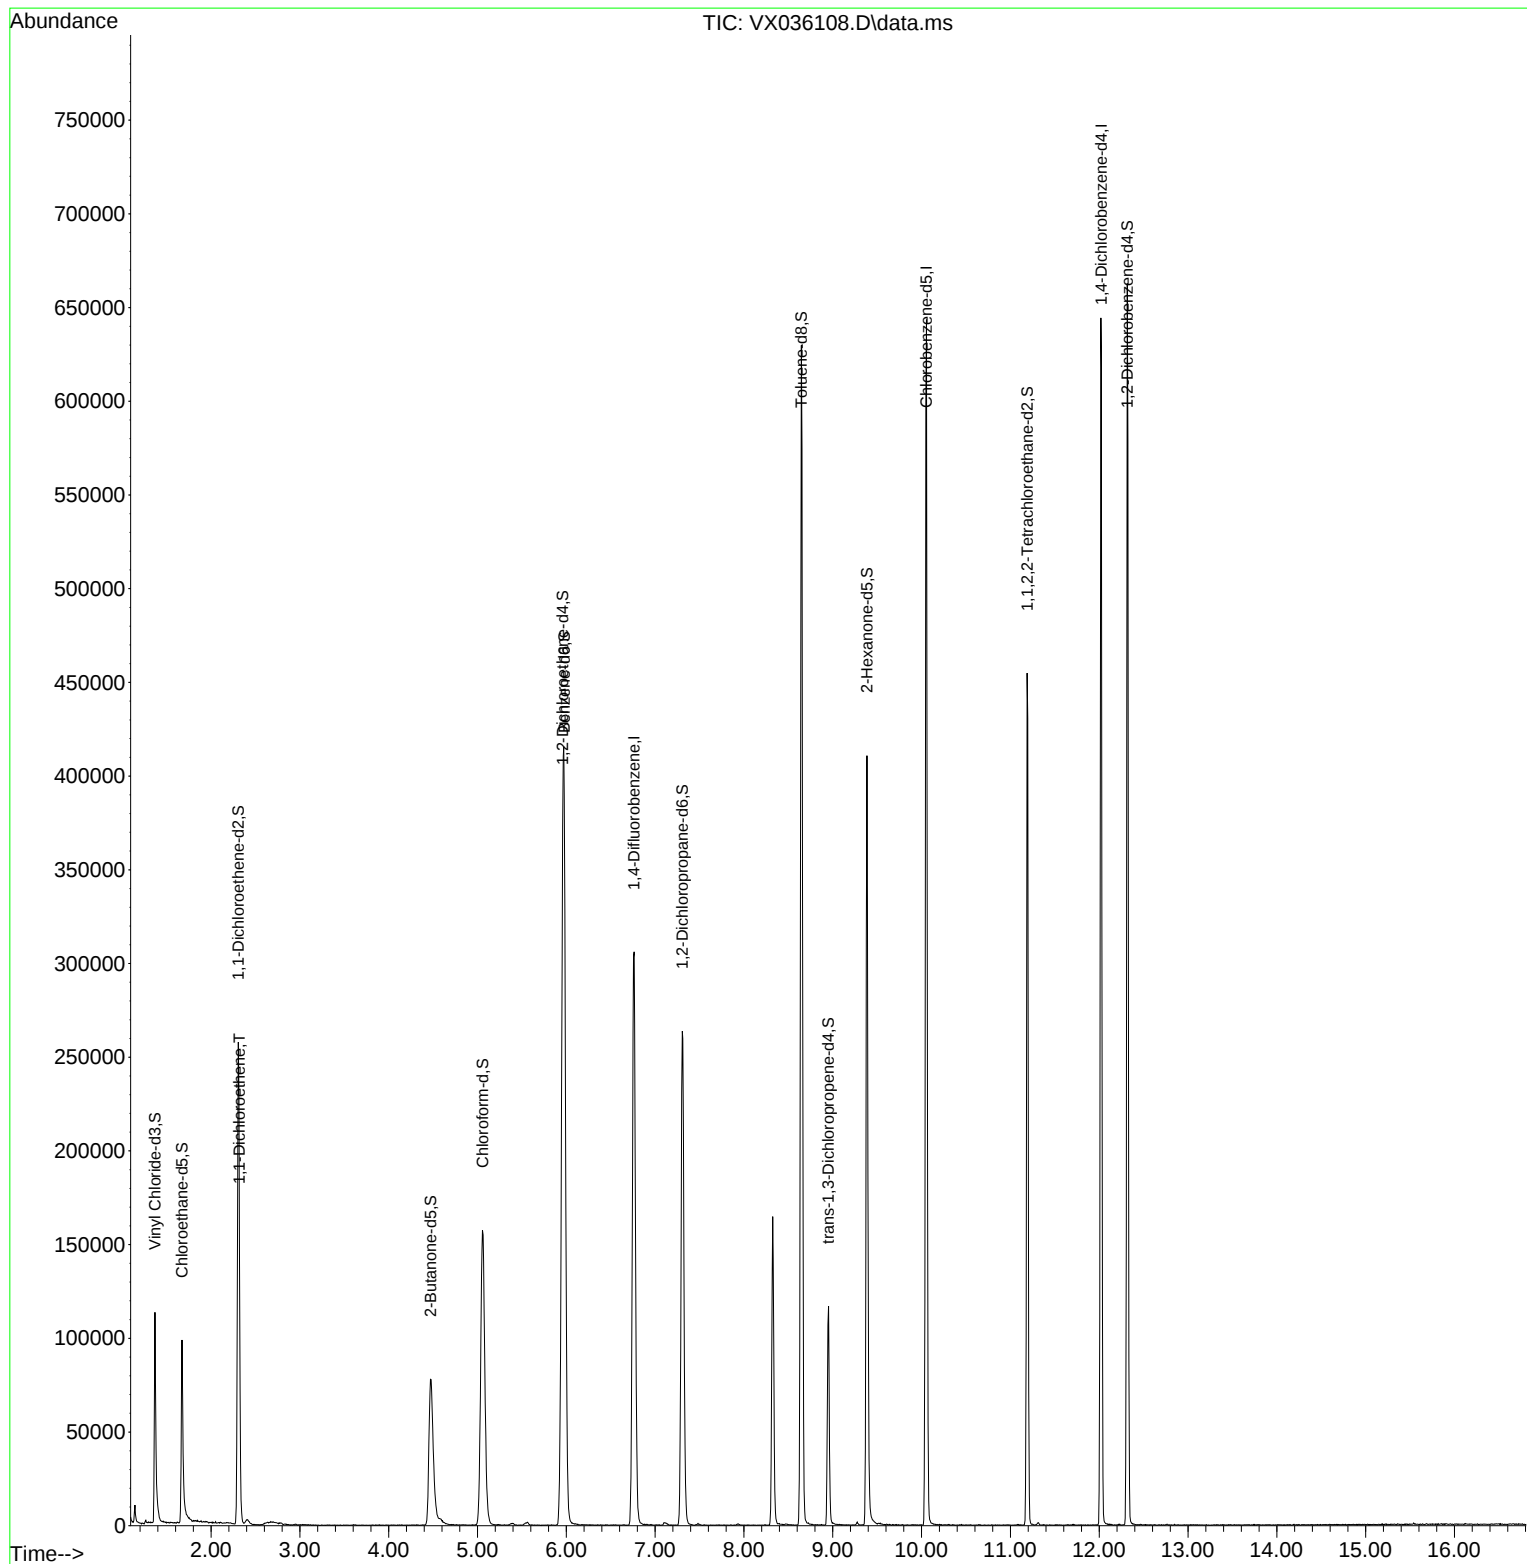

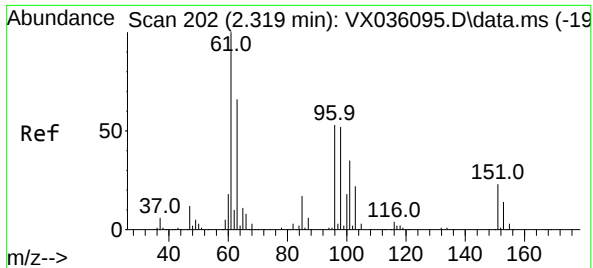

#12
 1,1-Dichloroethene
 Concen: 2.474 ug/L
 RT: 2.319 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VX036108.D
 Acq: 09 Jun 2023 15:05

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK2

Tgt Ion: 96 Resp: 4834
 Ion Ratio Lower Upper
 96 100
 61 352.8 132.5 246.1#
 63 1668.5 95.1 176.7#

