

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036110.D
 Acq On : 09 Jun 2023 15:52
 Operator : JC/MD
 Sample : 03107-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK5

Quant Time: Jun 10 00:16:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 10 00:08:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	289737	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	268479	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	120648	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	85510	43.439	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.880%
7) Chloroethane-d5	1.672	69	73459	48.658	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.320%
11) 1,1-Dichloroethene-d2	2.306	65	46655	46.745	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.500%
21) 2-Butanone-d5	4.471	46	162578	100.759	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.760%
24) Chloroform-d	5.056	84	195003	47.506	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.020%
26) 1,2-Dichloroethane-d4	5.958	65	151973	50.737	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.480%
32) Benzene-d6	5.976	84	388949	48.158	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.320%
36) 1,2-Dichloropropane-d6	7.306	67	122535	48.812	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.620%
41) Toluene-d8	8.647	98	350061	47.092	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.180%
43) trans-1,3-Dichloroprop...	8.952	79	51215	42.501	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.000%
47) 2-Hexanone-d5	9.384	63	111038	99.334	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.330%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	163889	47.796	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	12.317	152	118694	50.672	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.340%
Target Compounds						
13) Acetone	2.404	43	6440	3.778	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036110.D
Acq On : 09 Jun 2023 15:52
Operator : JC/MD
Sample : 03107-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK5

Quant Time: Jun 10 00:16:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM060623WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 10 00:08:47 2023
Response via : Initial Calibration

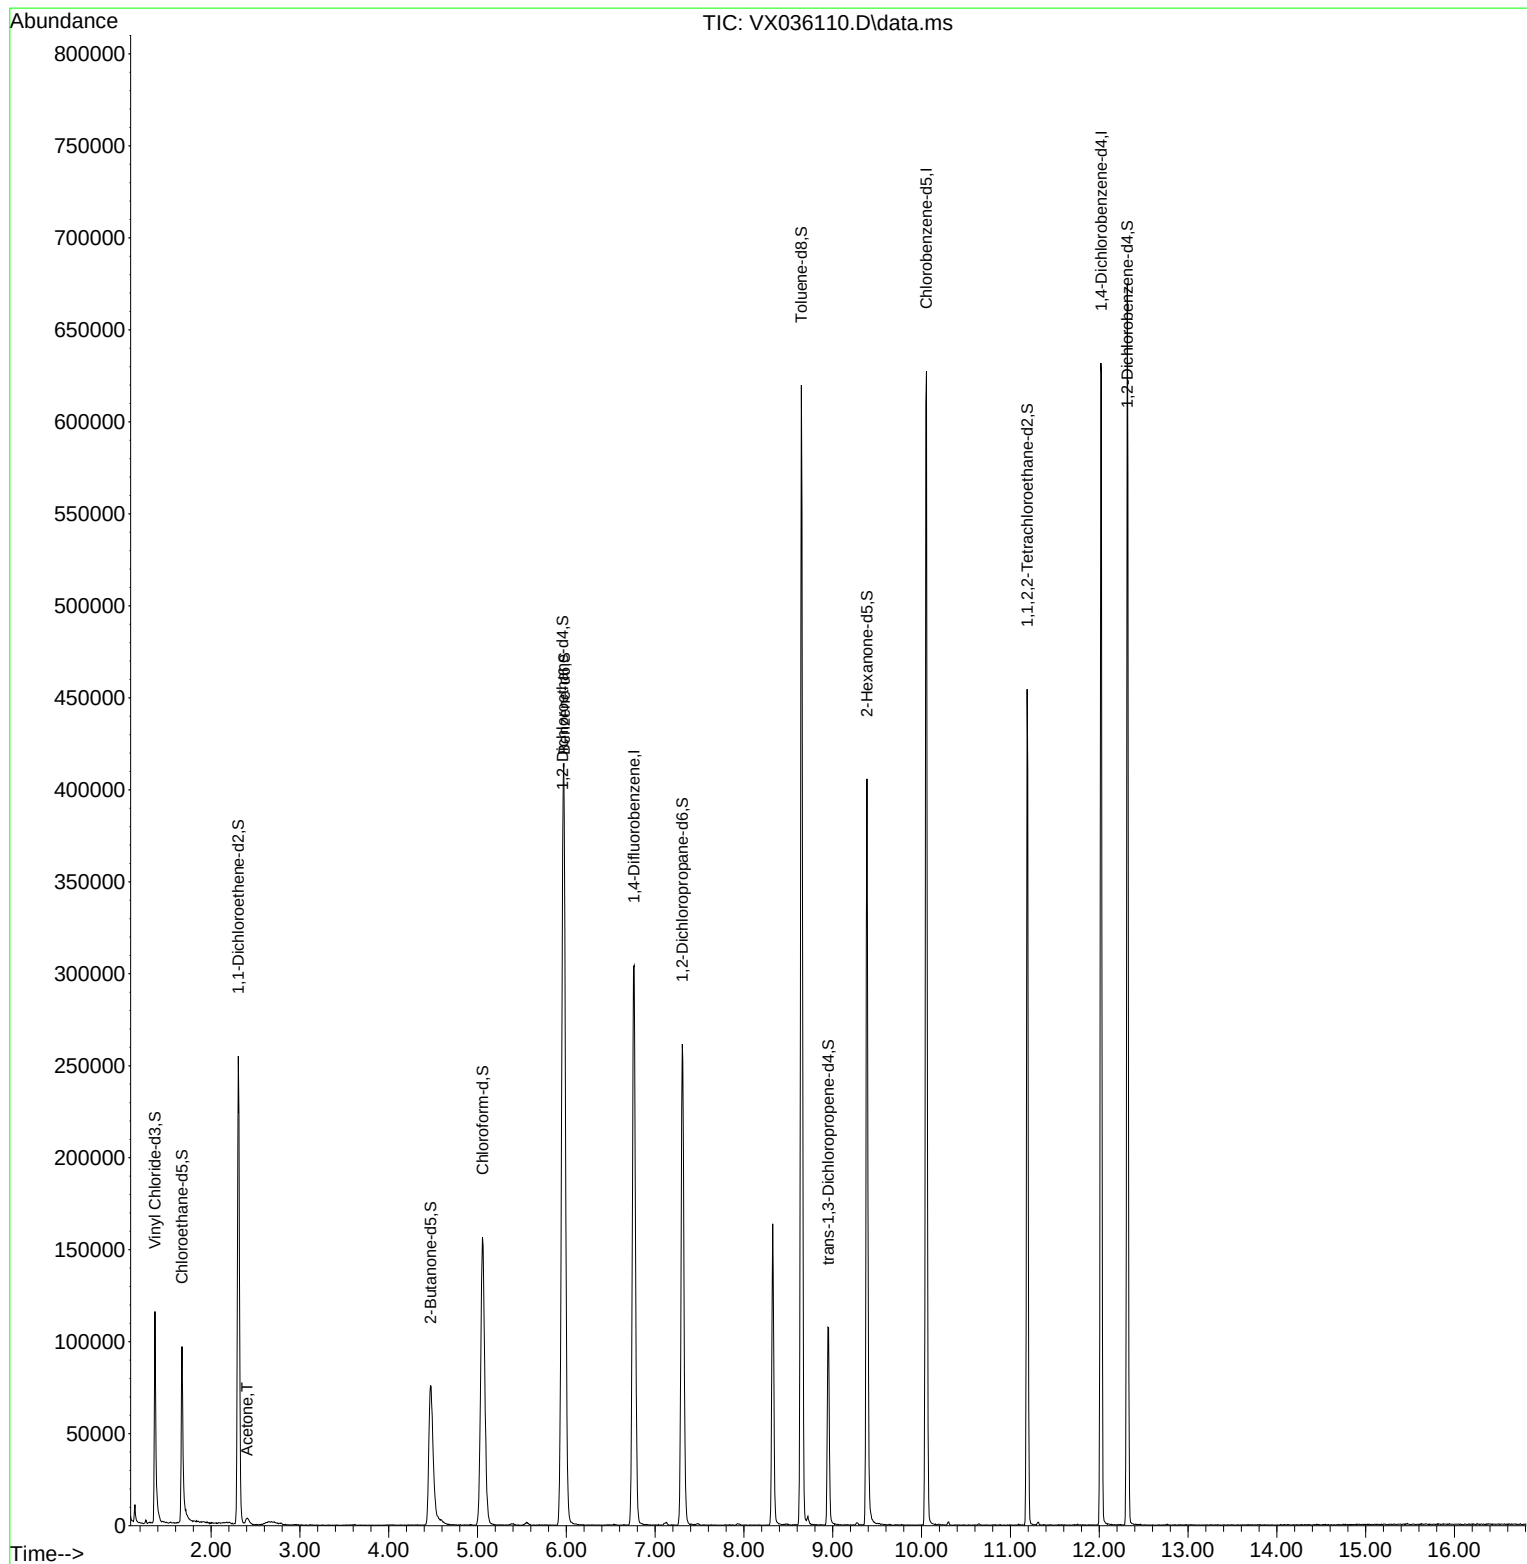

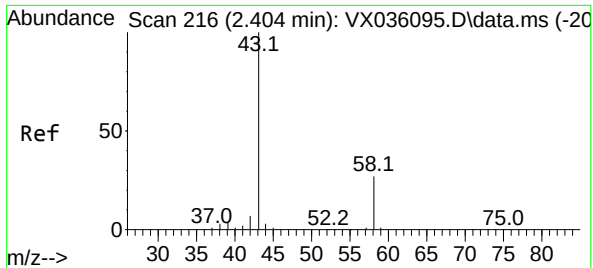

#13
 Acetone
 Concen: 3.778 ug/L
 RT: 2.404 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX036110.D
 Acq: 09 Jun 2023 15:52

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK5

Tgt Ion: 43 Resp: 6440
 Ion Ratio Lower Upper
 43 100
 58 27.3 0.0 55.4

