

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036096.D
 Acq On : 09 Jun 2023 09:10
 Operator : JC/MD
 Sample : VX0609WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK632

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	9804	10001	0.72%	0.097%
2	1.264	27	29	31	rBV2	1404	1224	0.09%	0.012%
3	1.368	42	46	59	rBV	127355	156059	11.29%	1.519%
4	1.673	91	96	113	rBV	106150	163604	11.84%	1.593%
5	2.307	193	200	210	rBV	277038	436506	31.58%	4.250%
6	2.788	276	279	283	rBV4	1839	2395	0.17%	0.023%
7	2.947	299	305	310	rVB4	853	1948	0.14%	0.019%
8	3.093	325	329	333	rBV4	475	730	0.05%	0.007%
9	3.227	348	351	354	rBV2	205	248	0.02%	0.002%
10	3.258	354	356	357	rVB	305	202	0.01%	0.002%
11	3.337	366	369	370	rBV2	235	285	0.02%	0.003%
12	3.380	373	376	377	rBV	208	157	0.01%	0.002%
13	3.434	383	385	387	rBV	269	255	0.02%	0.002%
14	3.459	387	389	392	rVB2	208	163	0.01%	0.002%
15	3.489	392	394	395	rBV	224	174	0.01%	0.002%
16	3.526	398	400	402	rBV2	177	177	0.01%	0.002%
17	3.605	410	413	417	rBV2	246	366	0.03%	0.004%
18	3.642	417	419	422	rVV2	181	217	0.02%	0.002%
19	3.739	430	435	437	rVB2	316	488	0.04%	0.005%
20	3.812	444	447	450	rVB2	205	208	0.02%	0.002%
21	3.867	454	456	459	rVB	330	209	0.02%	0.002%
22	3.898	459	461	463	rBV2	218	190	0.01%	0.002%
23	4.148	500	502	504	rBV2	239	183	0.01%	0.002%
24	4.471	542	555	571	rBV2	83391	303399	21.95%	2.954%
25	4.867	618	620	622	rBV3	298	319	0.02%	0.003%
26	5.050	639	650	669	rBV	174608	561237	40.60%	5.465%
27	5.306	688	692	693	rVB2	340	418	0.03%	0.004%
28	5.397	698	707	712	rBV4	1241	3285	0.24%	0.032%
29	5.550	723	732	742	rBV3	2368	6339	0.46%	0.062%
30	5.836	777	779	781	rVB	282	153	0.01%	0.001%
31	5.964	787	800	819	rBV2	458220	1382196	100.00%	13.458%
32	6.227	842	843	845	rVB	340	147	0.01%	0.001%
33	6.263	845	849	852	rBV2	204	292	0.02%	0.003%
34	6.306	855	856	859	rVB	271	199	0.01%	0.002%
35	6.422	872	875	876	rVB	346	277	0.02%	0.003%
36	6.452	876	880	881	rBV3	358	383	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036096.D
 Acq On : 09 Jun 2023 09:10
 Operator : JC/MD
 Sample : VX0609WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK632

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.538	890	894	896	rBV3	285	527	0.04%	0.005%
38	6.617	904	907	910	rBV2	313	368	0.03%	0.004%
39	6.757	921	930	945	rBV	333874	802679	58.07%	7.815%
40	7.074	980	982	983	rBV	329	151	0.01%	0.001%
41	7.111	983	988	996	rVB4	1814	4008	0.29%	0.039%
42	7.172	996	998	1000	rBV	183	176	0.01%	0.002%
43	7.306	1010	1020	1035	rVV	299972	646926	46.80%	6.299%
44	7.665	1078	1079	1081	rBV	201	159	0.01%	0.002%
45	7.879	1113	1114	1117	rBV2	204	199	0.01%	0.002%
46	7.928	1119	1122	1129	rVB3	741	1311	0.09%	0.013%
47	8.190	1162	1165	1166	rBV	300	371	0.03%	0.004%
48	8.263	1175	1177	1179	rBV2	248	330	0.02%	0.003%
49	8.324	1180	1187	1197	rVV	186544	306138	22.15%	2.981%
50	8.647	1233	1240	1249	rBV	699072	1090003	78.86%	10.613%
51	8.866	1274	1276	1277	rBV	290	141	0.01%	0.001%
52	8.946	1283	1289	1299	rBV	135752	203758	14.74%	1.984%
53	9.098	1312	1314	1315	rBV	270	196	0.01%	0.002%
54	9.275	1339	1343	1347	rBV2	582	822	0.06%	0.008%
55	9.385	1355	1361	1377	rBV	466961	670158	48.49%	6.525%
56	9.695	1409	1412	1419	rVB2	1431	2279	0.16%	0.022%
57	9.817	1431	1432	1437	rBV2	214	328	0.02%	0.003%
58	10.049	1464	1470	1491	rBV	680913	962128	69.61%	9.368%
59	10.189	1491	1493	1494	rBV2	571	568	0.04%	0.006%
60	10.232	1499	1500	1504	rVB2	382	375	0.03%	0.004%
61	10.299	1507	1511	1518	rBV4	763	1213	0.09%	0.012%
62	10.445	1533	1535	1539	rBV2	245	274	0.02%	0.003%
63	10.488	1539	1542	1545	rBV2	198	246	0.02%	0.002%
64	10.567	1553	1555	1556	rBV	206	186	0.01%	0.002%
65	10.616	1561	1563	1564	rVV	341	186	0.01%	0.002%
66	10.647	1564	1568	1576	rVV4	831	1781	0.13%	0.017%
67	10.744	1582	1584	1585	rBV2	260	139	0.01%	0.001%
68	10.787	1589	1591	1593	rBV	290	188	0.01%	0.002%
69	10.836	1596	1599	1601	rBV2	270	285	0.02%	0.003%
70	10.964	1618	1620	1626	rVB3	857	805	0.06%	0.008%
71	11.061	1634	1636	1637	rBV	205	137	0.01%	0.001%
72	11.079	1637	1639	1642	rVB3	814	693	0.05%	0.007%
73	11.189	1652	1657	1667	rBV	513445	651910	47.16%	6.347%
74	11.293	1673	1674	1675	rBV	289	169	0.01%	0.002%
75	11.396	1689	1691	1693	rVB2	164	138	0.01%	0.001%
76	11.457	1696	1701	1703	rVB3	511	757	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036096.D
 Acq On : 09 Jun 2023 09:10
 Operator : JC/MD
 Sample : VX0609WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK632

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.628	1725	1729	1732	rBV2	260	316	0.02%	0.003%
78	11.707	1739	1742	1744	rBV2	614	549	0.04%	0.005%
79	11.750	1747	1749	1753	rVB3	509	731	0.05%	0.007%
80	11.780	1753	1754	1756	rBV	244	214	0.02%	0.002%
81	11.969	1782	1785	1788	rBV	1267	1154	0.08%	0.011%
82	12.018	1788	1793	1807	rVV	736122	923601	66.82%	8.993%
83	12.317	1837	1842	1857	rVB	739586	941281	68.10%	9.165%
84	12.957	1946	1947	1948	rVB	392	143	0.01%	0.001%
85	12.975	1948	1950	1951	rBV	214	146	0.01%	0.001%
86	13.110	1969	1972	1979	rBV4	1412	2037	0.15%	0.020%
87	13.341	2009	2010	2015	rBV2	223	270	0.02%	0.003%
88	13.585	2047	2050	2054	rBV	1673	1945	0.14%	0.019%
89	13.670	2062	2064	2065	rBV2	269	165	0.01%	0.002%
90	13.774	2079	2081	2085	rVB	2132	2549	0.18%	0.025%
91	13.908	2099	2103	2104	rBV2	282	427	0.03%	0.004%
92	13.963	2108	2112	2117	rVB4	1872	2838	0.21%	0.028%
93	14.152	2141	2143	2147	rBV2	197	328	0.02%	0.003%
94	14.189	2147	2149	2151	rVB	385	287	0.02%	0.003%
95	14.457	2191	2193	2197	rBV2	532	552	0.04%	0.005%
96	14.695	2230	2232	2235	rVB	329	275	0.02%	0.003%
97	15.536	2368	2370	2375	rVB5	915	1377	0.10%	0.013%
98	15.761	2405	2407	2409	rVB	640	375	0.03%	0.004%
99	15.999	2444	2446	2450	rBV3	528	778	0.06%	0.008%
100	16.365	2505	2506	2508	rVB2	472	262	0.02%	0.003%




Sum of corrected areas: 10270439

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036096.D
Acq On : 09 Jun 2023 09:10
Operator : JC/MD
Sample : VX0609WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK632

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

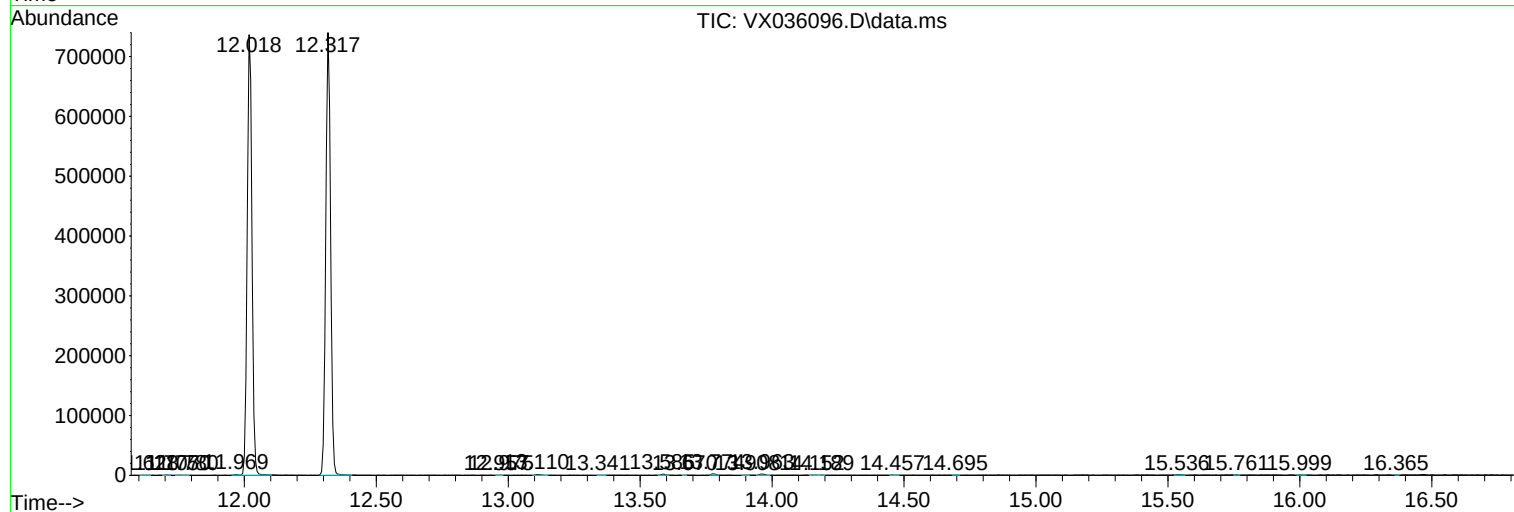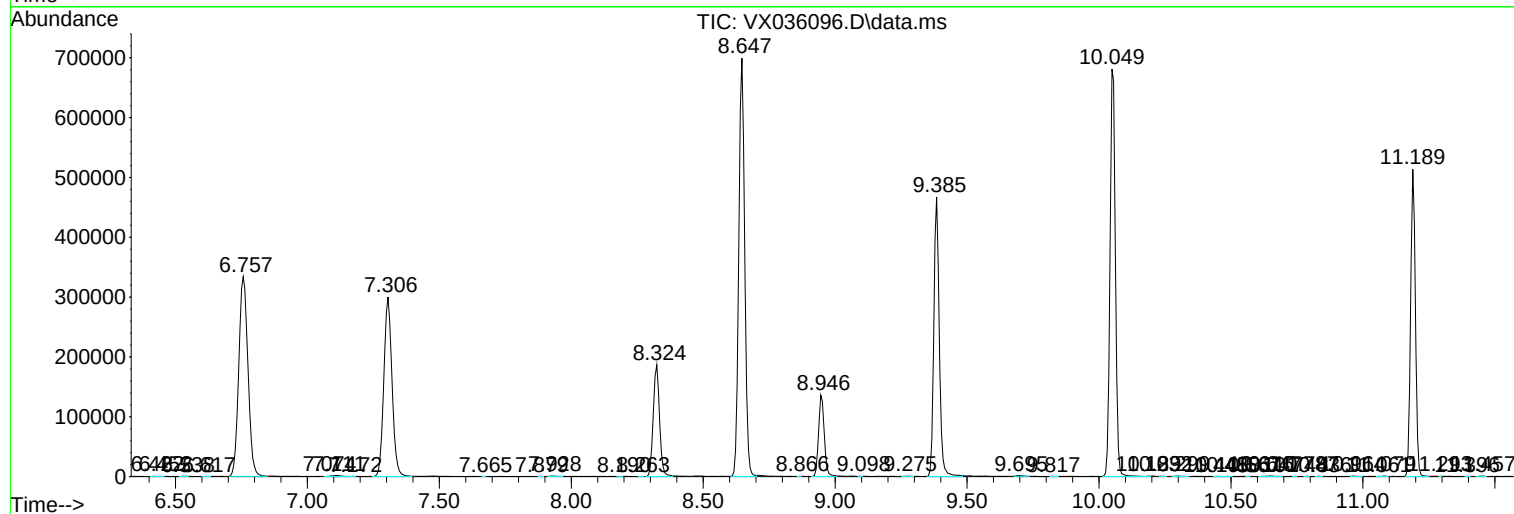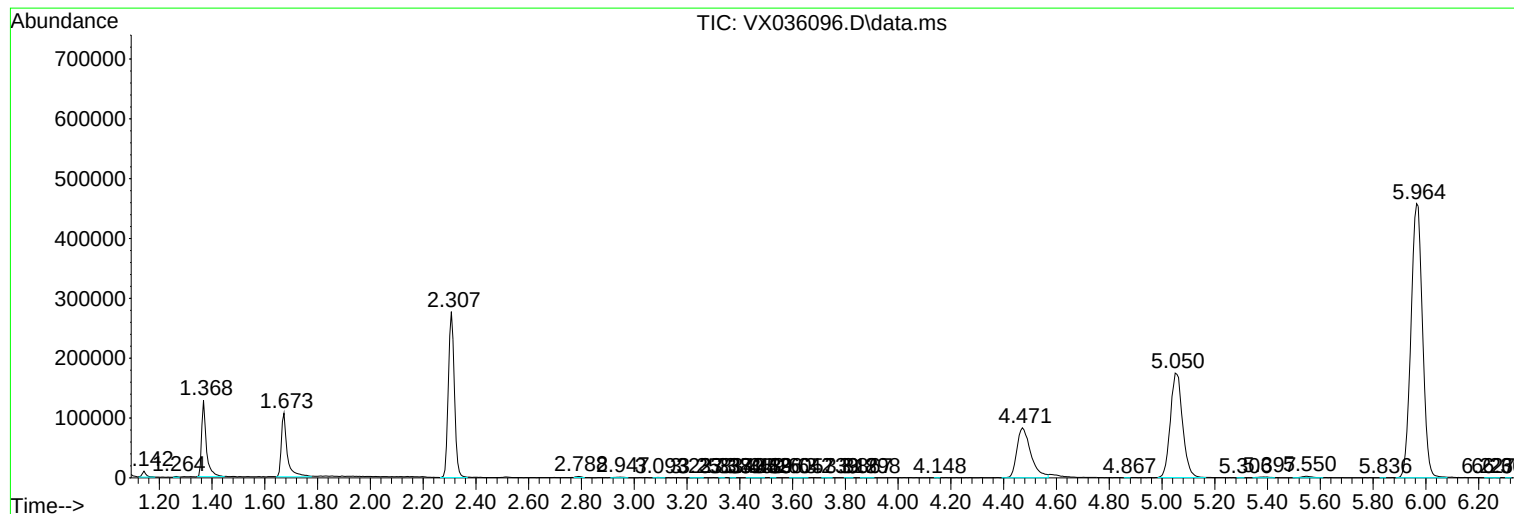

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036096.D
Acq On : 09 Jun 2023 09:10
Operator : JC/MD
Sample : VX0609WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK632

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036096.D
Acq On : 09 Jun 2023 09:10
Operator : JC/MD
Sample : VX0609WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK632

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc