

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036097.D
 Acq On : 09 Jun 2023 09:41
 Operator : JC/MD
 Sample : 03097-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEPO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB2	10059	11888	0.91%	0.123%
2	1.264	27	29	32	rBV2	1358	1290	0.10%	0.013%
3	1.368	42	46	57	rBV	131633	154260	11.81%	1.595%
4	1.672	91	96	110	rBV	102584	156147	11.95%	1.615%
5	2.306	194	200	212	rBV	274996	429917	32.90%	4.445%
6	2.514	230	234	241	rVB3	741	1464	0.11%	0.015%
7	2.776	275	277	278	rVV2	432	228	0.02%	0.002%
8	2.867	291	292	295	rBV2	261	272	0.02%	0.003%
9	2.898	295	297	299	rBV2	280	251	0.02%	0.003%
10	3.093	325	329	331	rBV3	375	653	0.05%	0.007%
11	3.111	331	332	333	rVB	564	211	0.02%	0.002%
12	3.209	345	348	352	rBV3	229	317	0.02%	0.003%
13	3.440	384	386	388	rBV	207	189	0.01%	0.002%
14	3.666	422	423	426	rBV	379	312	0.02%	0.003%
15	3.800	442	445	448	rBV2	199	283	0.02%	0.003%
16	3.873	456	457	460	rBV	215	188	0.01%	0.002%
17	4.330	530	532	535	rBV2	260	256	0.02%	0.003%
18	4.465	543	554	569	rBV	83059	256962	19.67%	2.657%
19	4.843	615	616	619	rBV2	269	264	0.02%	0.003%
20	4.958	634	635	638	rBV2	239	226	0.02%	0.002%
21	5.056	638	651	673	rVV	162701	527678	40.38%	5.456%
22	5.379	700	704	705	rBV3	665	851	0.07%	0.009%
23	5.519	725	727	728	rBV	540	438	0.03%	0.005%
24	5.544	728	731	741	rVB2	1340	2976	0.23%	0.031%
25	5.842	778	780	785	rVB2	218	300	0.02%	0.003%
26	5.964	787	800	818	rBV2	430768	1306679	100.00%	13.511%
27	6.287	851	853	854	rBV	367	238	0.02%	0.002%
28	6.342	858	862	863	rBV	376	311	0.02%	0.003%
29	6.373	863	867	869	rBV2	137	240	0.02%	0.002%
30	6.464	881	882	885	rVB2	329	278	0.02%	0.003%
31	6.562	896	898	899	rVB2	353	190	0.01%	0.002%
32	6.586	899	902	903	rVB2	233	229	0.02%	0.002%
33	6.604	903	905	907	rBV2	220	201	0.02%	0.002%
34	6.623	907	908	912	rVB2	161	194	0.01%	0.002%
35	6.757	920	930	942	rBV	327305	780872	59.76%	8.074%
36	6.946	960	961	963	rVB2	348	199	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036097.D
 Acq On : 09 Jun 2023 09:41
 Operator : JC/MD
 Sample : 03097-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEPO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.110	983	988	995	rBV6	1489	3485	0.27%	0.036%
38	7.306	1010	1020	1035	rBV	272117	607427	46.49%	6.281%
39	7.470	1042	1047	1049	rBV3	700	1136	0.09%	0.012%
40	7.720	1086	1088	1090	rBV	257	230	0.02%	0.002%
41	7.751	1090	1093	1095	rBV3	327	422	0.03%	0.004%
42	8.324	1180	1187	1200	rVV	176412	289401	22.15%	2.992%
43	8.470	1210	1211	1214	rVB2	621	430	0.03%	0.004%
44	8.647	1233	1240	1250	rBV	672096	1041213	79.68%	10.766%
45	8.799	1263	1265	1269	rVB2	639	627	0.05%	0.006%
46	8.946	1283	1289	1302	rBV	129031	188852	14.45%	1.953%
47	9.116	1315	1317	1321	rVB2	276	225	0.02%	0.002%
48	9.171	1324	1326	1329	rBV	363	513	0.04%	0.005%
49	9.220	1332	1334	1338	rVB2	210	233	0.02%	0.002%
50	9.275	1341	1343	1345	rVV2	420	294	0.02%	0.003%
51	9.384	1355	1361	1374	rBV	399649	581381	44.49%	6.011%
52	9.592	1393	1395	1398	rBV	268	316	0.02%	0.003%
53	9.665	1404	1407	1409	rVB2	320	328	0.03%	0.003%
54	9.732	1416	1418	1420	rBV2	299	253	0.02%	0.003%
55	9.897	1442	1445	1447	rBV2	286	321	0.02%	0.003%
56	10.049	1464	1470	1484	rBV	668254	935912	71.63%	9.677%
57	10.244	1498	1502	1503	rBV2	291	315	0.02%	0.003%
58	10.299	1508	1511	1515	rBV3	611	648	0.05%	0.007%
59	10.384	1522	1525	1528	rVB2	274	341	0.03%	0.004%
60	10.427	1528	1532	1533	rBV	217	219	0.02%	0.002%
61	10.488	1539	1542	1545	rBV2	235	369	0.03%	0.004%
62	10.646	1565	1568	1570	rBV	470	545	0.04%	0.006%
63	10.756	1584	1586	1588	rBV	268	301	0.02%	0.003%
64	10.866	1603	1604	1607	rBV2	273	192	0.01%	0.002%
65	10.890	1607	1608	1611	rVV2	189	189	0.01%	0.002%
66	10.921	1611	1613	1615	rVV2	258	214	0.02%	0.002%
67	10.970	1618	1621	1624	rVB2	284	398	0.03%	0.004%
68	11.000	1624	1626	1631	rVB2	243	371	0.03%	0.004%
69	11.085	1636	1640	1642	rVB3	476	548	0.04%	0.006%
70	11.189	1651	1657	1670	rBV	465955	591489	45.27%	6.116%
71	11.488	1704	1706	1711	rBV2	327	476	0.04%	0.005%
72	11.597	1722	1724	1727	rBV2	221	253	0.02%	0.003%
73	11.695	1738	1740	1742	rBV3	291	235	0.02%	0.002%
74	11.738	1745	1747	1748	rBV	306	240	0.02%	0.002%
75	11.780	1752	1754	1759	rVB	247	321	0.02%	0.003%
76	11.866	1766	1768	1770	rVB2	329	192	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036097.D
 Acq On : 09 Jun 2023 09:41
 Operator : JC/MD
 Sample : 03097-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEPO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.969	1782	1785	1788	rBV2	412	441	0.03%	0.005%
78	12.018	1788	1793	1803	rBV	731442	889796	68.10%	9.200%
79	12.225	1823	1827	1833	rVB5	1014	1600	0.12%	0.017%
80	12.317	1836	1842	1856	rBV	715107	881619	67.47%	9.116%
81	12.512	1871	1874	1879	rBV2	247	429	0.03%	0.004%
82	12.707	1904	1906	1908	rVB2	331	191	0.01%	0.002%
83	12.731	1908	1910	1913	rBV2	297	353	0.03%	0.004%
84	12.859	1928	1931	1937	rVB	455	606	0.05%	0.006%
85	12.957	1945	1947	1950	rVB2	451	388	0.03%	0.004%
86	12.987	1950	1952	1953	rBV	207	192	0.01%	0.002%
87	13.048	1960	1962	1965	rVB2	256	278	0.02%	0.003%
88	13.170	1980	1982	1985	rBV2	308	383	0.03%	0.004%
89	13.378	2014	2016	2017	rBV	234	201	0.02%	0.002%
90	13.426	2021	2024	2028	rBV2	345	491	0.04%	0.005%
91	13.475	2030	2032	2034	rBV	278	226	0.02%	0.002%
92	13.591	2047	2051	2054	rBV4	688	855	0.07%	0.009%
93	13.676	2064	2065	2068	rBV2	349	320	0.02%	0.003%
94	13.774	2078	2081	2086	rBV3	884	1072	0.08%	0.011%
95	13.957	2107	2111	2113	rBV	567	641	0.05%	0.007%
96	14.085	2131	2132	2134	rVV2	314	218	0.02%	0.002%
97	14.128	2137	2139	2140	rVV	430	254	0.02%	0.003%
98	15.066	2289	2293	2294	rBV2	460	519	0.04%	0.005%
99	15.536	2368	2370	2374	rBV4	896	1284	0.10%	0.013%
100	16.511	2528	2530	2533	rBV3	602	725	0.06%	0.007%




Sum of corrected areas: 9671389

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036097.D
Acq On : 09 Jun 2023 09:41
Operator : JC/MD
Sample : 03097-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEPO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

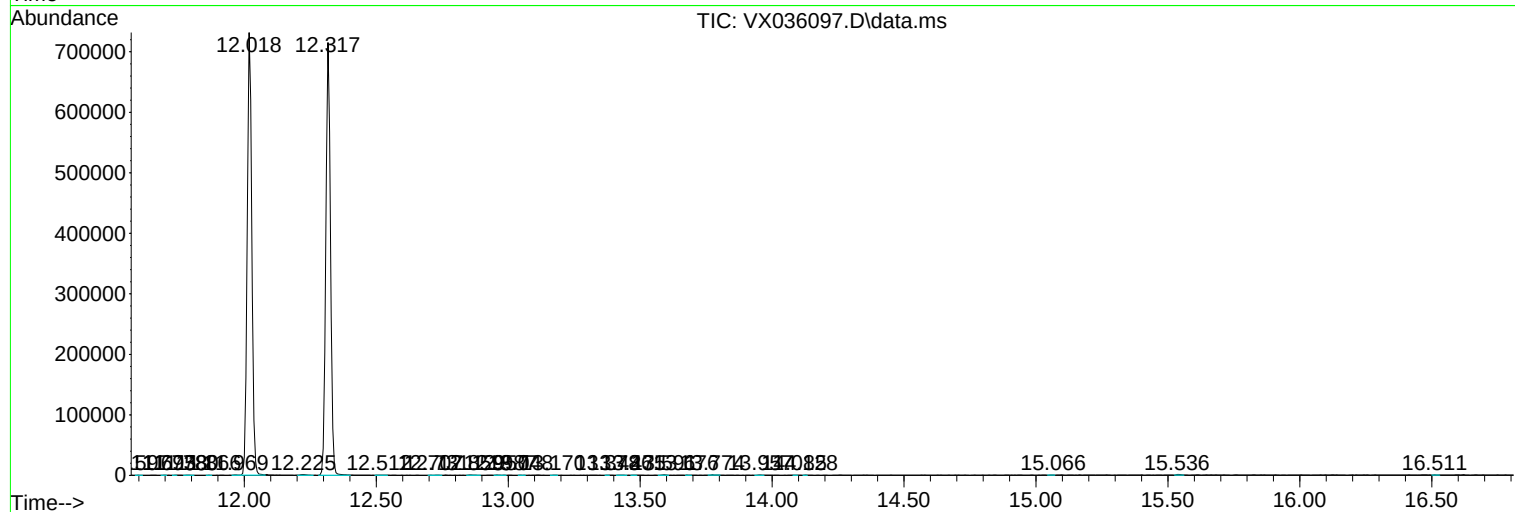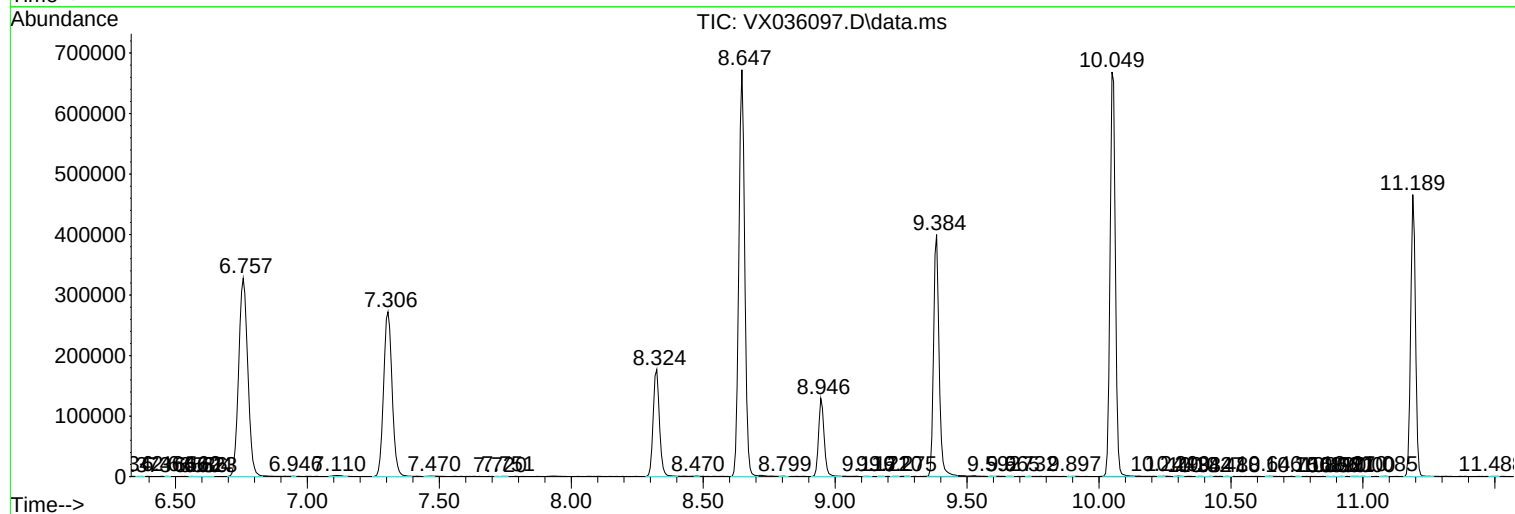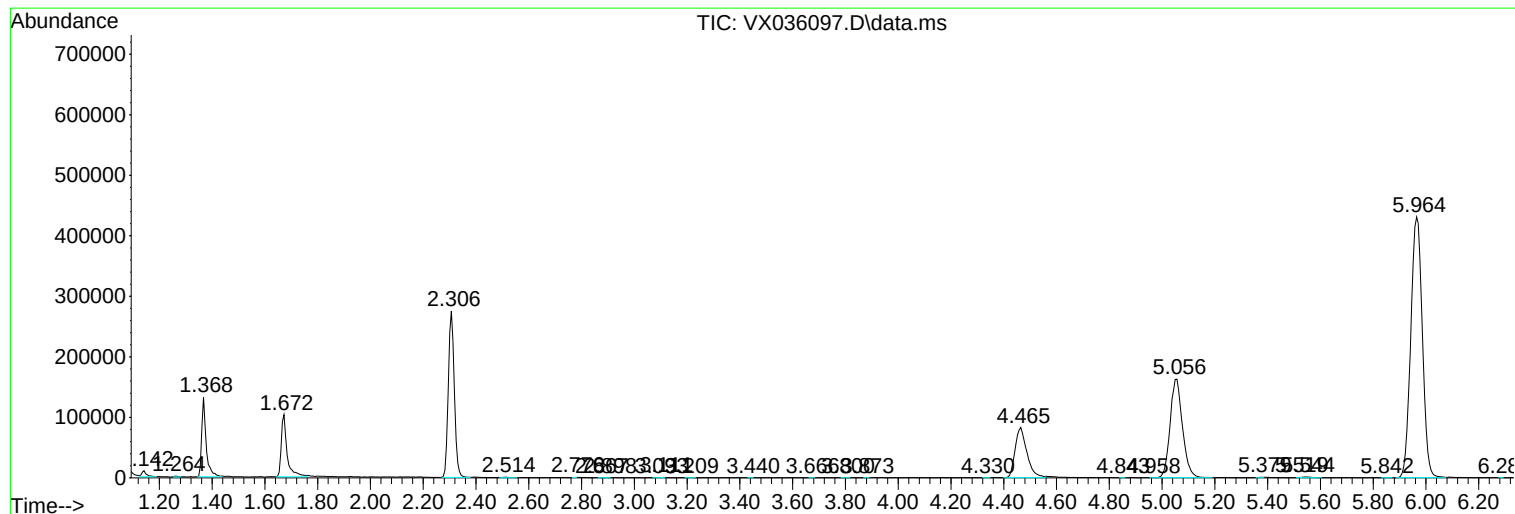

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036097.D
Acq On : 09 Jun 2023 09:41
Operator : JC/MD
Sample : 03097-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEPO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036097.D
Acq On : 09 Jun 2023 09:41
Operator : JC/MD
Sample : 03097-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEPO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc