

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036098.D
 Acq On : 09 Jun 2023 10:11
 Operator : JC/MD
 Sample : 03097-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB	8877	10280	0.76%	0.103%
2	1.368	42	46	58	rBV	120121	152721	11.30%	1.537%
3	1.673	91	96	113	rBV	98765	156371	11.57%	1.573%
4	2.307	193	200	210	rBV	265881	418045	30.93%	4.206%
5	2.508	229	233	237	rVB3	666	1031	0.08%	0.010%
6	2.556	240	241	242	rVB	479	175	0.01%	0.002%
7	2.697	262	264	265	rVB2	328	183	0.01%	0.002%
8	2.752	272	273	274	rVV	321	163	0.01%	0.002%
9	2.788	274	279	288	rVV4	1482	3204	0.24%	0.032%
10	2.849	288	289	293	rVV2	356	223	0.02%	0.002%
11	2.898	295	297	298	rVV2	260	210	0.02%	0.002%
12	2.941	300	304	310	rVV2	1804	3971	0.29%	0.040%
13	3.008	313	315	317	rVB2	247	208	0.02%	0.002%
14	3.050	317	322	323	rBV2	239	367	0.03%	0.004%
15	3.081	326	327	330	rVB2	311	240	0.02%	0.002%
16	3.197	345	346	347	rVV	373	168	0.01%	0.002%
17	3.251	353	355	358	rVV2	277	293	0.02%	0.003%
18	3.288	358	361	362	rVB	305	249	0.02%	0.003%
19	3.367	372	374	377	rBV2	166	156	0.01%	0.002%
20	3.703	426	429	430	rBV	141	160	0.01%	0.002%
21	3.831	448	450	452	rVB	245	203	0.02%	0.002%
22	3.904	460	462	467	rVB2	238	253	0.02%	0.003%
23	3.971	471	473	475	rBV2	356	351	0.03%	0.004%
24	4.111	495	496	500	rBV2	250	187	0.01%	0.002%
25	4.160	502	504	506	rVV2	247	171	0.01%	0.002%
26	4.276	521	523	526	rBV2	173	257	0.02%	0.003%
27	4.471	544	555	590	rBV	81466	304571	22.53%	3.064%
28	4.855	616	618	622	rBV2	292	389	0.03%	0.004%
29	5.056	638	651	669	rBV	168524	543402	40.20%	5.468%
30	5.336	695	697	701	rVV2	206	222	0.02%	0.002%
31	5.373	701	703	705	rVV3	380	423	0.03%	0.004%
32	5.404	705	708	710	rVB2	389	350	0.03%	0.004%
33	5.544	726	731	735	rBV4	509	1250	0.09%	0.013%
34	5.964	787	800	817	rBV2	456922	1351631	100.00%	13.600%
35	6.531	891	893	896	rBV2	376	382	0.03%	0.004%
36	6.641	909	911	914	rVB2	355	389	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036098.D
 Acq On : 09 Jun 2023 10:11
 Operator : JC/MD
 Sample : 03097-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.757	920	930	943	rBV	320826	764322	56.55%	7.690%
38	7.104	982	987	997	rVB3	1883	3785	0.28%	0.038%
39	7.306	1010	1020	1036	rBV	287099	624323	46.19%	6.282%
40	7.470	1045	1047	1053	rVB3	623	730	0.05%	0.007%
41	7.617	1066	1071	1072	rBV2	229	253	0.02%	0.003%
42	7.891	1115	1116	1119	rBV2	192	182	0.01%	0.002%
43	7.934	1119	1123	1129	rVV3	964	1913	0.14%	0.019%
44	8.104	1149	1151	1153	rBV	247	213	0.02%	0.002%
45	8.324	1180	1187	1199	rBV	179827	293758	21.73%	2.956%
46	8.470	1209	1211	1216	rBV4	510	916	0.07%	0.009%
47	8.647	1233	1240	1252	rBV	669190	1048092	77.54%	10.546%
48	8.946	1283	1289	1299	rBV	131086	194964	14.42%	1.962%
49	9.183	1326	1328	1329	rBV2	173	165	0.01%	0.002%
50	9.202	1330	1331	1334	rVB	311	250	0.02%	0.003%
51	9.269	1340	1342	1343	rBV	240	208	0.02%	0.002%
52	9.385	1355	1361	1373	rBV	452583	635352	47.01%	6.393%
53	9.634	1400	1402	1403	rBV	299	181	0.01%	0.002%
54	9.702	1409	1413	1418	rBV4	2548	3570	0.26%	0.036%
55	9.744	1418	1420	1422	rVV	340	207	0.02%	0.002%
56	9.891	1443	1444	1446	rBV	205	154	0.01%	0.002%
57	9.927	1449	1450	1453	rVB2	268	169	0.01%	0.002%
58	9.970	1455	1457	1462	rVB3	247	299	0.02%	0.003%
59	10.049	1465	1470	1483	rVV	663771	925876	68.50%	9.316%
60	10.220	1496	1498	1499	rVB	450	278	0.02%	0.003%
61	10.348	1516	1519	1520	rBV	198	221	0.02%	0.002%
62	10.665	1569	1571	1573	rVB	400	255	0.02%	0.003%
63	10.720	1578	1580	1581	rVB	228	162	0.01%	0.002%
64	10.787	1587	1591	1592	rBV	376	301	0.02%	0.003%
65	10.829	1596	1598	1601	rVB2	173	161	0.01%	0.002%
66	11.085	1638	1640	1643	rVB2	471	380	0.03%	0.004%
67	11.189	1652	1657	1669	rBV	504850	636055	47.06%	6.400%
68	11.268	1669	1670	1671	rVB	424	155	0.01%	0.002%
69	11.342	1680	1682	1684	rBV	180	155	0.01%	0.002%
70	11.591	1722	1723	1726	rBV2	180	198	0.01%	0.002%
71	11.622	1726	1728	1732	rVB	164	260	0.02%	0.003%
72	11.665	1732	1735	1736	rBV2	358	359	0.03%	0.004%
73	11.707	1740	1742	1748	rVV2	482	636	0.05%	0.006%
74	11.780	1752	1754	1758	rVB2	159	222	0.02%	0.002%
75	11.884	1767	1771	1772	rVB	231	218	0.02%	0.002%
76	12.018	1788	1793	1804	rBV	735545	903200	66.82%	9.088%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036098.D
 Acq On : 09 Jun 2023 10:11
 Operator : JC/MD
 Sample : 03097-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1852	rVB	769257	935668	69.23%	9.414%
78	12.457	1864	1865	1869	rVB3	395	450	0.03%	0.005%
79	12.494	1869	1871	1872	rBV	273	166	0.01%	0.002%
80	12.756	1912	1914	1916	rVB2	331	286	0.02%	0.003%
81	12.945	1943	1945	1948	rBV	321	313	0.02%	0.003%
82	13.085	1966	1968	1970	rBV	346	158	0.01%	0.002%
83	13.244	1990	1994	1996	rBV	254	353	0.03%	0.004%
84	13.506	2033	2037	2038	rBV2	237	276	0.02%	0.003%
85	13.585	2048	2050	2053	rVB3	236	238	0.02%	0.002%
86	13.683	2065	2066	2070	rBV	309	373	0.03%	0.004%
87	13.780	2078	2082	2083	rBV2	294	397	0.03%	0.004%
88	13.878	2094	2098	2099	rVB2	307	343	0.03%	0.003%
89	13.902	2099	2102	2103	rBV2	287	337	0.02%	0.003%
90	14.036	2122	2124	2125	rVB	351	197	0.01%	0.002%
91	14.158	2142	2144	2146	rVB3	274	191	0.01%	0.002%
92	14.231	2152	2156	2157	rBV2	319	285	0.02%	0.003%
93	14.371	2176	2179	2180	rBV	404	483	0.04%	0.005%
94	14.591	2207	2215	2217	rBV2	399	692	0.05%	0.007%
95	14.682	2229	2230	2231	rBV	376	193	0.01%	0.002%
96	14.731	2237	2238	2239	rBV	294	153	0.01%	0.002%
97	14.847	2255	2257	2260	rBV2	323	284	0.02%	0.003%
98	15.225	2318	2319	2321	rBV	331	178	0.01%	0.002%
99	15.835	2418	2419	2421	rBV2	426	255	0.02%	0.003%
100	16.639	2549	2551	2554	rBV	547	483	0.04%	0.005%


Sum of corrected areas: 9938699

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036098.D
Acq On : 09 Jun 2023 10:11
Operator : JC/MD
Sample : 03097-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

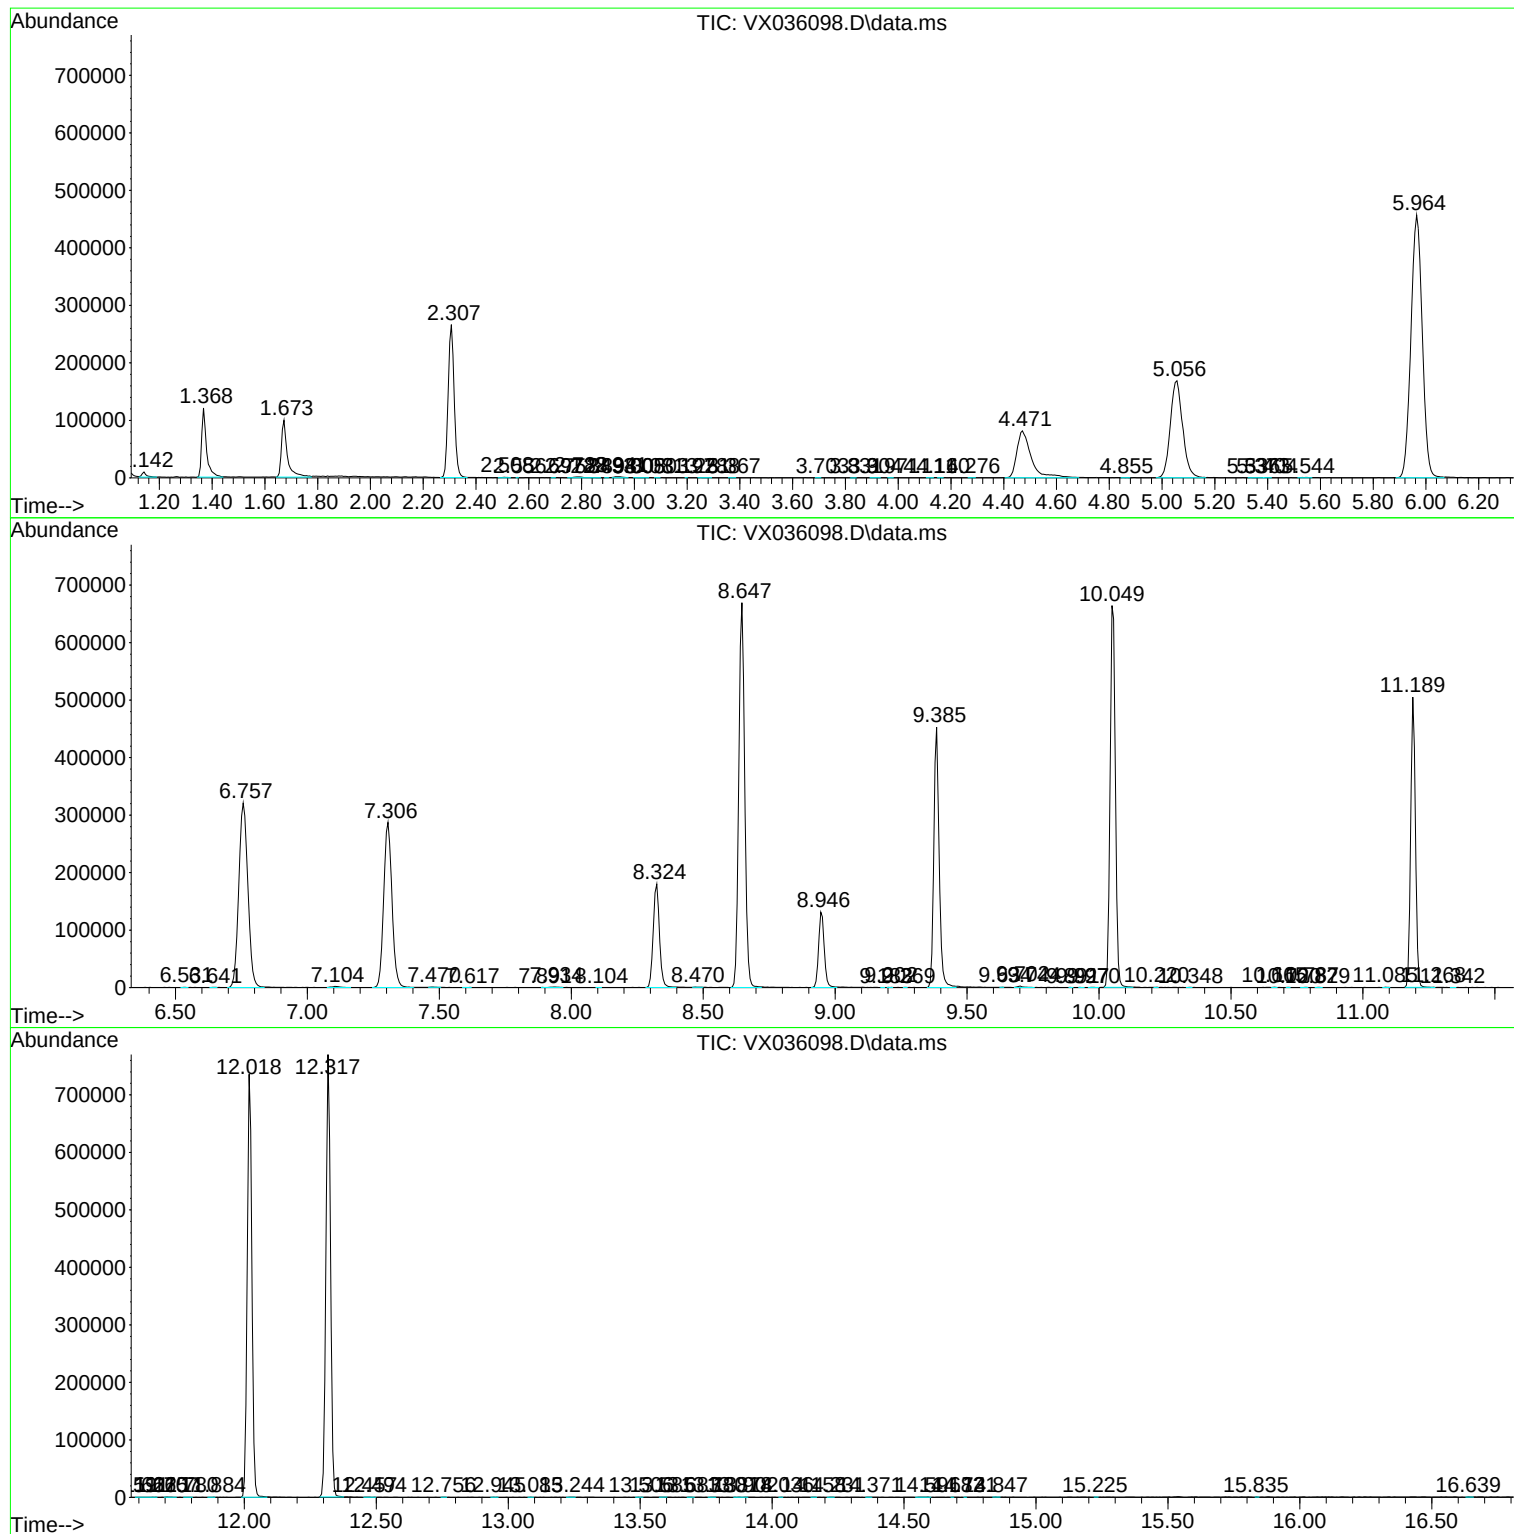

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036098.D
Acq On : 09 Jun 2023 10:11
Operator : JC/MD
Sample : 03097-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036098.D
Acq On : 09 Jun 2023 10:11
Operator : JC/MD
Sample : 03097-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc