

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036099.D
 Acq On : 09 Jun 2023 11:14
 Operator : JC/MD
 Sample : 03107-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	8192	9033	0.67%	0.090%
2	1.368	42	46	58	rBV	128651	160035	11.80%	1.597%
3	1.672	91	96	115	rBV	105605	163344	12.04%	1.630%
4	2.307	194	200	211	rBV	283571	442629	32.63%	4.416%
5	2.502	230	232	238	rBV4	612	958	0.07%	0.010%
6	2.709	263	266	269	rVB3	346	428	0.03%	0.004%
7	2.794	273	280	282	rVV3	495	877	0.06%	0.009%
8	2.861	289	291	292	rBV	385	181	0.01%	0.002%
9	3.160	338	340	341	rBV	269	182	0.01%	0.002%
10	3.251	352	355	357	rVB	236	174	0.01%	0.002%
11	3.294	359	362	366	rVB2	263	415	0.03%	0.004%
12	3.331	366	368	370	rBV2	164	183	0.01%	0.002%
13	3.410	378	381	383	rVB	189	217	0.02%	0.002%
14	3.562	404	406	409	rVB	179	201	0.01%	0.002%
15	3.684	422	426	429	rBV	202	251	0.02%	0.003%
16	3.715	429	431	434	rVB2	226	187	0.01%	0.002%
17	3.800	443	445	446	rVB	329	173	0.01%	0.002%
18	3.873	455	457	459	rBV2	213	195	0.01%	0.002%
19	4.026	480	482	484	rVB2	202	161	0.01%	0.002%
20	4.062	484	488	493	rBV2	319	609	0.04%	0.006%
21	4.184	504	508	509	rBV2	184	212	0.02%	0.002%
22	4.306	526	528	529	rVV2	219	149	0.01%	0.001%
23	4.361	535	537	538	rBV	252	165	0.01%	0.002%
24	4.465	544	554	573	rBV	81133	276782	20.40%	2.761%
25	4.879	619	622	624	rVB2	310	346	0.03%	0.003%
26	4.916	624	628	630	rBV2	280	378	0.03%	0.004%
27	4.965	634	636	637	rBV2	183	179	0.01%	0.002%
28	5.050	637	650	665	rBV	172064	546823	40.31%	5.455%
29	5.324	694	695	698	rVB2	274	218	0.02%	0.002%
30	5.367	700	702	703	rBV	347	271	0.02%	0.003%
31	5.690	753	755	760	rVB2	248	337	0.02%	0.003%
32	5.733	760	762	765	rBV2	172	259	0.02%	0.003%
33	5.812	773	775	778	rBV2	239	240	0.02%	0.002%
34	5.964	786	800	819	rBV2	451518	1356536	100.00%	13.533%
35	6.233	841	844	846	rBV2	207	232	0.02%	0.002%
36	6.318	854	858	860	rBV	224	244	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036099.D
 Acq On : 09 Jun 2023 11:14
 Operator : JC/MD
 Sample : 03107-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.379	867	868	870	rBV	251	184	0.01%	0.002%
38	6.397	870	871	874	rVV2	208	139	0.01%	0.001%
39	6.531	891	893	894	rBV2	261	190	0.01%	0.002%
40	6.751	920	929	944	rBV	331845	795805	58.66%	7.939%
41	7.104	982	987	990	rBV4	1379	2709	0.20%	0.027%
42	7.220	1004	1006	1008	rVB	226	159	0.01%	0.002%
43	7.300	1010	1019	1033	rBV	283285	631621	46.56%	6.301%
44	7.482	1043	1049	1052	rBV4	736	1379	0.10%	0.014%
45	7.635	1073	1074	1077	rVB2	180	148	0.01%	0.001%
46	7.678	1077	1081	1085	rBV	241	345	0.03%	0.003%
47	7.927	1117	1122	1127	rBV2	1026	1775	0.13%	0.018%
48	8.001	1131	1134	1138	rBV2	247	400	0.03%	0.004%
49	8.147	1157	1158	1161	rVB2	368	287	0.02%	0.003%
50	8.244	1172	1174	1179	rVB4	528	773	0.06%	0.008%
51	8.324	1179	1187	1198	rBV	180545	300119	22.12%	2.994%
52	8.507	1215	1217	1218	rVB	571	309	0.02%	0.003%
53	8.525	1218	1220	1223	rBV2	296	268	0.02%	0.003%
54	8.647	1233	1240	1254	rBV	677602	1081412	79.72%	10.788%
55	8.824	1268	1269	1271	rVB	325	142	0.01%	0.001%
56	8.946	1283	1289	1302	rBV	136590	196724	14.50%	1.963%
57	9.202	1329	1331	1334	rVB2	267	248	0.02%	0.002%
58	9.275	1340	1343	1346	rVB3	672	857	0.06%	0.009%
59	9.385	1355	1361	1380	rBV	412383	612385	45.14%	6.109%
60	9.775	1423	1425	1426	rBV	227	178	0.01%	0.002%
61	9.817	1430	1432	1433	rBV	214	160	0.01%	0.002%
62	9.866	1439	1440	1443	rBV3	256	228	0.02%	0.002%
63	9.958	1454	1455	1458	rBV	196	154	0.01%	0.002%
64	10.049	1465	1470	1487	rVB	706264	952847	70.24%	9.506%
65	10.451	1534	1536	1540	rBV2	248	374	0.03%	0.004%
66	10.561	1552	1554	1556	rBV2	227	175	0.01%	0.002%
67	10.586	1556	1558	1560	rBV2	161	171	0.01%	0.002%
68	10.842	1598	1600	1602	rBV	324	338	0.02%	0.003%
69	10.982	1622	1623	1626	rBV	214	147	0.01%	0.001%
70	11.006	1626	1627	1629	rBV	228	151	0.01%	0.002%
71	11.092	1638	1641	1643	rVB2	432	431	0.03%	0.004%
72	11.189	1652	1657	1666	rVV	492008	621056	45.78%	6.196%
73	11.317	1674	1678	1681	rVB2	485	703	0.05%	0.007%
74	11.591	1719	1723	1724	rBV	216	232	0.02%	0.002%
75	11.640	1730	1731	1736	rVB	293	261	0.02%	0.003%
76	11.689	1736	1739	1740	rBV2	298	302	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036099.D
 Acq On : 09 Jun 2023 11:14
 Operator : JC/MD
 Sample : 03107-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.750	1748	1749	1751	rBV2	349	177	0.01%	0.002%
78	11.811	1756	1759	1762	rBV2	255	310	0.02%	0.003%
79	11.963	1782	1784	1788	rBV2	273	410	0.03%	0.004%
80	12.018	1788	1793	1802	rBV	751047	921617	67.94%	9.194%
81	12.317	1837	1842	1849	rBV	743251	927045	68.34%	9.248%
82	12.518	1872	1875	1876	rBV	292	207	0.02%	0.002%
83	12.738	1909	1911	1912	rVB	260	185	0.01%	0.002%
84	12.768	1912	1916	1917	rBV	360	373	0.03%	0.004%
85	12.896	1935	1937	1938	rBV	361	290	0.02%	0.003%
86	13.036	1958	1960	1962	rVB2	261	150	0.01%	0.001%
87	13.109	1970	1972	1974	rVB	393	245	0.02%	0.002%
88	13.530	2039	2041	2044	rBV2	339	239	0.02%	0.002%
89	13.762	2077	2079	2081	rBV	269	259	0.02%	0.003%
90	13.853	2092	2094	2096	rVB2	271	179	0.01%	0.002%
91	13.896	2100	2101	2104	rBV	225	145	0.01%	0.001%
92	13.957	2109	2111	2112	rBV	321	242	0.02%	0.002%
93	14.079	2127	2131	2132	rBV	338	385	0.03%	0.004%
94	14.134	2139	2140	2142	rBV	504	290	0.02%	0.003%
95	14.225	2153	2155	2156	rVB	436	197	0.01%	0.002%
96	14.371	2177	2179	2180	rVB	389	176	0.01%	0.002%
97	14.609	2216	2218	2219	rBV	264	194	0.01%	0.002%
98	14.707	2232	2234	2235	rVB	434	283	0.02%	0.003%
99	14.749	2240	2241	2242	rBV	308	176	0.01%	0.002%
100	14.969	2276	2277	2279	rBV	329	224	0.02%	0.002%




Sum of corrected areas: 10024088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036099.D
Acq On : 09 Jun 2023 11:14
Operator : JC/MD
Sample : 03107-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

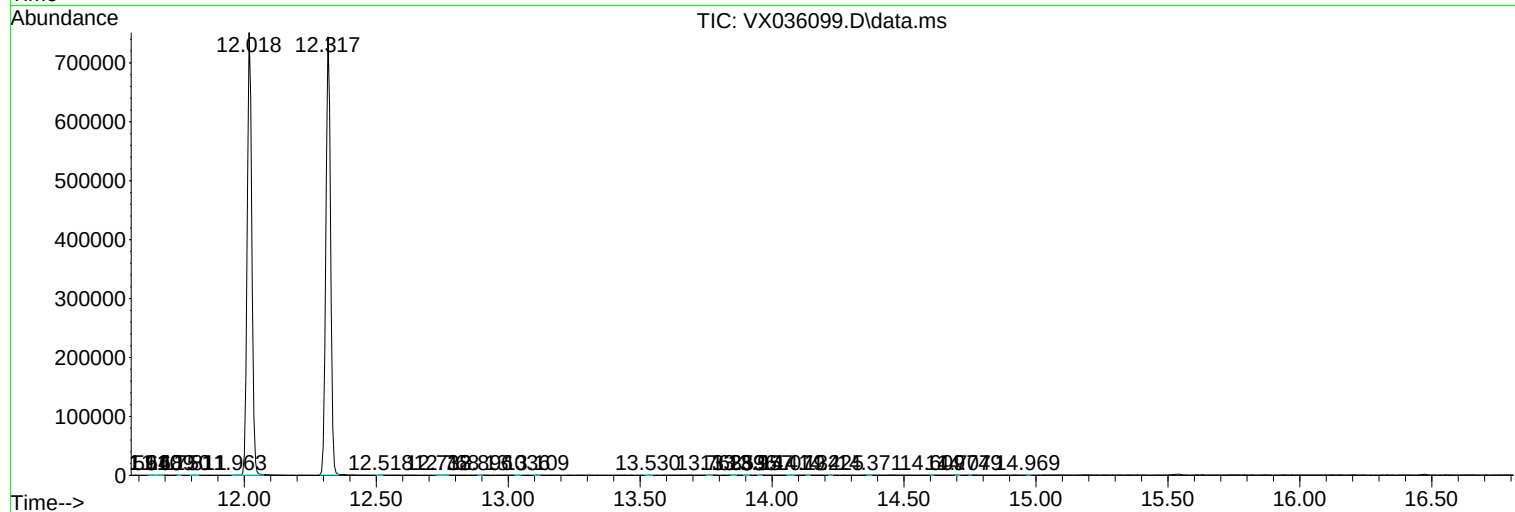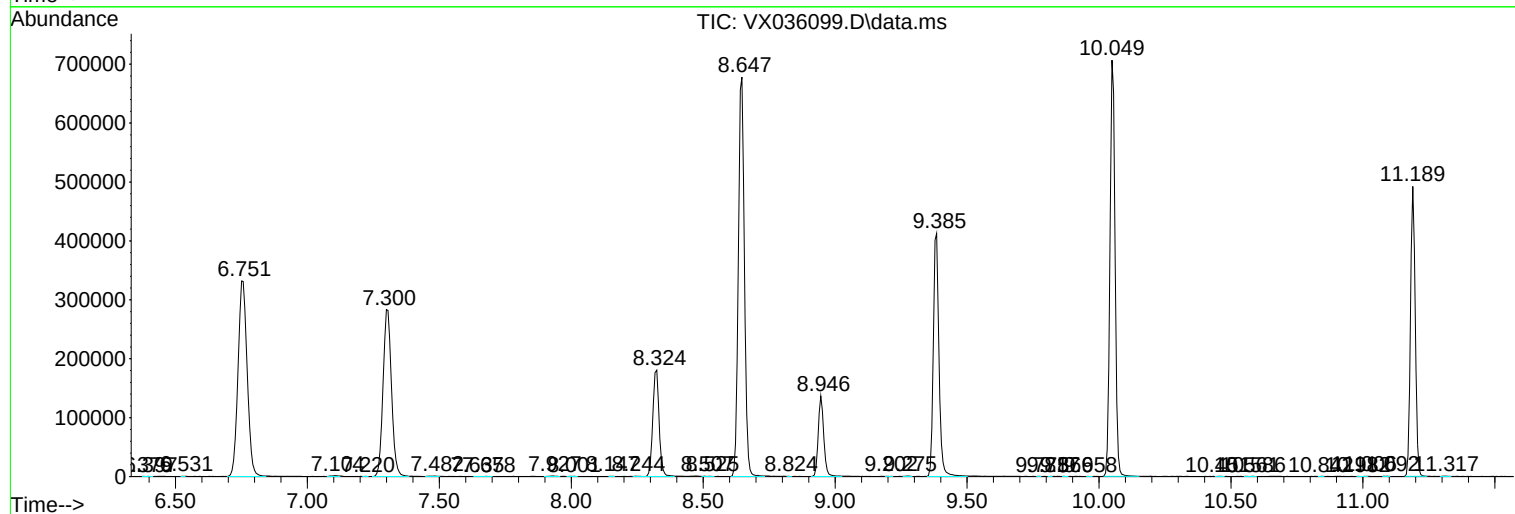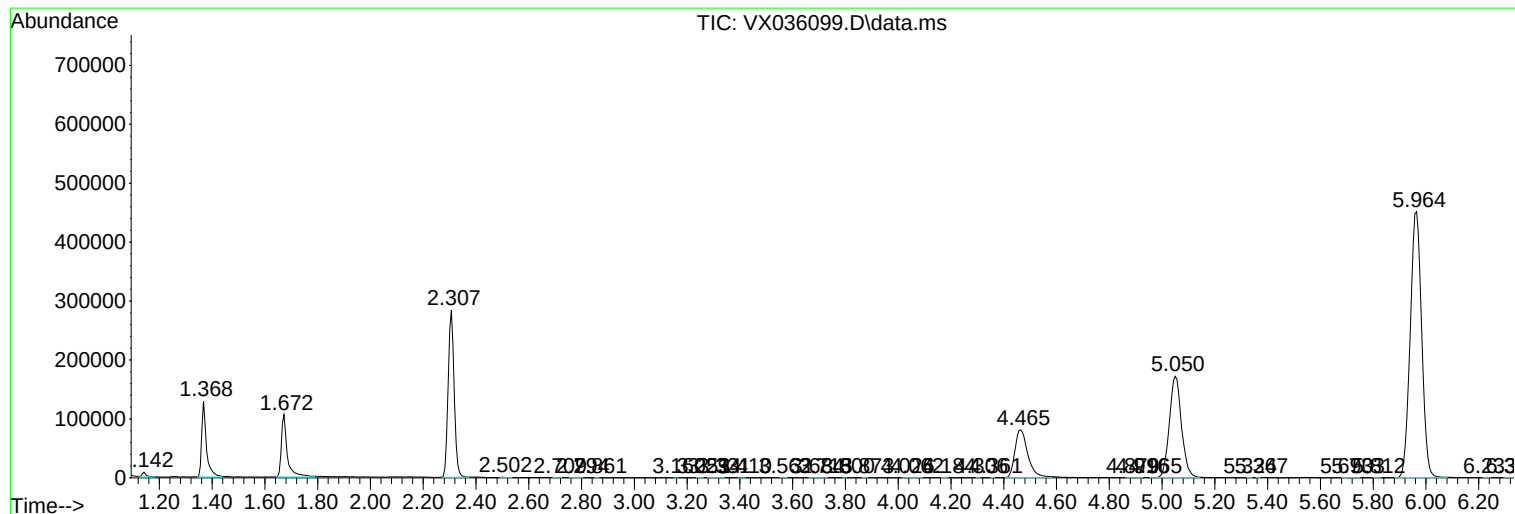

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036099.D
Acq On : 09 Jun 2023 11:14
Operator : JC/MD
Sample : 03107-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036099.D
Acq On : 09 Jun 2023 11:14
Operator : JC/MD
Sample : 03107-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc