

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036101.D
 Acq On : 09 Jun 2023 12:01
 Operator : JC/MD
 Sample : 03107-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB	10042	9649	0.75%	0.106%
2	1.264	27	29	32	rVB2	1466	1337	0.10%	0.015%
3	1.368	42	46	65	rVB	96513	128099	9.91%	1.403%
4	1.672	92	96	115	rBV	88813	140316	10.86%	1.537%
5	2.306	193	200	210	rBV	223592	346601	26.83%	3.796%
6	2.508	231	233	235	rBV2	618	686	0.05%	0.008%
7	2.593	246	247	250	rBV	218	179	0.01%	0.002%
8	2.654	253	257	259	rBV3	224	335	0.03%	0.004%
9	2.794	274	280	282	rBV5	702	1350	0.10%	0.015%
10	2.867	290	292	296	rBV2	386	566	0.04%	0.006%
11	2.898	296	297	299	rBV2	202	175	0.01%	0.002%
12	3.020	311	317	319	rBV2	250	450	0.03%	0.005%
13	3.087	326	328	332	rVB4	179	170	0.01%	0.002%
14	3.318	364	366	370	rVB2	342	356	0.03%	0.004%
15	3.367	373	374	376	rBV2	264	232	0.02%	0.003%
16	3.520	398	399	401	rVV2	214	189	0.01%	0.002%
17	3.696	426	428	429	rVB	303	184	0.01%	0.002%
18	3.709	429	430	433	rBV	365	240	0.02%	0.003%
19	3.837	450	451	455	rVB	294	232	0.02%	0.003%
20	3.891	455	460	461	rBV2	208	280	0.02%	0.003%
21	3.971	472	473	475	rBV	269	207	0.02%	0.002%
22	4.007	478	479	481	rBV	262	200	0.02%	0.002%
23	4.257	518	520	523	rBV2	187	207	0.02%	0.002%
24	4.477	546	556	581	rBV	74834	257206	19.91%	2.817%
25	4.769	602	604	605	rVB	407	175	0.01%	0.002%
26	5.062	638	652	668	rBV	165110	525302	40.66%	5.754%
27	5.379	701	704	706	rBV3	417	636	0.05%	0.007%
28	5.556	727	733	735	rBV5	784	1676	0.13%	0.018%
29	5.696	752	756	757	rBV2	215	187	0.01%	0.002%
30	5.830	772	778	781	rBV2	328	507	0.04%	0.006%
31	5.970	787	801	818	rBV2	428785	1292073	100.00%	14.153%
32	6.086	818	820	825	rVB4	670	900	0.07%	0.010%
33	6.190	835	837	841	rVV3	229	274	0.02%	0.003%
34	6.367	864	866	868	rVV	241	178	0.01%	0.002%
35	6.434	876	877	881	rBV2	219	234	0.02%	0.003%
36	6.489	883	886	889	rBV2	264	320	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036101.D
 Acq On : 09 Jun 2023 12:01
 Operator : JC/MD
 Sample : 03107-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.519	889	891	894	rBV3	355	266	0.02%	0.003%
38	6.556	894	897	900	rVB2	277	349	0.03%	0.004%
39	6.757	920	930	948	rBV	312753	752801	58.26%	8.246%
40	7.025	971	974	975	rBV2	216	242	0.02%	0.003%
41	7.110	982	988	994	rBV3	1391	2885	0.22%	0.032%
42	7.159	994	996	997	rBV	260	165	0.01%	0.002%
43	7.305	1010	1020	1033	rBV	275608	606391	46.93%	6.642%
44	7.458	1043	1045	1046	rBV2	381	387	0.03%	0.004%
45	7.696	1081	1084	1087	rVB2	222	292	0.02%	0.003%
46	7.763	1093	1095	1100	rBV3	335	402	0.03%	0.004%
47	7.933	1117	1123	1127	rBV4	814	1614	0.12%	0.018%
48	8.129	1154	1155	1157	rBV	209	192	0.01%	0.002%
49	8.269	1174	1178	1179	rBV2	195	270	0.02%	0.003%
50	8.324	1180	1187	1197	rBV	164416	273182	21.14%	2.992%
51	8.647	1233	1240	1252	rBV	632648	983882	76.15%	10.777%
52	8.945	1283	1289	1302	rBV	117794	181110	14.02%	1.984%
53	9.281	1339	1344	1349	rVB3	1062	1465	0.11%	0.016%
54	9.384	1355	1361	1379	rBV	392470	566456	43.84%	6.205%
55	10.055	1465	1471	1486	rVB	630425	890920	68.95%	9.759%
56	10.195	1492	1494	1498	rVB4	505	597	0.05%	0.007%
57	10.226	1498	1499	1504	rVB	398	376	0.03%	0.004%
58	10.293	1508	1510	1517	rVB4	611	910	0.07%	0.010%
59	10.390	1525	1526	1530	rVB	252	149	0.01%	0.002%
60	10.659	1568	1570	1572	rVB2	621	445	0.03%	0.005%
61	10.695	1572	1576	1580	rBV2	304	444	0.03%	0.005%
62	10.823	1594	1597	1599	rBV2	309	283	0.02%	0.003%
63	11.085	1638	1640	1641	rVB	497	274	0.02%	0.003%
64	11.189	1652	1657	1666	rVB	447103	567806	43.95%	6.219%
65	11.311	1674	1677	1681	rVB3	973	1223	0.09%	0.013%
66	11.378	1686	1688	1691	rBV2	224	161	0.01%	0.002%
67	11.634	1729	1730	1731	rBV	379	178	0.01%	0.002%
68	11.664	1733	1735	1736	rVV2	345	208	0.02%	0.002%
69	11.713	1740	1743	1744	rVB	449	422	0.03%	0.005%
70	11.756	1746	1750	1751	rBV2	245	255	0.02%	0.003%
71	11.969	1783	1785	1788	rBV2	395	431	0.03%	0.005%
72	12.018	1788	1793	1803	rBV	629726	782289	60.55%	8.569%
73	12.128	1810	1811	1813	rVB	406	220	0.02%	0.002%
74	12.158	1813	1816	1817	rBV2	259	245	0.02%	0.003%
75	12.250	1830	1831	1834	rBV2	223	219	0.02%	0.002%
76	12.317	1837	1842	1859	rVB	640072	790379	61.17%	8.657%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036101.D
 Acq On : 09 Jun 2023 12:01
 Operator : JC/MD
 Sample : 03107-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.469	1865	1867	1870	rVB2	465	380	0.03%	0.004%
78	12.585	1884	1886	1888	rBV2	320	311	0.02%	0.003%
79	12.609	1888	1890	1893	rVB	364	245	0.02%	0.003%
80	12.695	1902	1904	1908	rBV	274	341	0.03%	0.004%
81	12.774	1915	1917	1919	rBV3	217	196	0.02%	0.002%
82	12.914	1939	1940	1943	rBV	230	157	0.01%	0.002%
83	13.000	1953	1954	1956	rBV	403	220	0.02%	0.002%
84	13.054	1959	1963	1966	rVB	272	396	0.03%	0.004%
85	13.079	1966	1967	1971	rBV2	155	181	0.01%	0.002%
86	13.371	2012	2015	2017	rVB2	253	266	0.02%	0.003%
87	13.469	2029	2031	2032	rVB2	296	161	0.01%	0.002%
88	13.597	2048	2052	2057	rBV2	296	494	0.04%	0.005%
89	13.688	2065	2067	2069	rVB	550	484	0.04%	0.005%
90	13.774	2079	2081	2084	rBV2	212	172	0.01%	0.002%
91	13.914	2102	2104	2107	rBV	393	342	0.03%	0.004%
92	14.225	2153	2155	2157	rVV2	314	185	0.01%	0.002%
93	14.243	2157	2158	2161	rVB2	274	174	0.01%	0.002%
94	14.554	2207	2209	2210	rBV2	257	158	0.01%	0.002%
95	14.975	2276	2278	2279	rBV	295	171	0.01%	0.002%
96	15.139	2304	2305	2306	rVB	425	155	0.01%	0.002%
97	15.158	2306	2308	2311	rBV3	323	269	0.02%	0.003%
98	15.182	2311	2312	2313	rBV	499	241	0.02%	0.003%
99	15.487	2360	2362	2363	rBV	637	345	0.03%	0.004%
100	16.365	2503	2506	2508	rBV3	633	771	0.06%	0.008%


Sum of corrected areas: 9129508

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036101.D
Acq On : 09 Jun 2023 12:01
Operator : JC/MD
Sample : 03107-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

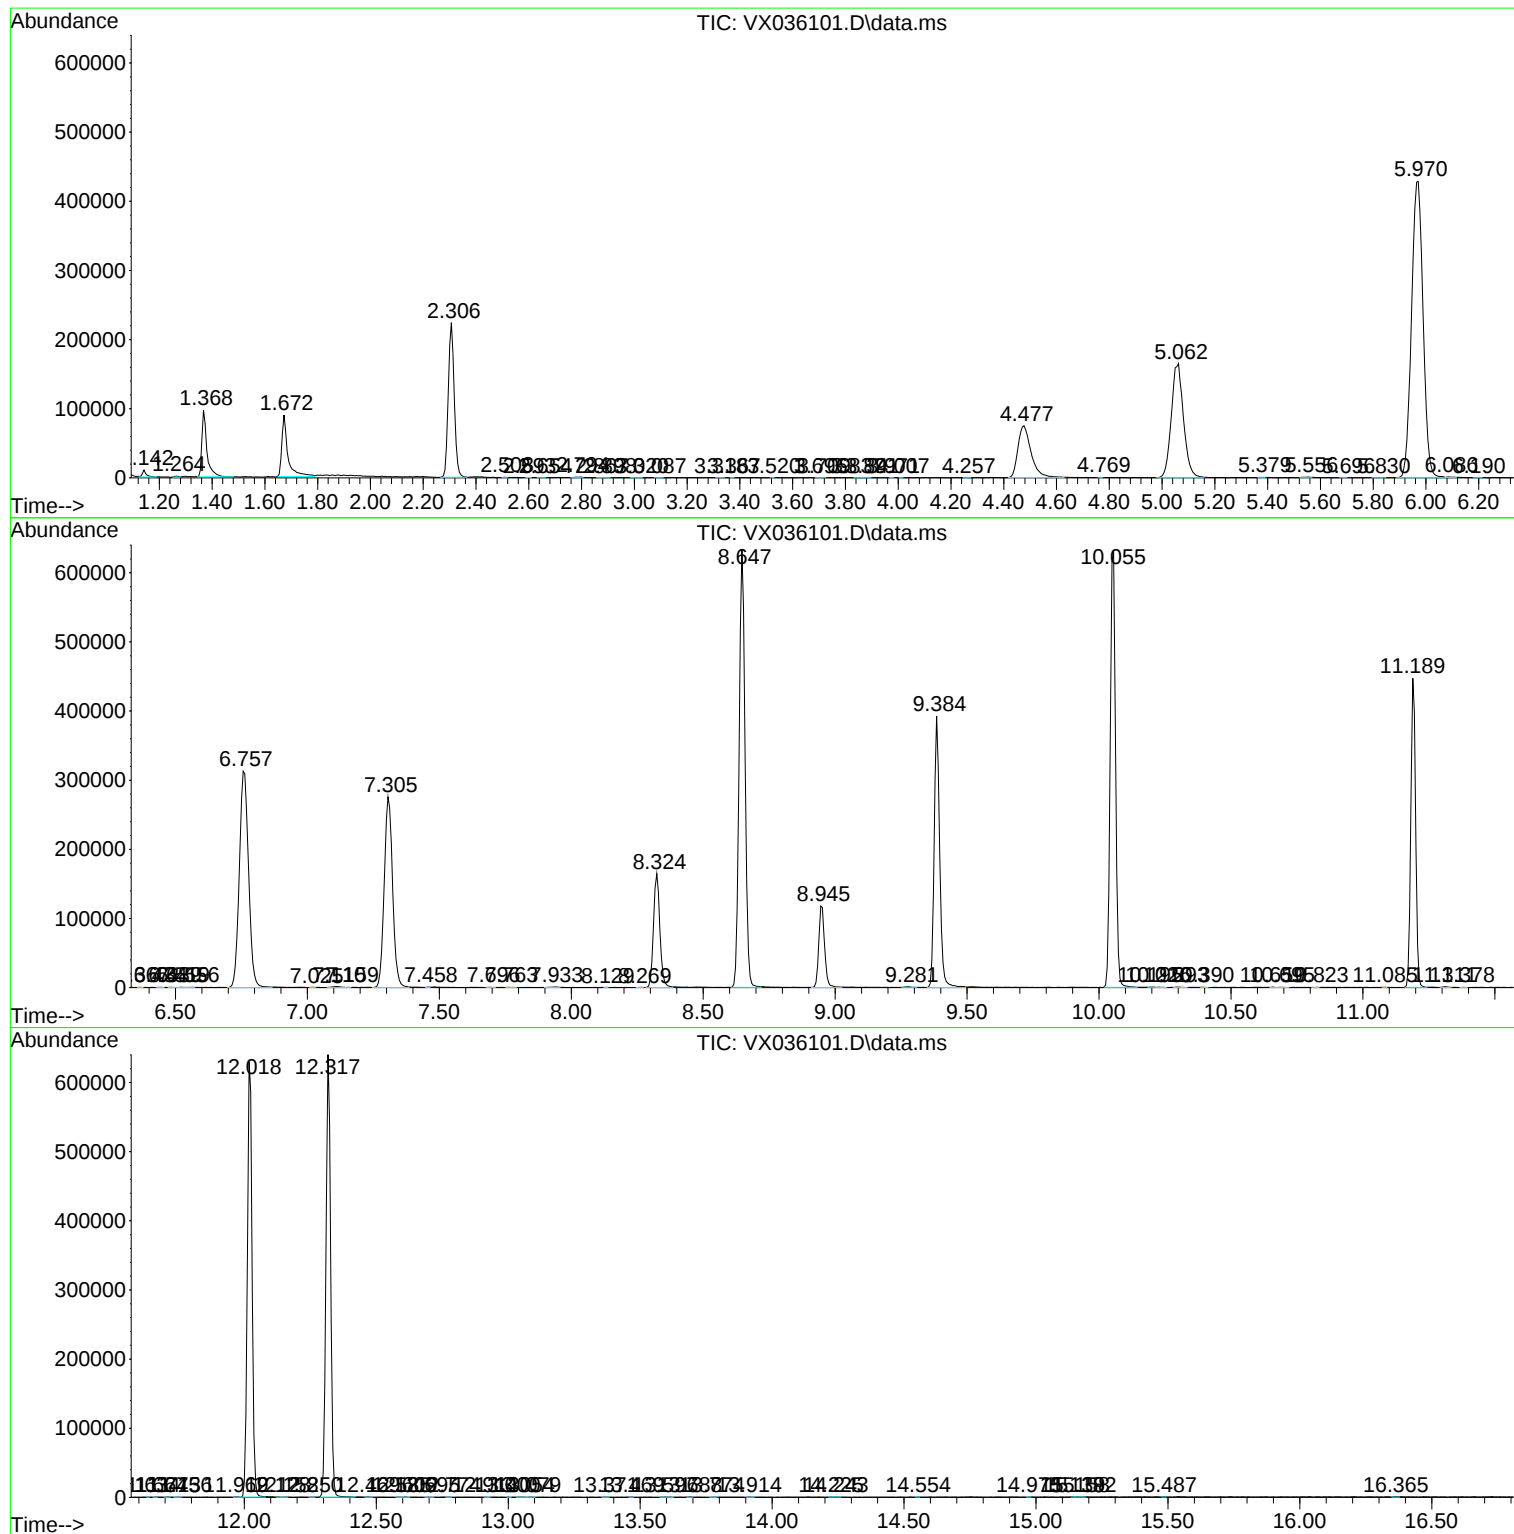

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036101.D
Acq On : 09 Jun 2023 12:01
Operator : JC/MD
Sample : 03107-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036101.D
Acq On : 09 Jun 2023 12:01
Operator : JC/MD
Sample : 03107-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------