

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036103.D
 Acq On : 09 Jun 2023 12:47
 Operator : JC/MD
 Sample : 03107-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rBV	8939	8822	0.68%	0.097%
2	1.264	26	29	32	rBV2	3378	3519	0.27%	0.039%
3	1.367	42	46	59	rVB	95280	122190	9.40%	1.340%
4	1.672	91	96	108	rBV	88247	138702	10.67%	1.521%
5	2.306	194	200	210	rVV	226555	346551	26.66%	3.799%
6	2.410	211	217	231	rVB2	5923	17649	1.36%	0.193%
7	2.568	240	243	244	rBV2	390	412	0.03%	0.005%
8	2.940	298	304	313	rVB	13639	31612	2.43%	0.347%
9	3.306	363	364	365	rBV	274	168	0.01%	0.002%
10	3.361	371	373	377	rBB3	178	231	0.02%	0.003%
11	3.452	387	388	391	rVB	299	172	0.01%	0.002%
12	3.611	412	414	417	rBV	227	250	0.02%	0.003%
13	3.647	419	420	423	rVB	278	188	0.01%	0.002%
14	3.727	429	433	434	rBV	193	176	0.01%	0.002%
15	3.794	441	444	446	rBV	168	203	0.02%	0.002%
16	3.855	452	454	457	rVB	286	260	0.02%	0.003%
17	3.885	457	459	462	rBV2	227	264	0.02%	0.003%
18	3.983	469	475	476	rBV2	228	372	0.03%	0.004%
19	4.476	546	556	568	rBV	75226	258207	19.86%	2.831%
20	5.056	639	651	671	rBV	160793	518586	39.89%	5.685%
21	5.287	687	689	692	rBV2	207	194	0.01%	0.002%
22	5.458	714	717	719	rBV	229	254	0.02%	0.003%
23	5.494	721	723	725	rVB2	274	284	0.02%	0.003%
24	5.543	727	731	732	rBV2	922	1170	0.09%	0.013%
25	5.970	787	801	821	rBV2	437184	1299923	100.00%	14.252%
26	6.287	849	853	856	rVB2	254	343	0.03%	0.004%
27	6.360	862	865	868	rBV	276	365	0.03%	0.004%
28	6.391	868	870	871	rBV2	266	173	0.01%	0.002%
29	6.537	892	894	896	rVB2	400	329	0.03%	0.004%
30	6.598	901	904	905	rBV2	223	246	0.02%	0.003%
31	6.756	921	930	947	rBV	298736	725127	55.78%	7.950%
32	7.110	983	988	994	rVB4	1530	2875	0.22%	0.032%
33	7.153	994	995	998	rBV2	262	264	0.02%	0.003%
34	7.305	1011	1020	1036	rBV	273601	610095	46.93%	6.689%
35	7.433	1039	1041	1043	rVB2	284	211	0.02%	0.002%
36	7.470	1043	1047	1048	rBV2	637	753	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036103.D
 Acq On : 09 Jun 2023 12:47
 Operator : JC/MD
 Sample : 03107-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.598	1066	1068	1074	rVB2	246	420	0.03%	0.005%
38	7.866	1109	1112	1115	rBV2	320	284	0.02%	0.003%
39	7.903	1115	1118	1119	rBV	164	207	0.02%	0.002%
40	7.939	1119	1124	1130	rVV5	756	1415	0.11%	0.016%
41	8.323	1180	1187	1200	rBV	166807	272395	20.95%	2.986%
42	8.451	1206	1208	1209	rBV	305	203	0.02%	0.002%
43	8.573	1226	1228	1230	rBV	401	322	0.02%	0.004%
44	8.646	1233	1240	1249	rBV	639172	993977	76.46%	10.897%
45	8.805	1265	1266	1269	rVB2	453	353	0.03%	0.004%
46	8.866	1275	1276	1279	rBV3	389	314	0.02%	0.003%
47	8.951	1284	1290	1299	rBV	118974	177911	13.69%	1.951%
48	9.274	1337	1343	1350	rVV3	2255	3667	0.28%	0.040%
49	9.384	1355	1361	1378	rBV	398660	572814	44.07%	6.280%
50	9.634	1401	1402	1409	rVB3	301	392	0.03%	0.004%
51	10.055	1465	1471	1482	rBV	624448	859891	66.15%	9.427%
52	10.219	1496	1498	1499	rBV	294	192	0.01%	0.002%
53	10.238	1499	1501	1505	rVB3	495	472	0.04%	0.005%
54	10.299	1510	1511	1517	rVB3	791	798	0.06%	0.009%
55	10.372	1522	1523	1526	rVB2	374	248	0.02%	0.003%
56	10.396	1526	1527	1531	rVB2	409	397	0.03%	0.004%
57	10.439	1531	1534	1537	rBV2	199	279	0.02%	0.003%
58	10.652	1565	1569	1576	rBV4	3699	5702	0.44%	0.063%
59	10.945	1615	1617	1618	rBV	169	162	0.01%	0.002%
60	11.054	1630	1635	1637	rBV2	326	521	0.04%	0.006%
61	11.085	1638	1640	1643	rVB2	630	517	0.04%	0.006%
62	11.189	1652	1657	1668	rVB	440667	565876	43.53%	6.204%
63	11.311	1674	1677	1683	rVB3	2374	3569	0.27%	0.039%
64	11.408	1690	1693	1695	rBV2	312	339	0.03%	0.004%
65	11.432	1695	1697	1700	rBV2	253	360	0.03%	0.004%
66	11.573	1718	1720	1723	rVB2	267	190	0.01%	0.002%
67	11.713	1739	1743	1747	rVB3	573	799	0.06%	0.009%
68	11.749	1747	1749	1750	rBV	258	223	0.02%	0.002%
69	11.798	1754	1757	1758	rVB2	221	198	0.02%	0.002%
70	11.835	1760	1763	1766	rVV3	354	465	0.04%	0.005%
71	11.969	1783	1785	1788	rBV	386	324	0.02%	0.004%
72	12.018	1788	1793	1803	rBV	582504	759533	58.43%	8.327%
73	12.158	1815	1816	1819	rVB	398	277	0.02%	0.003%
74	12.195	1819	1822	1823	rBV2	212	236	0.02%	0.003%
75	12.213	1823	1825	1826	rBV	499	340	0.03%	0.004%
76	12.316	1837	1842	1852	rBV	630087	794210	61.10%	8.707%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036103.D
 Acq On : 09 Jun 2023 12:47
 Operator : JC/MD
 Sample : 03107-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.438	1861	1862	1863	rBV	382	200	0.02%	0.002%
78	12.761	1913	1915	1919	rVB2	822	844	0.06%	0.009%
79	12.859	1928	1931	1934	rBV3	1221	1390	0.11%	0.015%
80	12.890	1934	1936	1939	rVB	235	243	0.02%	0.003%
81	12.950	1944	1946	1949	rBV	176	184	0.01%	0.002%
82	12.993	1951	1953	1955	rBV2	182	189	0.01%	0.002%
83	13.048	1960	1962	1964	rBV	264	181	0.01%	0.002%
84	13.091	1966	1969	1970	rBV2	199	232	0.02%	0.003%
85	13.396	2017	2019	2021	rBV2	211	244	0.02%	0.003%
86	13.469	2028	2031	2032	rBV2	207	208	0.02%	0.002%
87	13.530	2039	2041	2043	rVB2	413	317	0.02%	0.003%
88	13.627	2056	2057	2061	rBV	314	342	0.03%	0.004%
89	13.688	2066	2067	2071	rVB	577	453	0.03%	0.005%
90	13.847	2091	2093	2096	rVB2	221	213	0.02%	0.002%
91	14.072	2127	2130	2133	rBV	322	473	0.04%	0.005%
92	14.121	2137	2138	2143	rBV2	459	537	0.04%	0.006%
93	14.328	2170	2172	2175	rVB2	329	349	0.03%	0.004%
94	14.359	2175	2177	2178	rBV	328	187	0.01%	0.002%
95	14.401	2181	2184	2187	rBV4	410	527	0.04%	0.006%
96	15.212	2315	2317	2319	rBV	527	382	0.03%	0.004%
97	15.511	2365	2366	2367	rBV	558	252	0.02%	0.003%
98	15.609	2381	2382	2386	rBV3	502	789	0.06%	0.009%
99	15.737	2401	2403	2404	rBV2	296	175	0.01%	0.002%
100	16.663	2553	2555	2558	rVB2	472	433	0.03%	0.005%




Sum of corrected areas: 9121276

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036103.D
Acq On : 09 Jun 2023 12:47
Operator : JC/MD
Sample : 03107-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

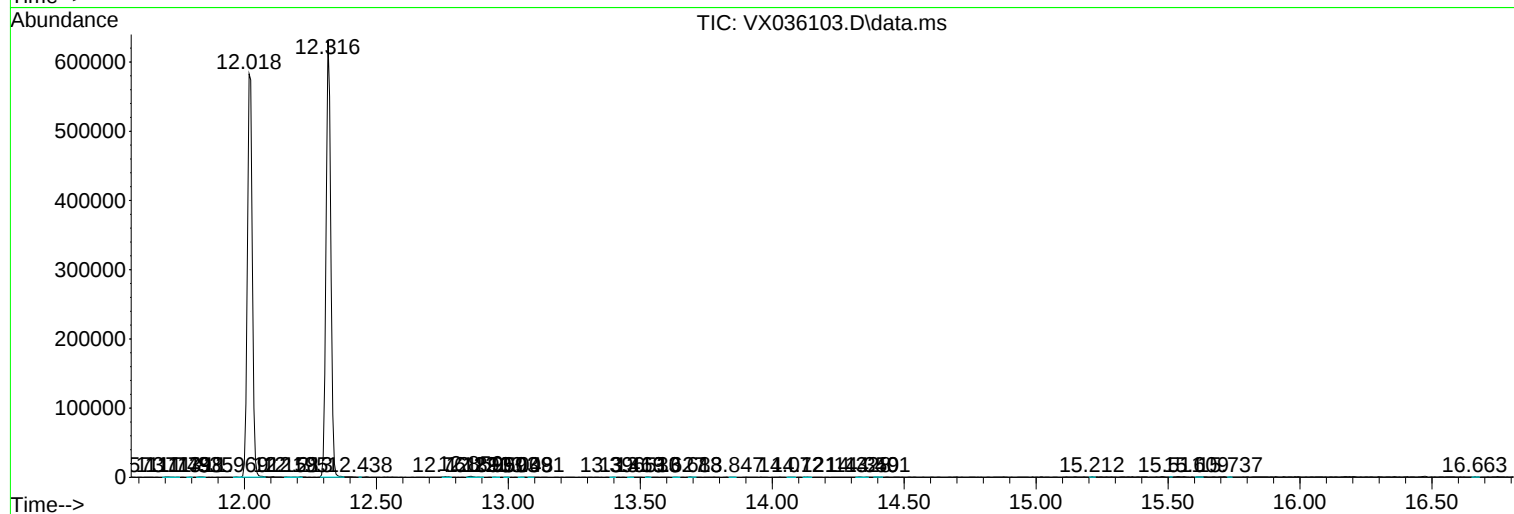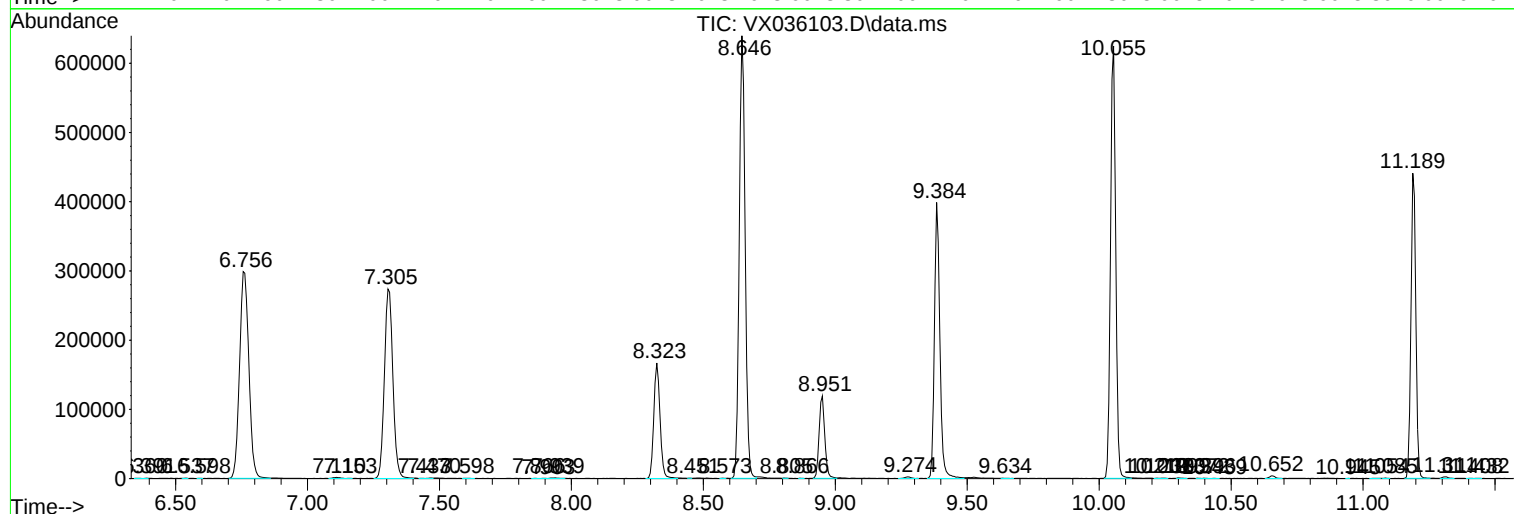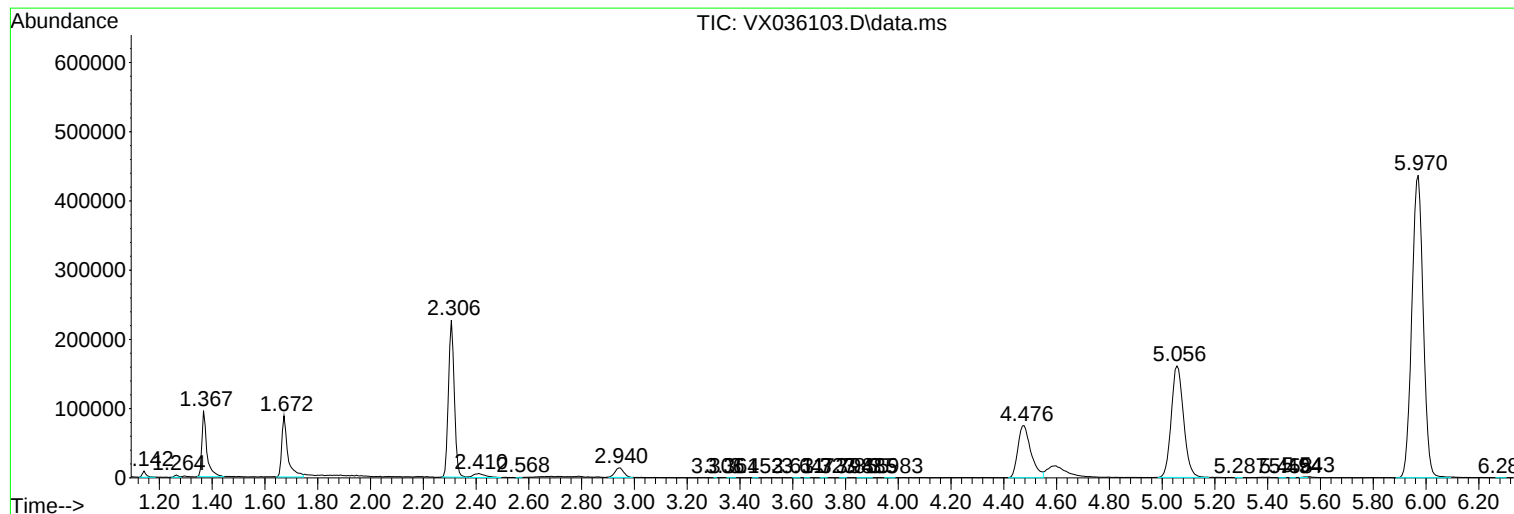

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036103.D
Acq On : 09 Jun 2023 12:47
Operator : JC/MD
Sample : 03107-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036103.D
Acq On : 09 Jun 2023 12:47
Operator : JC/MD
Sample : 03107-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------