

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036104.D
 Acq On : 09 Jun 2023 13:32
 Operator : JC/MD
 Sample : 03107-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	15	rVB2	8361	8886	1.01%	0.134%
2	1.264	27	29	32	rBV3	1283	1513	0.17%	0.023%
3	1.368	42	46	59	rVB	82302	100905	11.47%	1.516%
4	1.672	91	96	109	rBV	68060	105772	12.02%	1.590%
5	2.306	194	200	209	rBV	183604	284111	32.29%	4.270%
6	2.502	230	232	233	rBV2	422	310	0.04%	0.005%
7	2.934	301	303	304	rVB	291	130	0.01%	0.002%
8	2.953	304	306	309	rVB2	306	224	0.03%	0.003%
9	3.087	326	328	330	rVB	240	146	0.02%	0.002%
10	3.184	341	344	346	rBV3	227	312	0.04%	0.005%
11	3.209	346	348	351	rVV2	276	224	0.03%	0.003%
12	3.276	356	359	362	rVV2	208	240	0.03%	0.004%
13	3.300	362	363	365	rVB2	287	158	0.02%	0.002%
14	3.325	365	367	370	rBV2	281	326	0.04%	0.005%
15	3.520	397	399	400	rBV2	186	171	0.02%	0.003%
16	3.568	404	407	409	rVV2	204	250	0.03%	0.004%
17	3.648	417	420	423	rBV2	140	196	0.02%	0.003%
18	3.727	431	433	434	rVB2	249	155	0.02%	0.002%
19	3.757	434	438	439	rBV	279	312	0.04%	0.005%
20	3.812	445	447	451	rVB	207	154	0.02%	0.002%
21	3.928	464	466	469	rVB2	150	96	0.01%	0.001%
22	3.983	473	475	476	rBV2	164	136	0.02%	0.002%
23	4.172	504	506	507	rBV2	211	132	0.02%	0.002%
24	4.190	507	509	512	rBV2	227	255	0.03%	0.004%
25	4.458	543	553	569	rBV	73179	230937	26.25%	3.470%
26	4.836	614	615	617	rVB	322	161	0.02%	0.002%
27	4.910	625	627	629	rBV2	302	239	0.03%	0.004%
28	4.946	631	633	636	rVB	484	352	0.04%	0.005%
29	5.050	636	650	667	rBV	107462	361038	41.03%	5.426%
30	5.227	678	679	680	rBV	186	95	0.01%	0.001%
31	5.275	685	687	689	rBV2	116	121	0.01%	0.002%
32	5.379	700	704	708	rBV4	612	1137	0.13%	0.017%
33	5.501	723	724	725	rVB	266	97	0.01%	0.001%
34	5.544	725	731	734	rBV4	1060	2008	0.23%	0.030%
35	5.672	750	752	753	rBV	203	108	0.01%	0.002%
36	5.714	757	759	760	rBB	228	103	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036104.D
 Acq On : 09 Jun 2023 13:32
 Operator : JC/MD
 Sample : 03107-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	5.964	786	800	816	rBV2	292392	879892	100.00%	13.223%
38	6.409	871	873	875	rBV2	128	150	0.02%	0.002%
39	6.501	886	888	889	rBV	167	146	0.02%	0.002%
40	6.611	905	906	907	rBV	143	95	0.01%	0.001%
41	6.757	920	930	950	rBV	227269	549657	62.47%	8.260%
42	7.110	982	988	996	rBV5	1297	3160	0.36%	0.047%
43	7.306	1011	1020	1035	rVB2	183288	407597	46.32%	6.125%
44	7.470	1045	1047	1053	rVV2	498	586	0.07%	0.009%
45	7.586	1064	1066	1068	rBV	222	244	0.03%	0.004%
46	7.684	1081	1082	1083	rBV	160	101	0.01%	0.002%
47	7.702	1083	1085	1088	rVV2	221	215	0.02%	0.003%
48	7.927	1118	1122	1129	rVB3	632	1247	0.14%	0.019%
49	8.110	1150	1152	1153	rBV	264	132	0.02%	0.002%
50	8.220	1168	1170	1172	rBV	213	141	0.02%	0.002%
51	8.324	1180	1187	1199	rBV	106930	180981	20.57%	2.720%
52	8.543	1222	1223	1226	rBV2	225	301	0.03%	0.005%
53	8.598	1230	1232	1233	rBV	275	134	0.02%	0.002%
54	8.647	1233	1240	1249	rBV	436463	684340	77.78%	10.284%
55	8.946	1284	1289	1300	rBV	78939	115932	13.18%	1.742%
56	9.220	1332	1334	1338	rBV2	220	270	0.03%	0.004%
57	9.275	1338	1343	1348	rVB3	3626	5609	0.64%	0.084%
58	9.317	1348	1350	1352	rBV	249	186	0.02%	0.003%
59	9.384	1355	1361	1377	rBV	335230	486981	55.35%	7.318%
60	9.573	1390	1392	1394	rBV	449	355	0.04%	0.005%
61	9.628	1399	1401	1406	rVB2	382	369	0.04%	0.006%
62	9.665	1406	1407	1409	rBV	224	192	0.02%	0.003%
63	10.049	1465	1470	1477	rBV	461417	643000	73.08%	9.663%
64	10.232	1499	1500	1504	rBV	257	204	0.02%	0.003%
65	10.281	1506	1508	1509	rVV	188	95	0.01%	0.001%
66	10.299	1509	1511	1515	rVB3	539	629	0.07%	0.009%
67	10.451	1533	1536	1537	rBV	226	206	0.02%	0.003%
68	10.902	1609	1610	1612	rBV2	277	183	0.02%	0.003%
69	10.963	1619	1620	1621	rBV	237	97	0.01%	0.001%
70	11.189	1652	1657	1669	rVB	342501	436669	49.63%	6.562%
71	11.311	1673	1677	1682	rVB2	3781	4633	0.53%	0.070%
72	11.610	1724	1726	1729	rBV2	217	293	0.03%	0.004%
73	11.640	1729	1731	1733	rVB	302	168	0.02%	0.003%
74	11.707	1741	1742	1744	rVB2	288	149	0.02%	0.002%
75	11.969	1783	1785	1788	rBV3	327	397	0.05%	0.006%
76	12.018	1788	1793	1801	rBV	460416	582201	66.17%	8.749%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036104.D
 Acq On : 09 Jun 2023 13:32
 Operator : JC/MD
 Sample : 03107-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.219	1824	1826	1828	rVB2	430	299	0.03%	0.004%
78	12.317	1837	1842	1851	rVB	445679	556059	63.20%	8.356%
79	12.457	1863	1865	1869	rVB3	404	599	0.07%	0.009%
80	12.573	1882	1884	1885	rBV	242	152	0.02%	0.002%
81	12.609	1888	1890	1893	rBV2	178	158	0.02%	0.002%
82	12.762	1911	1915	1921	rBV3	1163	1625	0.18%	0.024%
83	12.823	1923	1925	1927	rBV2	247	291	0.03%	0.004%
84	12.853	1927	1930	1934	rBV3	450	651	0.07%	0.010%
85	12.969	1947	1949	1953	rBV2	265	218	0.02%	0.003%
86	13.140	1975	1977	1979	rVB2	305	217	0.02%	0.003%
87	13.158	1979	1980	1981	rBV	280	149	0.02%	0.002%
88	13.237	1992	1993	1995	rBV2	167	104	0.01%	0.002%
89	13.554	2043	2045	2046	rBV	184	94	0.01%	0.001%
90	13.689	2064	2067	2071	rBV3	664	858	0.10%	0.013%
91	13.780	2079	2082	2084	rBV3	261	390	0.04%	0.006%
92	13.963	2110	2112	2113	rBV	195	139	0.02%	0.002%
93	14.121	2136	2138	2139	rBV	432	277	0.03%	0.004%
94	14.164	2143	2145	2146	rBV	277	225	0.03%	0.003%
95	14.377	2178	2180	2183	rBV3	402	510	0.06%	0.008%
96	15.243	2320	2322	2324	rBV2	355	262	0.03%	0.004%
97	15.883	2426	2427	2430	rVB2	525	438	0.05%	0.007%
98	15.981	2442	2443	2444	rBV	389	168	0.02%	0.003%
99	16.462	2520	2522	2525	rBV3	729	660	0.08%	0.010%
100	16.731	2565	2566	2568	rBV2	555	362	0.04%	0.005%

Sum of corrected areas: 6654352


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036104.D
Acq On : 09 Jun 2023 13:32
Operator : JC/MD
Sample : 03107-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

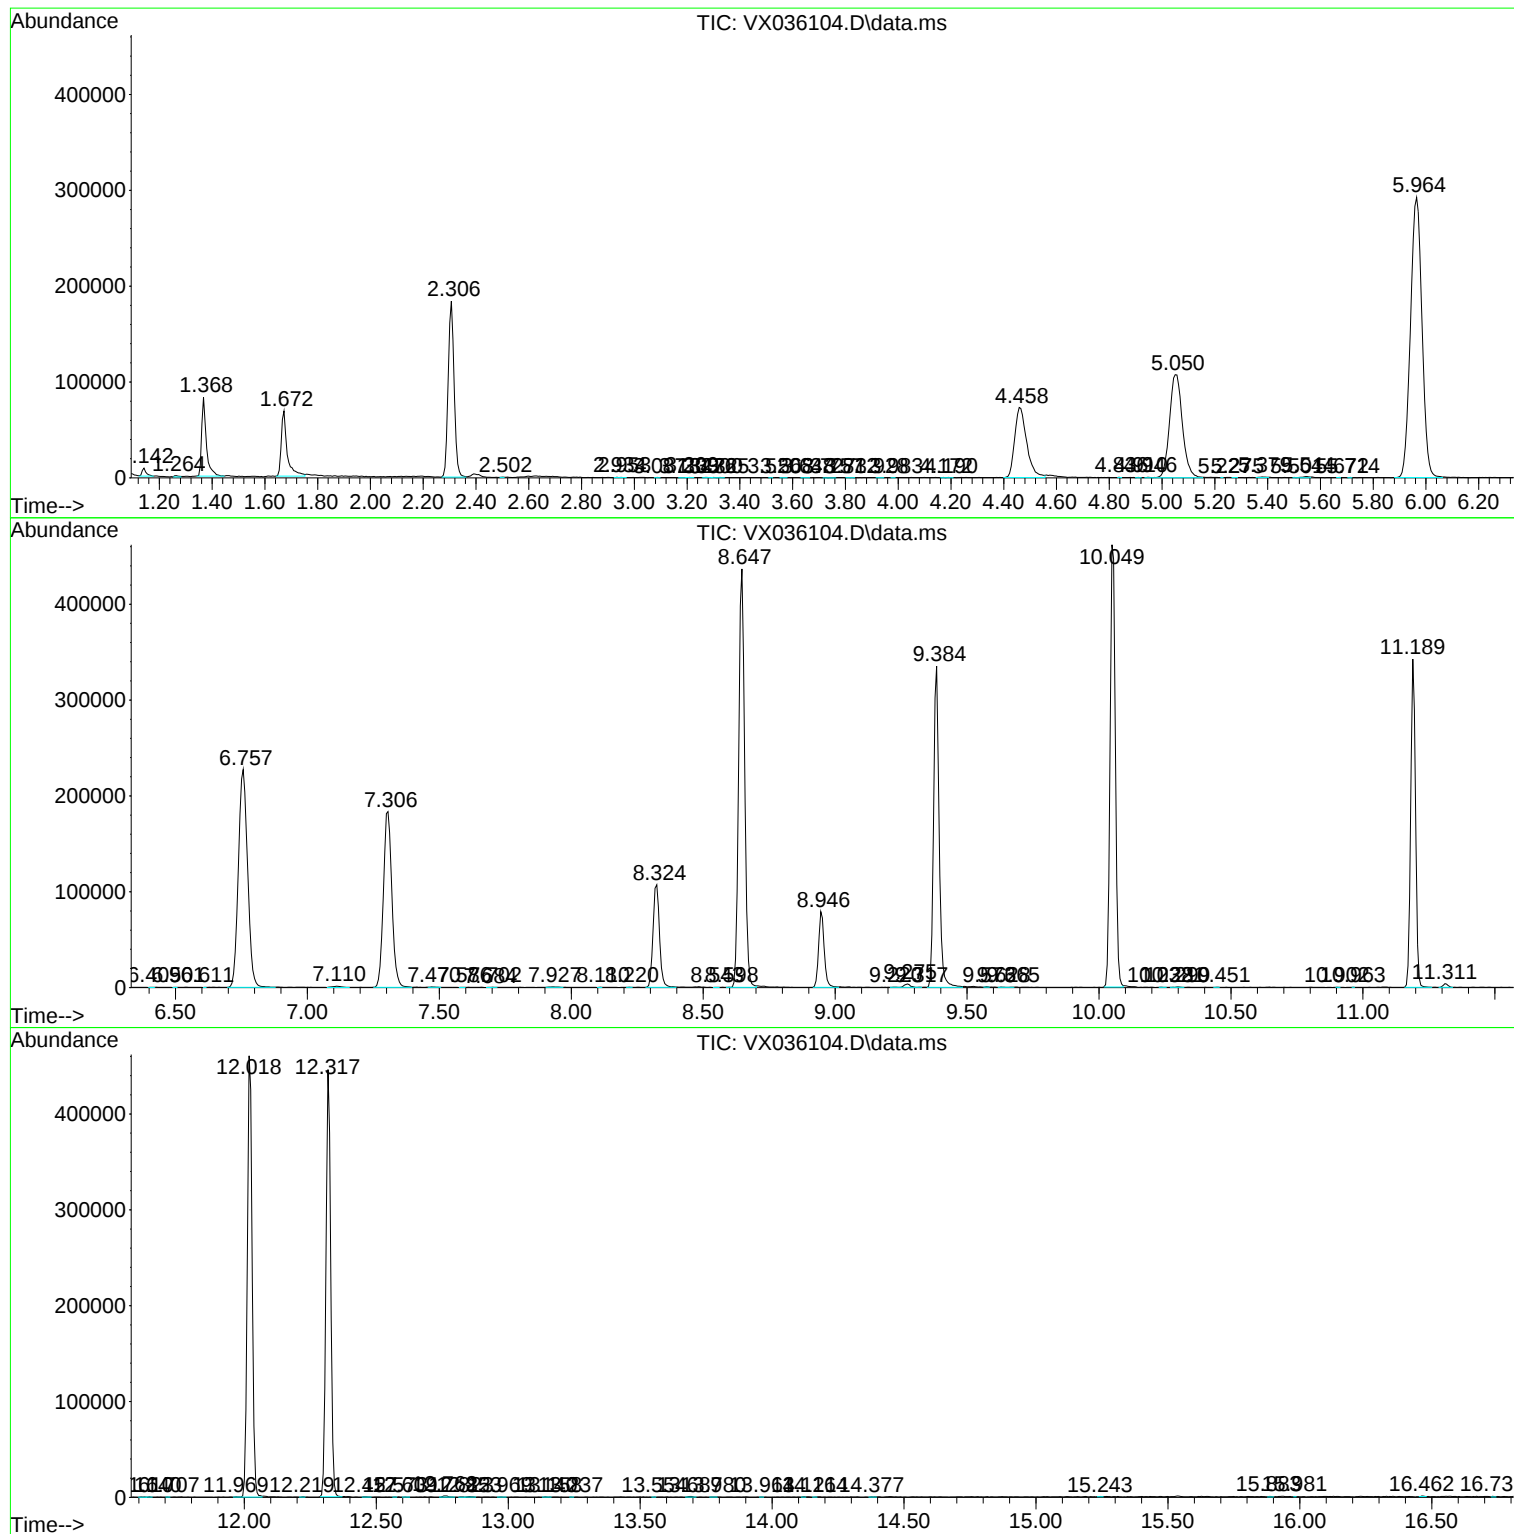

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036104.D
Acq On : 09 Jun 2023 13:32
Operator : JC/MD
Sample : 03107-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036104.D
Acq On : 09 Jun 2023 13:32
Operator : JC/MD
Sample : 03107-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc