

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036105.D
 Acq On : 09 Jun 2023 13:55
 Operator : JC/MD
 Sample : 03107-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	15	rVB	8574	9827	0.90%	0.119%
2	1.264	26	29	32	rBV4	1783	1875	0.17%	0.023%
3	1.368	42	46	59	rBV	91418	116986	10.73%	1.413%
4	1.672	91	96	113	rBV	73519	126416	11.60%	1.527%
5	2.306	194	200	210	rVB	208480	330179	30.29%	3.987%
6	2.404	212	216	217	rBV3	1831	2377	0.22%	0.029%
7	2.502	229	232	240	rVB4	451	918	0.08%	0.011%
8	2.623	248	252	253	rBV3	732	874	0.08%	0.011%
9	2.873	292	293	297	rVB2	277	243	0.02%	0.003%
10	2.934	300	303	304	rBV3	352	352	0.03%	0.004%
11	3.014	312	316	317	rBV3	336	514	0.05%	0.006%
12	3.318	363	366	368	rVV	260	352	0.03%	0.004%
13	3.355	370	372	374	rVV	285	217	0.02%	0.003%
14	3.392	376	378	380	rVV	348	225	0.02%	0.003%
15	3.422	380	383	386	rVV2	246	359	0.03%	0.004%
16	3.465	388	390	392	rVV	244	233	0.02%	0.003%
17	3.489	392	394	397	rVV2	202	217	0.02%	0.003%
18	3.605	412	413	416	rVB2	307	232	0.02%	0.003%
19	3.642	416	419	421	rBV2	262	331	0.03%	0.004%
20	3.666	421	423	426	rVB	184	184	0.02%	0.002%
21	3.721	431	432	436	rVB	222	192	0.02%	0.002%
22	3.757	436	438	440	rBV	325	316	0.03%	0.004%
23	3.831	447	450	452	rBV	286	244	0.02%	0.003%
24	3.977	472	474	477	rBV2	285	305	0.03%	0.004%
25	4.050	484	486	489	rVB2	189	217	0.02%	0.003%
26	4.227	511	515	516	rVB	245	277	0.03%	0.003%
27	4.245	516	518	519	rBV	236	186	0.02%	0.002%
28	4.471	545	555	573	rBV	78719	266725	24.47%	3.221%
29	4.806	608	610	611	rBV	442	278	0.03%	0.003%
30	5.056	639	651	670	rVV2	133639	445798	40.90%	5.384%
31	5.379	698	704	705	rBV4	1405	2496	0.23%	0.030%
32	5.556	727	733	738	rVB3	999	2212	0.20%	0.027%
33	5.964	788	800	817	rBV2	365509	1089925	100.00%	13.162%
34	6.336	859	861	864	rVB	263	218	0.02%	0.003%
35	6.543	893	895	897	rBV3	208	223	0.02%	0.003%
36	6.598	902	904	906	rBV2	179	217	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036105.D
 Acq On : 09 Jun 2023 13:55
 Operator : JC/MD
 Sample : 03107-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.757	921	930	951	rVV	287398	681576	62.53%	8.231%
38	6.958	961	963	966	rVB3	299	304	0.03%	0.004%
39	7.123	982	990	1005	rBV2	59961	137718	12.64%	1.663%
40	7.306	1010	1020	1035	rBV	234953	510743	46.86%	6.168%
41	7.482	1045	1049	1055	rVB4	536	1053	0.10%	0.013%
42	7.531	1055	1057	1060	rVB2	223	221	0.02%	0.003%
43	7.927	1119	1122	1124	rBV3	574	716	0.07%	0.009%
44	7.976	1127	1130	1132	rBV2	238	245	0.02%	0.003%
45	8.043	1139	1141	1143	rBV	286	221	0.02%	0.003%
46	8.208	1166	1168	1172	rBV2	209	239	0.02%	0.003%
47	8.324	1180	1187	1199	rBV	138344	226886	20.82%	2.740%
48	8.513	1216	1218	1219	rVB	364	204	0.02%	0.002%
49	8.586	1227	1230	1233	rBV2	350	470	0.04%	0.006%
50	8.647	1233	1240	1249	rBV	535082	827226	75.90%	9.990%
51	8.763	1258	1259	1261	rVB	346	178	0.02%	0.002%
52	8.952	1283	1290	1299	rBV	96729	148877	13.66%	1.798%
53	9.220	1332	1334	1336	rBV2	228	198	0.02%	0.002%
54	9.275	1338	1343	1352	rBV3	2174	4317	0.40%	0.052%
55	9.384	1355	1361	1379	rBV	398421	563467	51.70%	6.805%
56	9.720	1414	1416	1419	rVB2	224	227	0.02%	0.003%
57	9.836	1432	1435	1438	rBV2	237	331	0.03%	0.004%
58	9.915	1445	1448	1452	rBV3	259	311	0.03%	0.004%
59	10.055	1465	1471	1482	rBV	581286	813878	74.67%	9.829%
60	10.244	1499	1502	1507	rBV2	360	422	0.04%	0.005%
61	10.305	1508	1512	1514	rVV3	568	798	0.07%	0.010%
62	10.628	1563	1565	1568	rVV	236	259	0.02%	0.003%
63	10.659	1568	1570	1572	rVV	415	376	0.03%	0.005%
64	10.835	1596	1599	1601	rVB2	228	179	0.02%	0.002%
65	11.085	1636	1640	1643	rVB3	348	534	0.05%	0.006%
66	11.189	1652	1657	1667	rVV	421535	527618	48.41%	6.372%
67	11.311	1674	1677	1683	rVB2	2158	2838	0.26%	0.034%
68	11.457	1699	1701	1703	rBV2	261	266	0.02%	0.003%
69	11.549	1714	1716	1719	rBV2	201	242	0.02%	0.003%
70	11.634	1728	1730	1732	rVB2	281	185	0.02%	0.002%
71	12.018	1788	1793	1803	rBV	567068	722556	66.29%	8.726%
72	12.225	1825	1827	1831	rVB4	254	230	0.02%	0.003%
73	12.317	1837	1842	1849	rBV	547454	690054	63.31%	8.333%
74	12.762	1911	1915	1919	rBV2	1043	1287	0.12%	0.016%
75	12.817	1922	1924	1928	rBV2	260	371	0.03%	0.004%
76	12.853	1928	1930	1934	rVB3	592	695	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036105.D
 Acq On : 09 Jun 2023 13:55
 Operator : JC/MD
 Sample : 03107-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	13.158	1978	1980	1982	rBV2	316	211	0.02%	0.003%
78	13.219	1989	1990	1993	rVB3	324	297	0.03%	0.004%
79	13.390	2017	2018	2022	rBV2	281	254	0.02%	0.003%
80	13.439	2024	2026	2031	rVB2	225	366	0.03%	0.004%
81	13.493	2033	2035	2037	rBV2	227	248	0.02%	0.003%
82	13.579	2047	2049	2051	rBV2	227	292	0.03%	0.004%
83	13.682	2064	2066	2069	rVB2	529	518	0.05%	0.006%
84	13.780	2080	2082	2085	rVB2	360	308	0.03%	0.004%
85	14.042	2123	2125	2129	rVB2	367	355	0.03%	0.004%
86	14.127	2136	2139	2142	rBV2	614	702	0.06%	0.008%
87	14.213	2151	2153	2155	rBV2	287	313	0.03%	0.004%
88	14.286	2164	2165	2167	rBV2	408	331	0.03%	0.004%
89	14.457	2190	2193	2196	rBV2	575	799	0.07%	0.010%
90	14.573	2210	2212	2213	rBV	332	184	0.02%	0.002%
91	14.999	2281	2282	2283	rBV	439	276	0.03%	0.003%
92	15.219	2316	2318	2322	rBV2	647	860	0.08%	0.010%
93	15.335	2335	2337	2339	rBV3	504	459	0.04%	0.006%
94	15.396	2345	2347	2348	rBV	412	213	0.02%	0.003%
95	15.475	2358	2360	2361	rBV	346	288	0.03%	0.003%
96	15.572	2374	2376	2379	rBV3	528	572	0.05%	0.007%
97	15.639	2385	2387	2389	rBV2	610	384	0.04%	0.005%
98	15.780	2408	2410	2413	rBV3	420	434	0.04%	0.005%
99	16.578	2539	2541	2545	rBV3	583	435	0.04%	0.005%
100	16.700	2559	2561	2562	rBV2	375	211	0.02%	0.003%


Sum of corrected areas: 8280566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036105.D
Acq On : 09 Jun 2023 13:55
Operator : JC/MD
Sample : 03107-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

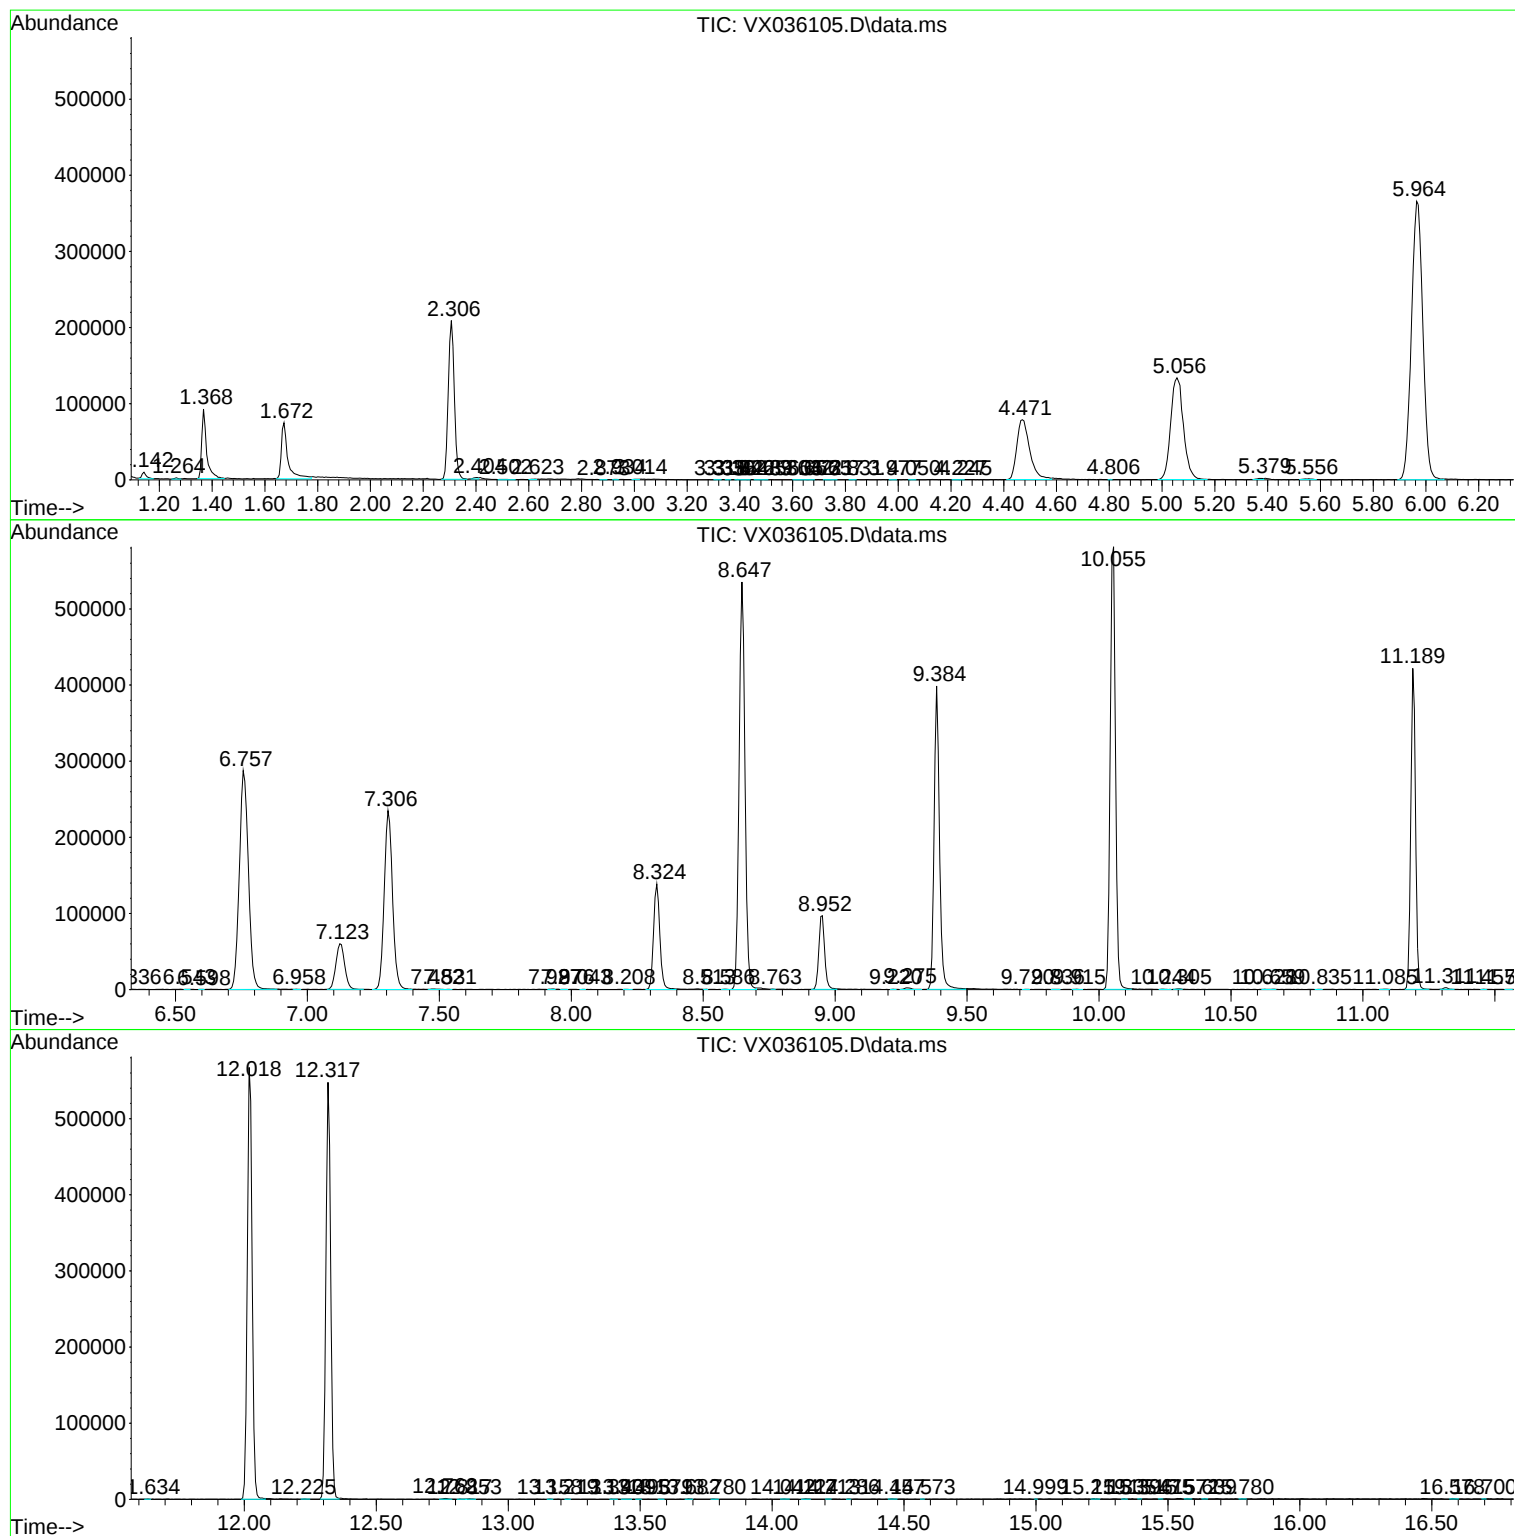

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036105.D
Acq On : 09 Jun 2023 13:55
Operator : JC/MD
Sample : 03107-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036105.D
Acq On : 09 Jun 2023 13:55
Operator : JC/MD
Sample : 03107-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc