

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036106.D
 Acq On : 09 Jun 2023 14:19
 Operator : JC/MD
 Sample : 03107-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	18	rVB2	9068	10505	0.87%	0.118%
2	1.264	26	29	32	rBV3	1812	2000	0.17%	0.023%
3	1.368	42	46	63	rBV	114955	139862	11.62%	1.577%
4	1.672	91	96	109	rBV	94448	139366	11.58%	1.571%
5	2.306	194	200	211	rBV	244895	385423	32.02%	4.345%
6	2.569	239	243	244	rBV2	381	420	0.03%	0.005%
7	3.111	330	332	335	rVV2	243	180	0.01%	0.002%
8	3.227	349	351	353	rBV2	245	290	0.02%	0.003%
9	3.312	362	365	368	rVB2	246	283	0.02%	0.003%
10	3.501	394	396	399	rBV2	206	223	0.02%	0.003%
11	3.568	404	407	408	rBV2	183	195	0.02%	0.002%
12	3.593	408	411	412	rBV	306	229	0.02%	0.003%
13	3.971	470	473	474	rBV2	289	253	0.02%	0.003%
14	4.001	474	478	481	rBV2	134	253	0.02%	0.003%
15	4.135	497	500	502	rBV2	192	239	0.02%	0.003%
16	4.294	523	526	528	rBV	232	297	0.02%	0.003%
17	4.477	545	556	573	rBV	72502	257845	21.42%	2.907%
18	4.806	608	610	611	rVB2	304	188	0.02%	0.002%
19	4.830	611	614	615	rBV	243	233	0.02%	0.003%
20	5.056	639	651	670	rBV	151892	486411	40.42%	5.484%
21	5.391	700	706	711	rBV4	1269	2479	0.21%	0.028%
22	5.556	725	733	740	rVV5	1563	4233	0.35%	0.048%
23	5.757	764	766	770	rVB2	214	188	0.02%	0.002%
24	5.867	781	784	785	rBV	219	185	0.02%	0.002%
25	5.970	788	801	818	rBV2	401495	1203511	100.00%	13.569%
26	6.501	886	888	889	rBV2	263	222	0.02%	0.003%
27	6.544	893	895	897	rVV	265	274	0.02%	0.003%
28	6.665	912	915	920	rVB2	288	449	0.04%	0.005%
29	6.757	920	930	947	rBV	295271	706786	58.73%	7.969%
30	7.111	982	988	994	rBV3	1211	2632	0.22%	0.030%
31	7.196	1000	1002	1004	rBV2	373	320	0.03%	0.004%
32	7.306	1011	1020	1036	rBV	255439	558954	46.44%	6.302%
33	7.458	1044	1045	1047	rBV2	386	307	0.03%	0.003%
34	7.806	1100	1102	1104	rVB2	211	194	0.02%	0.002%
35	7.830	1104	1106	1107	rBV	242	201	0.02%	0.002%
36	7.879	1110	1114	1116	rVB2	194	227	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036106.D
 Acq On : 09 Jun 2023 14:19
 Operator : JC/MD
 Sample : 03107-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.927	1116	1122	1129	rBV5	706	1865	0.15%	0.021%
38	8.324	1180	1187	1201	rBV	155437	252083	20.95%	2.842%
39	8.482	1208	1213	1216	rBV5	800	1351	0.11%	0.015%
40	8.574	1224	1228	1230	rBV2	363	518	0.04%	0.006%
41	8.647	1233	1240	1250	rBV	616247	946057	78.61%	10.666%
42	8.848	1272	1273	1278	rVB2	369	330	0.03%	0.004%
43	8.952	1284	1290	1301	rBV	108334	165268	13.73%	1.863%
44	9.147	1320	1322	1325	rBV2	211	284	0.02%	0.003%
45	9.275	1339	1343	1348	rVB2	1636	2027	0.17%	0.023%
46	9.384	1355	1361	1378	rBV	397428	570069	47.37%	6.427%
47	9.622	1399	1400	1404	rVV3	279	224	0.02%	0.003%
48	9.671	1406	1408	1410	rBV2	303	292	0.02%	0.003%
49	9.695	1410	1412	1415	rVB2	278	215	0.02%	0.002%
50	9.787	1425	1427	1430	rVB2	282	305	0.03%	0.003%
51	9.817	1430	1432	1434	rBV	295	222	0.02%	0.003%
52	10.055	1465	1471	1479	rBV	612191	837458	69.58%	9.442%
53	10.195	1492	1494	1496	rBV	424	338	0.03%	0.004%
54	10.281	1505	1508	1509	rBV	291	284	0.02%	0.003%
55	10.457	1535	1537	1540	rVV2	238	272	0.02%	0.003%
56	10.488	1540	1542	1543	rVV2	232	198	0.02%	0.002%
57	10.531	1546	1549	1551	rVB2	384	410	0.03%	0.005%
58	10.610	1558	1562	1565	rVB2	172	220	0.02%	0.002%
59	10.640	1565	1567	1569	rBV	290	312	0.03%	0.004%
60	10.732	1579	1582	1583	rVB2	329	189	0.02%	0.002%
61	10.799	1589	1593	1594	rBV	212	216	0.02%	0.002%
62	11.122	1643	1646	1647	rVB2	274	193	0.02%	0.002%
63	11.140	1647	1649	1652	rBV	208	248	0.02%	0.003%
64	11.189	1652	1657	1670	rVV	437830	566101	47.04%	6.383%
65	11.311	1674	1677	1681	rVV2	1815	2054	0.17%	0.023%
66	11.354	1682	1684	1686	rVB	328	202	0.02%	0.002%
67	11.756	1745	1750	1752	rBV	253	365	0.03%	0.004%
68	12.018	1788	1793	1801	rBV	611293	785200	65.24%	8.853%
69	12.164	1815	1817	1818	rVB2	354	201	0.02%	0.002%
70	12.195	1818	1822	1823	rBV	410	347	0.03%	0.004%
71	12.317	1837	1842	1850	rBV	644017	817726	67.95%	9.219%
72	12.500	1871	1872	1874	rBV2	327	273	0.02%	0.003%
73	12.573	1883	1884	1886	rBV	311	205	0.02%	0.002%
74	12.701	1904	1905	1907	rVB	318	188	0.02%	0.002%
75	12.725	1907	1909	1910	rBV	256	203	0.02%	0.002%
76	12.859	1929	1931	1932	rVB	410	272	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036106.D
 Acq On : 09 Jun 2023 14:19
 Operator : JC/MD
 Sample : 03107-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.902	1936	1938	1939	rBV2	301	245	0.02%	0.003%
78	13.176	1981	1983	1985	rBV2	267	225	0.02%	0.003%
79	13.244	1991	1994	2000	rVB2	135	261	0.02%	0.003%
80	13.445	2025	2027	2030	rBV2	378	364	0.03%	0.004%
81	13.628	2053	2057	2058	rBV2	272	373	0.03%	0.004%
82	13.670	2061	2064	2065	rBV2	188	205	0.02%	0.002%
83	13.682	2065	2066	2070	rVB2	342	348	0.03%	0.004%
84	13.865	2095	2096	2100	rVB2	319	192	0.02%	0.002%
85	13.896	2100	2101	2104	rBV	270	193	0.02%	0.002%
86	14.030	2121	2123	2124	rBV2	480	278	0.02%	0.003%
87	14.213	2151	2153	2154	rBV2	255	199	0.02%	0.002%
88	14.231	2154	2156	2157	rVV	346	195	0.02%	0.002%
89	14.304	2166	2168	2171	rVB2	318	330	0.03%	0.004%
90	14.908	2265	2267	2270	rBV4	259	305	0.03%	0.003%
91	14.993	2279	2281	2284	rBV3	410	533	0.04%	0.006%
92	15.164	2307	2309	2311	rBV2	459	346	0.03%	0.004%
93	15.377	2341	2344	2346	rBV2	569	861	0.07%	0.010%
94	15.542	2369	2371	2374	rBV3	578	798	0.07%	0.009%
95	16.237	2483	2485	2487	rVB2	462	369	0.03%	0.004%
96	16.261	2487	2489	2492	rBV3	722	766	0.06%	0.009%
97	16.304	2494	2496	2498	rVB2	669	542	0.05%	0.006%
98	16.383	2508	2509	2511	rBV2	429	273	0.02%	0.003%
99	16.469	2521	2523	2524	rBV2	554	380	0.03%	0.004%
100	16.597	2542	2544	2546	rBV2	348	346	0.03%	0.004%


Sum of corrected areas: 8869569

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036106.D
Acq On : 09 Jun 2023 14:19
Operator : JC/MD
Sample : 03107-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

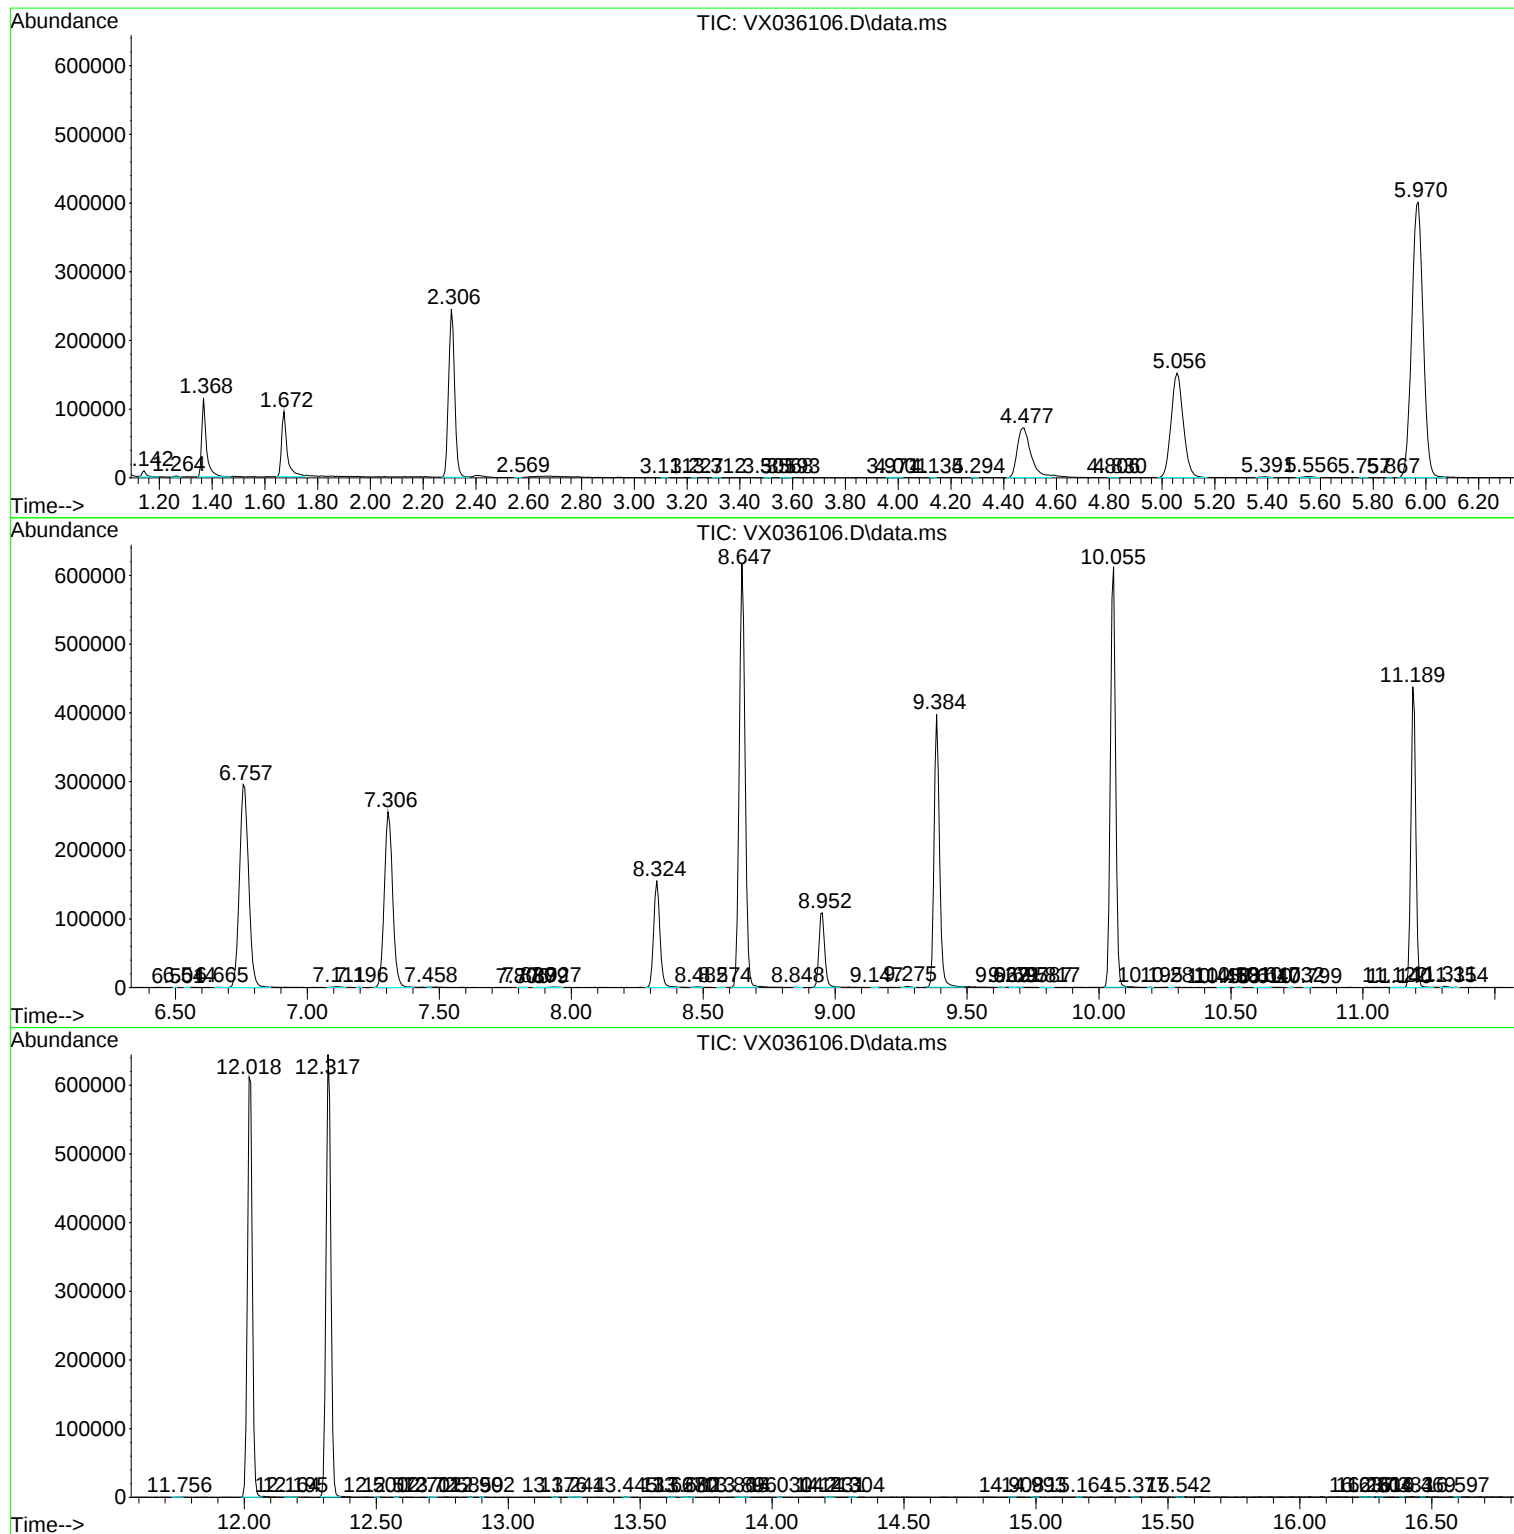

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036106.D
Acq On : 09 Jun 2023 14:19
Operator : JC/MD
Sample : 03107-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036106.D
Acq On : 09 Jun 2023 14:19
Operator : JC/MD
Sample : 03107-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc