

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036107.D
 Acq On : 09 Jun 2023 14:42
 Operator : JC/MD
 Sample : 03107-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	15	rVB2	9513	9770	0.77%	0.101%
2	1.264	27	29	33	rBV2	1842	1581	0.13%	0.016%
3	1.368	42	46	59	rBV	120536	149488	11.85%	1.540%
4	1.673	91	96	115	rBV	99188	149834	11.88%	1.543%
5	2.307	194	200	211	rBV	263293	422140	33.47%	4.348%
6	2.508	230	233	235	rBV2	336	363	0.03%	0.004%
7	2.624	241	252	253	rBV5	1617	4057	0.32%	0.042%
8	2.904	295	298	300	rVB2	330	334	0.03%	0.003%
9	2.989	308	312	315	rBV2	302	471	0.04%	0.005%
10	3.117	330	333	334	rVB2	262	238	0.02%	0.002%
11	3.142	334	337	338	rBV2	443	490	0.04%	0.005%
12	3.252	353	355	357	rBV2	305	186	0.01%	0.002%
13	3.508	395	397	400	rVB2	223	177	0.01%	0.002%
14	3.556	403	405	410	rBV	190	215	0.02%	0.002%
15	3.617	410	415	420	rVB4	531	1070	0.08%	0.011%
16	3.825	447	449	451	rVB2	294	199	0.02%	0.002%
17	3.861	451	455	456	rBV2	196	238	0.02%	0.002%
18	4.196	508	510	513	rBV2	190	217	0.02%	0.002%
19	4.264	519	521	524	rVB	369	317	0.03%	0.003%
20	4.294	524	526	527	rBV	278	170	0.01%	0.002%
21	4.349	532	535	536	rBV2	241	255	0.02%	0.003%
22	4.471	545	555	572	rBV2	80020	283919	22.51%	2.924%
23	5.056	638	651	669	rBV	166474	512154	40.61%	5.275%
24	5.251	681	683	686	rVB3	505	467	0.04%	0.005%
25	5.282	686	688	691	rBV2	257	278	0.02%	0.003%
26	5.391	698	706	715	rVB6	3317	10186	0.81%	0.105%
27	5.550	724	732	741	rBV3	1980	5680	0.45%	0.058%
28	5.660	748	750	752	rBV2	338	234	0.02%	0.002%
29	5.696	755	756	759	rBV	256	215	0.02%	0.002%
30	5.782	768	770	772	rVB	180	163	0.01%	0.002%
31	5.971	788	801	817	rBV2	420912	1261213	100.00%	12.989%
32	6.336	860	861	865	rVB2	238	215	0.02%	0.002%
33	6.373	865	867	872	rBV2	170	250	0.02%	0.003%
34	6.434	875	877	880	rVB2	322	318	0.03%	0.003%
35	6.458	880	881	883	rBV	370	318	0.03%	0.003%
36	6.519	889	891	894	rVB2	234	184	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036107.D
 Acq On : 09 Jun 2023 14:42
 Operator : JC/MD
 Sample : 03107-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.598	903	904	906	rBV2	178	168	0.01%	0.002%
38	6.763	921	931	944	rBV	322569	772277	61.23%	7.954%
39	6.989	966	968	970	rBV	322	267	0.02%	0.003%
40	7.123	982	990	1007	rBV	144785	327295	25.95%	3.371%
41	7.306	1011	1020	1033	rBV	268126	584103	46.31%	6.016%
42	7.470	1043	1047	1048	rBV2	687	787	0.06%	0.008%
43	7.696	1082	1084	1086	rVB	333	164	0.01%	0.002%
44	7.775	1094	1097	1098	rBV2	218	213	0.02%	0.002%
45	7.928	1119	1122	1123	rBV2	921	757	0.06%	0.008%
46	8.220	1169	1170	1173	rBV2	229	233	0.02%	0.002%
47	8.324	1181	1187	1200	rBV	165880	267614	21.22%	2.756%
48	8.549	1223	1224	1228	rBV3	355	403	0.03%	0.004%
49	8.647	1232	1240	1252	rBV	633415	989155	78.43%	10.187%
50	8.952	1284	1290	1304	rVV	112456	171360	13.59%	1.765%
51	9.104	1313	1315	1317	rVB	408	269	0.02%	0.003%
52	9.129	1317	1319	1320	rVB2	339	174	0.01%	0.002%
53	9.226	1333	1335	1339	rBV2	304	482	0.04%	0.005%
54	9.275	1339	1343	1347	rVB3	1463	2327	0.18%	0.024%
55	9.385	1355	1361	1379	rBV	409425	587941	46.62%	6.055%
56	9.732	1416	1418	1419	rBV	265	230	0.02%	0.002%
57	9.817	1428	1432	1434	rBV2	285	427	0.03%	0.004%
58	9.903	1444	1446	1449	rVB	287	218	0.02%	0.002%
59	10.055	1465	1471	1485	rVV	674223	922952	73.18%	9.505%
60	10.250	1500	1503	1505	rVB2	246	282	0.02%	0.003%
61	10.275	1505	1507	1508	rBV2	192	180	0.01%	0.002%
62	10.293	1508	1510	1513	rVB3	328	335	0.03%	0.003%
63	10.384	1523	1525	1527	rBV2	385	346	0.03%	0.004%
64	10.409	1527	1529	1531	rVB2	218	163	0.01%	0.002%
65	10.464	1536	1538	1539	rVB2	310	225	0.02%	0.002%
66	10.525	1546	1548	1552	rVB2	238	191	0.02%	0.002%
67	10.567	1553	1555	1558	rVB	357	247	0.02%	0.003%
68	10.933	1614	1615	1618	rBV	220	251	0.02%	0.003%
69	11.085	1637	1640	1641	rBV2	414	306	0.02%	0.003%
70	11.189	1652	1657	1669	rVV	456039	576466	45.71%	5.937%
71	11.311	1672	1677	1681	rBV3	1454	2199	0.17%	0.023%
72	11.463	1699	1702	1705	rBV2	285	425	0.03%	0.004%
73	11.549	1715	1716	1719	rBV2	172	197	0.02%	0.002%
74	11.756	1748	1750	1752	rVB2	247	174	0.01%	0.002%
75	11.787	1752	1755	1757	rBV2	294	341	0.03%	0.004%
76	11.829	1760	1762	1763	rBV2	280	184	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036107.D
 Acq On : 09 Jun 2023 14:42
 Operator : JC/MD
 Sample : 03107-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.860	1765	1767	1768	rVB	297	184	0.01%	0.002%
78	11.890	1768	1772	1773	rBV2	224	259	0.02%	0.003%
79	12.018	1788	1793	1803	rBV	689439	847761	67.22%	8.731%
80	12.317	1837	1842	1850	rBV	662992	823985	65.33%	8.486%
81	12.573	1882	1884	1885	rBV	269	193	0.02%	0.002%
82	12.664	1897	1899	1901	rVB	300	236	0.02%	0.002%
83	12.695	1901	1904	1905	rBV	255	201	0.02%	0.002%
84	12.756	1911	1914	1918	rBV4	577	926	0.07%	0.010%
85	12.853	1929	1930	1936	rBV3	321	509	0.04%	0.005%
86	13.122	1969	1974	1977	rBV2	427	579	0.05%	0.006%
87	13.170	1981	1982	1986	rVV	301	227	0.02%	0.002%
88	14.024	2120	2122	2124	rVB2	324	260	0.02%	0.003%
89	14.085	2131	2132	2137	rBV	202	292	0.02%	0.003%
90	14.183	2146	2148	2149	rBV2	392	251	0.02%	0.003%
91	14.231	2155	2156	2160	rVB2	321	398	0.03%	0.004%
92	14.304	2167	2168	2170	rVB	312	174	0.01%	0.002%
93	14.347	2173	2175	2176	rBV2	334	286	0.02%	0.003%
94	14.518	2201	2203	2205	rBV	305	261	0.02%	0.003%
95	15.420	2349	2351	2352	rVB	474	206	0.02%	0.002%
96	15.530	2367	2369	2374	rVB4	561	939	0.07%	0.010%
97	15.621	2380	2384	2385	rBV3	432	459	0.04%	0.005%
98	15.676	2392	2393	2395	rBV	594	395	0.03%	0.004%
99	16.621	2546	2548	2550	rVB2	660	483	0.04%	0.005%
100	16.645	2550	2552	2554	rBV2	467	469	0.04%	0.005%

Sum of corrected areas: 9709865




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036107.D
Acq On : 09 Jun 2023 14:42
Operator : JC/MD
Sample : 03107-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

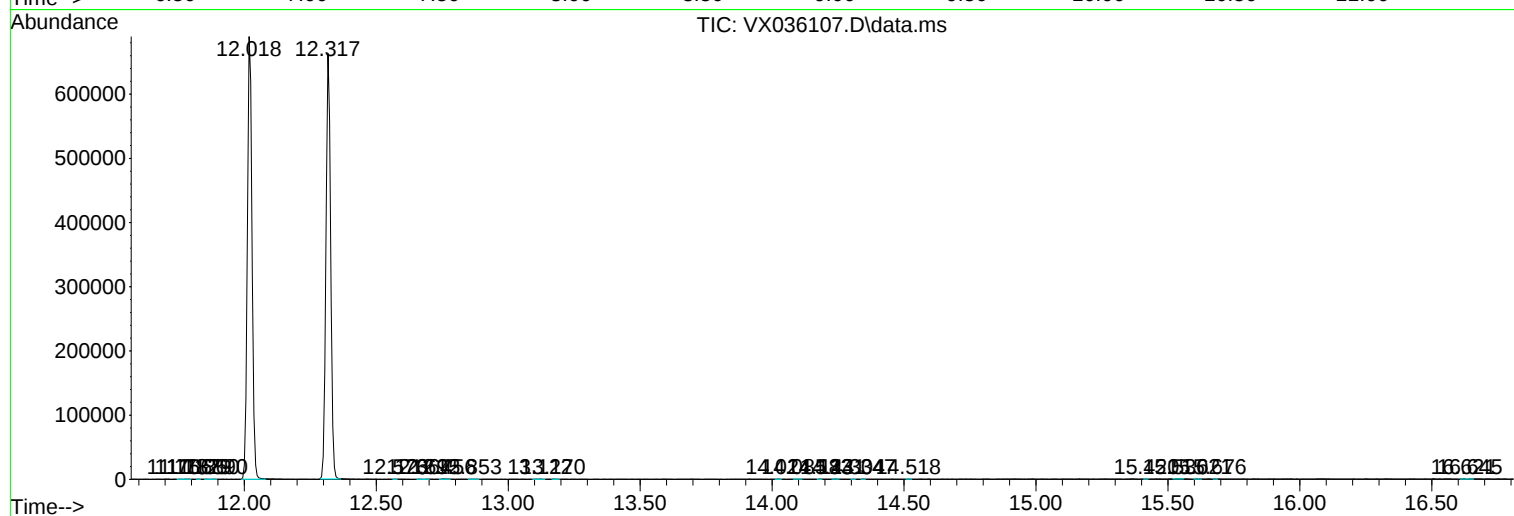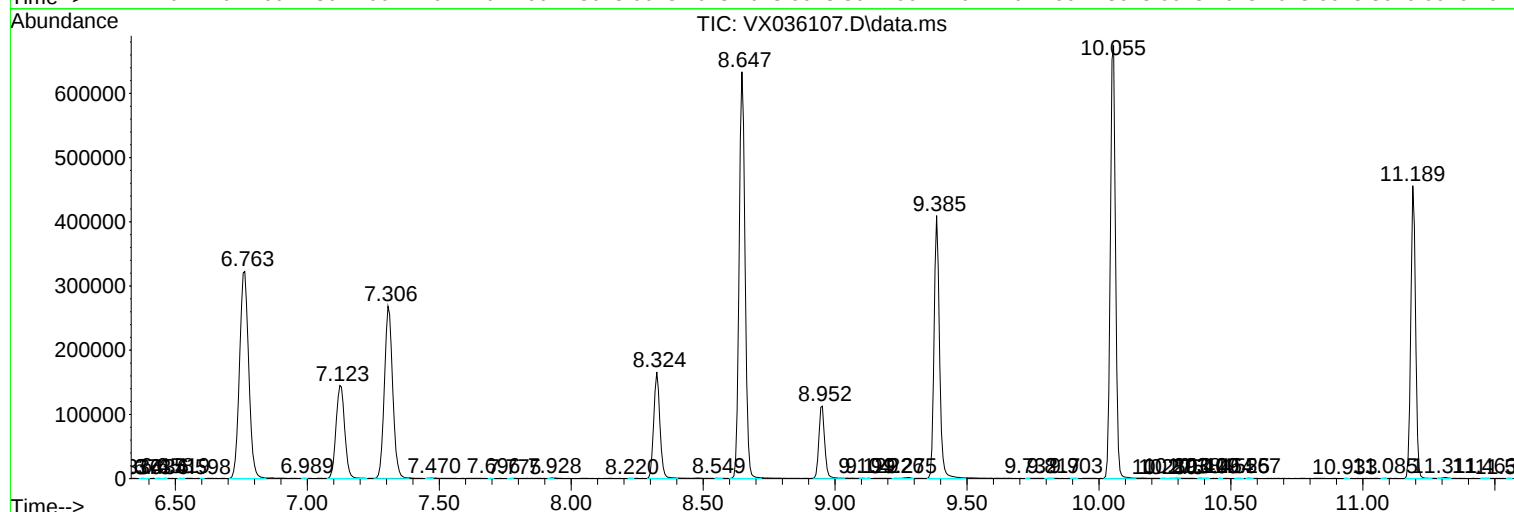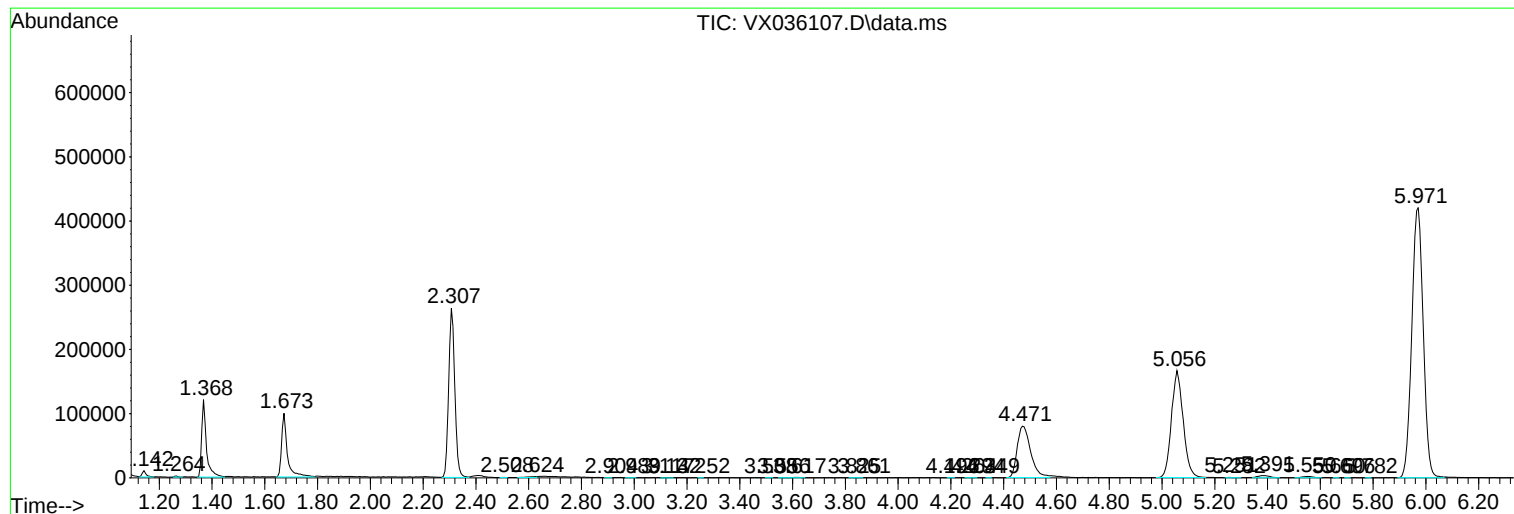

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036107.D
Acq On : 09 Jun 2023 14:42
Operator : JC/MD
Sample : 03107-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036107.D
Acq On : 09 Jun 2023 14:42
Operator : JC/MD
Sample : 03107-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc