

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036108.D
 Acq On : 09 Jun 2023 15:05
 Operator : JC/MD
 Sample : 03107-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB	9529	9889	0.79%	0.107%
2	1.264	26	29	31	rBV2	1924	1951	0.16%	0.021%
3	1.368	42	46	58	rBV	112101	137871	10.97%	1.489%
4	1.672	91	96	115	rBV	97540	145887	11.61%	1.575%
5	2.306	194	200	210	rBV	257086	410911	32.70%	4.437%
6	2.605	245	249	250	rBV3	731	808	0.06%	0.009%
7	2.898	296	297	300	rBV2	259	226	0.02%	0.002%
8	2.928	300	302	303	rVV	295	264	0.02%	0.003%
9	2.947	303	305	309	rVB2	469	573	0.05%	0.006%
10	3.312	361	365	366	rBV2	211	265	0.02%	0.003%
11	3.495	392	395	397	rBV2	235	203	0.02%	0.002%
12	3.599	410	412	415	rVV2	356	337	0.03%	0.004%
13	3.745	434	436	439	rVV2	179	176	0.01%	0.002%
14	3.818	444	448	452	rVV2	263	398	0.03%	0.004%
15	3.855	452	454	455	rVV	335	170	0.01%	0.002%
16	3.879	456	458	460	rVV	232	190	0.02%	0.002%
17	3.898	460	461	463	rVB2	310	177	0.01%	0.002%
18	3.971	471	473	476	rBV2	165	169	0.01%	0.002%
19	4.032	479	483	485	rBV2	240	306	0.02%	0.003%
20	4.123	495	498	499	rVB2	206	182	0.01%	0.002%
21	4.471	545	555	571	rBV	77660	270069	21.49%	2.916%
22	5.056	639	651	671	rBV	157402	514155	40.92%	5.551%
23	5.233	678	680	682	rBV	414	420	0.03%	0.005%
24	5.379	700	704	705	rBV2	853	1049	0.08%	0.011%
25	5.538	723	730	732	rBV2	1277	2317	0.18%	0.025%
26	5.611	741	742	746	rVB2	220	239	0.02%	0.003%
27	5.970	786	801	816	rBV2	415384	1256488	100.00%	13.567%
28	6.287	851	853	855	rBV2	294	268	0.02%	0.003%
29	6.348	862	863	867	rVB	214	186	0.01%	0.002%
30	6.385	867	869	871	rBV2	200	202	0.02%	0.002%
31	6.440	876	878	879	rBV	275	170	0.01%	0.002%
32	6.458	879	881	884	rVB	254	266	0.02%	0.003%
33	6.513	886	890	891	rBV2	246	264	0.02%	0.003%
34	6.531	891	893	894	rBV	238	202	0.02%	0.002%
35	6.763	918	931	948	rVV	306087	744269	59.23%	8.036%
36	6.909	952	955	960	rVB2	505	765	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036108.D
 Acq On : 09 Jun 2023 15:05
 Operator : JC/MD
 Sample : 03107-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.952	960	962	963	rBV	381	240	0.02%	0.003%
38	7.110	983	988	997	rVV6	1441	3774	0.30%	0.041%
39	7.305	1012	1020	1042	rVB	263605	586731	46.70%	6.335%
40	7.482	1042	1049	1051	rBV3	912	1406	0.11%	0.015%
41	7.555	1058	1061	1062	rBV2	308	329	0.03%	0.004%
42	7.622	1071	1072	1075	rVB2	226	200	0.02%	0.002%
43	7.653	1075	1077	1079	rBV2	206	215	0.02%	0.002%
44	7.854	1107	1110	1112	rBV2	252	238	0.02%	0.003%
45	7.933	1118	1123	1128	rVB5	652	1197	0.10%	0.013%
46	8.238	1171	1173	1174	rVB	316	170	0.01%	0.002%
47	8.324	1181	1187	1196	rBV	164565	266155	21.18%	2.874%
48	8.470	1209	1211	1212	rBV2	416	433	0.03%	0.005%
49	8.647	1233	1240	1251	rBV	629510	982960	78.23%	10.613%
50	8.952	1284	1290	1304	rBV	116653	174762	13.91%	1.887%
51	9.159	1323	1324	1326	rBV2	229	203	0.02%	0.002%
52	9.275	1340	1343	1350	rVB2	1560	1666	0.13%	0.018%
53	9.384	1355	1361	1380	rBV	410607	591562	47.08%	6.387%
54	9.604	1395	1397	1401	rVV3	442	554	0.04%	0.006%
55	9.640	1401	1403	1407	rVB2	480	548	0.04%	0.006%
56	9.677	1407	1409	1410	rBV	430	305	0.02%	0.003%
57	9.714	1413	1415	1416	rVB	446	286	0.02%	0.003%
58	9.738	1416	1419	1420	rBV	364	297	0.02%	0.003%
59	9.781	1424	1426	1429	rVB2	338	352	0.03%	0.004%
60	9.842	1434	1436	1440	rBV2	209	283	0.02%	0.003%
61	9.903	1444	1446	1447	rVB2	322	201	0.02%	0.002%
62	10.055	1465	1471	1484	rBV	643150	886385	70.54%	9.570%
63	10.311	1509	1513	1515	rVB2	368	440	0.04%	0.005%
64	10.348	1517	1519	1522	rBV2	243	218	0.02%	0.002%
65	10.427	1531	1532	1535	rBV2	226	285	0.02%	0.003%
66	10.713	1574	1579	1580	rBV2	159	175	0.01%	0.002%
67	10.750	1583	1585	1588	rVB2	207	190	0.02%	0.002%
68	10.787	1588	1591	1594	rBV2	253	348	0.03%	0.004%
69	11.085	1637	1640	1642	rVB2	445	532	0.04%	0.006%
70	11.189	1652	1657	1666	rBV	454365	588086	46.80%	6.350%
71	11.280	1670	1672	1673	rBV	219	186	0.01%	0.002%
72	11.311	1674	1677	1685	rVB	1294	1817	0.14%	0.020%
73	11.439	1696	1698	1700	rVB	242	184	0.01%	0.002%
74	11.549	1714	1716	1719	rVV2	187	226	0.02%	0.002%
75	11.597	1722	1724	1725	rBV2	210	209	0.02%	0.002%
76	11.707	1740	1742	1743	rBV	424	304	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036108.D
 Acq On : 09 Jun 2023 15:05
 Operator : JC/MD
 Sample : 03107-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.786	1753	1755	1757	rVB	277	193	0.02%	0.002%
78	11.847	1763	1765	1767	rBV2	280	176	0.01%	0.002%
79	12.018	1788	1793	1808	rBV	644064	820838	65.33%	8.863%
80	12.231	1825	1828	1830	rVV2	470	477	0.04%	0.005%
81	12.317	1837	1842	1860	rVB	662487	836836	66.60%	9.035%
82	12.463	1864	1866	1870	rBV3	366	484	0.04%	0.005%
83	12.524	1875	1876	1877	rBV	380	183	0.01%	0.002%
84	12.762	1911	1915	1919	rVB3	510	815	0.06%	0.009%
85	12.792	1919	1920	1923	rBV2	206	219	0.02%	0.002%
86	12.847	1927	1929	1931	rBV2	360	197	0.02%	0.002%
87	13.103	1969	1971	1973	rBV	340	259	0.02%	0.003%
88	13.292	2000	2002	2003	rBV	251	187	0.01%	0.002%
89	13.365	2012	2014	2017	rVV	172	186	0.01%	0.002%
90	14.109	2134	2136	2137	rBV	215	169	0.01%	0.002%
91	14.280	2163	2164	2166	rBV2	292	271	0.02%	0.003%
92	14.353	2172	2176	2179	rBV3	334	541	0.04%	0.006%
93	14.920	2267	2269	2270	rBV	337	264	0.02%	0.003%
94	15.359	2339	2341	2342	rBV	504	370	0.03%	0.004%
95	15.463	2356	2358	2361	rBV2	334	304	0.02%	0.003%
96	15.542	2369	2371	2373	rVB2	678	378	0.03%	0.004%
97	15.639	2385	2387	2391	rVB	433	298	0.02%	0.003%
98	15.816	2415	2416	2418	rBV	552	325	0.03%	0.004%
99	16.005	2444	2447	2448	rBV3	449	455	0.04%	0.005%
100	16.725	2564	2565	2568	rBV2	395	320	0.03%	0.003%


Sum of corrected areas: 9261679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036108.D
Acq On : 09 Jun 2023 15:05
Operator : JC/MD
Sample : 03107-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

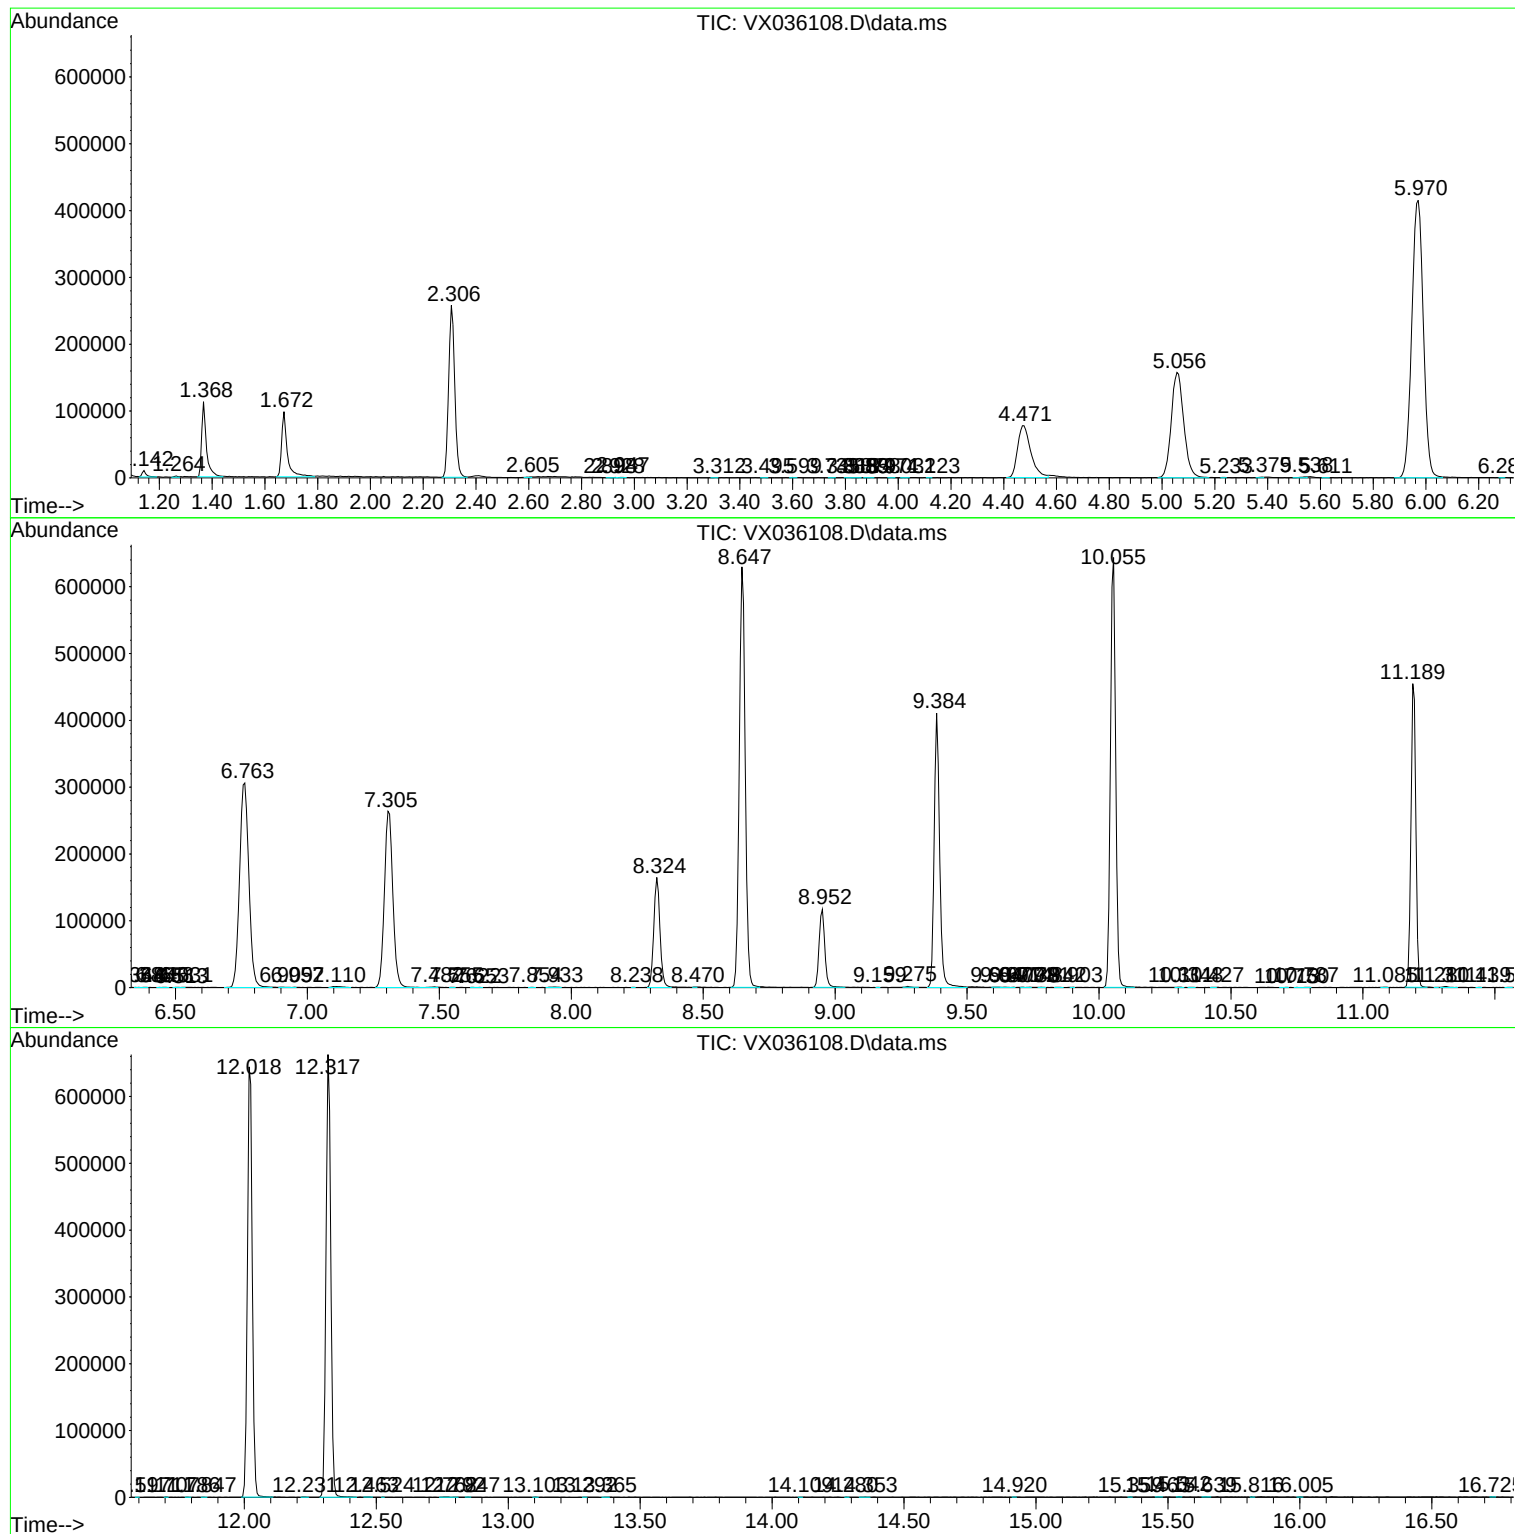

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036108.D
Acq On : 09 Jun 2023 15:05
Operator : JC/MD
Sample : 03107-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036108.D
Acq On : 09 Jun 2023 15:05
Operator : JC/MD
Sample : 03107-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc