

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036109.D
 Acq On : 09 Jun 2023 15:29
 Operator : JC/MD
 Sample : 03107-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036109.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	20	rVB3	9914	12810	1.03%	0.131%
2	1.264	27	29	33	rVB2	1701	1176	0.09%	0.012%
3	1.368	42	46	60	rBV	118128	145287	11.66%	1.491%
4	1.673	91	96	106	rBV	91514	141336	11.34%	1.450%
5	2.307	194	200	210	rBV	263039	421317	33.81%	4.324%
6	2.788	277	279	282	rBV3	690	690	0.06%	0.007%
7	2.861	289	291	294	rBV3	284	312	0.03%	0.003%
8	3.160	338	340	343	rVV2	150	185	0.01%	0.002%
9	3.325	365	367	370	rVV2	270	350	0.03%	0.004%
10	3.380	373	376	379	rVB2	168	214	0.02%	0.002%
11	3.410	379	381	385	rBV	246	332	0.03%	0.003%
12	3.532	398	401	402	rBV	271	196	0.02%	0.002%
13	3.593	408	411	412	rBV	490	333	0.03%	0.003%
14	3.745	434	436	438	rBV2	239	169	0.01%	0.002%
15	3.770	438	440	442	rVB2	249	195	0.02%	0.002%
16	3.800	442	445	447	rBV2	161	211	0.02%	0.002%
17	3.837	449	451	454	rVV	234	176	0.01%	0.002%
18	3.953	468	470	473	rVB2	196	168	0.01%	0.002%
19	4.111	494	496	499	rVB2	292	253	0.02%	0.003%
20	4.166	503	505	507	rVV	301	195	0.02%	0.002%
21	4.373	535	539	540	rVB2	195	191	0.02%	0.002%
22	4.471	545	555	581	rBV	79078	282860	22.70%	2.903%
23	4.800	608	609	611	rVB	307	193	0.02%	0.002%
24	4.952	631	634	636	rVB	237	234	0.02%	0.002%
25	5.062	638	652	671	rBV	160647	509707	40.90%	5.231%
26	5.227	677	679	683	rVB3	317	256	0.02%	0.003%
27	5.367	697	702	703	rBV2	1820	1857	0.15%	0.019%
28	5.562	723	734	742	rBV4	1614	4383	0.35%	0.045%
29	5.684	751	754	755	rBV	242	196	0.02%	0.002%
30	5.702	755	757	758	rBV	404	187	0.02%	0.002%
31	5.721	758	760	762	rVV2	250	224	0.02%	0.002%
32	5.843	779	780	784	rVB	263	277	0.02%	0.003%
33	5.891	784	788	789	rBV2	254	312	0.03%	0.003%
34	5.971	789	801	822	rVV2	413262	1246104	100.00%	12.788%
35	6.221	840	842	843	rBV2	213	165	0.01%	0.002%
36	6.281	850	852	854	rVB2	317	202	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036109.D
 Acq On : 09 Jun 2023 15:29
 Operator : JC/MD
 Sample : 03107-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.446	876	879	881	rBV2	215	234	0.02%	0.002%
38	6.672	914	916	920	rBV2	228	198	0.02%	0.002%
39	6.763	920	931	950	rBV	311495	753040	60.43%	7.728%
40	7.123	982	990	1003	rBV	215042	470182	37.73%	4.825%
41	7.306	1011	1020	1034	rBV	269020	583032	46.79%	5.983%
42	7.610	1068	1070	1074	rVB2	192	165	0.01%	0.002%
43	7.781	1096	1098	1101	rBV	200	228	0.02%	0.002%
44	7.812	1101	1103	1109	rVB2	339	404	0.03%	0.004%
45	7.934	1118	1123	1127	rBV2	818	1302	0.10%	0.013%
46	8.123	1151	1154	1157	rVB2	235	317	0.03%	0.003%
47	8.153	1157	1159	1160	rBV	319	251	0.02%	0.003%
48	8.184	1163	1164	1167	rBV2	181	210	0.02%	0.002%
49	8.324	1180	1187	1203	rBV	159835	262876	21.10%	2.698%
50	8.476	1210	1212	1218	rVB4	857	1182	0.09%	0.012%
51	8.568	1225	1227	1229	rVB	413	229	0.02%	0.002%
52	8.647	1233	1240	1254	rBV	632188	981171	78.74%	10.069%
53	8.885	1278	1279	1282	rVB2	193	168	0.01%	0.002%
54	8.946	1284	1289	1302	rVV	112159	171217	13.74%	1.757%
55	9.116	1314	1317	1318	rBV2	288	315	0.03%	0.003%
56	9.159	1321	1324	1326	rVB2	397	369	0.03%	0.004%
57	9.281	1339	1344	1348	rVB	2192	3248	0.26%	0.033%
58	9.385	1355	1361	1376	rBV	405301	580983	46.62%	5.962%
59	9.720	1414	1416	1418	rBV	260	243	0.02%	0.002%
60	9.860	1437	1439	1441	rBV	184	223	0.02%	0.002%
61	10.055	1465	1471	1482	rBV	642281	896275	71.93%	9.198%
62	10.787	1588	1591	1592	rBV2	313	266	0.02%	0.003%
63	11.037	1629	1632	1633	rVB2	268	212	0.02%	0.002%
64	11.079	1637	1639	1642	rBV3	326	413	0.03%	0.004%
65	11.189	1652	1657	1664	rBV	459416	578058	46.39%	5.932%
66	11.317	1674	1678	1684	rVB	2355	3233	0.26%	0.033%
67	11.378	1684	1688	1691	rVB2	280	390	0.03%	0.004%
68	11.427	1691	1696	1699	rBV3	258	453	0.04%	0.005%
69	11.488	1704	1706	1710	rVB	267	309	0.02%	0.003%
70	11.524	1710	1712	1715	rBV2	167	201	0.02%	0.002%
71	11.707	1739	1742	1745	rBV	322	530	0.04%	0.005%
72	12.018	1788	1793	1804	rBV	664395	836048	67.09%	8.580%
73	12.171	1816	1818	1819	rBV2	236	182	0.01%	0.002%
74	12.219	1823	1826	1828	rBV3	444	473	0.04%	0.005%
75	12.317	1837	1842	1851	rBV	660223	833832	66.92%	8.557%
76	12.500	1871	1872	1875	rBV	280	202	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036109.D
 Acq On : 09 Jun 2023 15:29
 Operator : JC/MD
 Sample : 03107-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.549	1879	1880	1882	rBV	247	186	0.01%	0.002%
78	12.756	1912	1914	1918	rVB4	922	1137	0.09%	0.012%
79	12.853	1927	1930	1935	rVB3	489	748	0.06%	0.008%
80	12.896	1935	1937	1938	rBV	216	190	0.02%	0.002%
81	12.927	1940	1942	1944	rBV	179	192	0.02%	0.002%
82	13.561	2044	2046	2049	rVB3	381	337	0.03%	0.003%
83	13.622	2052	2056	2057	rBV2	244	260	0.02%	0.003%
84	13.780	2079	2082	2084	rBV2	291	356	0.03%	0.004%
85	13.926	2104	2106	2109	rBV2	231	220	0.02%	0.002%
86	14.048	2124	2126	2129	rBV	278	324	0.03%	0.003%
87	14.115	2136	2137	2138	rBV	332	231	0.02%	0.002%
88	14.225	2152	2155	2157	rBV2	322	342	0.03%	0.004%
89	14.500	2198	2200	2202	rBV	234	240	0.02%	0.002%
90	14.524	2202	2204	2205	rVB2	381	188	0.02%	0.002%
91	14.597	2214	2216	2219	rBV3	361	465	0.04%	0.005%
92	14.877	2260	2262	2263	rBV2	271	178	0.01%	0.002%
93	14.993	2278	2281	2283	rBV3	421	507	0.04%	0.005%
94	15.158	2306	2308	2310	rBV	318	217	0.02%	0.002%
95	15.176	2310	2311	2312	rBV	363	201	0.02%	0.002%
96	15.371	2342	2343	2346	rVB2	656	432	0.03%	0.004%
97	15.414	2346	2350	2352	rBV	434	540	0.04%	0.006%
98	16.322	2497	2499	2500	rVB	574	267	0.02%	0.003%
99	16.347	2502	2503	2506	rBV3	427	413	0.03%	0.004%
100	16.505	2527	2529	2531	rBV2	342	248	0.02%	0.003%




Sum of corrected areas: 9744536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036109.D
Acq On : 09 Jun 2023 15:29
Operator : JC/MD
Sample : 03107-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

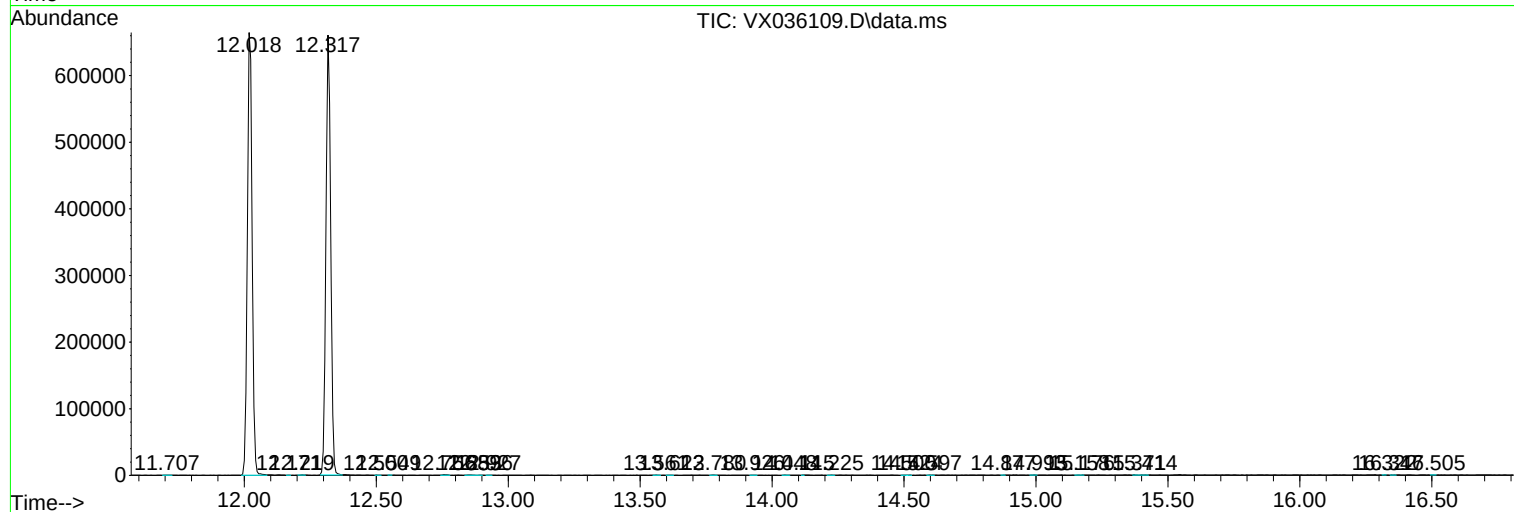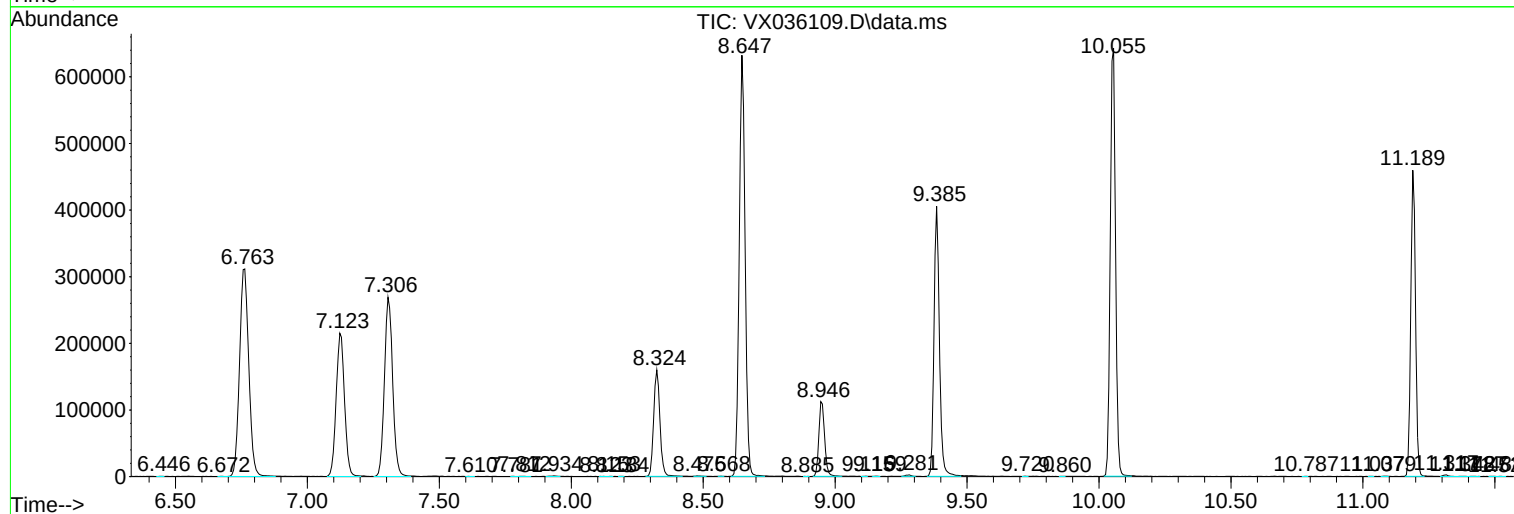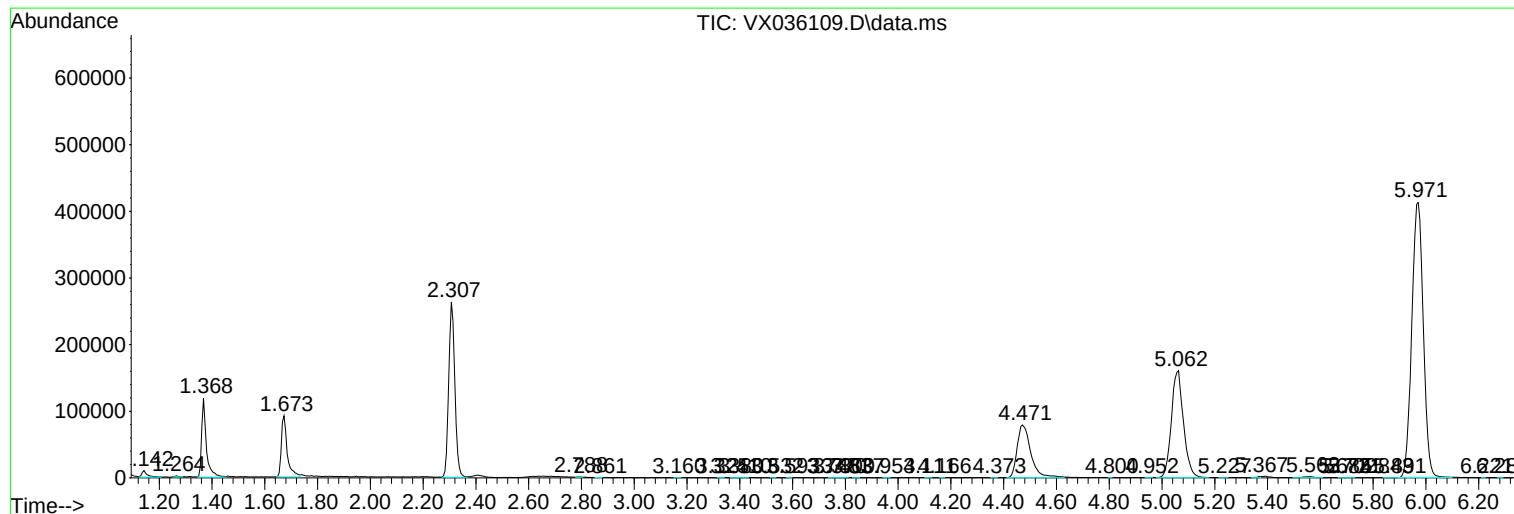

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036109.D
Acq On : 09 Jun 2023 15:29
Operator : JC/MD
Sample : 03107-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036109.D
Acq On : 09 Jun 2023 15:29
Operator : JC/MD
Sample : 03107-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------