

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036110.D
 Acq On : 09 Jun 2023 15:52
 Operator : JC/MD
 Sample : 03107-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB2	9864	10200	0.82%	0.111%
2	1.264	27	29	32	rVB3	1880	1584	0.13%	0.017%
3	1.368	42	46	58	rBV	114526	140413	11.32%	1.533%
4	1.672	91	96	114	rBV	95434	144025	11.61%	1.573%
5	2.306	194	200	209	rBV	254110	398088	32.09%	4.347%
6	2.404	212	216	226	rVV	3483	9745	0.79%	0.106%
7	2.569	241	243	245	rBV2	460	485	0.04%	0.005%
8	3.062	322	324	328	rVB2	248	339	0.03%	0.004%
9	3.105	328	331	332	rBV2	357	266	0.02%	0.003%
10	3.257	355	356	360	rVB	289	253	0.02%	0.003%
11	3.410	380	381	385	rBV2	245	258	0.02%	0.003%
12	4.471	545	555	573	rBV	75727	265380	21.39%	2.898%
13	4.806	608	610	612	rVB	302	217	0.02%	0.002%
14	4.873	619	621	625	rBV2	168	230	0.02%	0.003%
15	5.056	638	651	673	rBV	156488	502250	40.49%	5.485%
16	5.385	698	705	707	rBV3	879	1725	0.14%	0.019%
17	5.513	725	726	727	rBV	388	257	0.02%	0.003%
18	5.550	727	732	738	rVV5	1363	2833	0.23%	0.031%
19	5.727	759	761	763	rBV	187	226	0.02%	0.002%
20	5.842	778	780	785	rBV2	184	353	0.03%	0.004%
21	5.970	788	801	815	rBV2	414224	1240478	100.00%	13.546%
22	6.196	836	838	840	rBV2	290	235	0.02%	0.003%
23	6.537	892	894	896	rBV	467	300	0.02%	0.003%
24	6.556	896	897	901	rVB2	299	211	0.02%	0.002%
25	6.647	909	912	913	rBV2	372	297	0.02%	0.003%
26	6.763	920	931	945	rBV	304180	737207	59.43%	8.050%
27	7.117	984	989	990	rBV4	1169	1973	0.16%	0.022%
28	7.306	1011	1020	1034	rBV	261550	576567	46.48%	6.296%
29	7.403	1034	1036	1037	rVV	717	585	0.05%	0.006%
30	7.440	1041	1042	1044	rVV2	356	232	0.02%	0.003%
31	7.488	1044	1050	1055	rVB4	852	1908	0.15%	0.021%
32	7.537	1055	1058	1059	rBV2	177	209	0.02%	0.002%
33	7.793	1094	1100	1104	rBV2	244	433	0.03%	0.005%
34	7.873	1111	1113	1117	rVB2	269	274	0.02%	0.003%
35	7.927	1117	1122	1125	rBV3	862	1564	0.13%	0.017%
36	8.068	1144	1145	1149	rBV2	227	217	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036110.D
 Acq On : 09 Jun 2023 15:52
 Operator : JC/MD
 Sample : 03107-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	8.116	1151	1153	1155	rBV2	234	215	0.02%	0.002%
38	8.324	1180	1187	1198	rBV	163865	260885	21.03%	2.849%
39	8.574	1224	1228	1229	rBV2	310	338	0.03%	0.004%
40	8.647	1233	1240	1249	rBV	619486	971410	78.31%	10.608%
41	8.945	1284	1289	1301	rBV	107686	171408	13.82%	1.872%
42	9.232	1335	1336	1339	rBV2	222	254	0.02%	0.003%
43	9.275	1339	1343	1346	rVV4	1109	1798	0.14%	0.020%
44	9.384	1355	1361	1379	rBV	405587	586224	47.26%	6.401%
45	9.634	1398	1402	1403	rBV2	412	450	0.04%	0.005%
46	9.708	1409	1414	1416	rBV2	410	566	0.05%	0.006%
47	9.750	1420	1421	1424	rBV	205	259	0.02%	0.003%
48	9.994	1460	1461	1465	rBV3	286	369	0.03%	0.004%
49	10.055	1465	1471	1487	rVV	626988	879007	70.86%	9.599%
50	10.305	1508	1512	1517	rVB3	1784	2276	0.18%	0.025%
51	10.366	1520	1522	1526	rBV2	241	342	0.03%	0.004%
52	10.476	1539	1540	1544	rVB	296	266	0.02%	0.003%
53	10.646	1564	1568	1571	rBV2	703	904	0.07%	0.010%
54	10.805	1590	1594	1597	rBV2	263	348	0.03%	0.004%
55	10.963	1618	1620	1623	rBV	211	255	0.02%	0.003%
56	10.988	1623	1624	1627	rVB	298	208	0.02%	0.002%
57	11.018	1627	1629	1632	rBV	209	311	0.03%	0.003%
58	11.091	1639	1641	1643	rVB2	521	316	0.03%	0.003%
59	11.134	1646	1648	1652	rVB2	351	432	0.03%	0.005%
60	11.189	1652	1657	1665	rBV	454438	580959	46.83%	6.344%
61	11.311	1674	1677	1681	rBV3	1549	2086	0.17%	0.023%
62	11.378	1686	1688	1690	rBV2	378	273	0.02%	0.003%
63	11.439	1696	1698	1699	rBV2	392	367	0.03%	0.004%
64	11.610	1724	1726	1728	rBV2	276	253	0.02%	0.003%
65	11.658	1732	1734	1739	rVB2	249	387	0.03%	0.004%
66	11.719	1741	1744	1745	rBV2	263	278	0.02%	0.003%
67	11.756	1748	1750	1753	rBV2	498	425	0.03%	0.005%
68	11.817	1758	1760	1762	rBV	405	300	0.02%	0.003%
69	11.847	1762	1765	1767	rVB	263	290	0.02%	0.003%
70	11.884	1770	1771	1774	rBV2	300	266	0.02%	0.003%
71	11.951	1780	1782	1784	rBV2	225	254	0.02%	0.003%
72	12.018	1788	1793	1802	rBV	631663	811769	65.44%	8.864%
73	12.140	1812	1813	1817	rVB2	395	358	0.03%	0.004%
74	12.201	1820	1823	1825	rBV2	287	336	0.03%	0.004%
75	12.317	1837	1842	1854	rBV	674649	828875	66.82%	9.051%
76	12.677	1896	1901	1904	rBV2	230	381	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036110.D
 Acq On : 09 Jun 2023 15:52
 Operator : JC/MD
 Sample : 03107-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.719	1907	1908	1912	rBV2	259	363	0.03%	0.004%
78	12.768	1914	1916	1918	rVB	373	230	0.02%	0.003%
79	12.975	1948	1950	1951	rBV	339	242	0.02%	0.003%
80	13.561	2044	2046	2047	rBV2	293	251	0.02%	0.003%
81	13.664	2062	2063	2065	rBV	296	230	0.02%	0.003%
82	13.707	2068	2070	2072	rBV2	314	274	0.02%	0.003%
83	13.804	2084	2086	2089	rVB2	369	425	0.03%	0.005%
84	13.847	2089	2093	2094	rBV2	259	230	0.02%	0.003%
85	14.042	2123	2125	2130	rVB2	533	719	0.06%	0.008%
86	14.085	2130	2132	2135	rBV2	502	638	0.05%	0.007%
87	14.127	2135	2139	2142	rVV2	301	472	0.04%	0.005%
88	14.256	2158	2160	2162	rBV	205	221	0.02%	0.002%
89	14.316	2168	2170	2172	rBV	345	298	0.02%	0.003%
90	14.365	2175	2178	2179	rVB2	365	279	0.02%	0.003%
91	14.505	2199	2201	2204	rBV2	238	260	0.02%	0.003%
92	14.615	2216	2219	2221	rBV3	273	290	0.02%	0.003%
93	14.749	2239	2241	2244	rBV2	442	413	0.03%	0.005%
94	14.774	2244	2245	2247	rBV	372	222	0.02%	0.002%
95	14.993	2279	2281	2283	rBV2	341	321	0.03%	0.004%
96	15.207	2313	2316	2322	rBV4	452	942	0.08%	0.010%
97	15.420	2349	2351	2352	rBV	371	267	0.02%	0.003%
98	15.944	2436	2437	2439	rBV2	432	273	0.02%	0.003%
99	16.115	2463	2465	2470	rBV2	462	708	0.06%	0.008%
100	16.255	2486	2488	2490	rBV2	679	526	0.04%	0.006%




Sum of corrected areas: 9157609

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036110.D
Acq On : 09 Jun 2023 15:52
Operator : JC/MD
Sample : 03107-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

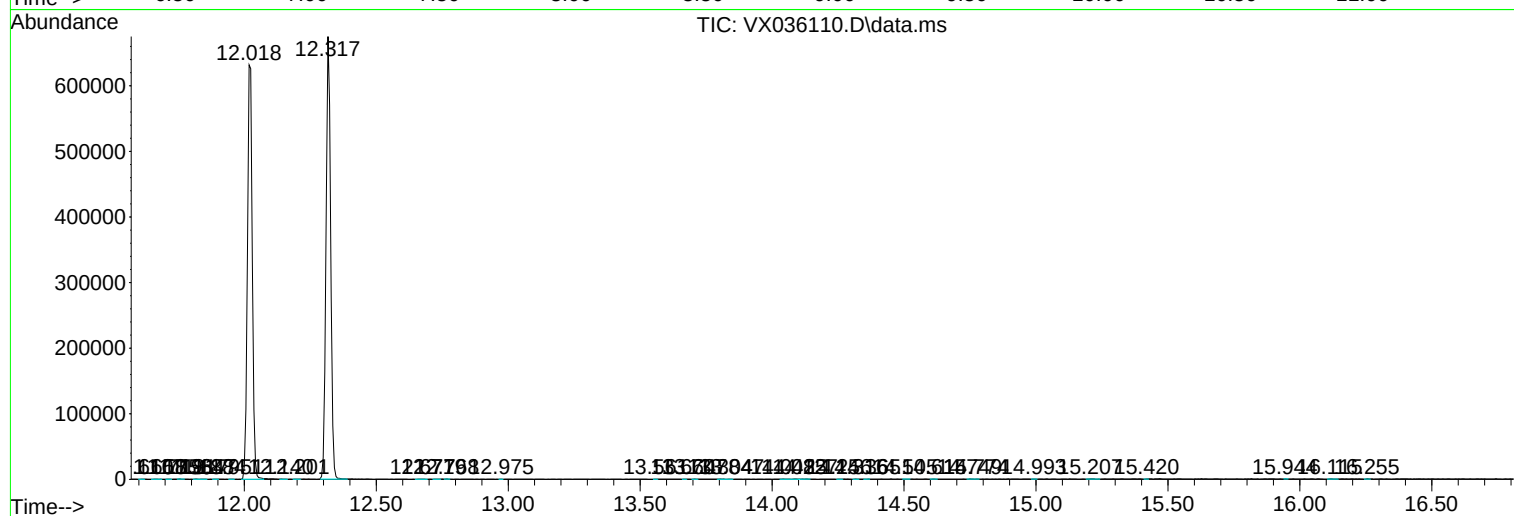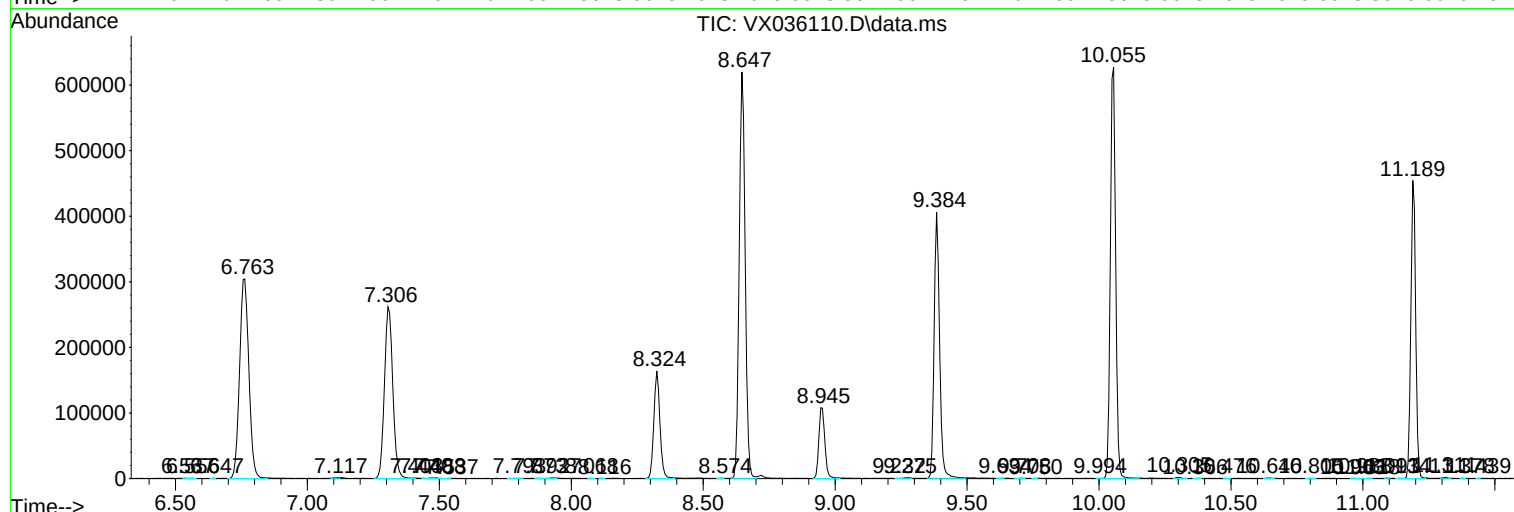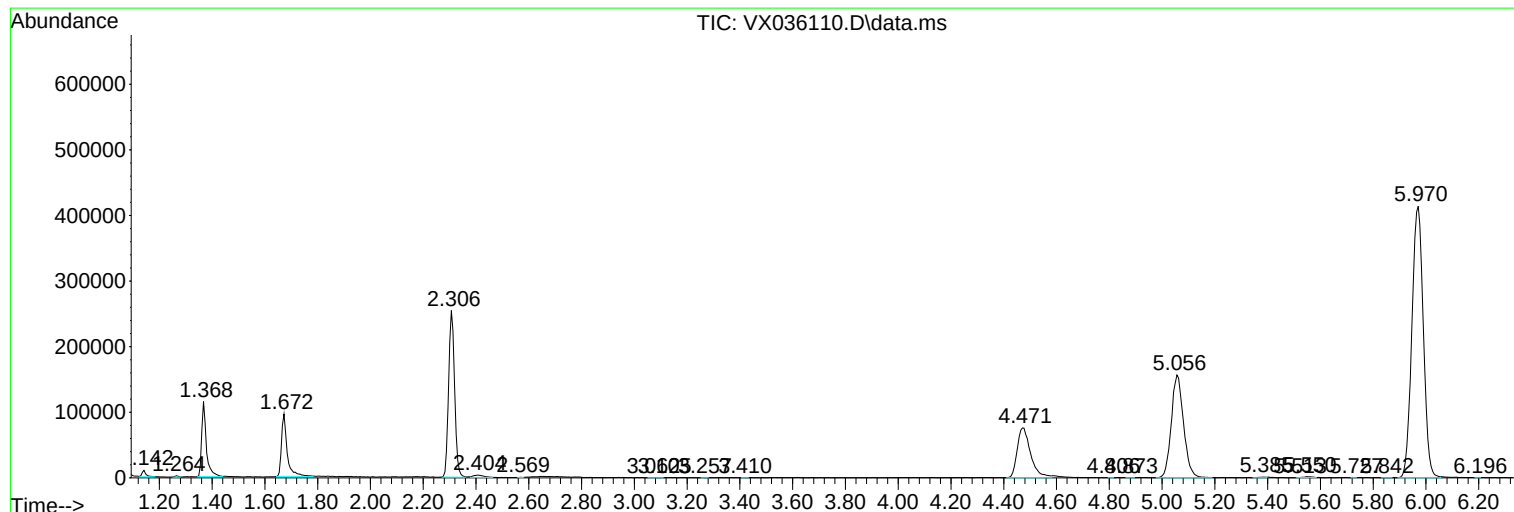

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036110.D
Acq On : 09 Jun 2023 15:52
Operator : JC/MD
Sample : 03107-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036110.D
Acq On : 09 Jun 2023 15:52
Operator : JC/MD
Sample : 03107-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc