

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036111.D
 Acq On : 09 Jun 2023 16:15
 Operator : JC/MD
 Sample : 03107-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M

Title : VOC Analysis

Signal : TIC: VX036111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB3	10500	12031	0.95%	0.119%
2	1.264	27	29	31	rBV	1718	1687	0.13%	0.017%
3	1.368	42	46	59	rBV	124184	144254	11.39%	1.422%
4	1.672	91	96	114	rBV	98888	145862	11.52%	1.437%
5	2.307	194	200	209	rBV2	278747	452870	35.77%	4.463%
6	2.508	232	233	239	rVB3	466	759	0.06%	0.007%
7	2.569	239	243	244	rBV	405	502	0.04%	0.005%
8	2.611	244	250	251	rBV3	1264	2091	0.17%	0.021%
9	2.843	286	288	290	rBV2	506	485	0.04%	0.005%
10	2.947	301	305	307	rBV2	369	491	0.04%	0.005%
11	2.971	307	309	311	rVV2	307	276	0.02%	0.003%
12	3.020	315	317	319	rVB	363	311	0.02%	0.003%
13	3.044	319	321	323	rBV2	355	305	0.02%	0.003%
14	3.093	327	329	334	rVB3	244	313	0.02%	0.003%
15	3.233	349	352	355	rVB3	218	295	0.02%	0.003%
16	3.489	391	394	399	rBV2	255	490	0.04%	0.005%
17	3.611	405	414	418	rBV3	967	1938	0.15%	0.019%
18	3.892	459	460	463	rBV	175	228	0.02%	0.002%
19	4.007	477	479	481	rBV	260	173	0.01%	0.002%
20	4.032	481	483	487	rVB2	218	255	0.02%	0.003%
21	4.471	546	555	579	rBV	87516	305657	24.14%	3.012%
22	4.855	616	618	619	rBV2	323	185	0.01%	0.002%
23	4.873	619	621	623	rBV2	233	217	0.02%	0.002%
24	4.928	628	630	632	rBV	143	169	0.01%	0.002%
25	5.056	639	651	667	rBV	158101	516044	40.76%	5.085%
26	5.330	693	696	697	rBV2	190	254	0.02%	0.003%
27	5.379	697	704	713	rVV5	5533	16253	1.28%	0.160%
28	5.556	727	733	739	rVB6	1930	4102	0.32%	0.040%
29	5.708	757	758	761	rVB	323	275	0.02%	0.003%
30	5.830	777	778	780	rBV	318	180	0.01%	0.002%
31	5.970	788	801	822	rBV2	420590	1266117	100.00%	12.477%
32	6.202	837	839	840	rVB2	296	168	0.01%	0.002%
33	6.342	858	862	865	rBV	190	259	0.02%	0.003%
34	6.763	921	931	951	rBV	306428	735909	58.12%	7.252%
35	7.123	981	990	1008	rBV	391692	867388	68.51%	8.547%
36	7.306	1011	1020	1034	rBV	271262	590465	46.64%	5.819%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036111.D
 Acq On : 09 Jun 2023 16:15
 Operator : JC/MD
 Sample : 03107-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.482	1045	1049	1051	rBV4	729	868	0.07%	0.009%
38	7.677	1079	1081	1083	rBV2	234	187	0.01%	0.002%
39	7.934	1117	1123	1127	rBV4	824	1468	0.12%	0.014%
40	8.098	1148	1150	1152	rBV2	230	236	0.02%	0.002%
41	8.232	1170	1172	1175	rVB	349	232	0.02%	0.002%
42	8.263	1175	1177	1180	rBV2	143	169	0.01%	0.002%
43	8.324	1180	1187	1203	rBV	162426	265974	21.01%	2.621%
44	8.647	1233	1240	1256	rBV	632961	1001702	79.12%	9.871%
45	8.878	1276	1278	1281	rBV	312	246	0.02%	0.002%
46	8.952	1284	1290	1305	rVV	113208	173556	13.71%	1.710%
47	9.153	1321	1323	1329	rVB	535	673	0.05%	0.007%
48	9.275	1339	1343	1349	rVB2	1830	2855	0.23%	0.028%
49	9.385	1355	1361	1373	rBV	409870	575320	45.44%	5.669%
50	9.683	1408	1410	1411	rBV2	272	163	0.01%	0.002%
51	9.866	1436	1440	1442	rBV3	269	308	0.02%	0.003%
52	9.951	1452	1454	1456	rBV	226	287	0.02%	0.003%
53	10.055	1465	1471	1482	rBV	636906	864192	68.26%	8.516%
54	10.262	1503	1505	1508	rVB2	234	200	0.02%	0.002%
55	10.299	1508	1511	1515	rBV2	908	997	0.08%	0.010%
56	10.427	1530	1532	1535	rBV2	281	367	0.03%	0.004%
57	10.604	1560	1561	1563	rBV2	259	199	0.02%	0.002%
58	10.653	1567	1569	1572	rVB	316	287	0.02%	0.003%
59	10.866	1602	1604	1607	rVB2	181	184	0.01%	0.002%
60	10.939	1612	1616	1617	rBV	229	264	0.02%	0.003%
61	10.976	1621	1622	1624	rVB	395	173	0.01%	0.002%
62	10.994	1624	1625	1627	rBV	211	180	0.01%	0.002%
63	11.079	1638	1639	1641	rBV	405	243	0.02%	0.002%
64	11.189	1652	1657	1667	rBV	439161	568942	44.94%	5.606%
65	11.317	1674	1678	1682	rVB4	1616	2372	0.19%	0.023%
66	11.439	1695	1698	1699	rBV	215	236	0.02%	0.002%
67	11.591	1721	1723	1726	rVB2	232	175	0.01%	0.002%
68	11.671	1734	1736	1737	rBV2	276	193	0.02%	0.002%
69	11.768	1748	1752	1753	rBV	250	214	0.02%	0.002%
70	12.018	1788	1793	1803	rBV	629968	785966	62.08%	7.745%
71	12.213	1823	1825	1827	rVV2	343	343	0.03%	0.003%
72	12.232	1827	1828	1832	rVV2	404	316	0.02%	0.003%
73	12.317	1837	1842	1856	rVV	667469	820045	64.77%	8.081%
74	12.579	1883	1885	1886	rVB2	310	201	0.02%	0.002%
75	12.683	1901	1902	1904	rBV	360	219	0.02%	0.002%
76	12.707	1904	1906	1909	rBV2	287	323	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036111.D
 Acq On : 09 Jun 2023 16:15
 Operator : JC/MD
 Sample : 03107-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0FK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.762	1912	1915	1920	rVB2	588	771	0.06%	0.008%
78	12.799	1920	1921	1923	rBV2	337	233	0.02%	0.002%
79	13.195	1983	1986	1988	rBV2	342	399	0.03%	0.004%
80	13.250	1991	1995	1997	rBV2	200	221	0.02%	0.002%
81	13.506	2035	2037	2040	rVB2	247	229	0.02%	0.002%
82	13.536	2040	2042	2046	rVB2	286	318	0.03%	0.003%
83	13.664	2059	2063	2065	rBV	201	216	0.02%	0.002%
84	13.695	2065	2068	2070	rBV	473	485	0.04%	0.005%
85	13.926	2104	2106	2107	rVB	315	166	0.01%	0.002%
86	14.024	2121	2122	2125	rBV2	286	280	0.02%	0.003%
87	14.207	2149	2152	2153	rBV	256	203	0.02%	0.002%
88	14.402	2182	2184	2187	rBV2	243	313	0.02%	0.003%
89	14.566	2209	2211	2212	rBV2	322	195	0.02%	0.002%
90	14.634	2220	2222	2225	rBV3	389	458	0.04%	0.005%
91	14.688	2229	2231	2234	rVV2	247	282	0.02%	0.003%
92	14.743	2238	2240	2241	rBV	370	244	0.02%	0.002%
93	14.792	2245	2248	2249	rBV2	399	361	0.03%	0.004%
94	15.085	2295	2296	2300	rBV3	304	365	0.03%	0.004%
95	15.176	2309	2311	2312	rBV	377	218	0.02%	0.002%
96	15.255	2322	2324	2325	rBV	316	238	0.02%	0.002%
97	15.615	2381	2383	2385	rBV2	462	376	0.03%	0.004%
98	15.639	2385	2387	2390	rVB2	511	542	0.04%	0.005%
99	15.798	2411	2413	2415	rVB2	369	236	0.02%	0.002%
100	16.066	2455	2457	2459	rVB2	365	297	0.02%	0.003%

Sum of corrected areas: 10147979




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036111.D
Acq On : 09 Jun 2023 16:15
Operator : JC/MD
Sample : 03107-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

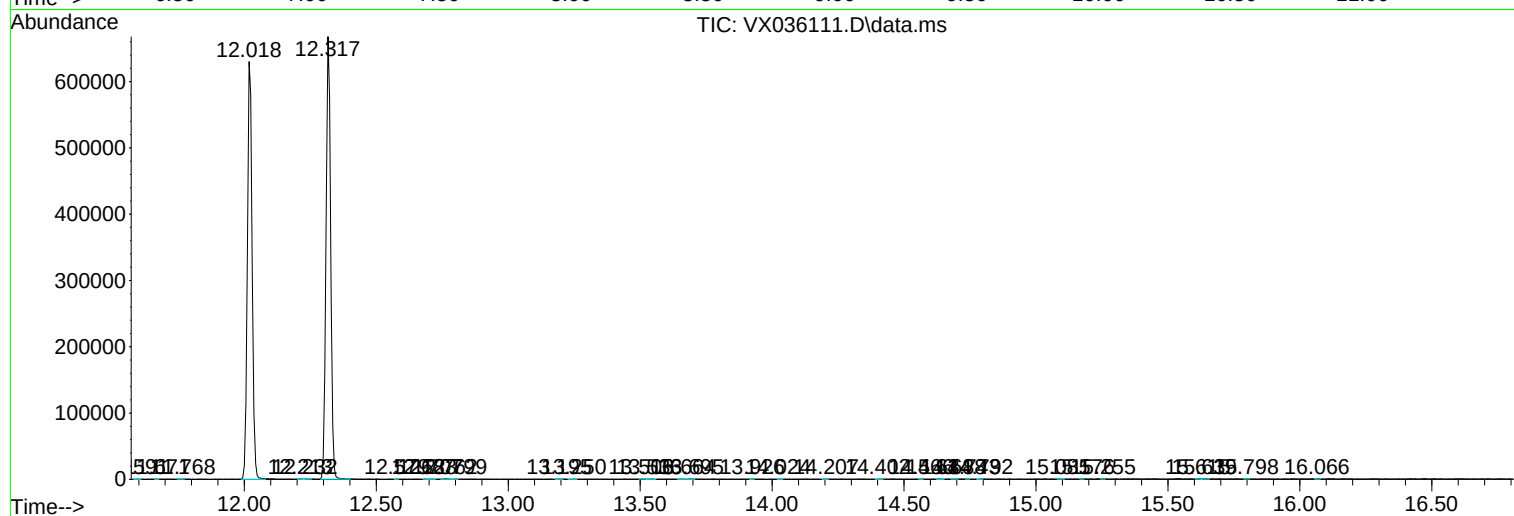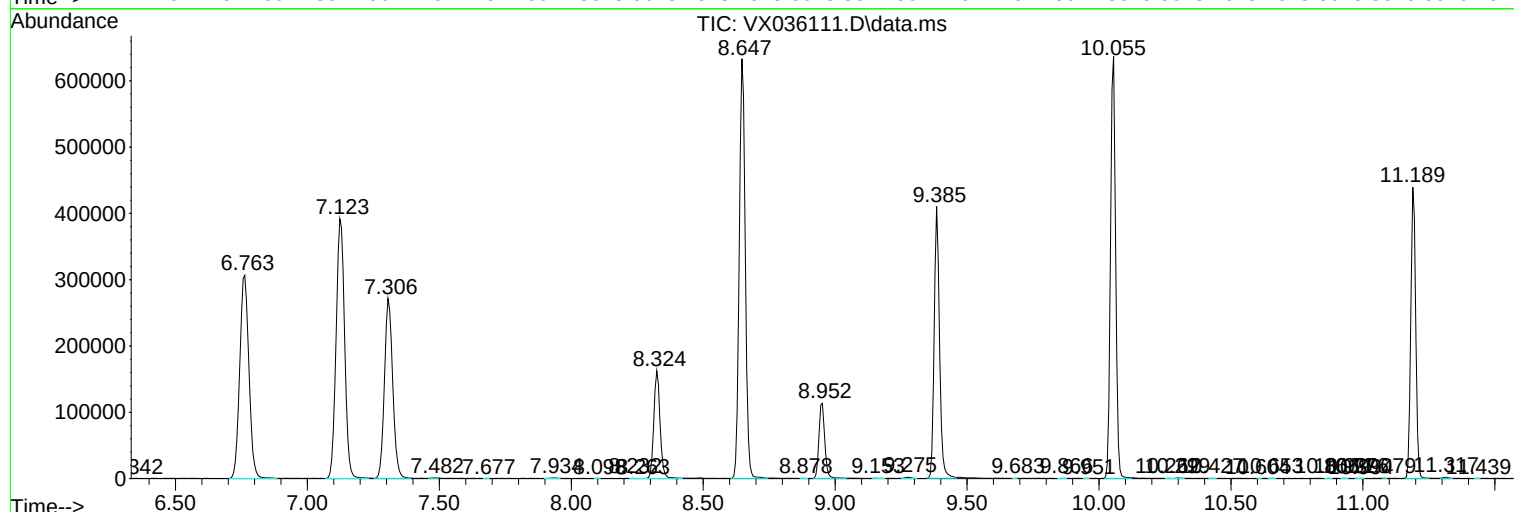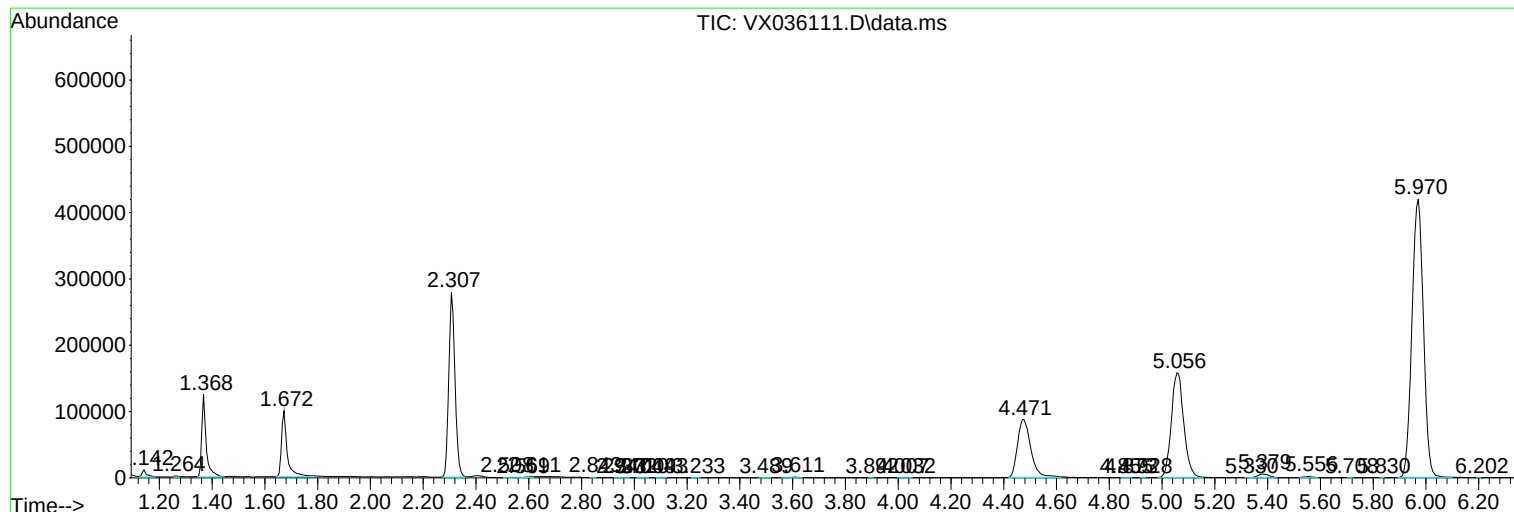

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036111.D
Acq On : 09 Jun 2023 16:15
Operator : JC/MD
Sample : 03107-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036111.D
Acq On : 09 Jun 2023 16:15
Operator : JC/MD
Sample : 03107-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0FK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc