

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036113.D
 Acq On : 09 Jun 2023 17:02
 Operator : JC/MD
 Sample : 03107-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	15	rVB	10195	10858	0.82%	0.110%
2	1.264	26	29	30	rBV2	1703	1329	0.10%	0.013%
3	1.368	42	46	61	rVB	121747	154646	11.70%	1.564%
4	1.672	91	96	107	rBV	95002	152301	11.52%	1.540%
5	2.306	193	200	211	rVB	275163	426417	32.25%	4.312%
6	2.477	226	228	230	rBV	377	318	0.02%	0.003%
7	2.508	230	233	236	rVV3	397	573	0.04%	0.006%
8	2.587	245	246	249	rBV2	361	299	0.02%	0.003%
9	2.642	253	255	256	rVB2	475	268	0.02%	0.003%
10	2.745	270	272	275	rBV3	231	210	0.02%	0.002%
11	2.788	275	279	285	rVB	1707	2729	0.21%	0.028%
12	2.880	292	294	296	rVB2	294	273	0.02%	0.003%
13	2.947	298	305	311	rVB4	1350	3365	0.25%	0.034%
14	3.026	316	318	320	rBV2	276	213	0.02%	0.002%
15	3.117	331	333	336	rVB2	315	256	0.02%	0.003%
16	3.215	345	349	350	rBV2	191	198	0.01%	0.002%
17	3.337	367	369	371	rBV2	321	327	0.02%	0.003%
18	3.501	394	396	398	rVB	230	210	0.02%	0.002%
19	3.562	404	406	409	rVB2	250	276	0.02%	0.003%
20	3.605	409	413	414	rBV	271	327	0.02%	0.003%
21	3.678	422	425	427	rBV2	186	213	0.02%	0.002%
22	3.855	451	454	457	rBV	262	302	0.02%	0.003%
23	3.959	469	471	472	rBV	190	194	0.01%	0.002%
24	4.202	509	511	514	rBV2	189	194	0.01%	0.002%
25	4.471	545	555	570	rBV	88972	287797	21.77%	2.910%
26	4.806	607	610	614	rBV2	277	381	0.03%	0.004%
27	5.056	637	651	669	rBV	160864	534120	40.40%	5.401%
28	5.294	687	690	692	rBV2	230	225	0.02%	0.002%
29	5.385	699	705	707	rBV3	722	1281	0.10%	0.013%
30	5.550	726	732	740	rBV5	1521	3479	0.26%	0.035%
31	5.824	775	777	779	rVB	271	223	0.02%	0.002%
32	5.970	788	801	818	rBV2	441153	1322136	100.00%	13.369%
33	6.214	839	841	844	rBV2	239	262	0.02%	0.003%
34	6.269	848	850	853	rVB2	272	253	0.02%	0.003%
35	6.678	916	917	921	rBV2	284	333	0.03%	0.003%
36	6.763	921	931	948	rBV	348285	830174	62.79%	8.395%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036113.D
 Acq On : 09 Jun 2023 17:02
 Operator : JC/MD
 Sample : 03107-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.940	958	960	961	rBV2	333	222	0.02%	0.002%
38	7.123	981	990	994	rVB8	1722	4279	0.32%	0.043%
39	7.306	1011	1020	1032	rBV	282970	617673	46.72%	6.246%
40	7.464	1043	1046	1047	rBV2	401	444	0.03%	0.004%
41	7.927	1118	1122	1128	rBV4	1025	1860	0.14%	0.019%
42	8.043	1139	1141	1144	rVB2	196	194	0.01%	0.002%
43	8.074	1144	1146	1151	rBV2	176	311	0.02%	0.003%
44	8.153	1158	1159	1162	rVB2	262	225	0.02%	0.002%
45	8.238	1172	1173	1177	rVB	282	241	0.02%	0.002%
46	8.324	1181	1187	1201	rBV	163028	270756	20.48%	2.738%
47	8.476	1210	1212	1218	rVB3	826	1039	0.08%	0.011%
48	8.580	1226	1229	1231	rBV2	366	351	0.03%	0.004%
49	8.647	1233	1240	1250	rBV	686522	1032367	78.08%	10.439%
50	8.848	1271	1273	1274	rBV2	280	240	0.02%	0.002%
51	8.903	1279	1282	1283	rBV2	180	216	0.02%	0.002%
52	8.952	1283	1290	1302	rBV	113933	177508	13.43%	1.795%
53	9.183	1325	1328	1330	rVB2	233	192	0.01%	0.002%
54	9.226	1333	1335	1337	rVB	256	207	0.02%	0.002%
55	9.275	1341	1343	1351	rVB3	1300	1866	0.14%	0.019%
56	9.342	1351	1354	1355	rBV2	285	277	0.02%	0.003%
57	9.384	1355	1361	1382	rBV	454411	634381	47.98%	6.415%
58	9.610	1396	1398	1399	rBV2	289	268	0.02%	0.003%
59	9.702	1409	1413	1417	rVV2	1706	2401	0.18%	0.024%
60	9.756	1420	1422	1424	rBV2	242	209	0.02%	0.002%
61	10.000	1458	1462	1465	rBV2	223	361	0.03%	0.004%
62	10.055	1465	1471	1480	rBV	708398	986814	74.64%	9.979%
63	10.195	1490	1494	1498	rVB	863	985	0.07%	0.010%
64	10.244	1498	1502	1504	rBV	311	549	0.04%	0.006%
65	10.299	1508	1511	1516	rVV2	741	955	0.07%	0.010%
66	10.366	1520	1522	1525	rVB2	341	304	0.02%	0.003%
67	10.390	1525	1526	1530	rBV2	171	199	0.02%	0.002%
68	10.494	1541	1543	1548	rBV2	224	337	0.03%	0.003%
69	10.653	1564	1569	1571	rBV2	316	429	0.03%	0.004%
70	10.842	1597	1600	1601	rBV2	242	250	0.02%	0.003%
71	10.970	1616	1621	1624	rBB3	474	740	0.06%	0.007%
72	11.043	1629	1633	1635	rVV2	279	288	0.02%	0.003%
73	11.079	1637	1639	1645	rVV2	195	371	0.03%	0.004%
74	11.189	1652	1657	1666	rBV	480362	615376	46.54%	6.223%
75	11.311	1674	1677	1681	rVV3	900	1100	0.08%	0.011%
76	11.616	1725	1727	1728	rBV	329	236	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
 Data File : VX036113.D
 Acq On : 09 Jun 2023 17:02
 Operator : JC/MD
 Sample : 03107-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.744	1747	1748	1753	rVB4	375	538	0.04%	0.005%
78	11.817	1756	1760	1761	rVB2	276	239	0.02%	0.002%
79	11.835	1761	1763	1765	rBV	231	202	0.02%	0.002%
80	11.921	1774	1777	1780	rBV2	285	415	0.03%	0.004%
81	11.951	1780	1782	1784	rBV2	292	236	0.02%	0.002%
82	11.969	1784	1785	1788	rVB2	598	303	0.02%	0.003%
83	12.018	1788	1793	1803	rBV	727093	912792	69.04%	9.230%
84	12.189	1818	1821	1823	rBV3	365	378	0.03%	0.004%
85	12.317	1837	1842	1850	rBV	702843	873939	66.10%	8.837%
86	12.475	1866	1868	1869	rVB	353	192	0.01%	0.002%
87	12.640	1894	1895	1898	rBV2	273	268	0.02%	0.003%
88	12.762	1912	1915	1921	rVB2	783	1046	0.08%	0.011%
89	12.872	1929	1933	1934	rBV2	207	234	0.02%	0.002%
90	13.774	2079	2081	2084	rVB2	418	389	0.03%	0.004%
91	13.859	2092	2095	2097	rVB2	296	330	0.02%	0.003%
92	14.134	2134	2140	2142	rBV3	531	856	0.06%	0.009%
93	14.219	2153	2154	2157	rVB2	315	316	0.02%	0.003%
94	14.249	2157	2159	2161	rBV	431	385	0.03%	0.004%
95	14.518	2201	2203	2205	rBV2	240	259	0.02%	0.003%
96	14.810	2249	2251	2254	rBV	310	388	0.03%	0.004%
97	16.048	2453	2454	2455	rBV	499	264	0.02%	0.003%
98	16.121	2465	2466	2468	rBV2	583	371	0.03%	0.004%
99	16.304	2494	2496	2498	rBV2	486	480	0.04%	0.005%
100	16.462	2520	2522	2524	rBV2	529	488	0.04%	0.005%



Sum of corrected areas: 9889289

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036113.D
Acq On : 09 Jun 2023 17:02
Operator : JC/MD
Sample : 03107-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

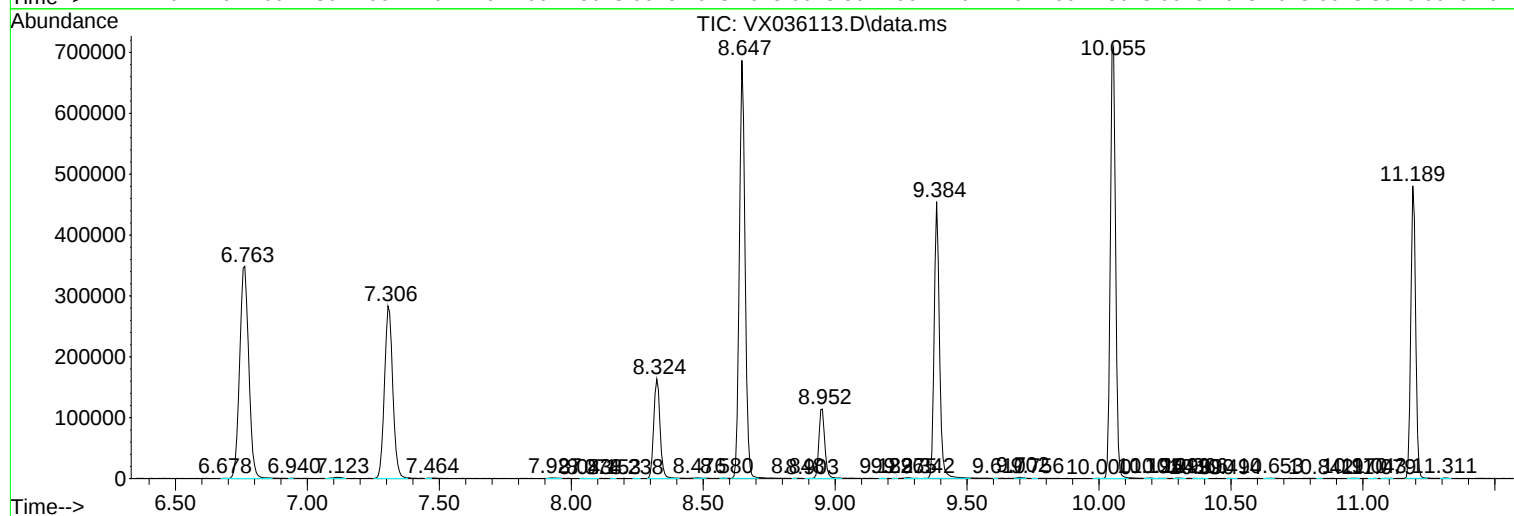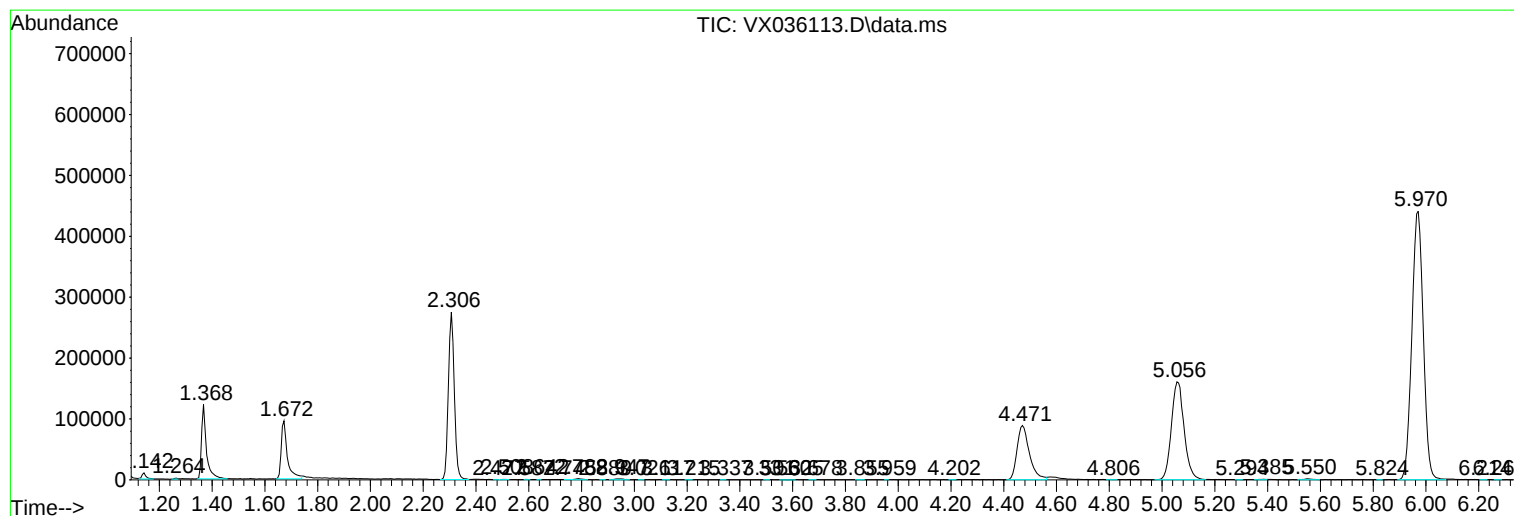

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036113.D
Acq On : 09 Jun 2023 17:02
Operator : JC/MD
Sample : 03107-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036113.D
Acq On : 09 Jun 2023 17:02
Operator : JC/MD
Sample : 03107-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------