


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060923\
Data File : VX036094.D
Acq On : 09 Jun 2023 08:00
Operator : JC/MD
Sample : BFB630
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB630

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM060623WMA.M
Title : VOC Analysis
Last Update : Sat Jun 10 00:08:47 2023

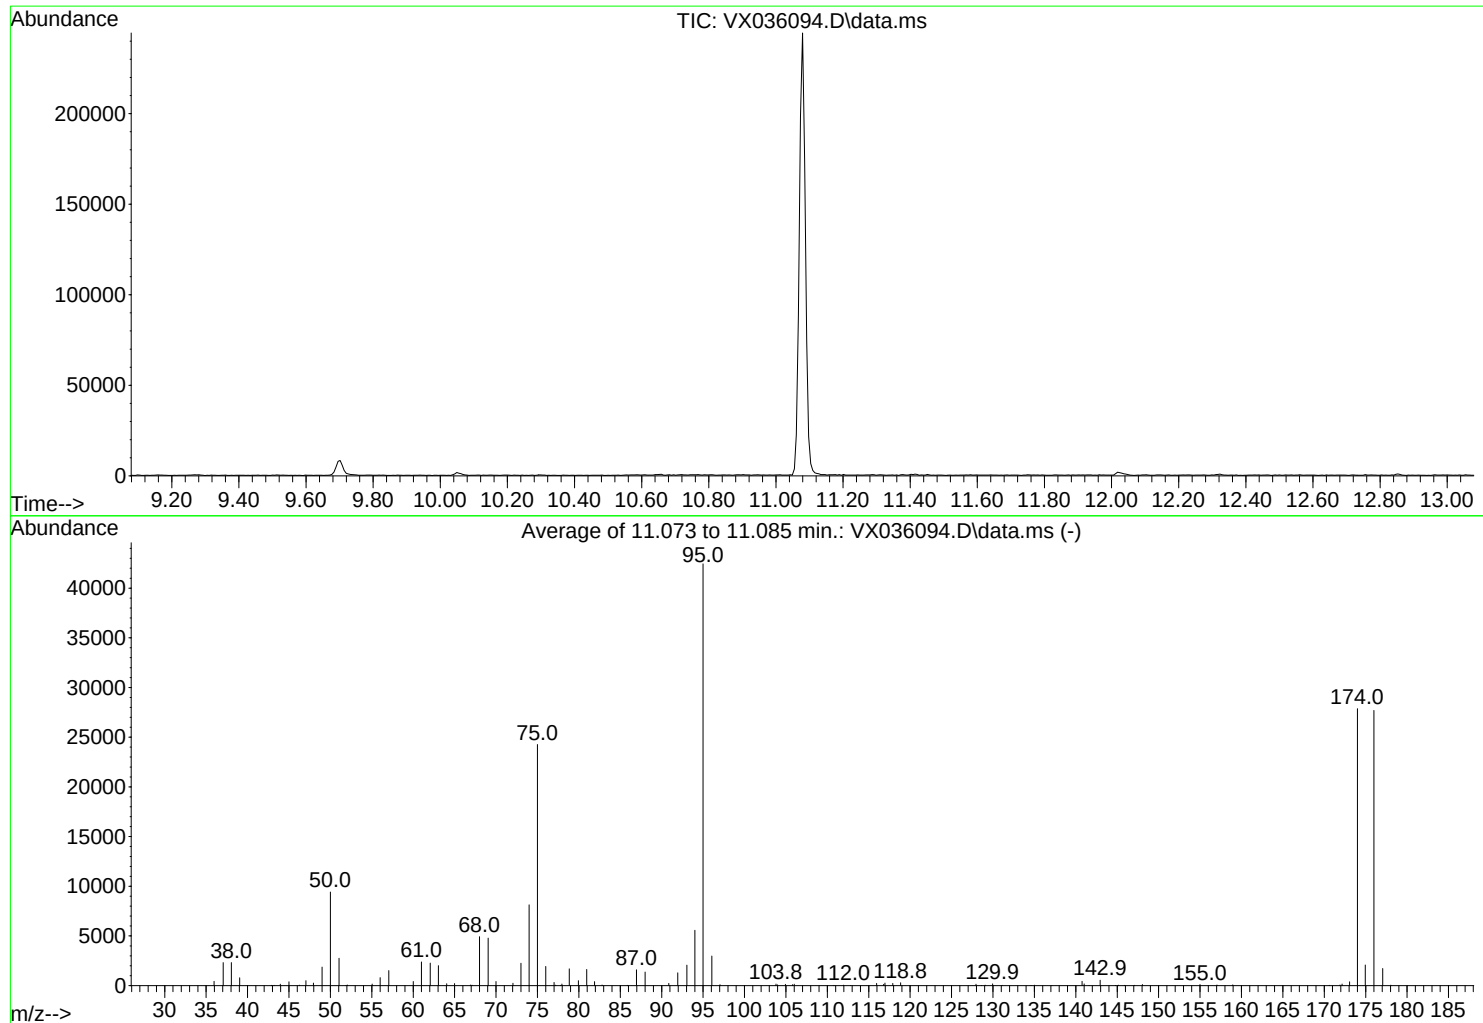

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	9419	PASS
75	95	30	80	57.2	24259	PASS
95	95	100	100	100.0	42445	PASS
96	95	5	9	7.0	2972	PASS
173	174	0.00	2	1.4	387	PASS
174	95	50	120	65.6	27864	PASS
175	174	5	9	7.5	2077	PASS
176	174	95	101	99.4	27691	PASS
177	176	5	9	6.2	1730	PASS

m/z	Abundance
35.90	161.0
40.00	226.0
43.90	226.0

Instrument :
MSVOA_X
ClientSampleId :
BFB630

m/z	Abundance
36.00	640.0
37.10	2390.0
38.00	2521.0
39.10	854.0
40.10	225.0
43.20	111.0
44.00	364.0
45.00	414.0
47.10	350.0
48.00	315.0
49.00	2238.0
50.00	10535.0
51.00	2891.0
51.90	99.0
55.00	198.0
56.00	835.0
57.10	1841.0
60.00	502.0
61.00	2252.0
62.00	2398.0
63.00	2030.0
64.00	166.0
65.00	166.0
66.90	81.0
68.00	4935.0
69.10	5007.0
70.00	344.0
72.10	224.0
73.00	2062.0
74.00	8436.0
75.00	24232.0
76.00	1995.0
77.10	384.0
77.80	122.0
78.00	123.0
78.80	1422.0
79.90	494.0
80.90	1594.0
81.90	344.0
85.90	54.0
86.90	1476.0
88.10	1272.0
90.90	200.0
92.00	1105.0
93.00	2337.0
94.00	5619.0
95.00	42880.0
96.00	3350.0
97.10	148.0
103.80	252.0
105.00	112.0
105.80	279.0
116.00	213.0
116.80	377.0
117.90	259.0
118.90	240.0
127.90	116.0
130.10	148.0
134.60	65.0
135.00	60.0
141.00	525.0
142.90	468.0
148.00	93.0
155.00	115.0
157.10	59.0
158.90	65.0
171.90	208.0
173.00	384.0
174.00	23616.0
175.00	1881.0
176.00	22624.0
177.00	1440.0
178.10	80.0

Instrument :
MSVOA_X
ClientSampleId :
BFB630

m/z	Abundance
36.00	740.0
37.00	2866.0
38.10	2741.0
39.10	883.0
40.00	180.0
42.90	114.0
43.90	346.0
45.00	489.0
46.30	61.0
47.10	715.0
47.90	231.0
49.00	2051.0
50.00	10850.0
51.10	3193.0
52.10	115.0
55.10	146.0
56.10	925.0
57.00	1720.0
60.00	451.0
61.00	2913.0
62.00	2640.0
63.10	2287.0
64.00	242.0
65.00	264.0
66.90	112.0
68.00	5868.0
69.00	5692.0
70.00	622.0
72.10	248.0
73.00	2868.0
74.00	9606.0
75.00	29216.0
76.00	2237.0
76.90	444.0
78.00	205.0
78.90	1958.0
80.00	655.0
81.00	2111.0
81.90	437.0
82.80	77.0
85.90	68.0
87.00	1925.0
87.90	1801.0
90.80	268.0
92.00	1722.0
93.10	2268.0
94.00	6408.0
95.00	49992.0
96.10	3656.0
97.00	81.0
103.80	247.0
105.00	163.0
106.00	240.0
110.80	80.0
111.90	72.0
115.90	259.0
117.00	386.0
117.90	266.0
118.80	314.0
128.00	171.0
129.00	82.0
129.90	204.0
135.00	98.0
140.70	710.0
143.00	615.0
145.10	75.0
145.90	123.0
147.10	66.0
148.10	100.0
155.00	125.0
157.00	134.0
159.00	90.0
170.60	52.0
172.20	220.0
173.00	448.0
174.00	33184.0
175.00	2492.0
176.00	33344.0
177.00	2364.0
178.00	71.0

Instrument :
MSVOA_X
ClientSampleId :
BFB630

m/z	Abundance
36.00	427.0
37.10	1680.0
38.10	1679.0
39.00	629.0
40.00	198.0
44.10	385.0
44.90	269.0
46.20	70.0
46.90	415.0
47.90	215.0
49.10	1306.0
50.10	6873.0
51.00	2192.0
52.00	69.0
55.10	123.0
55.90	638.0
57.10	1002.0
60.00	283.0
61.00	2003.0
62.10	1794.0
63.00	1727.0
64.10	170.0
65.00	176.0
67.10	131.0
68.00	3994.0
69.10	3660.0
70.00	281.0
72.00	238.0
73.00	1850.0
74.00	6364.0
75.00	19328.0
76.00	1578.0
76.90	138.0
77.20	163.0
77.90	151.0
78.90	1682.0
79.90	331.0
80.90	1193.0
81.90	412.0
82.80	104.0
86.90	1387.0
88.00	1052.0
90.90	215.0
91.90	1063.0
93.00	1577.0
94.00	4680.0
95.00	34464.0
96.10	1911.0
97.00	66.0
104.00	251.0
104.90	102.0
106.00	181.0
112.00	56.0
112.80	74.0
115.90	191.0
116.90	393.0
117.90	160.0
118.90	333.0
128.00	168.0
128.60	62.0
129.10	55.0
129.80	166.0
131.10	89.0
137.10	55.0
140.80	581.0
141.60	66.0
142.90	564.0
144.80	52.0
145.20	51.0
147.10	58.0
148.00	134.0
155.00	101.0
158.90	68.0
170.60	53.0
172.10	267.0
173.10	330.0
174.00	26792.0
174.90	1857.0
176.00	27104.0
177.10	1385.0

Instrument :
MSVOA_X
ClientSampleId :
BFB630