

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061019\
 Data File : VX010210.D
 Acq On : 11 Jun 2019 05:00
 Operator : JC/SP
 Sample : PB120437TB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB120437TB

Quant Time: Jun 11 08:46:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 08 02:12:13 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	258896	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	393114	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	357680	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	168506	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	116253	46.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.00%	
35) Dibromofluoromethane	5.50	113	121258	50.01	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.02%	
50) Toluene-d8	8.71	98	463615	51.01	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.02%	
62) 4-Bromofluorobenzene	11.13	95	159255	46.92	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.84%	
Target Compounds						
16) Acetone	2.44	43	7754	6.524	ug/l #	82
20) Methylene Chloride	2.85	84	4128	1.581	ug/l #	69
43) Isopropyl Acetate	6.45	43	11332	2.031	ug/l #	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061019\
Data File : VX010210.D
Acq On : 11 Jun 2019 05:00
Operator : JC/SP
Sample : PB120437TB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB120437TB

Quant Time: Jun 11 08:46:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 08 02:12:13 2019
Response via : Initial Calibration

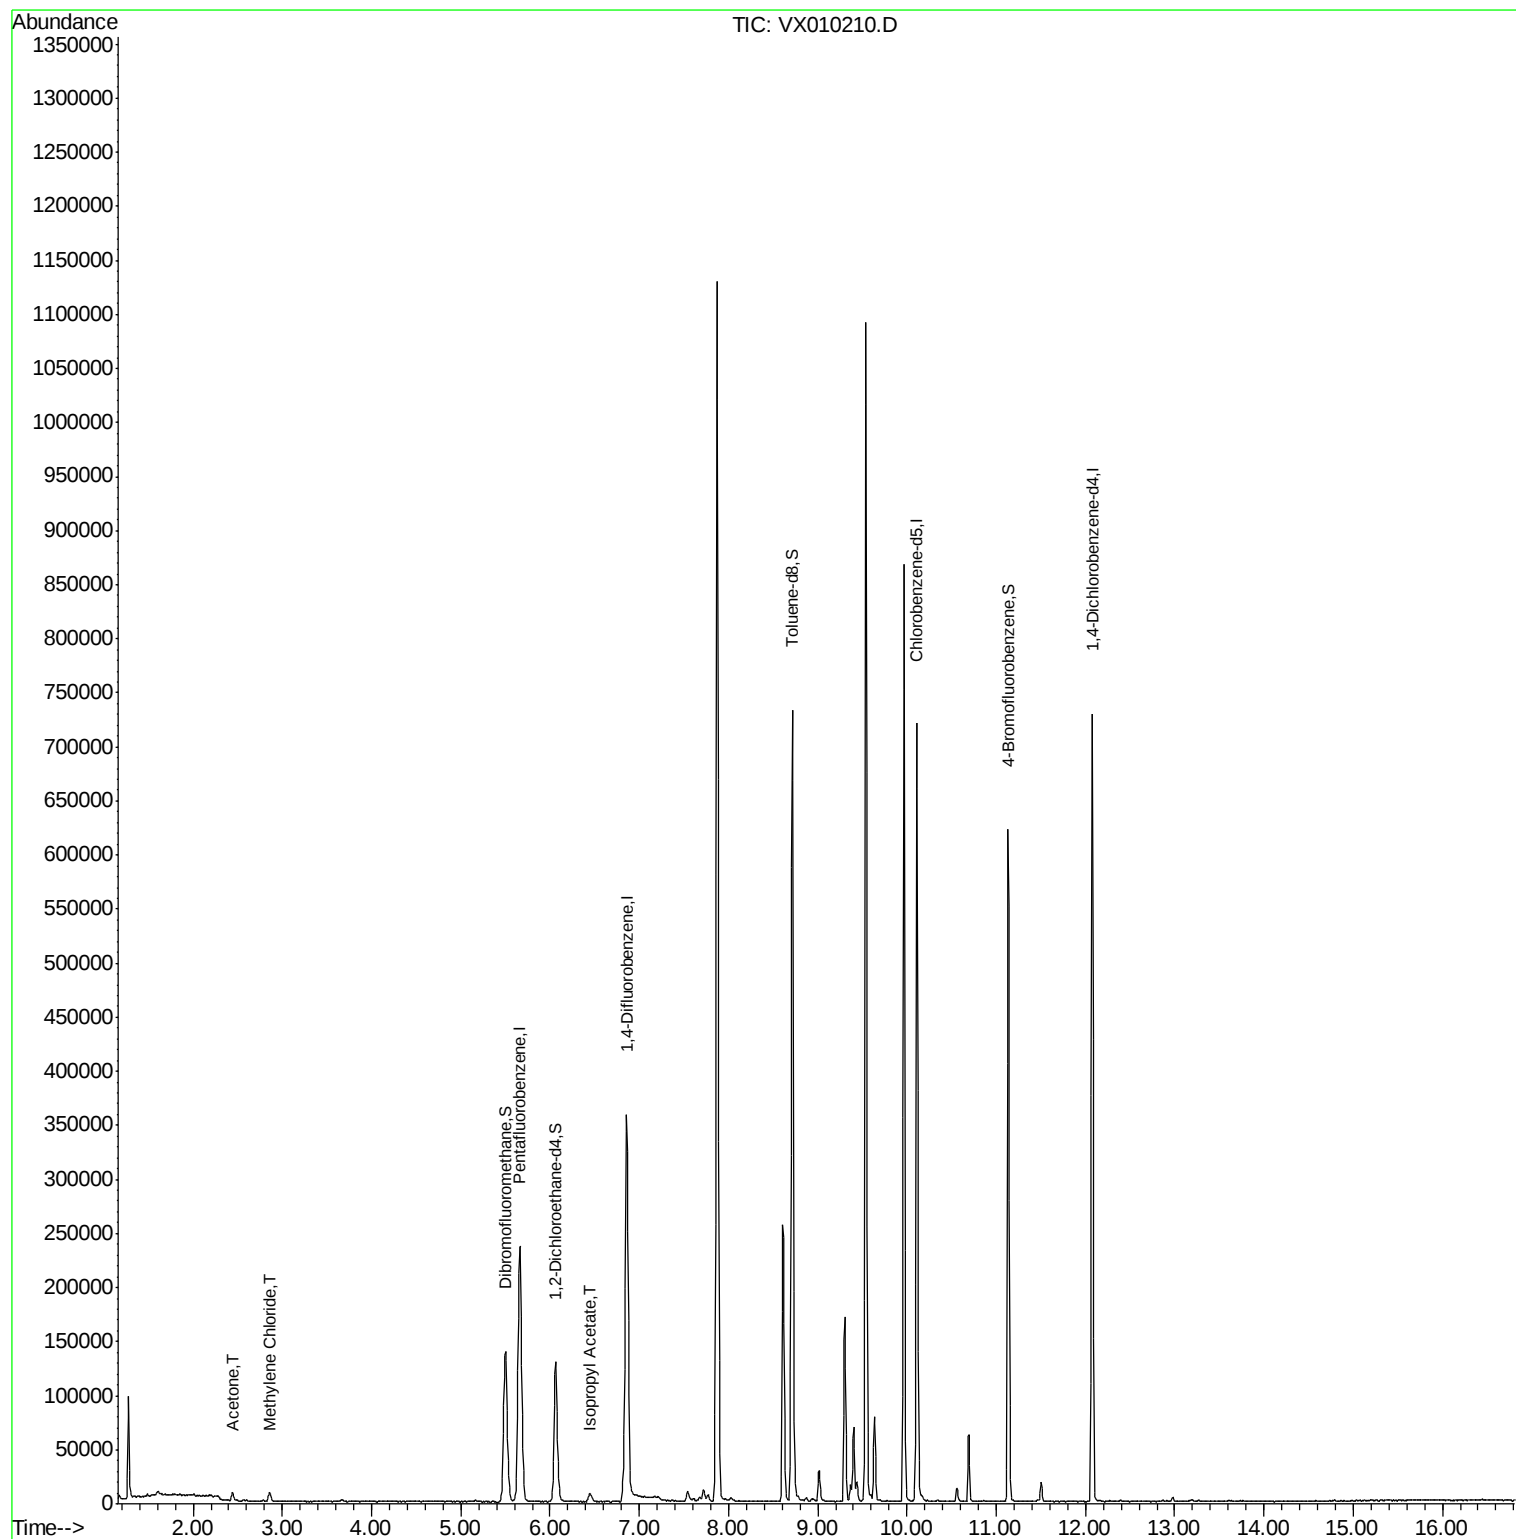



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX010210.D

Acq: 11 Jun 2019 05:00

Instrument :

MSVOA_X

ClientSampleId :


PB120437TB

Tot Ion:168 Resp: 258896

Ion Ratio Lower Upper




168 100

99 45.5 43.0 64.6

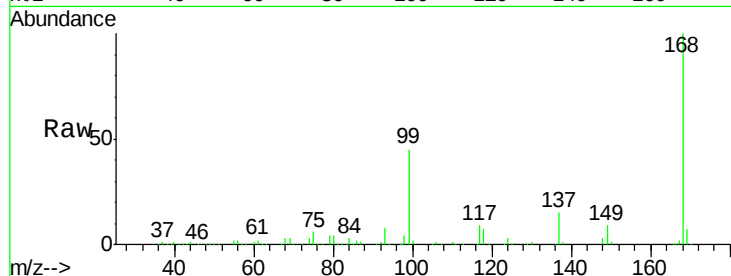

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

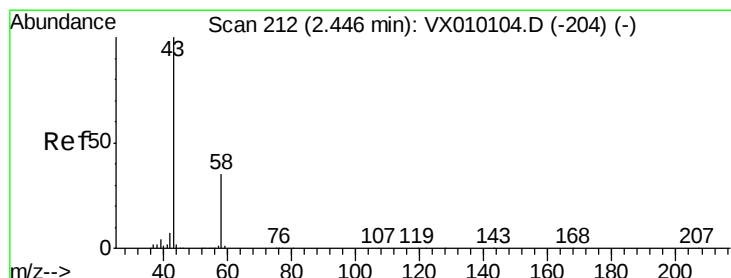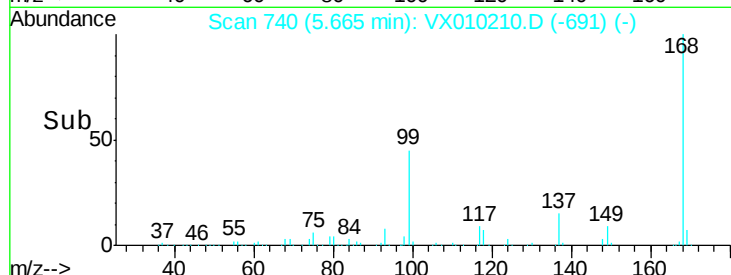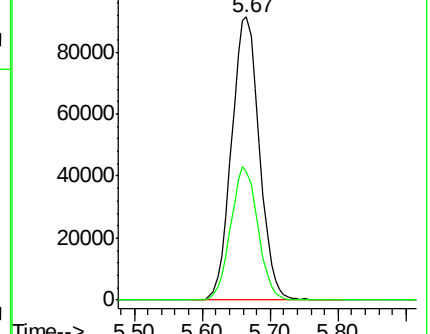

#16

Acetone

Concen: 6.524 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX010210.D


Acq: 11 Jun 2019 05:00

Tgt Ion: 43 Resp: 7754

Ion Ratio Lower Upper



43 100


58 38.5 23.2 34.8#

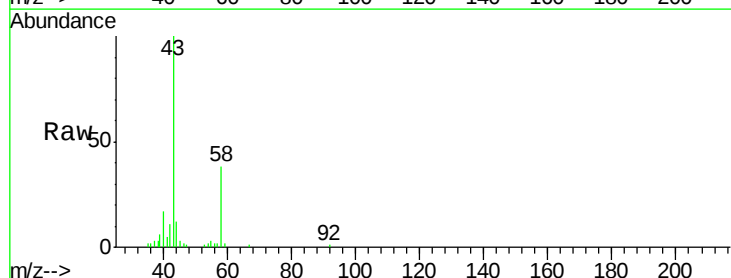

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



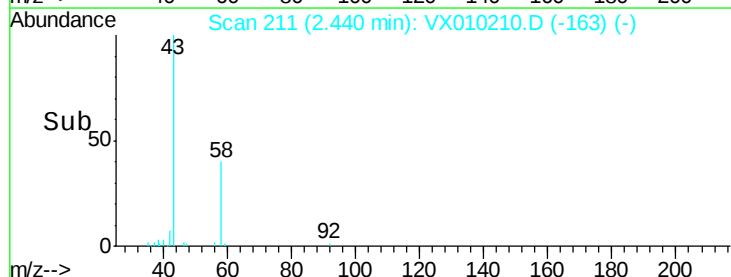
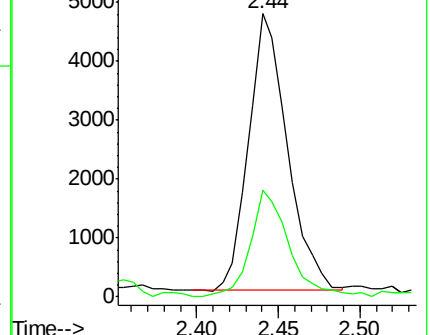


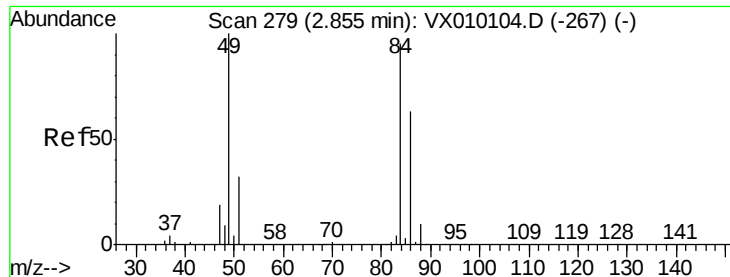

#20
Methvlene Chloride
Concen: 1.581 ug/l
RT: 2.85 min Scan# 279
Delta R.T. -0.00 min
Lab File: VX010210.D
Acq: 11 Jun 2019 05:00




Instrument :
MSVOA_X
ClientSampleId :
PB120437TB


Tot Ion: 84 Resp: 4128
Ion Ratio Lower Upper
84 100
49 94.7 115.8 173.6#
51 29.6 34.4 51.6#
86 73.9 49.7 74.5

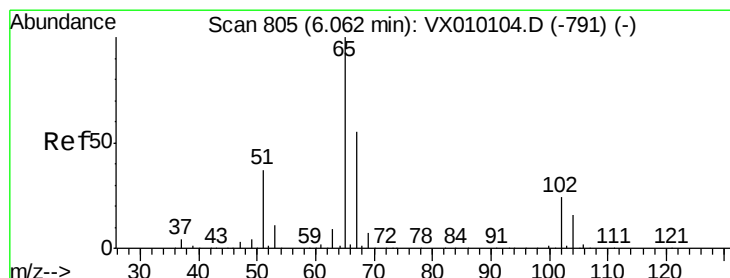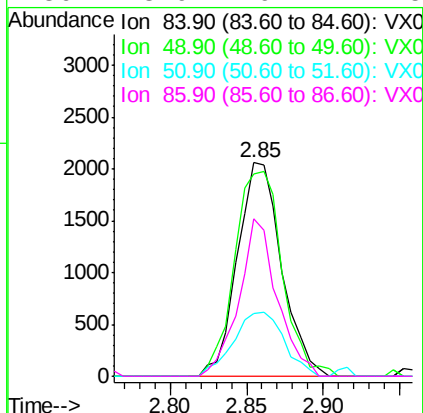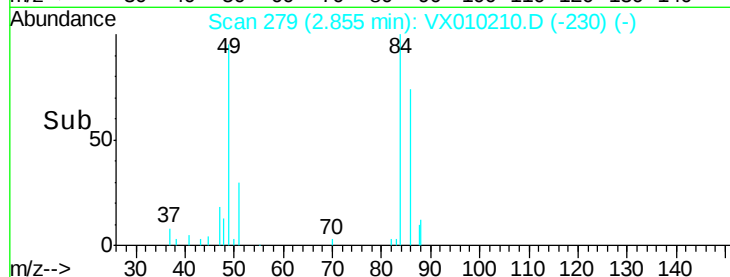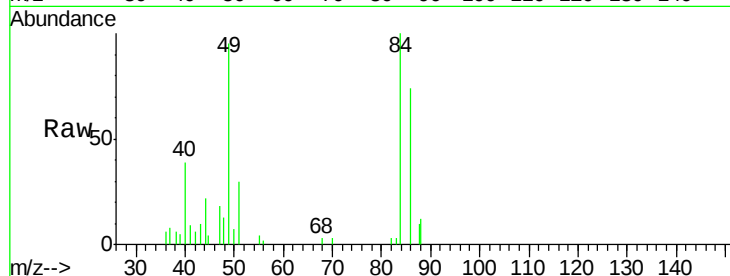

#33
1,2-Dichloroethane-d4
Concen: 46.002 ug/l
RT: 6.06 min Scan# 805
Delta R.T. 0.00 min
Lab File: VX010210.D
Acq: 11 Jun 2019 05:00

Tgt Ion: 65 Resp: 116253
Ion Ratio Lower Upper
65 100
67 55.1 0.0 108.4

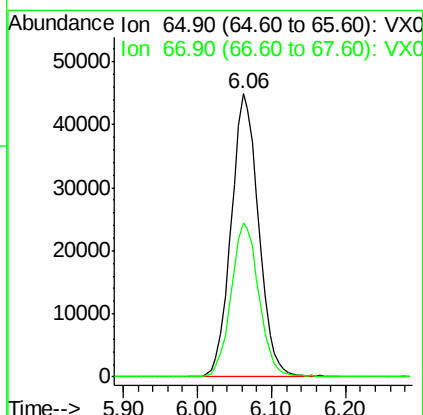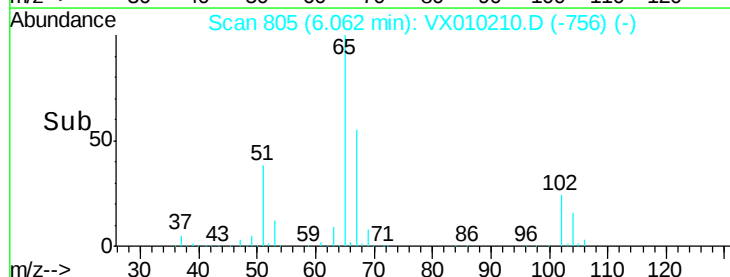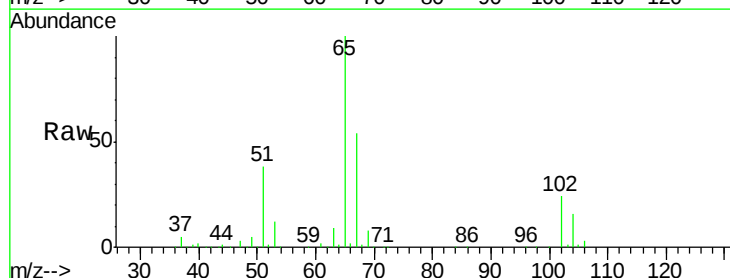

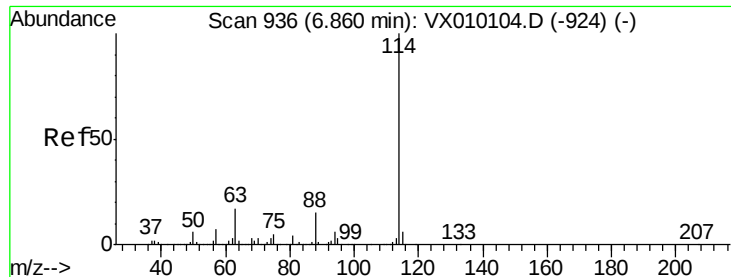

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX010210.D

Acq: 11 Jun 2019 05:00

Instrument :

MSVOA_X

ClientSampleId :

PB120437TB


Tot Ion:114 Resp: 393114

Ion Ratio Lower Upper

114 100

63 16.6 0.0 47.4




88 14.4 0.0 33.0

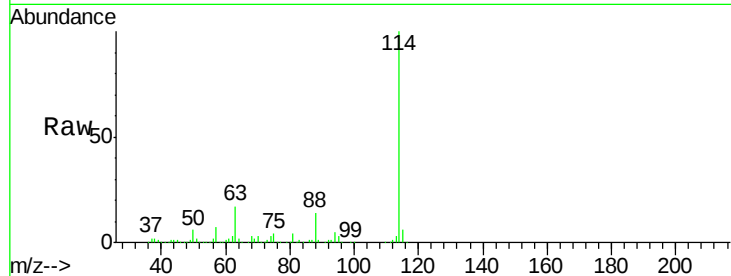

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

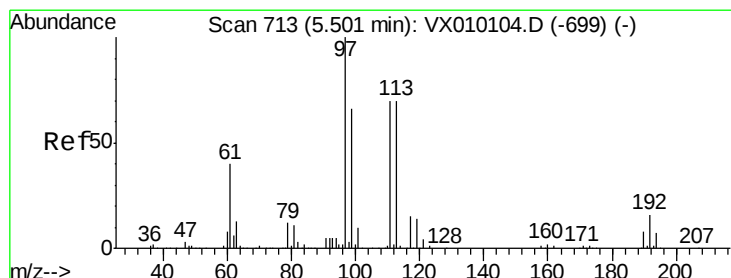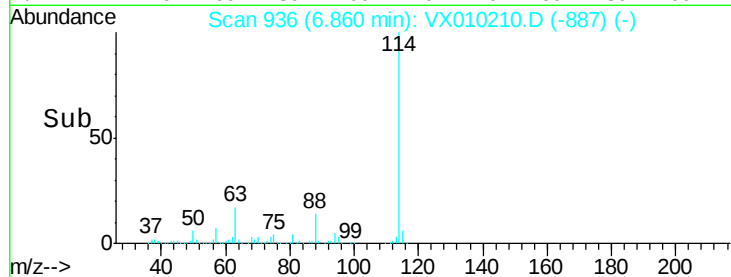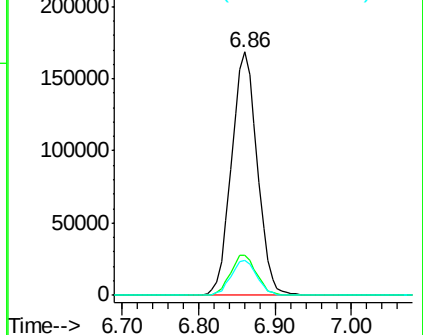

#35

Dibromofluoromethane

Concen: 50.007 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX010210.D

Acq: 11 Jun 2019 05:00


Tgt Ion:113 Resp: 121258

Ion Ratio Lower Upper

113 100

111 101.5 82.2 123.2



192 22.7 17.1 25.7

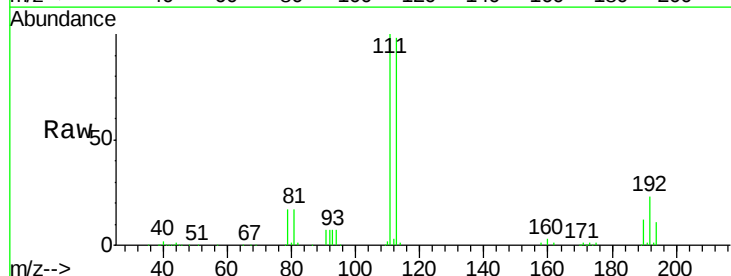


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

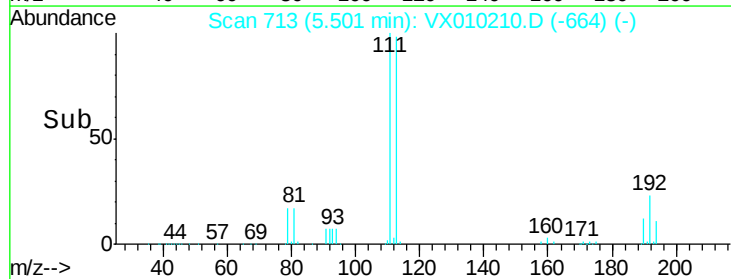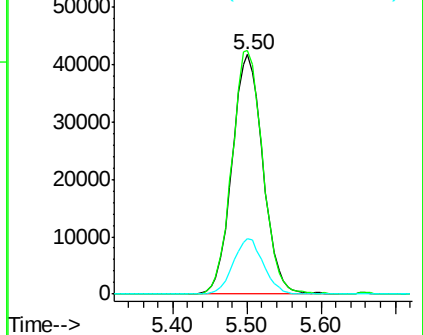

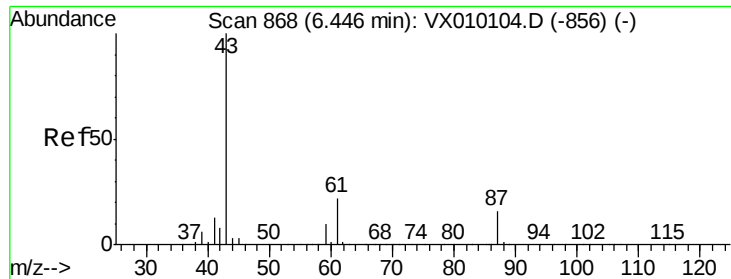

#43

Isopropyl Acetate

Concen: 2.031 ug/l

RT: 6.45 min Scan# 869

Delta R.T. 0.01 min

Lab File: VX010210.D

Acq: 11 Jun 2019 05:00

Instrument :

MSVOA_X

ClientSampled :

PB120437TB


Tot Ion: 43 Resp: 11332

Ion Ratio Lower Upper

43 100

61 23.8 14.6 21.8#




87 16.3 8.7 13.1#

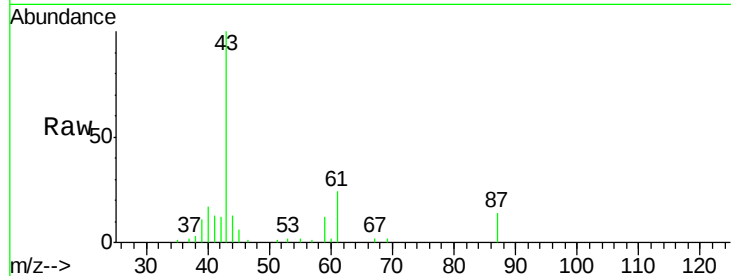

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

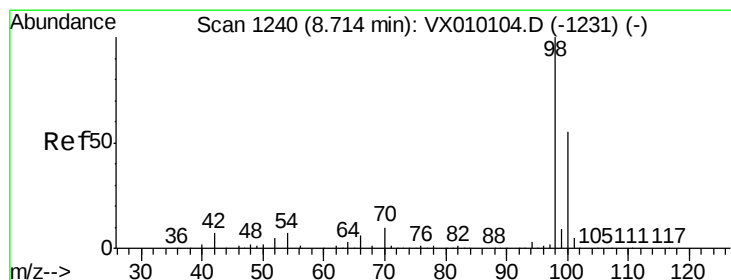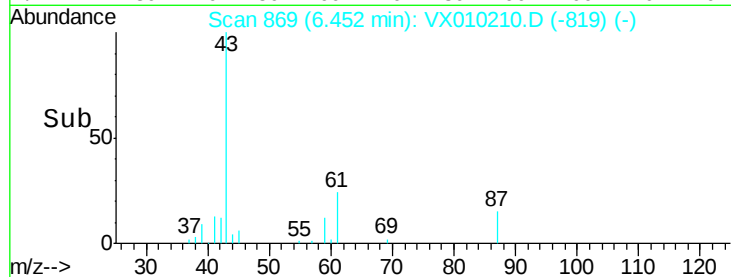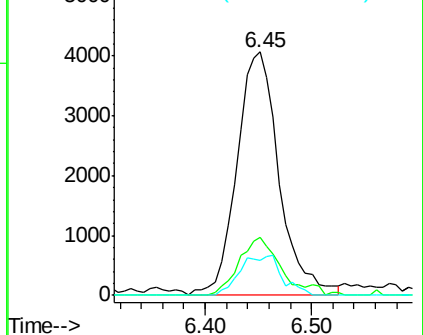

#50

Toluene-d8

Concen: 51.015 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX010210.D


Acq: 11 Jun 2019 05:00

Tgt Ion: 98 Resp: 463615

Ion Ratio Lower Upper



98 100


100 64.6 51.5 77.3

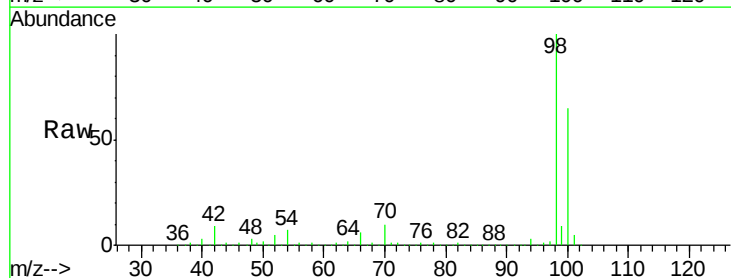

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

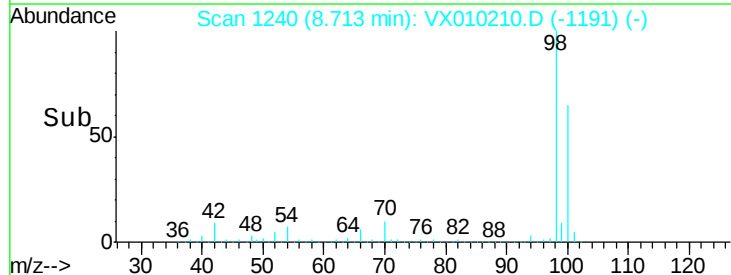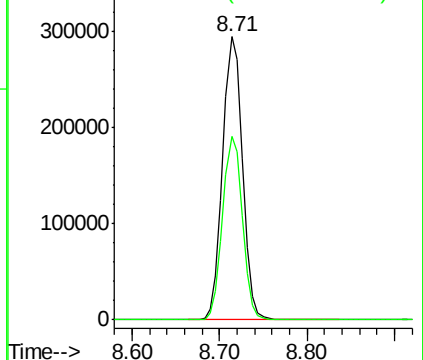

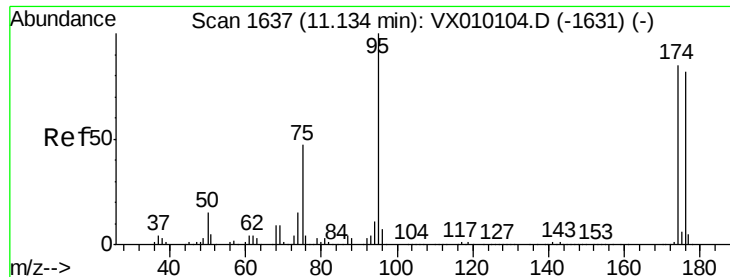

#62

4-Bromofluorobenzene

Concen: 46.923 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX010210.D

Acq: 11 Jun 2019 05:00

Instrument :

MSVOA_X

ClientSampleId :

PB120437TB


Tot Ion: 95 Resp: 159255

Ion Ratio Lower Upper

95 100

174 94.7 0.0 160.4




176 92.1 0.0 154.6

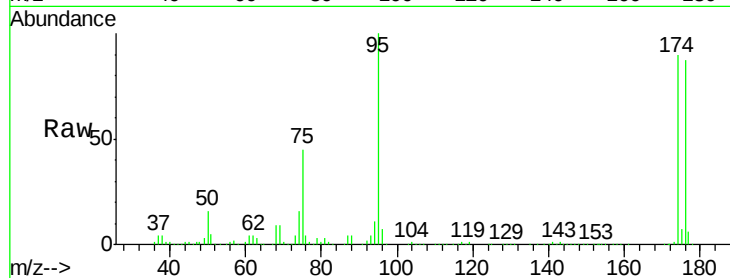

Abundance Ion 94.90 (94.60 to 95.60): VX010210.D (-1588) (-)

Ion 173.80 (173.50 to 174.50): VX010210.D (-1588) (-)

Ion 175.80 (175.50 to 176.50): VX010210.D (-1588) (-)

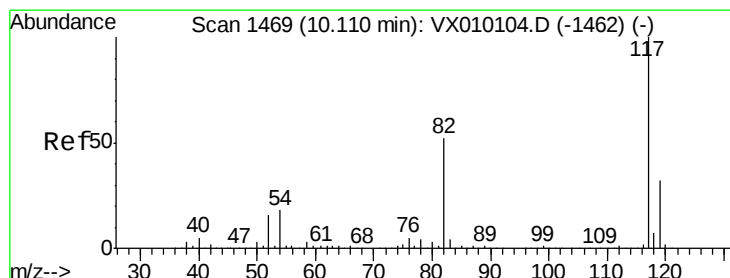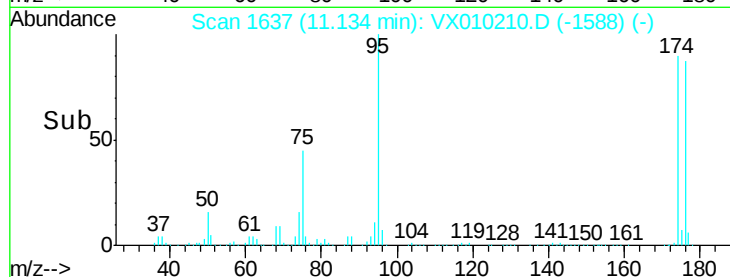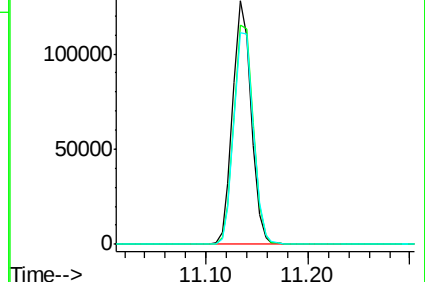

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX010210.D

Acq: 11 Jun 2019 05:00


Tgt Ion: 117 Resp: 357680

Ion Ratio Lower Upper

117 100

82 50.6 49.2 73.8



119 33.1 25.2 37.8

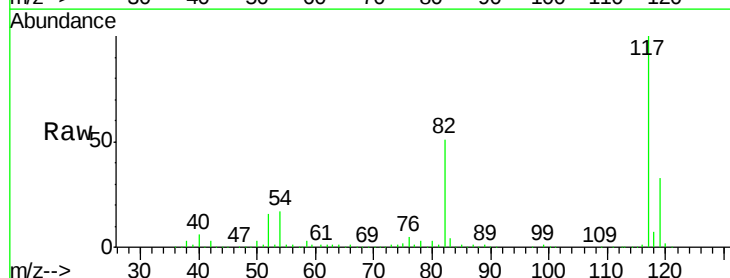


Abundance Ion 116.90 (116.60 to 117.60): VX010210.D (-1420) (-)

Ion 82.00 (81.70 to 82.70): VX010210.D (-1420) (-)

Ion 118.90 (118.60 to 119.60): VX010210.D (-1420) (-)

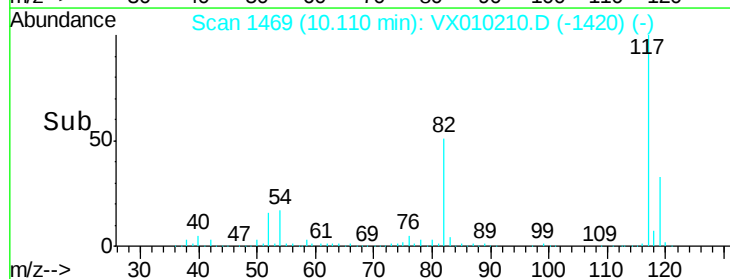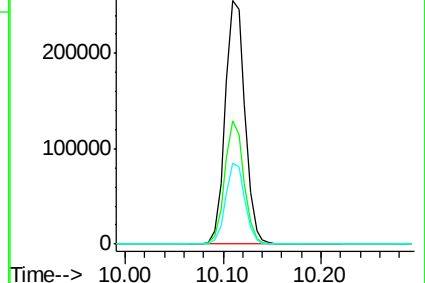

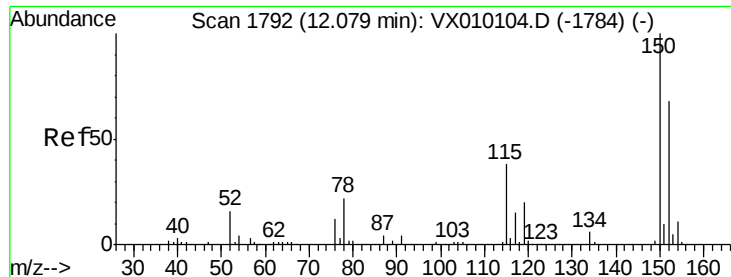

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX010210.D

Acq: 11 Jun 2019 05:00

Instrument :

MSVOA_X

ClientSampleId :

PB120437TB


Tot Ion:152 Resp: 168506

Ion Ratio Lower Upper

152 100

115 53.2 41.4 124.2

150 156.0 0.0 345.2

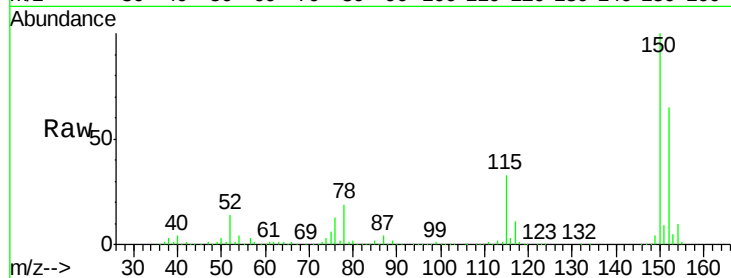

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

