

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061021\
 Data File : VX022653.D
 Acq On : 10 Jun 2021 19:16
 Operator : JC/MD
 Sample : M2645-03 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BUR-1041

Quant Time: Jun 11 06:47:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 10 12:20:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	58541	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	118322	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	105380	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	42081	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	49490	47.006	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.020%
35) Dibromofluoromethane	5.391	113	35551	47.092	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.180%
50) Toluene-d8	8.653	98	147001	49.396	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.800%
62) 4-Bromofluorobenzene	11.085	95	52475	46.623	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.240%

Target Compounds				Qvalue		
5) Bromomethane	1.605	94	207	0.467	ug/l #	51
10) Methyl Iodide	2.459	142	242	0.301	ug/l #	91
11) Tert butyl alcohol	2.953	59	1224	5.021	ug/l #	73
13) Acrolein	2.239	56	8234	80.601	ug/l	98
15) Acrylonitrile	3.081	53	108	0.226	ug/l #	35
16) Acetone	2.386	43	12139	25.749	ug/l	96
17) Carbon Disulfide	2.508	76	1070	0.669	ug/l #	75
18) Methyl Acetate	2.709	43	504	0.355	ug/l #	47
20) Methylene Chloride	2.794	84	526	0.302	ug/l #	77
21) trans-1,2-Dichloroethene	3.105	96	173	0.220	ug/l #	30
22) Diisopropyl ether	3.873	45	765	0.281	ug/l #	1
25) 2-Butanone	4.568	43	13204	17.270	ug/l	91
29) Tetrahydrofuran	5.038	42	114	0.256	ug/l #	59
36) 1,1-Dichloropropene	5.562	75	5681	4.819	ug/l #	45
37) Ethyl Acetate	4.727	43	3770	2.516	ug/l #	87
38) Carbon Tetrachloride	5.562	117	7095	7.035	ug/l #	16
41) Methacrylonitrile	5.025	41	275	0.342	ug/l #	18
43) Isopropyl Acetate	6.367	43	3724	1.574	ug/l #	57
46) Dibromomethane	7.592	93	22	1.380	ug/l #	2
49) 1,4-Dioxane	7.915	88	20	0.925	ug/l #	1
51) 4-Methyl-2-Pentanone	8.555	43	6227	4.146	ug/l #	32
53) t-1,3-Dichloropropene	8.982	75	82	3.312	ug/l #	44
54) cis-1,3-Dichloropropene	8.391	75	21	2.509	ug/l #	57
59) 2-Hexanone	9.439	43	760	0.662	ug/l	72
64) Tetrachloroethene	9.281	164	148	0.222	ug/l #	17
68) m/p-Xylenes	10.305	106	321	0.219	ug/l	76
70) Styrene	10.659	104	164	1.515	ug/l #	29
76) 1,2,3-Trichloropropane	11.085	75	27399	24.557	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	27399	61.938	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.756	105	734	0.251	ug/l	89
85) sec-Butylbenzene	11.896	105	728	0.206	ug/l	82
86) p-Isopropyltoluene	12.012	119	671	0.230	ug/l #	69
87) 1,3-Dichlorobenzene	11.975	146	356	0.254	ug/l	92
88) 1,4-Dichlorobenzene	11.975	146	356	0.247	ug/l	92
89) n-Butylbenzene	12.341	91	1364	0.489	ug/l	87
93) 1,2,4-Trichlorobenzene	13.597	180	492	0.601	ug/l	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061021\
Data File : VX022653.D
Acq On : 10 Jun 2021 19:16
Operator : JC/MD
Sample : M2645-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1041

Quant Time: Jun 11 06:47:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 12:20:00 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
94) Hexachlorobutadiene	13.731	225	114	0.388	ug/l #	49
95) Naphthalene	13.780	128	1410	1.857	ug/l #	94
96) 1,2,3-Trichlorobenzene	13.969	180	393	0.492	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061021\
Data File : VX022653.D
Acq On : 10 Jun 2021 19:16
Operator : JC/MD
Sample : M2645-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Quant Time: Jun 11 06:47:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 12:20:00 2021
Response via : Initial Calibration

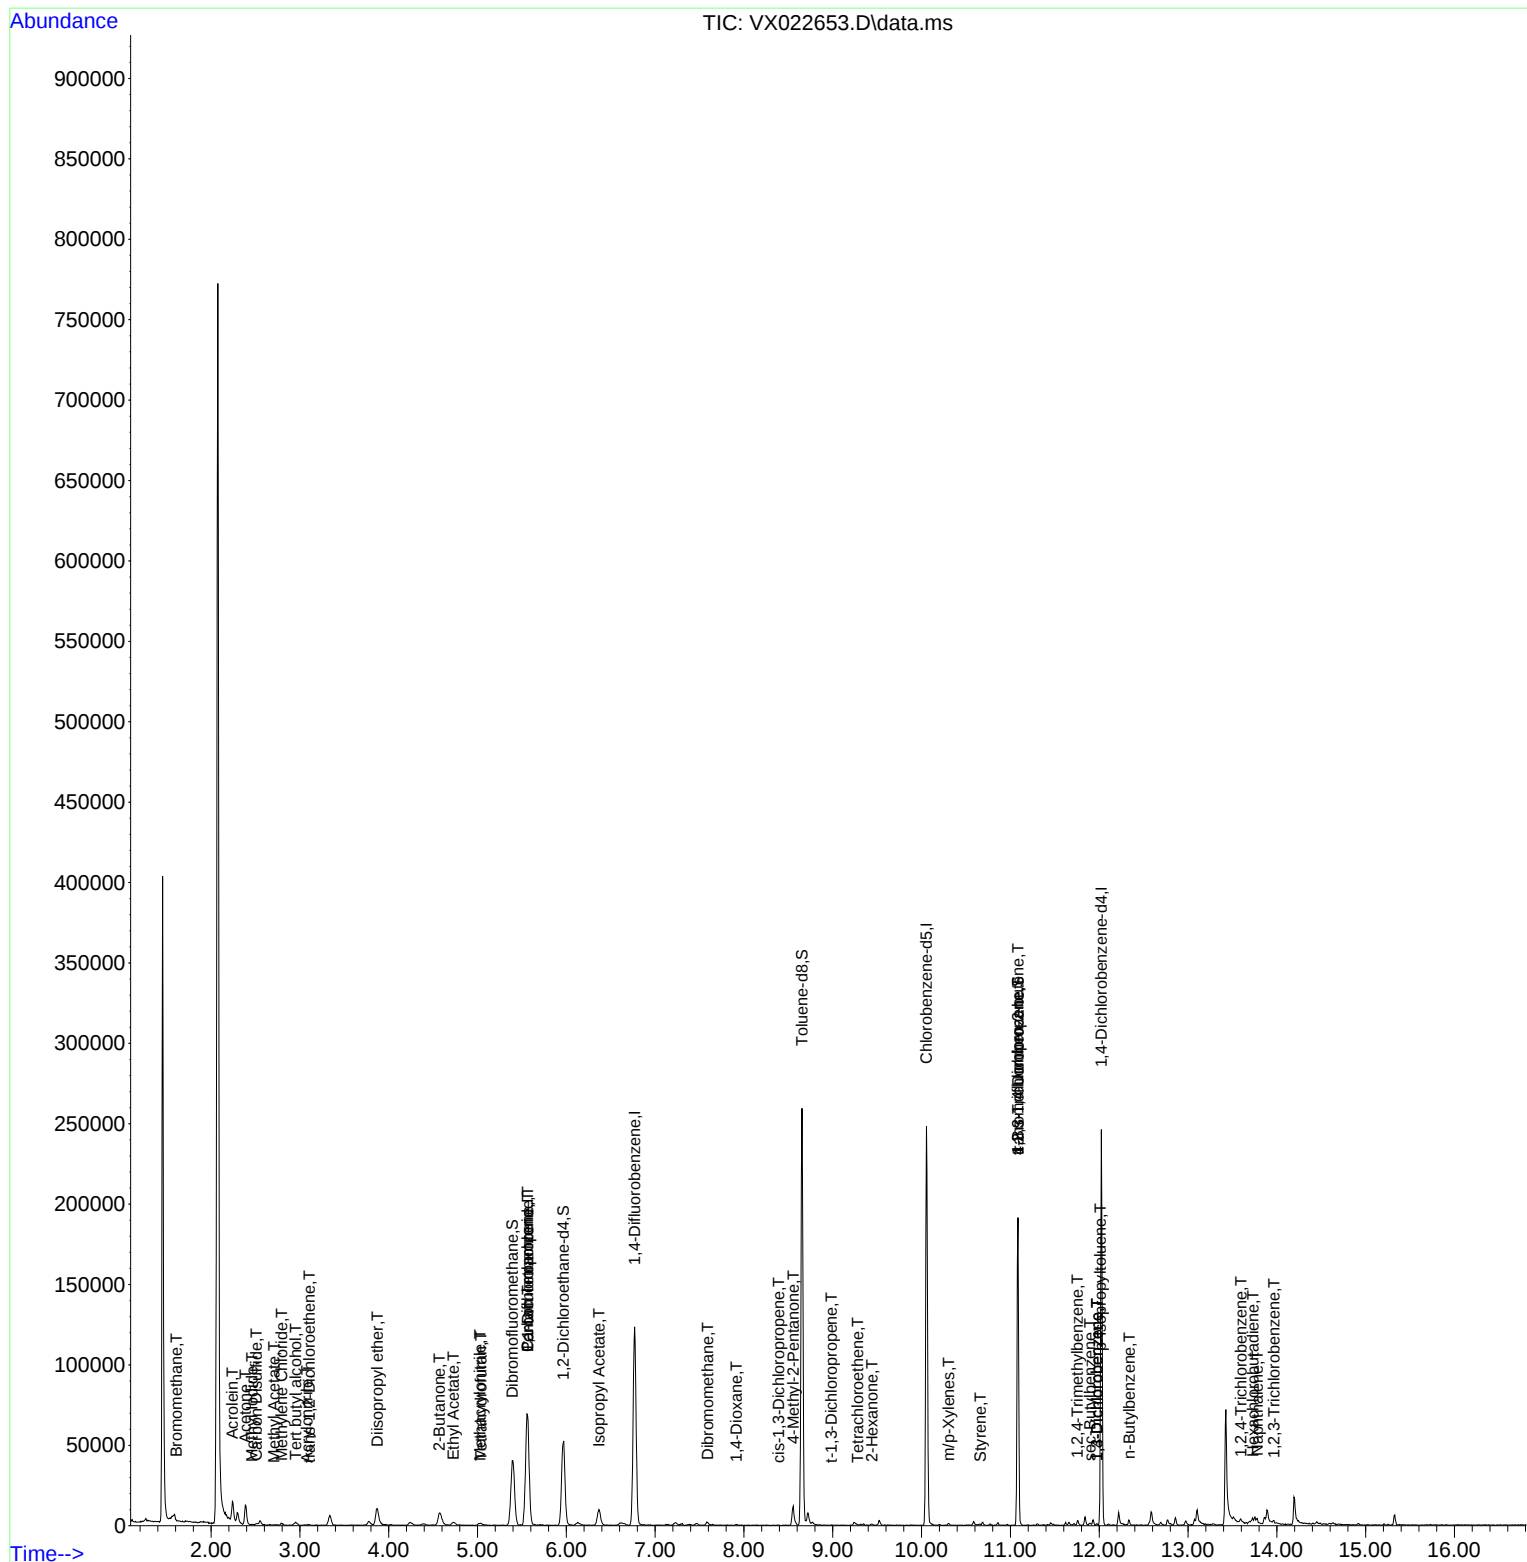






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Instrument :
MSVOA_X
ClientSampleID :
BUR-1041



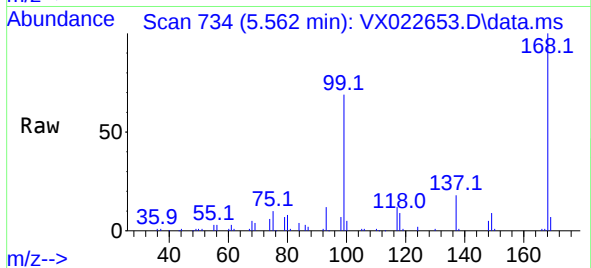



Tgt Ion:168 Resp: 58541
Ion Ratio Lower Upper
168 100
99 68.9 45.8 68.6#



#5
Bromomethane
Concen: 0.467 ug/l
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 94 Resp: 207
Ion Ratio Lower Upper
94 100
96 48.1 76.4 114.6#


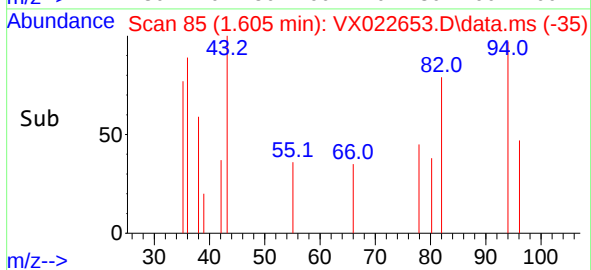






#10
Methyl Iodide
Concen: 0.301 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion:142 Resp: 242
Ion Ratio Lower Upper
142 100
127 41.3 33.3 49.9
141 0.0 11.4 17.0#

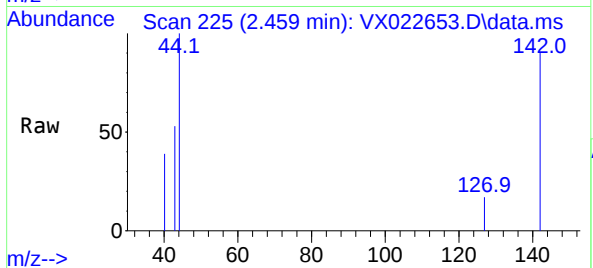

#11
Tert butyl alcohol
Concen: 5.021 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.030 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 59 Resp: 1224
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


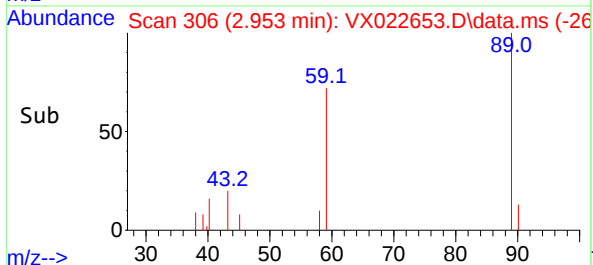

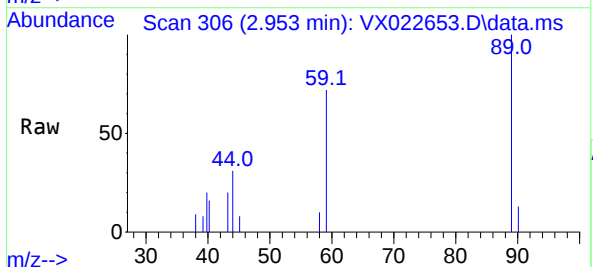




#13
Acrolein
Concen: 80.601 ug/l
RT: 2.239 min Scan# 189
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion: 56 Resp: 8234
Ion Ratio Lower Upper
56 100
55 68.5 56.4 84.6

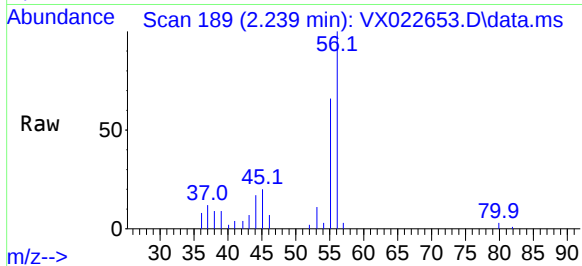

#15
Acrylonitrile
Concen: 0.226 ug/l
RT: 3.081 min Scan# 327
Delta R.T. 0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 53 Resp: 108
Ion Ratio Lower Upper
53 100
52 141.7 65.3 97.9#
51 0.0 28.2 42.2#


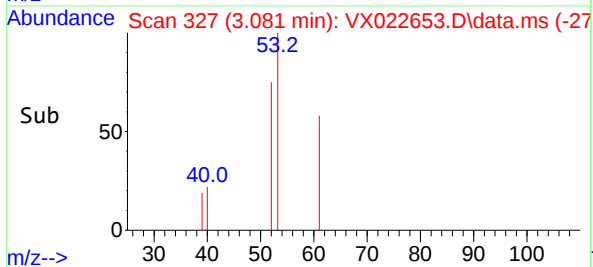

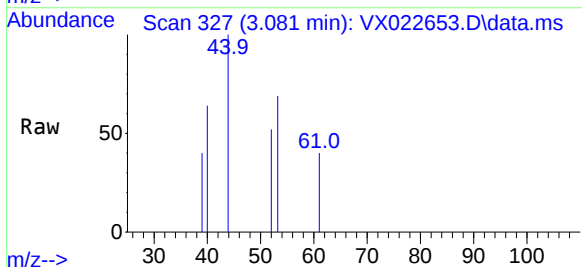




#16
Acetone
Concen: 25.749 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampled :
BUR-1041


Tgt Ion: 43 Resp: 12139
Ion Ratio Lower Upper
43 100
58 32.5 27.8 41.8



#17
Carbon Disulfide
Concen: 0.669 ug/l
RT: 2.508 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 76 Resp: 1070
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


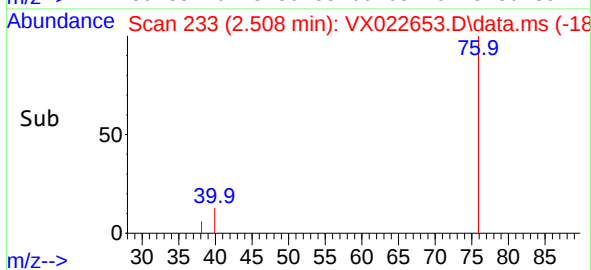




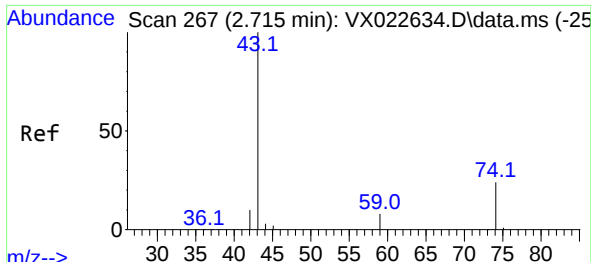

#18
Methyl Acetate
Concen: 0.355 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion: 43 Resp: 504
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

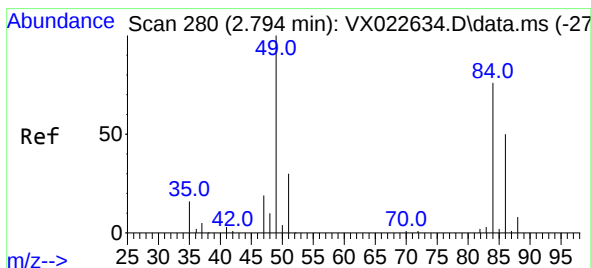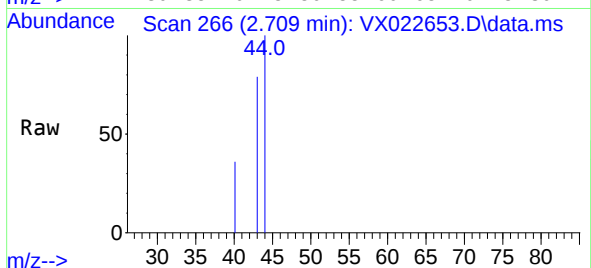

#20
Methylene Chloride
Concen: 0.302 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 84 Resp: 526
Ion Ratio Lower Upper
84 100
49 91.9 88.6 132.8
51 18.7 27.0 40.6#
86 40.4 50.3 75.5#


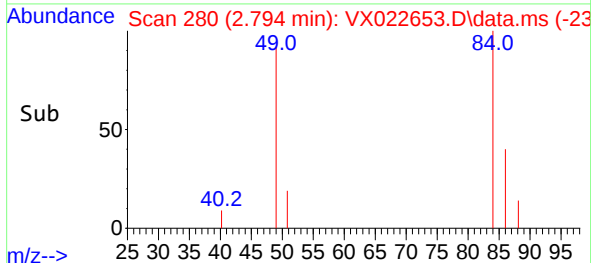
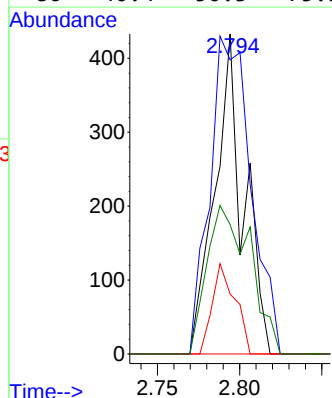
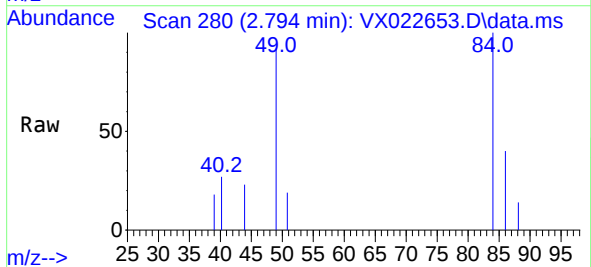




#21
trans-1,2-Dichloroethene
Concen: 0.220 ug/l
RT: 3.105 min Scan# 331
Delta R.T. 0.012 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion: 96 Resp: 173
Ion Ratio Lower Upper
96 100
61 57.1 107.7 161.5#
98 0.0 50.4 75.6#

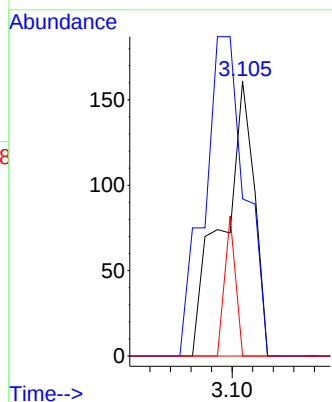

#22
Diisopropyl ether
Concen: 0.281 ug/l
RT: 3.873 min Scan# 457
Delta R.T. 0.103 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 45 Resp: 765
Ion Ratio Lower Upper
45 100
43 178.6 58.0 87.0#
87 0.0 25.4 38.0#
59 611.5 10.2 15.2#


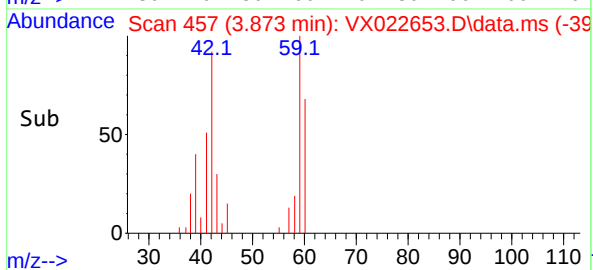






#25
2-Butanone
Concen: 17.270 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampled :
BUR-1041


Tgt Ion: 43 Resp: 13204
Ion Ratio Lower Upper
43 100
72 24.9 23.7 35.5

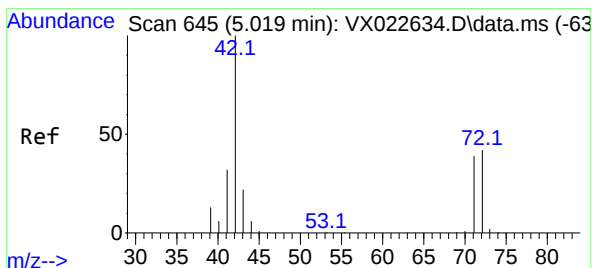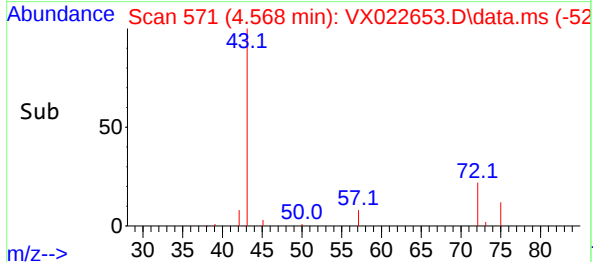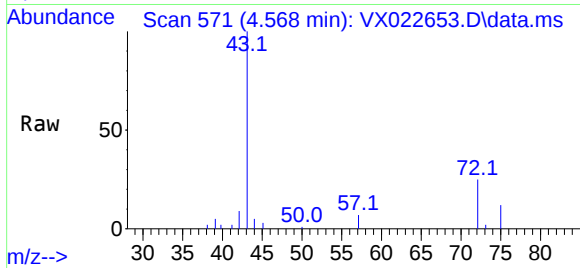

#29
Tetrahydrofuran
Concen: 0.256 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.025 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 42 Resp: 114
Ion Ratio Lower Upper
42 100
72 42.1 41.7 62.5
71 0.0 38.4 57.6#


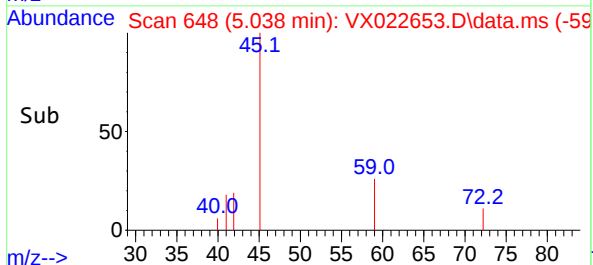
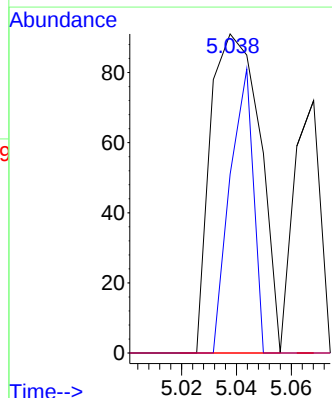
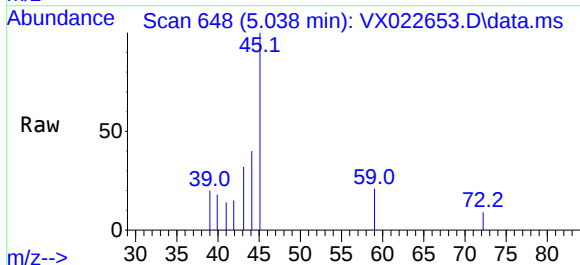




#33
1,2-Dichloroethane-d4
Concen: 47.006 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampled :
BUR-1041


Tgt Ion: 65 Resp: 49490
Ion Ratio Lower Upper
65 100
67 51.3 0.0 105.4



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 114 Resp: 118322
Ion Ratio Lower Upper
114 100
63 20.8 0.0 40.8
88 16.3 0.0 32.8

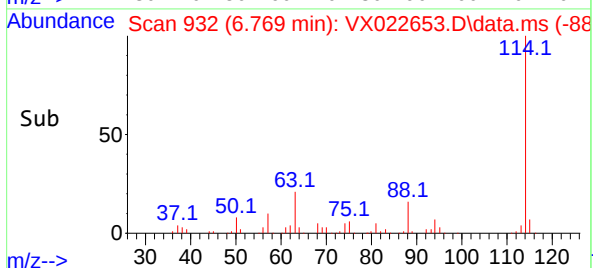

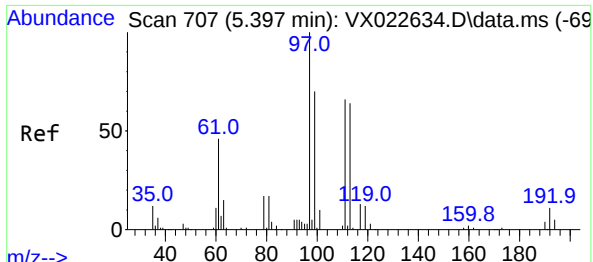

#35

Dibromofluoromethane

Concen: 47.092 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX022653.D

Acq: 10 Jun 2021 19:16





Tgt Ion:113 Resp: 35551

Ion Ratio Lower Upper

113 100

111 102.3 81.9 122.9

192 15.5 16.7 25.1#

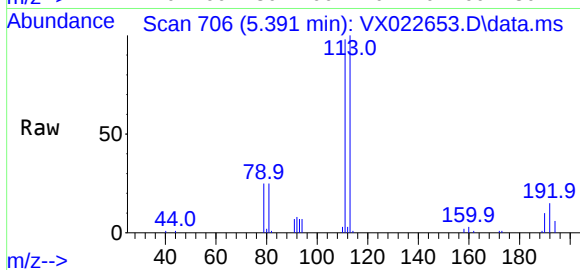

#36

1,1-Dichloropropene

Concen: 4.819 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.140 min

Lab File: VX022653.D

Acq: 10 Jun 2021 19:16




Tgt Ion: 75 Resp: 5681


Ion Ratio Lower Upper

75 100

110 4.7 18.1 54.4#

77 0.0 25.3 37.9#

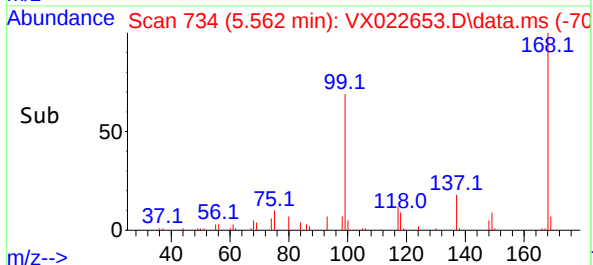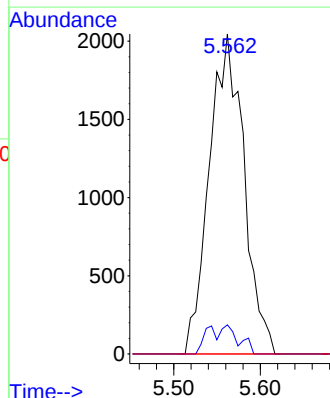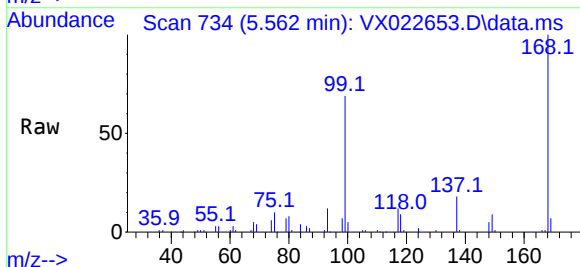



#37

Ethyl Acetate

Concen: 2.516 ug/l

RT: 4.727 min Scan# 597

Delta R.T. -0.000 min

Lab File: VX022653.D

Acq: 10 Jun 2021 19:16





Instrument :

MSVOA_X

ClientSampleId :

BUR-1041

Tgt Ion:	43	Resp:	3770
Ion	Ratio	Lower	Upper
43	100		
61	13.3	12.8	19.2
70	4.4	10.5	15.7#

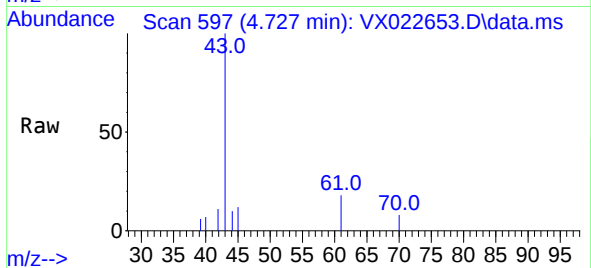

#38

Carbon Tetrachloride

Concen: 7.035 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.116 min

Lab File: VX022653.D

Acq: 10 Jun 2021 19:16

Tgt Ion:	117	Resp:	7095
Ion	Ratio	Lower	Upper
117	100		
119	4.6	76.2	114.2#
121	0.0	24.8	37.2#

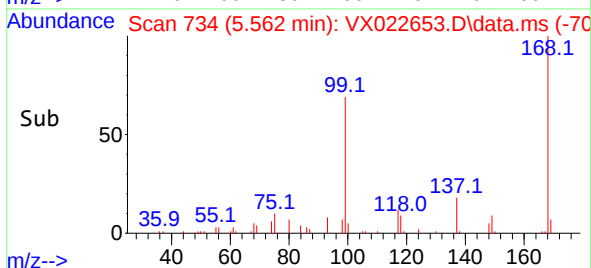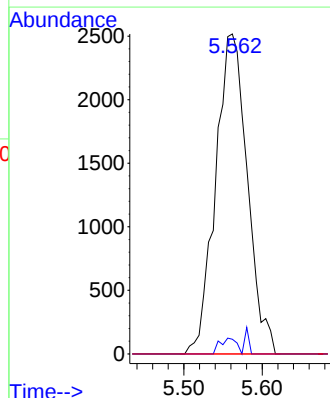




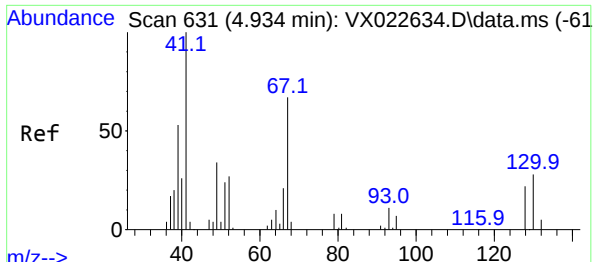


#41
Methacrylonitrile
Concen: 0.342 ug/l
RT: 5.025 min Scan# 646
Delta R.T. 0.097 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Instrument :
MSVOA_X
ClientSampleId :
BUR-1041

Tgt Ion: 41 Resp: 275




Ion	Ratio	Lower	Upper
41	100		
39	110.9	42.5	63.7#
67	0.0	65.0	97.6#
52	0.0	25.3	37.9#

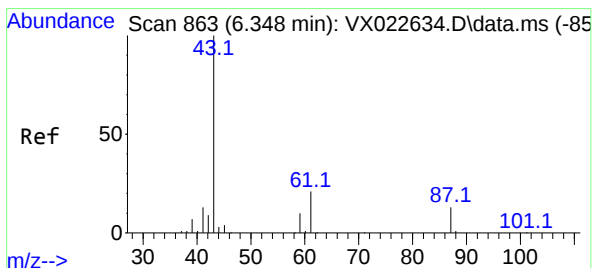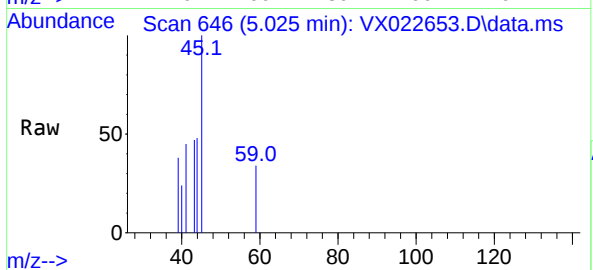


#43
Isopropyl Acetate
Concen: 1.574 ug/l
RT: 6.367 min Scan# 866
Delta R.T. 0.019 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 43 Resp: 3724

Ion	Ratio	Lower	Upper
43	100		
61	0.0	18.2	27.4#
87	0.0	12.5	18.7#


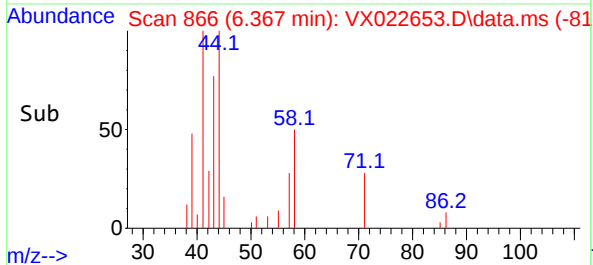

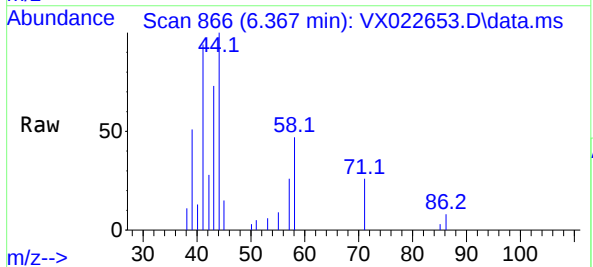




#46
Dibromomethane
Concen: 1.380 ug/l
RT: 7.592 min Scan# 1067
Delta R.T. 0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion: 93 Resp: 22
Ion Ratio Lower Upper
93 100
95 0.0 66.8 100.2#
174 0.0 83.1 124.7#



#49
1,4-Dioxane
Concen: 0.925 ug/l
RT: 7.915 min Scan# 1120
Delta R.T. 0.250 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 88 Resp: 20
Ion Ratio Lower Upper
88 100
43 1650.0 23.2 34.8#
58 0.0 55.0 82.4#


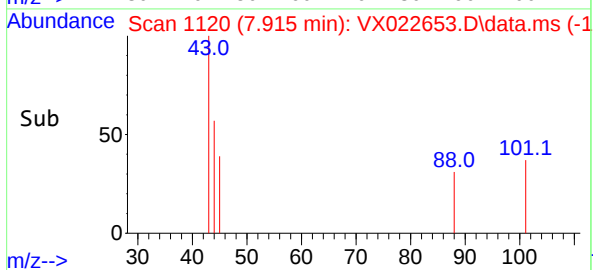






#50
Toluene-d8
Concen: 49.396 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion: 98 Resp: 147001
Ion Ratio Lower Upper
98 100
100 64.2 51.9 77.9

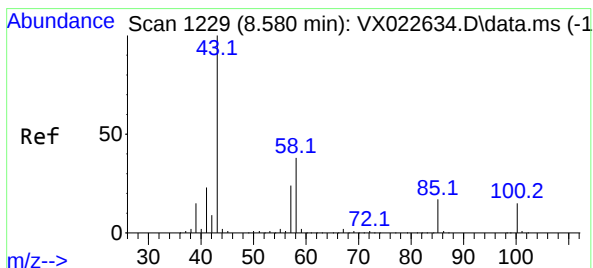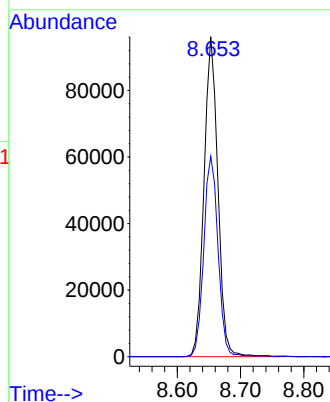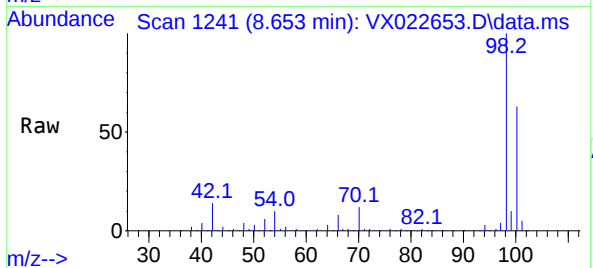

#51
4-Methyl-2-Pentanone
Concen: 4.146 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.025 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 43 Resp: 6227
Ion Ratio Lower Upper
43 100
58 0.0 35.4 53.0#


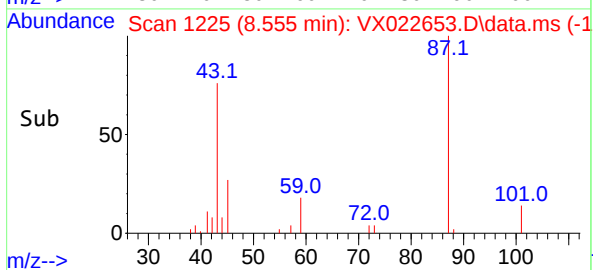
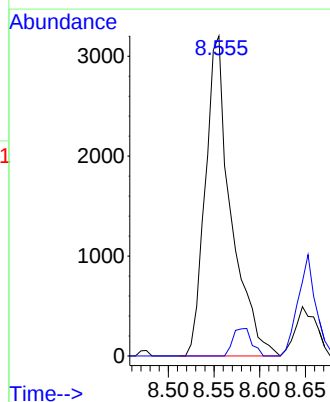
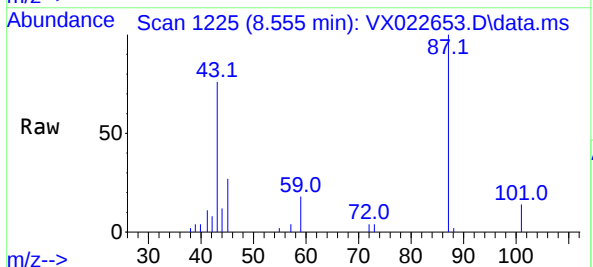




#53
t-1,3-Dichloropropene
Concen: 3.312 ug/l
RT: 8.982 min Scan# 1295
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion: 75 Resp: 82
Ion Ratio Lower Upper
75 100
77 0.0 24.9 37.3#

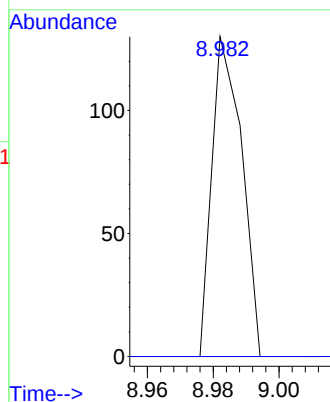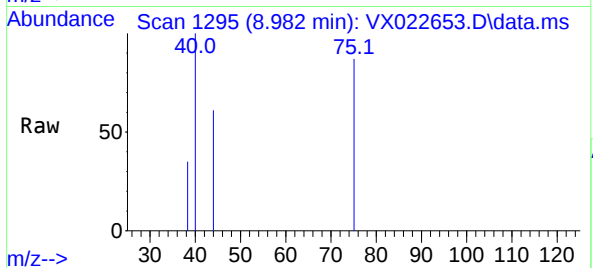

#54
cis-1,3-Dichloropropene
Concen: 2.509 ug/l
RT: 8.391 min Scan# 1198
Delta R.T. 0.019 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 75 Resp: 21
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#
39 22.4 35.1 52.7#


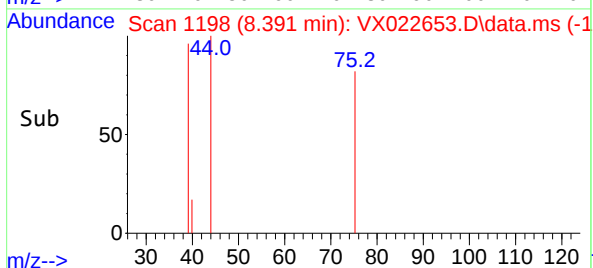






#59
2-Hexanone
Concen: 0.662 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion: 43 Resp: 760
Ion Ratio Lower Upper
43 100
58 40.7 30.9 92.8



#62
4-Bromofluorobenzene
Concen: 46.623 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 95 Resp: 52475
Ion Ratio Lower Upper
95 100
174 61.5 0.0 154.6
176 57.4 0.0 155.8


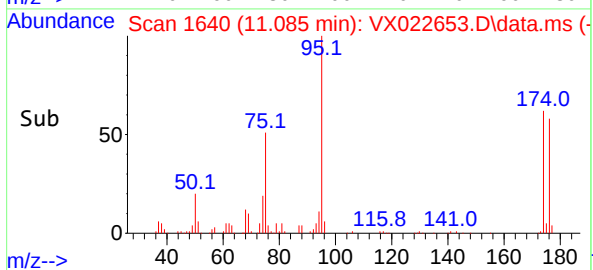






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion:117 Resp: 105380
Ion Ratio Lower Upper
117 100
82 62.1 47.4 71.2
119 31.1 26.6 39.8

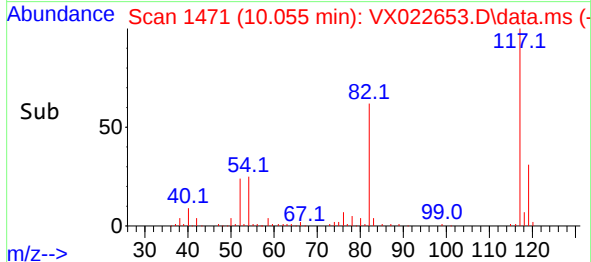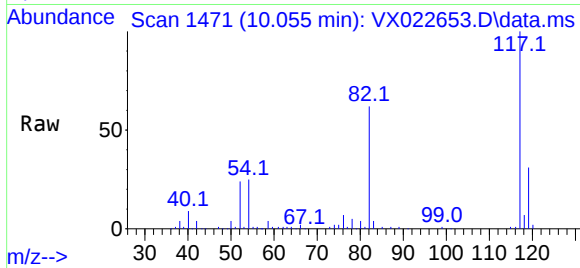

#64
Tetrachloroethene
Concen: 0.222 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion:164 Resp: 148
Ion Ratio Lower Upper
164 100
166 52.7 103.4 155.2#
129 0.0 70.8 106.2#
131 0.0 72.5 108.7#


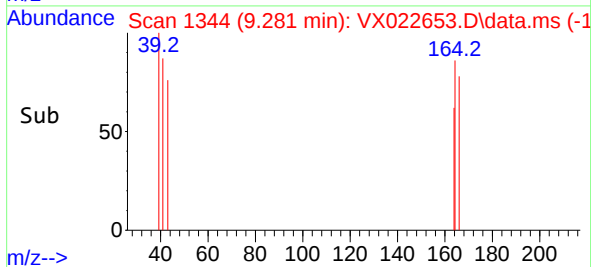

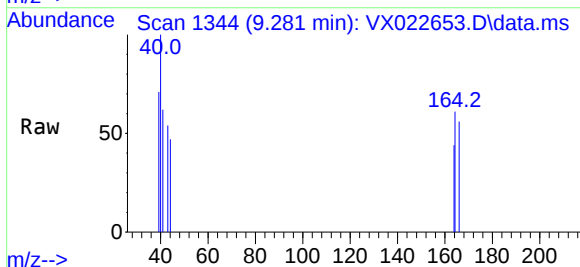




#68
m/p-Xylenes
Concen: 0.219 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampled :
BUR-1041


Tgt Ion:106 Resp: 321
Ion Ratio Lower Upper
106 100
91 240.5 162.8 244.2

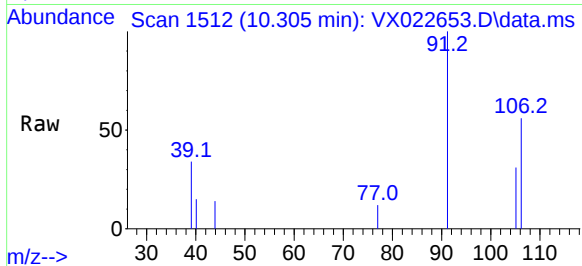

#70
Styrene
Concen: 1.515 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion:104 Resp: 164
Ion Ratio Lower Upper
104 100
78 87.8 40.0 60.0#
103 115.2 43.4 65.0#


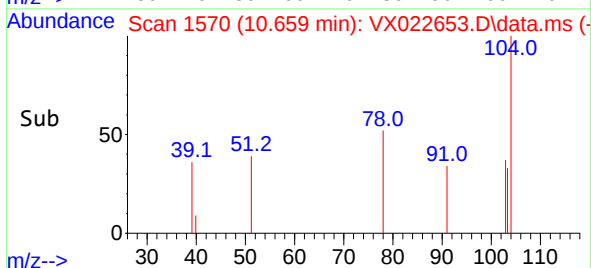
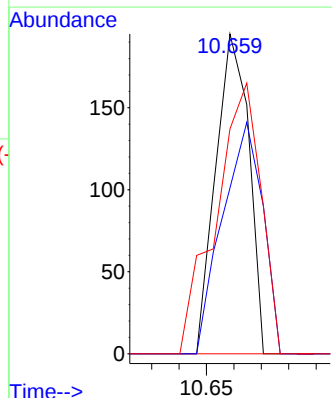
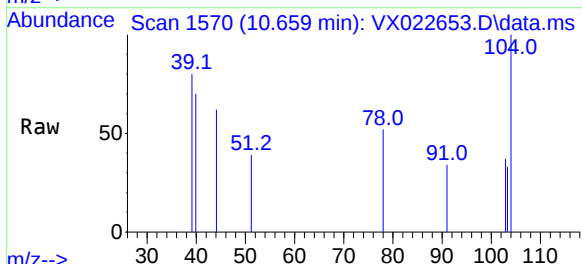




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampled :
BUR-1041


Tgt Ion:152 Resp: 42081
Ion Ratio Lower Upper
152 100
115 68.5 41.1 123.3
150 158.6 0.0 349.0

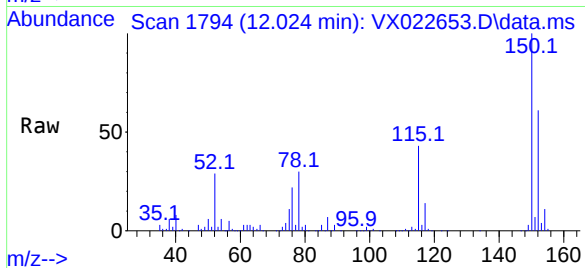

#76
1,2,3-Trichloropropane
Concen: 24.557 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 75 Resp: 27399
Ion Ratio Lower Upper
75 100
77 0.8 19.1 57.5#


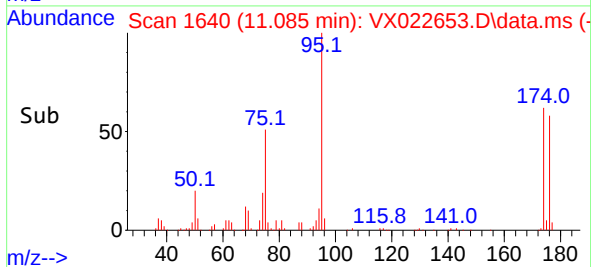

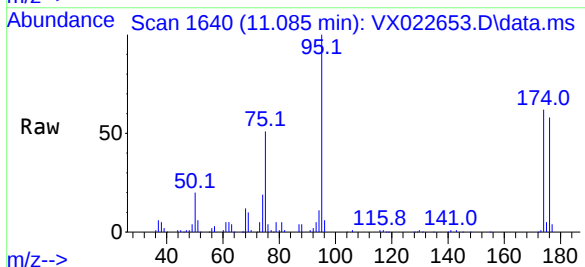




#81
trans-1,4-Dichloro-2-butene
Concen: 61.938 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16




Instrument :
MSVOA_X
ClientSampleId :
BUR-1041


Tgt Ion: 75 Resp: 27399
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

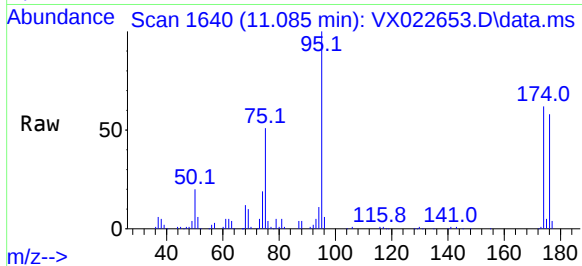

#84
1,2,4-Trimethylbenzene
Concen: 0.251 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 105 Resp: 734
Ion Ratio Lower Upper
105 100
120 37.7 22.4 67.3


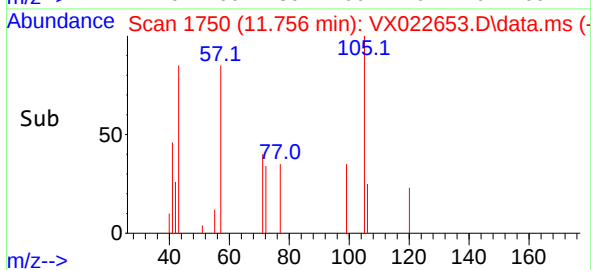

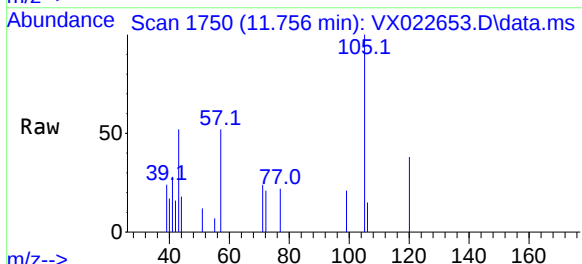




#85
 sec-Butylbenzene
 Concen: 0.206 ug/l
 RT: 11.896 min Scan# 1773
 Delta R.T. 0.000 min
 Lab File: VX022653.D
 Acq: 10 Jun 2021 19:16




Instrument :
 MSVOA_X
 ClientSampleId :
 BUR-1041


Tgt Ion:105 Resp: 728
 Ion Ratio Lower Upper
 105 100
 134 11.7 10.0 29.8

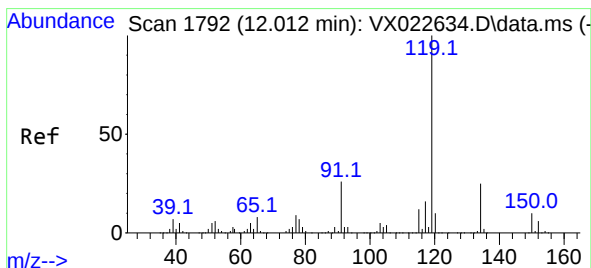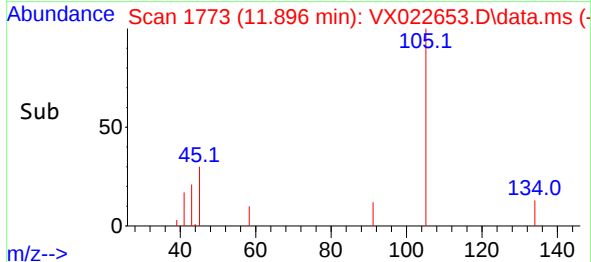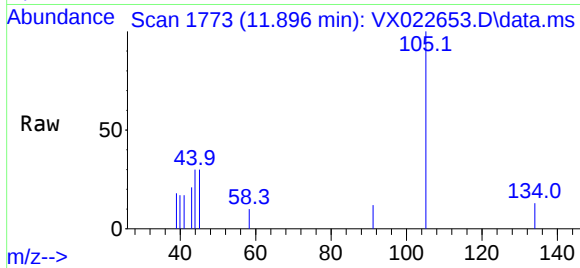

#86
 p-Isopropyltoluene
 Concen: 0.230 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.000 min
 Lab File: VX022653.D
 Acq: 10 Jun 2021 19:16

Tgt Ion:119 Resp: 671
 Ion Ratio Lower Upper
 119 100
 134 26.7 12.9 38.7
 91 53.8 11.7 35.0#

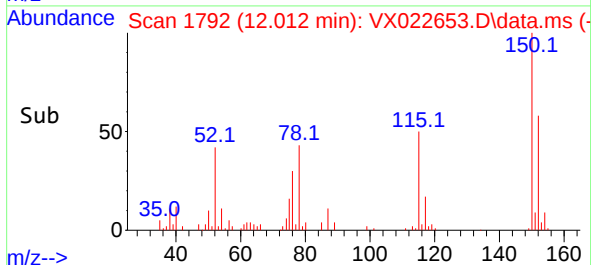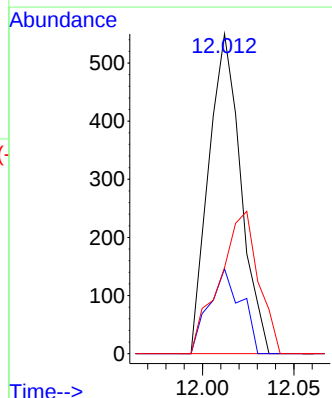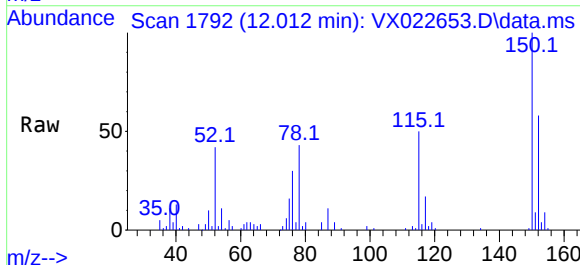







#87
1,3-Dichlorobenzene
Concen: 0.254 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Instrument :
MSVOA_X
ClientSampleId :
BUR-1041

Tgt Ion:146 Resp: 356




Ion	Ratio	Lower	Upper
146	100		
111	43.0	20.2	60.5
148	56.2	31.9	95.7

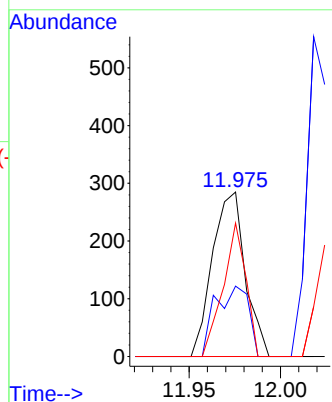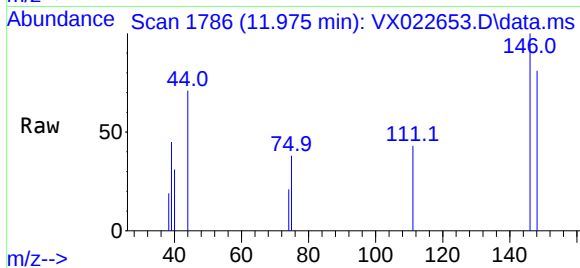


#88
1,4-Dichlorobenzene
Concen: 0.247 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.068 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion:146 Resp: 356

Ion	Ratio	Lower	Upper
146	100		
111	43.0	19.6	58.8
148	56.2	31.6	95.0

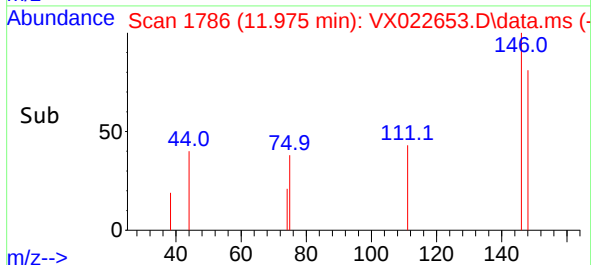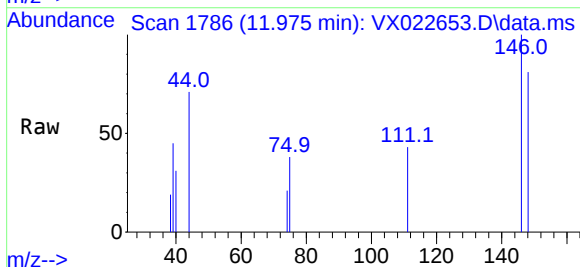







#89
n-Butylbenzene
Concen: 0.489 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Instrument :
MSVOA_X
ClientSampled :
BUR-1041

Tgt Ion: 91 Resp: 1364




Ion	Ratio	Lower	Upper
91	100		
92	45.3	27.4	82.0
134	20.3	13.2	39.5

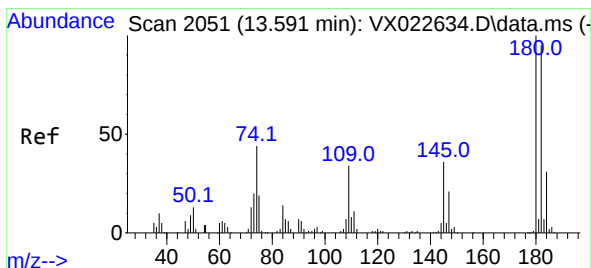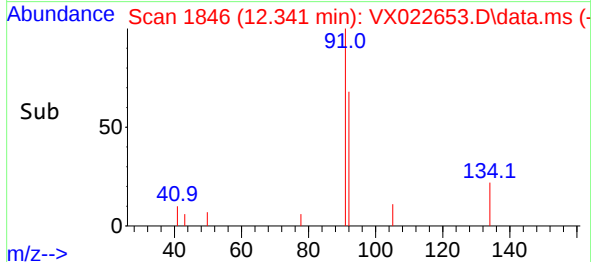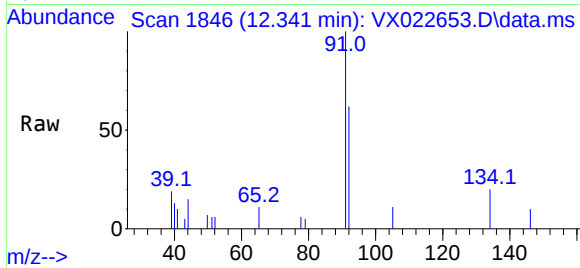


#93
1,2,4-Trichlorobenzene
Concen: 0.601 ug/l
RT: 13.597 min Scan# 2052
Delta R.T. 0.006 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

Tgt Ion: 180 Resp: 492


Ion	Ratio	Lower	Upper
180	100		
182	101.0	47.7	143.1
145	35.6	15.0	45.0

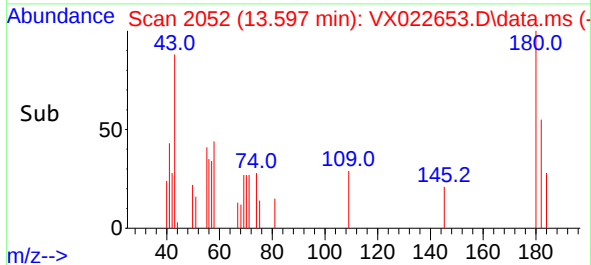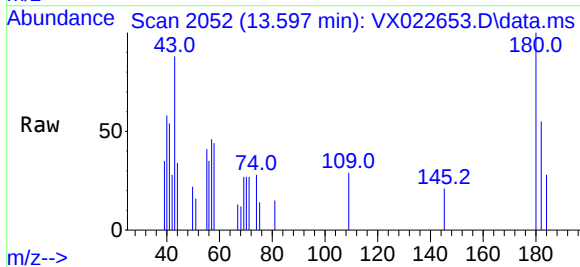






#94
Hexachlorobutadiene
Concen: 0.388 ug/l
RT: 13.731 min Scan# 2074
Delta R.T. 0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16


Instrument :
MSVOA_X
ClientSampled :
BUR-1041

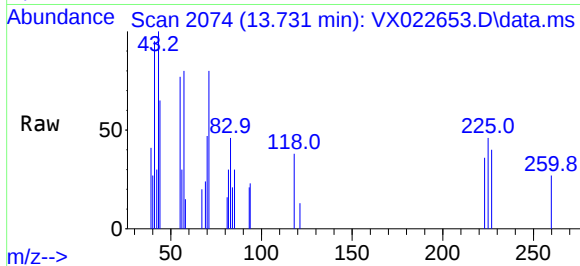



Tgt Ion:225 Resp: 114
Ion Ratio Lower Upper
225 100
223 119.3 31.1 93.2#
227 86.0 31.6 95.0




#95
Naphthalene
Concen: 1.857 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022653.D
Acq: 10 Jun 2021 19:16

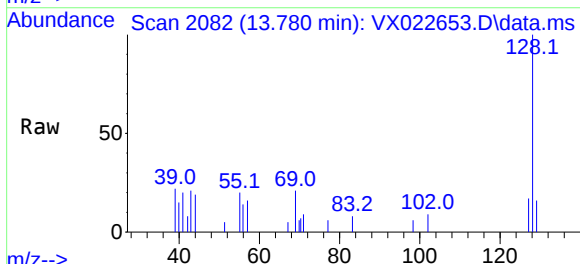


Tgt Ion:128 Resp: 1410
Ion Ratio Lower Upper
128 100
127 15.2 10.3 15.5
129 13.7 8.8 13.2#

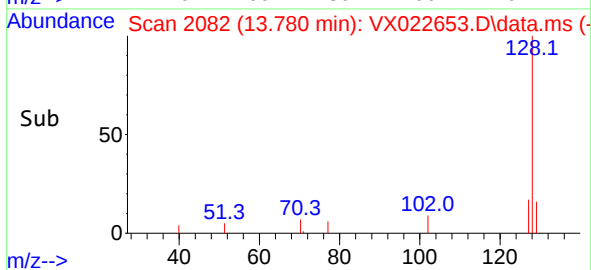



#96
 1,2,3-Trichlorobenzene
 Concen: 0.492 ug/l
 RT: 13.969 min Scan# 2113
 Delta R.T. 0.006 min
 Lab File: VX022653.D
 Acq: 10 Jun 2021 19:16

Instrument :
 MSVOA_X
 ClientSampleId :
 BUR-1041

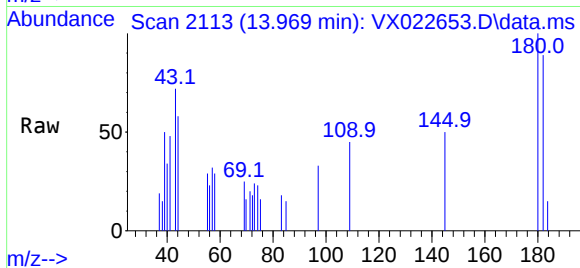

Tgt Ion:180 Resp: 393

Ion	Ratio	Lower	Upper
180	100		
182	94.7	47.6	142.9
145	45.5	16.1	48.3

