

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061021\
 Data File : VX022637.D
 Acq On : 10 Jun 2021 12:12
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
 Title : SW846 8260

Signal : TIC: VX022637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	33	rVB	4229	4225	1.15%	0.217%
2	1.563	73	78	84	rVB5	3513	5945	1.61%	0.305%
3	2.514	229	234	240	rBV3	2284	4467	1.21%	0.229%
4	2.953	300	306	314	rVB5	1993	4345	1.18%	0.223%
5	3.093	322	329	336	rVB5	2066	4269	1.16%	0.219%
6	4.593	564	575	584	rVB2	2355	7715	2.09%	0.396%
7	5.397	696	707	720	rBV	38785	109579	29.74%	5.627%
8	5.562	724	734	748	rVB2	65494	182959	49.66%	9.395%
9	5.964	790	800	812	rBV2	50359	132945	36.08%	6.827%
10	6.769	922	932	944	rBV2	112770	267038	72.48%	13.712%
11	7.385	1028	1033	1041	rVB5	1936	3987	1.08%	0.205%
12	8.653	1234	1241	1250	rBV	239978	368445	100.00%	18.920%
13	10.055	1466	1471	1484	rBV	226182	311835	84.64%	16.013%
14	10.305	1508	1512	1518	rBV2	4084	5076	1.38%	0.261%
15	11.085	1634	1640	1649	rBV	176988	219690	59.63%	11.281%
16	11.311	1671	1677	1680	rBV2	3046	3783	1.03%	0.194%
17	11.457	1697	1701	1705	rBV3	5189	6527	1.77%	0.335%
18	11.896	1769	1773	1777	rBV	3602	4434	1.20%	0.228%
19	11.975	1781	1786	1789	rBV2	2945	4144	1.12%	0.213%
20	12.024	1789	1794	1803	rVB	221637	272655	74.00%	14.001%
21	12.335	1841	1845	1849	rVB	7989	8951	2.43%	0.460%
22	13.591	2047	2051	2057	rVB	4587	5052	1.37%	0.259%
23	13.780	2077	2082	2086	rVB2	3894	4968	1.35%	0.255%
24	13.963	2109	2112	2116	rBV2	3719	4386	1.19%	0.225%


Sum of corrected areas: 1947420

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061021\
Data File : VX022637.D
Acq On : 10 Jun 2021 12:12
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

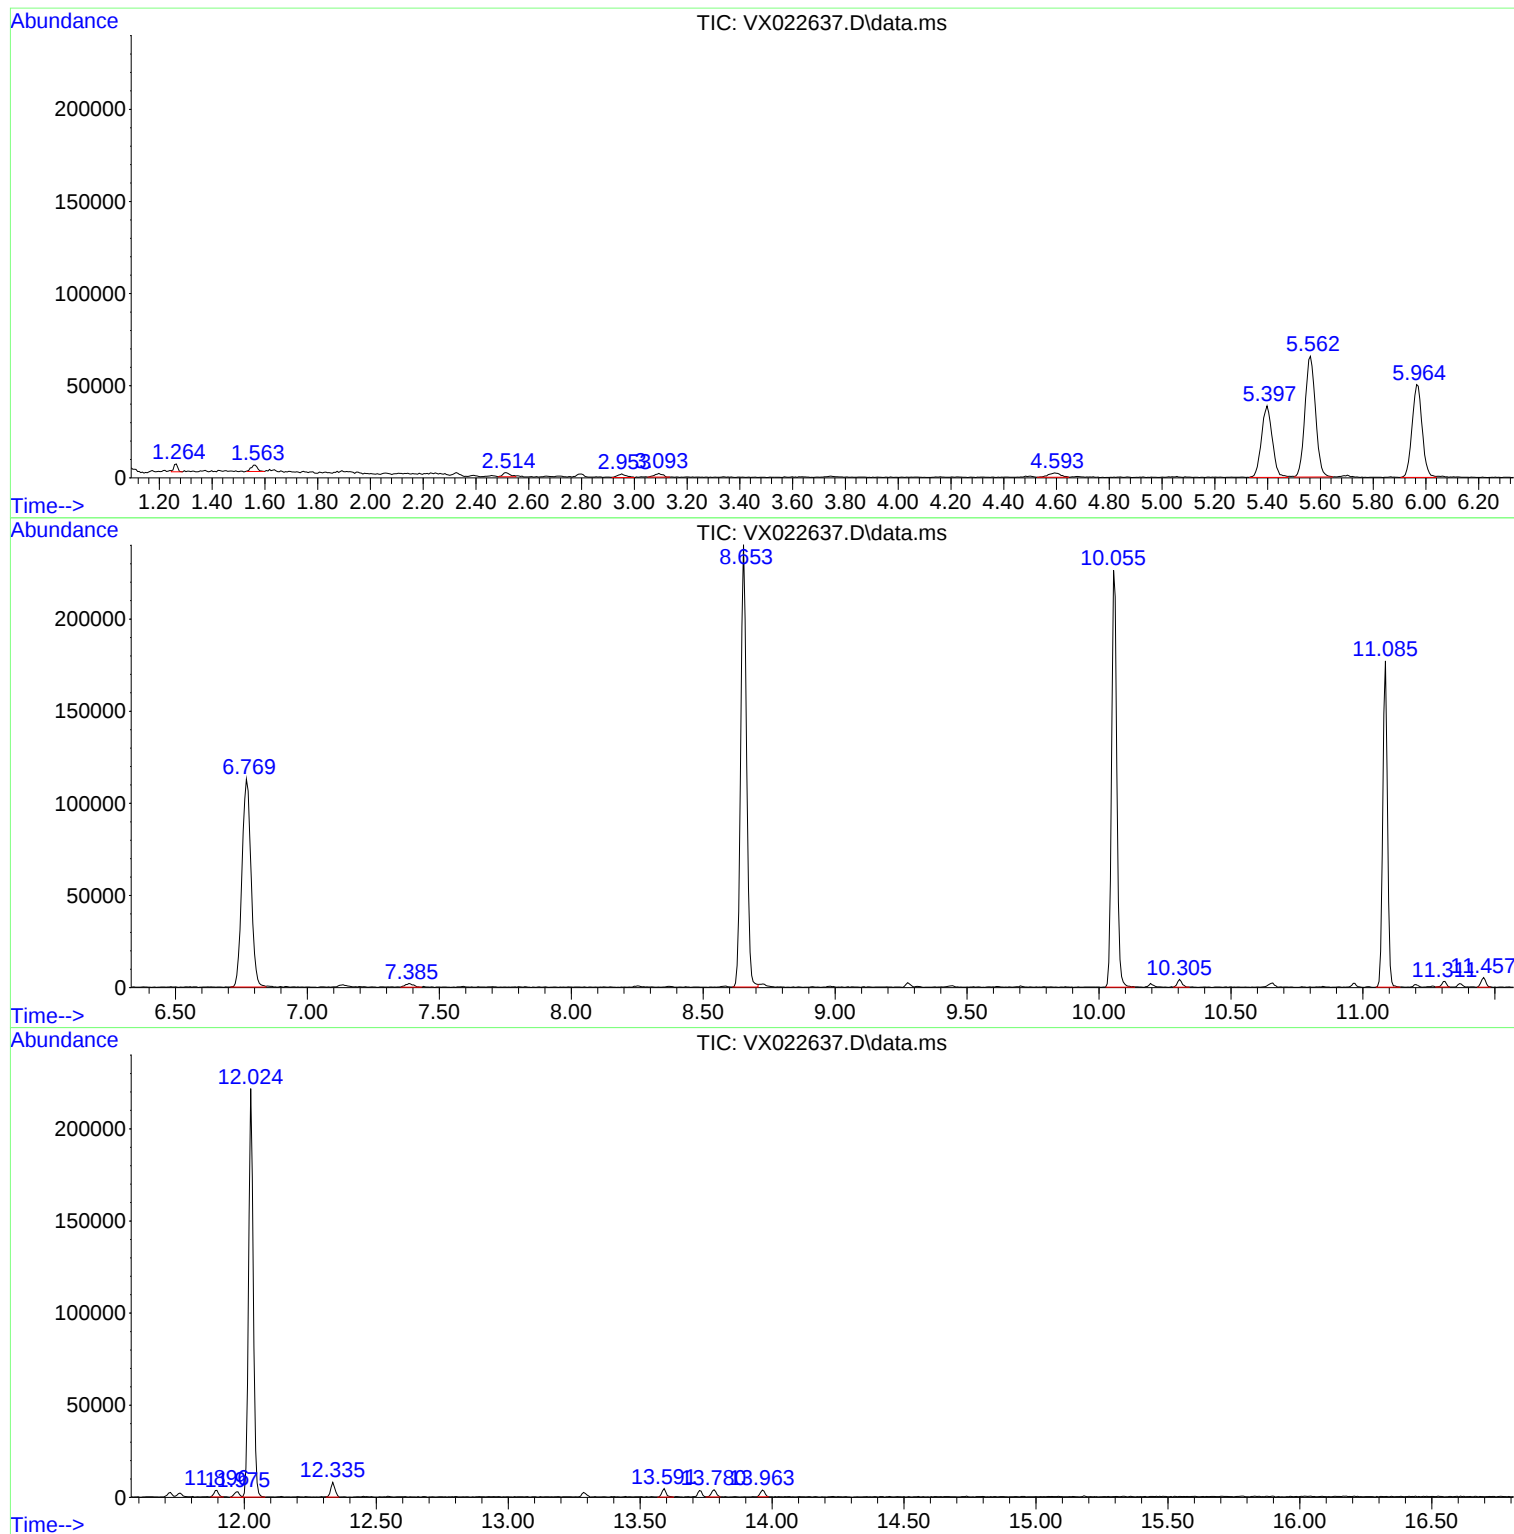

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061021\
Data File : VX022637.D
Acq On : 10 Jun 2021 12:12
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061021\
Data File : VX022637.D
Acq On : 10 Jun 2021 12:12
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
