


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061022\
 Data File : VX029361.D
 Acq On : 10 Jun 2022 09:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
 Title : SW846 8260
 Last Update : Wed Jun 08 03:00:38 2022

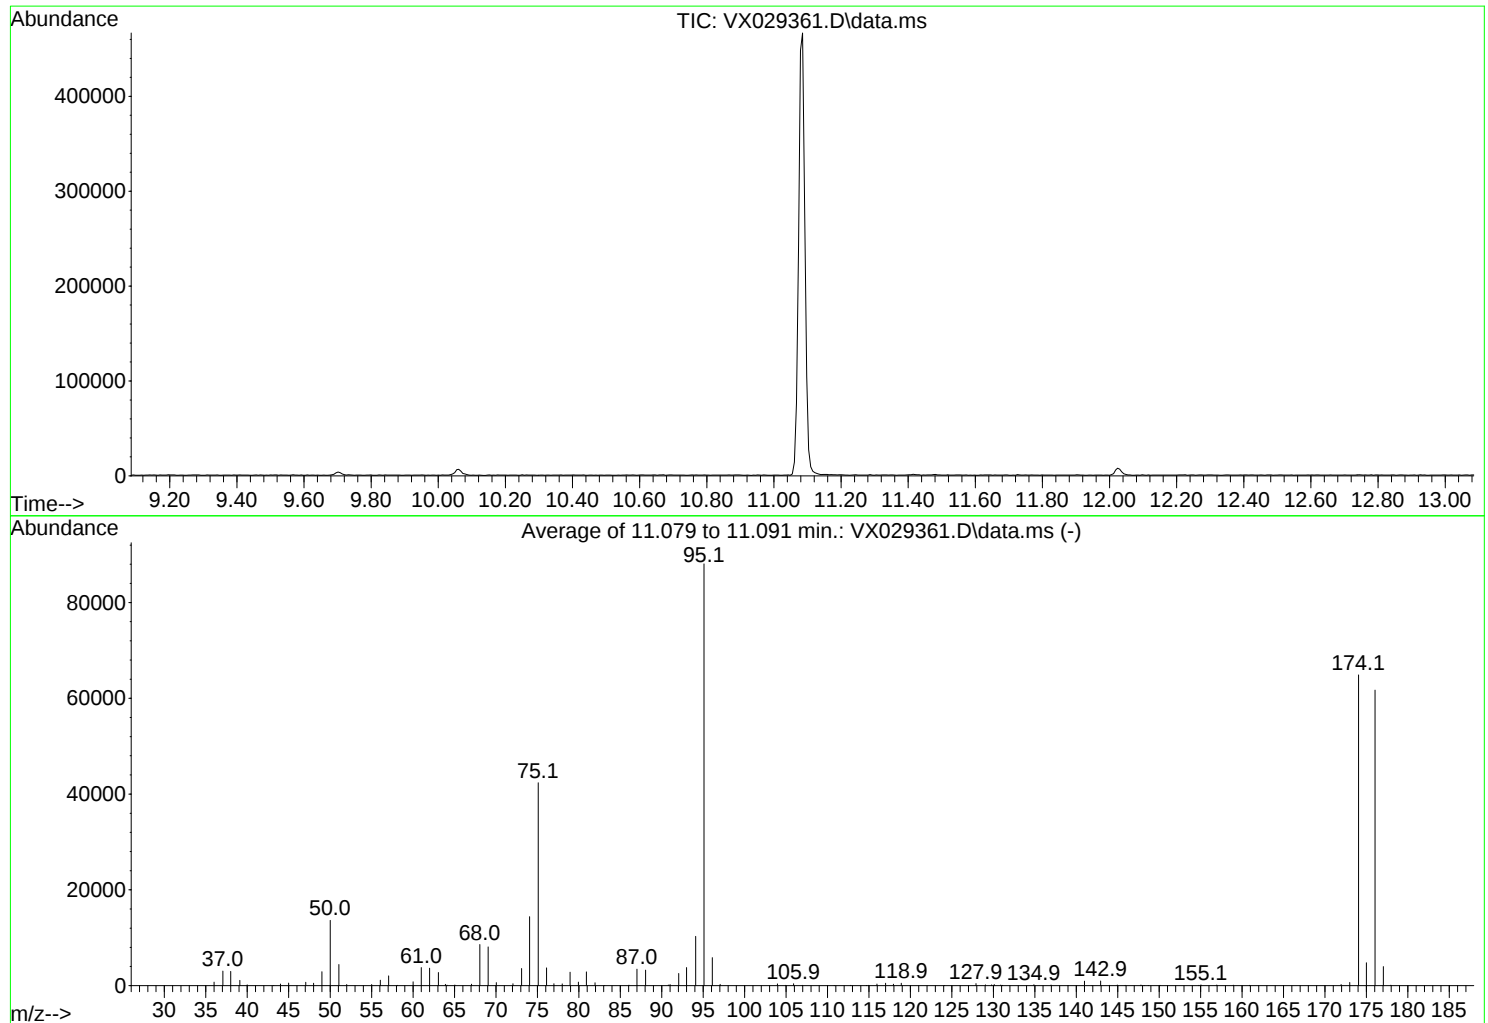

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	13643	PASS
75	95	30	60	48.1	42384	PASS
95	95	100	100	100.0	88085	PASS
96	95	5	9	6.6	5840	PASS
173	174	0.00	2	1.0	662	PASS
174	95	50	100	73.7	64899	PASS
175	174	5	9	7.3	4766	PASS
176	174	95	101	95.1	61720	PASS
177	176	5	9	6.5	3984	PASS