

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX061024\  
 Data File : VX041805.D  
 Acq On : 10 Jun 2024 13:12  
 Operator : JC/MD  
 Sample : P2796-03  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 STORAGE-BLANK-WATER-REF-4

Quant Time: Jun 11 03:47:36 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X052924W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu May 30 07:36:24 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon  | Response | Conc     | Units | Dev(Min) |
|-----------------------------|--------|-------|----------|----------|-------|----------|
| -----                       |        |       |          |          |       |          |
| Internal Standards          |        |       |          |          |       |          |
| 1) Pentafluorobenzene       | 5.550  | 168   | 143442   | 50.000   | ug/l  | # 0.00   |
| 34) 1,4-Difluorobenzene     | 6.763  | 114   | 223297   | 50.000   | ug/l  | 0.00     |
| 63) Chlorobenzene-d5        | 10.055 | 117   | 222787   | 50.000   | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4  | 12.024 | 152   | 109233   | 50.000   | ug/l  | 0.00     |
| System Monitoring Compounds |        |       |          |          |       |          |
| 33) 1,2-Dichloroethane-d4   | 5.952  | 65    | 84866    | 48.239   | ug/l  | 0.00     |
| Spiked Amount               | 50.000 | Range | 78 - 117 | Recovery | =     | 96.480%  |
| 35) Dibromofluoromethane    | 5.385  | 113   | 70471    | 45.646   | ug/l  | 0.00     |
| Spiked Amount               | 50.000 | Range | 75 - 124 | Recovery | =     | 91.300%  |
| 50) Toluene-d8              | 8.647  | 98    | 267773   | 49.639   | ug/l  | 0.00     |
| Spiked Amount               | 50.000 | Range | 92 - 112 | Recovery | =     | 99.280%  |
| 62) 4-Bromofluorobenzene    | 11.079 | 95    | 98816    | 49.632   | ug/l  | 0.00     |
| Spiked Amount               | 50.000 | Range | 83 - 123 | Recovery | =     | 99.260%  |


|                  |        |
|------------------|--------|
| Target Compounds | Qvalue |
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX061024\  
Data File : VX041805.D  
Acq On : 10 Jun 2024 13:12  
Operator : JC/MD  
Sample : P2796-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
STORAGE-BLANK-WATER-REF-4

Quant Time: Jun 11 03:47:36 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X052924W.M  
Quant Title : SW846 8260  
QLast Update : Thu May 30 07:36:24 2024  
Response via : Initial Calibration




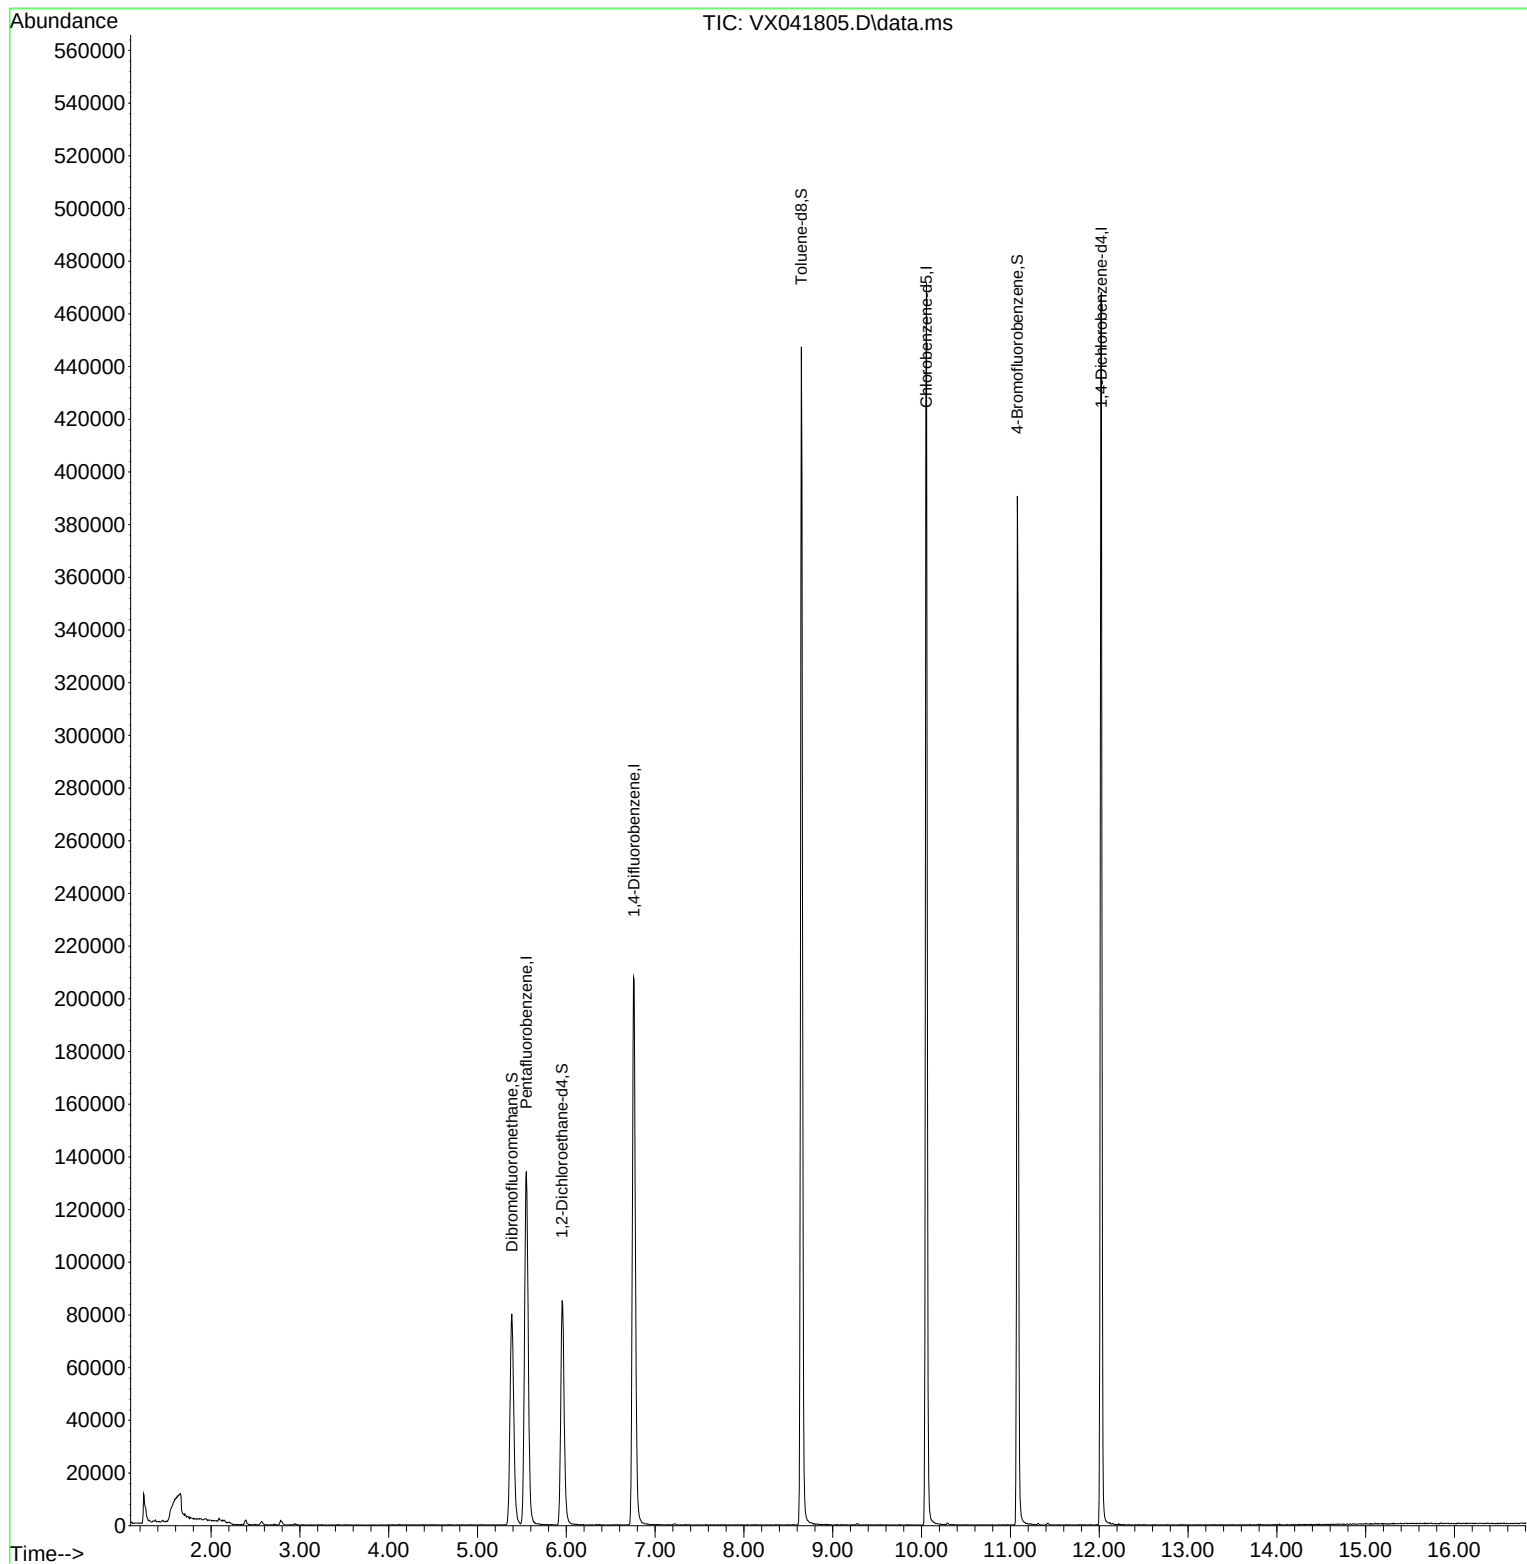


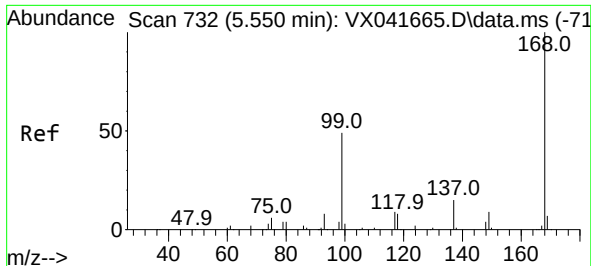

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 732  
Delta R.T. -0.000 min  
Lab File: VX041805.D  
Acq: 10 Jun 2024 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 143442  
Ion Ratio Lower Upper  
168 100  
99 50.9 56.6 85.0#

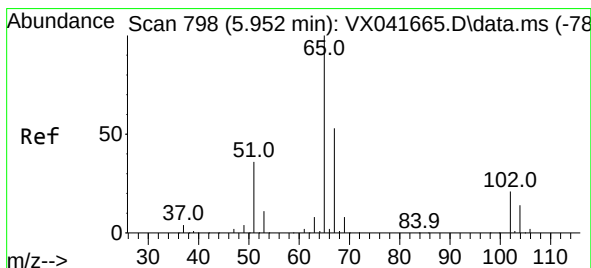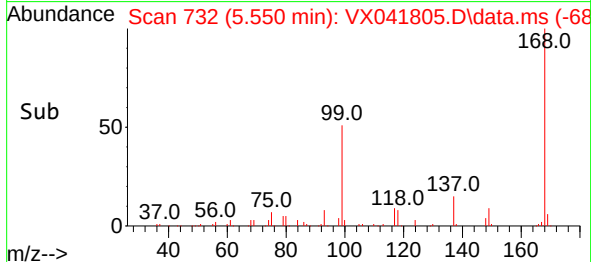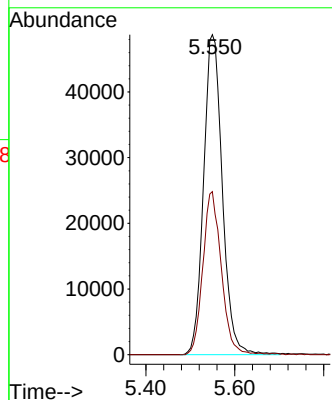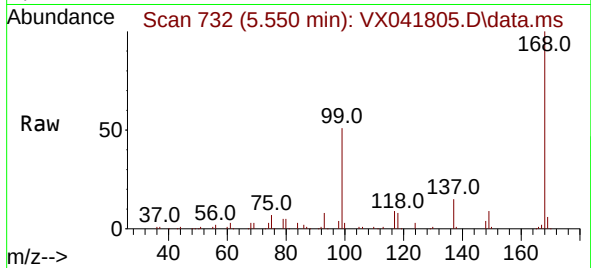

#33  
1,2-Dichloroethane-d4  
Concen: 48.239 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. 0.000 min  
Lab File: VX041805.D  
Acq: 10 Jun 2024 13:12

Tgt Ion: 65 Resp: 84866  
Ion Ratio Lower Upper  
65 100  
67 52.2 0.0 100.2


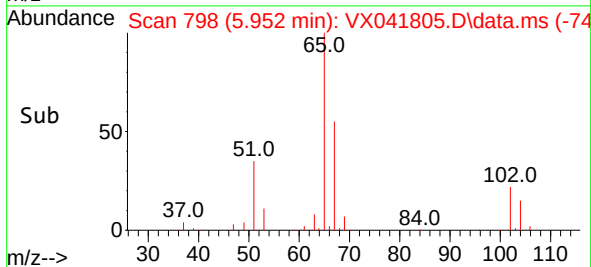
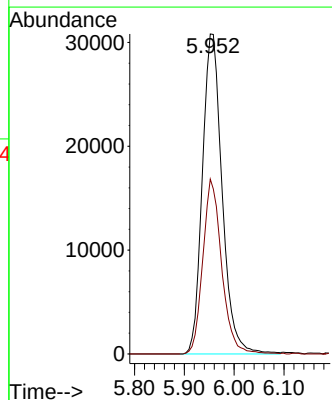
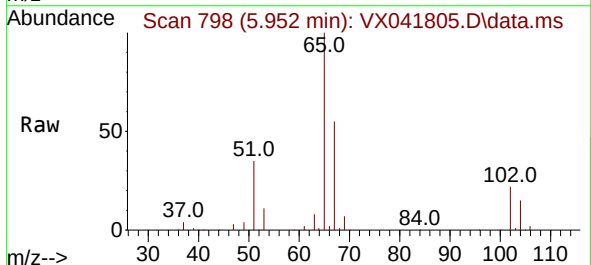


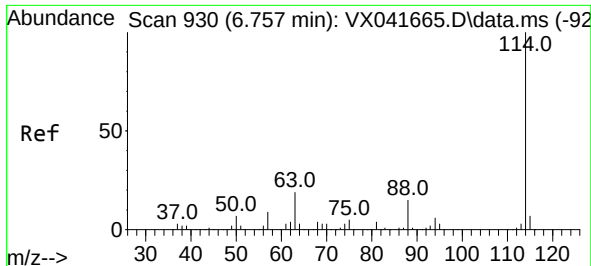

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 911  
Delta R.T. 0.006 min  
Lab File: VX041805.D  
Acq: 10 Jun 2024 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 223297  
Ion Ratio Lower Upper  
114 100  
63 19.0 0.0 45.0  
88 14.7 0.0 36.6

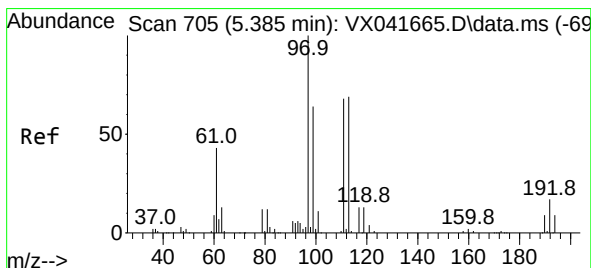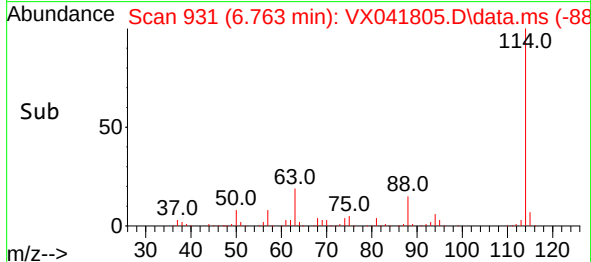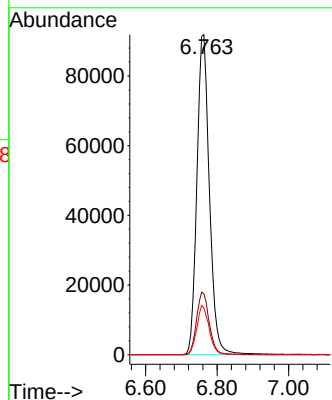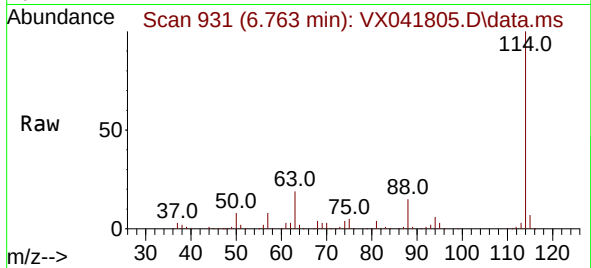

#35  
Dibromofluoromethane  
Concen: 45.646 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.000 min  
Lab File: VX041805.D  
Acq: 10 Jun 2024 13:12

Tgt Ion:113 Resp: 70471  
Ion Ratio Lower Upper  
113 100  
111 101.5 82.9 124.3  
192 23.5 13.3 19.9#


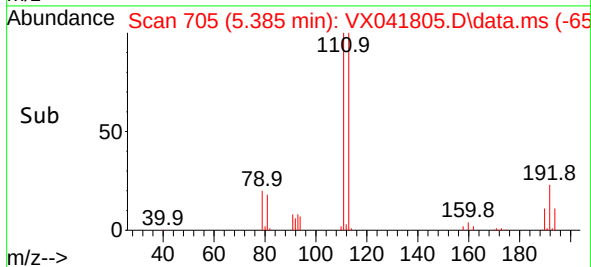
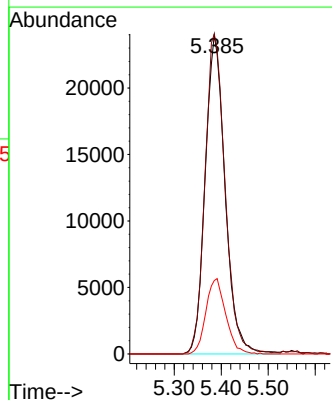
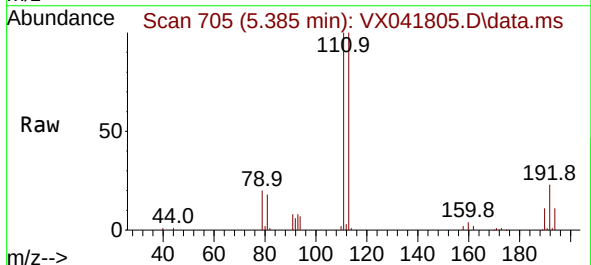


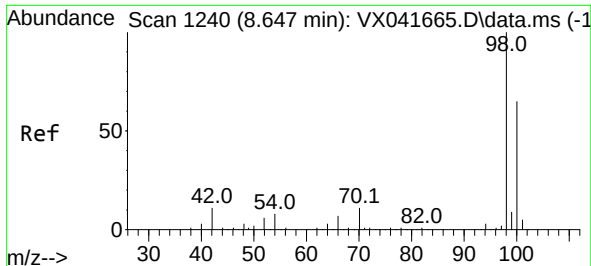

#50  
Toluene-d8  
Concen: 49.639 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX041805.D  
Acq: 10 Jun 2024 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 267773  
Ion Ratio Lower Upper  
98 100  
100 65.8 53.1 79.7

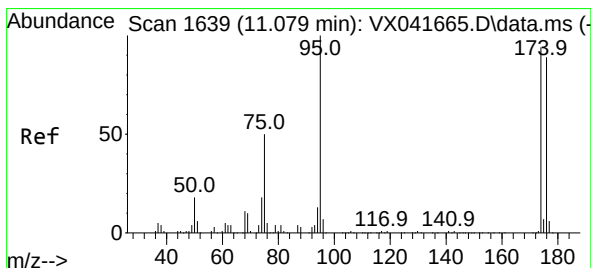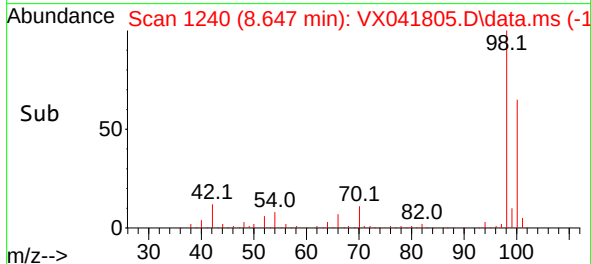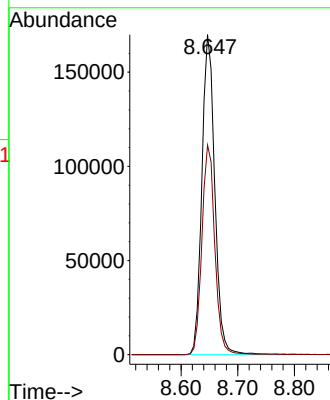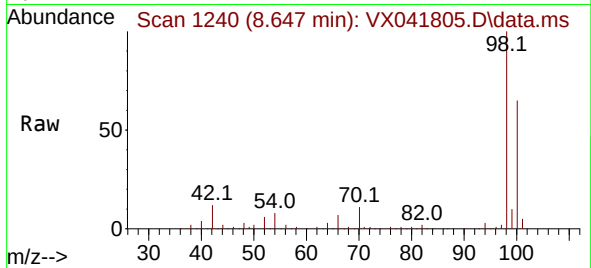

#62  
4-Bromofluorobenzene  
Concen: 49.632 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.000 min  
Lab File: VX041805.D  
Acq: 10 Jun 2024 13:12

Tgt Ion: 95 Resp: 98816  
Ion Ratio Lower Upper  
95 100  
174 95.9 0.0 135.6  
176 91.7 0.0 131.0

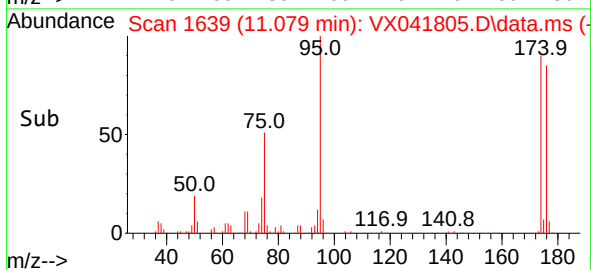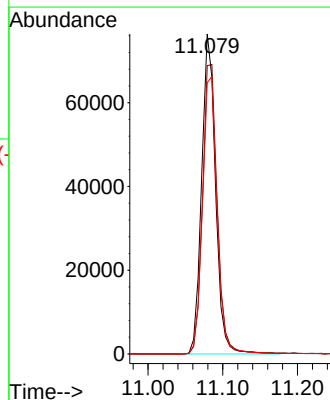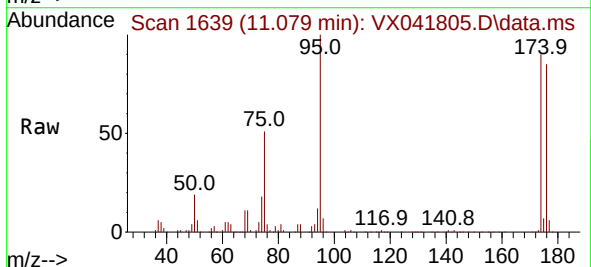

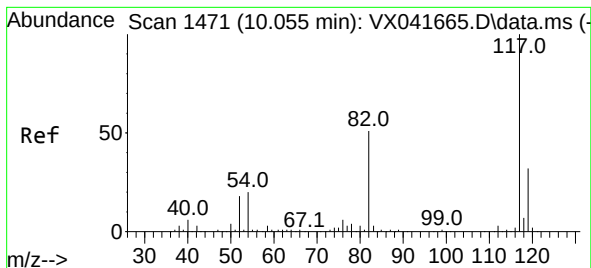

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX041805.D

Acq: 10 Jun 2024 13:12

Instrument :

MSVOA\_X

ClientSampleId :

STORAGE-BLANK-WATER-REF-4





Tgt Ion:117 Resp: 222787

Ion Ratio Lower Upper

117 100

82 51.3 46.2 69.4

119 32.3 25.5 38.3

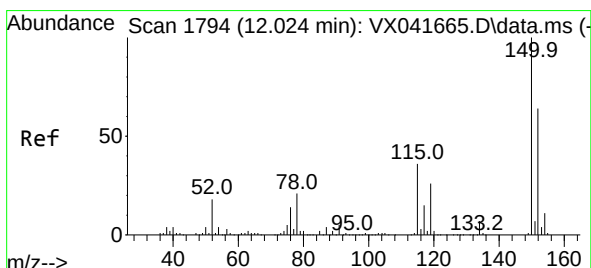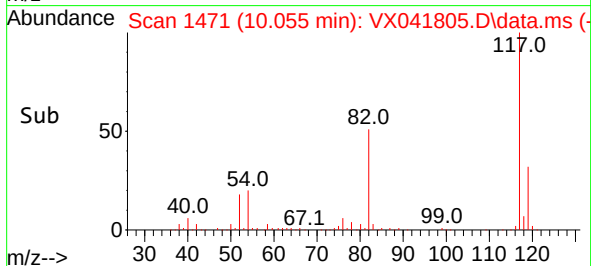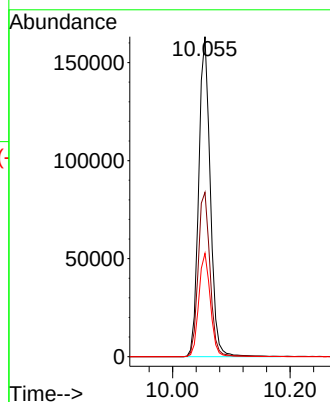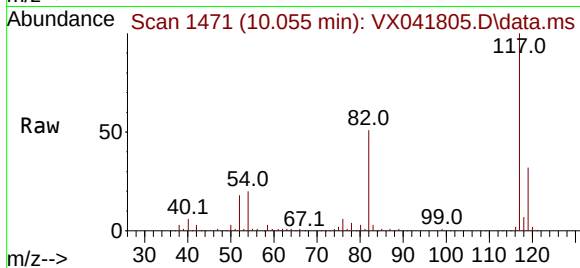

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX041805.D

Acq: 10 Jun 2024 13:12

Tgt Ion:152 Resp: 109233

Ion Ratio Lower Upper

152 100

115 53.8 43.3 129.9

150 154.8 0.0 345.0

