

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061024\
 Data File : VX041807.D
 Acq On : 10 Jun 2024 13:58
 Operator : JC/MD
 Sample : P2767-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRIP-BLANK

Quant Time: Jun 11 03:48:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 30 07:36:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	146453	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	229360	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	225249	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	111856	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	89327	49.731	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	99.460%
35) Dibromofluoromethane	5.391	113	73105	46.100	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.200%
50) Toluene-d8	8.647	98	272132	49.113	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.220%
62) 4-Bromofluorobenzene	11.079	95	101747	49.753	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061024\
Data File : VX041807.D
Acq On : 10 Jun 2024 13:58
Operator : JC/MD
Sample : P2767-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Quant Time: Jun 11 03:48:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260
QLast Update : Thu May 30 07:36:24 2024
Response via : Initial Calibration




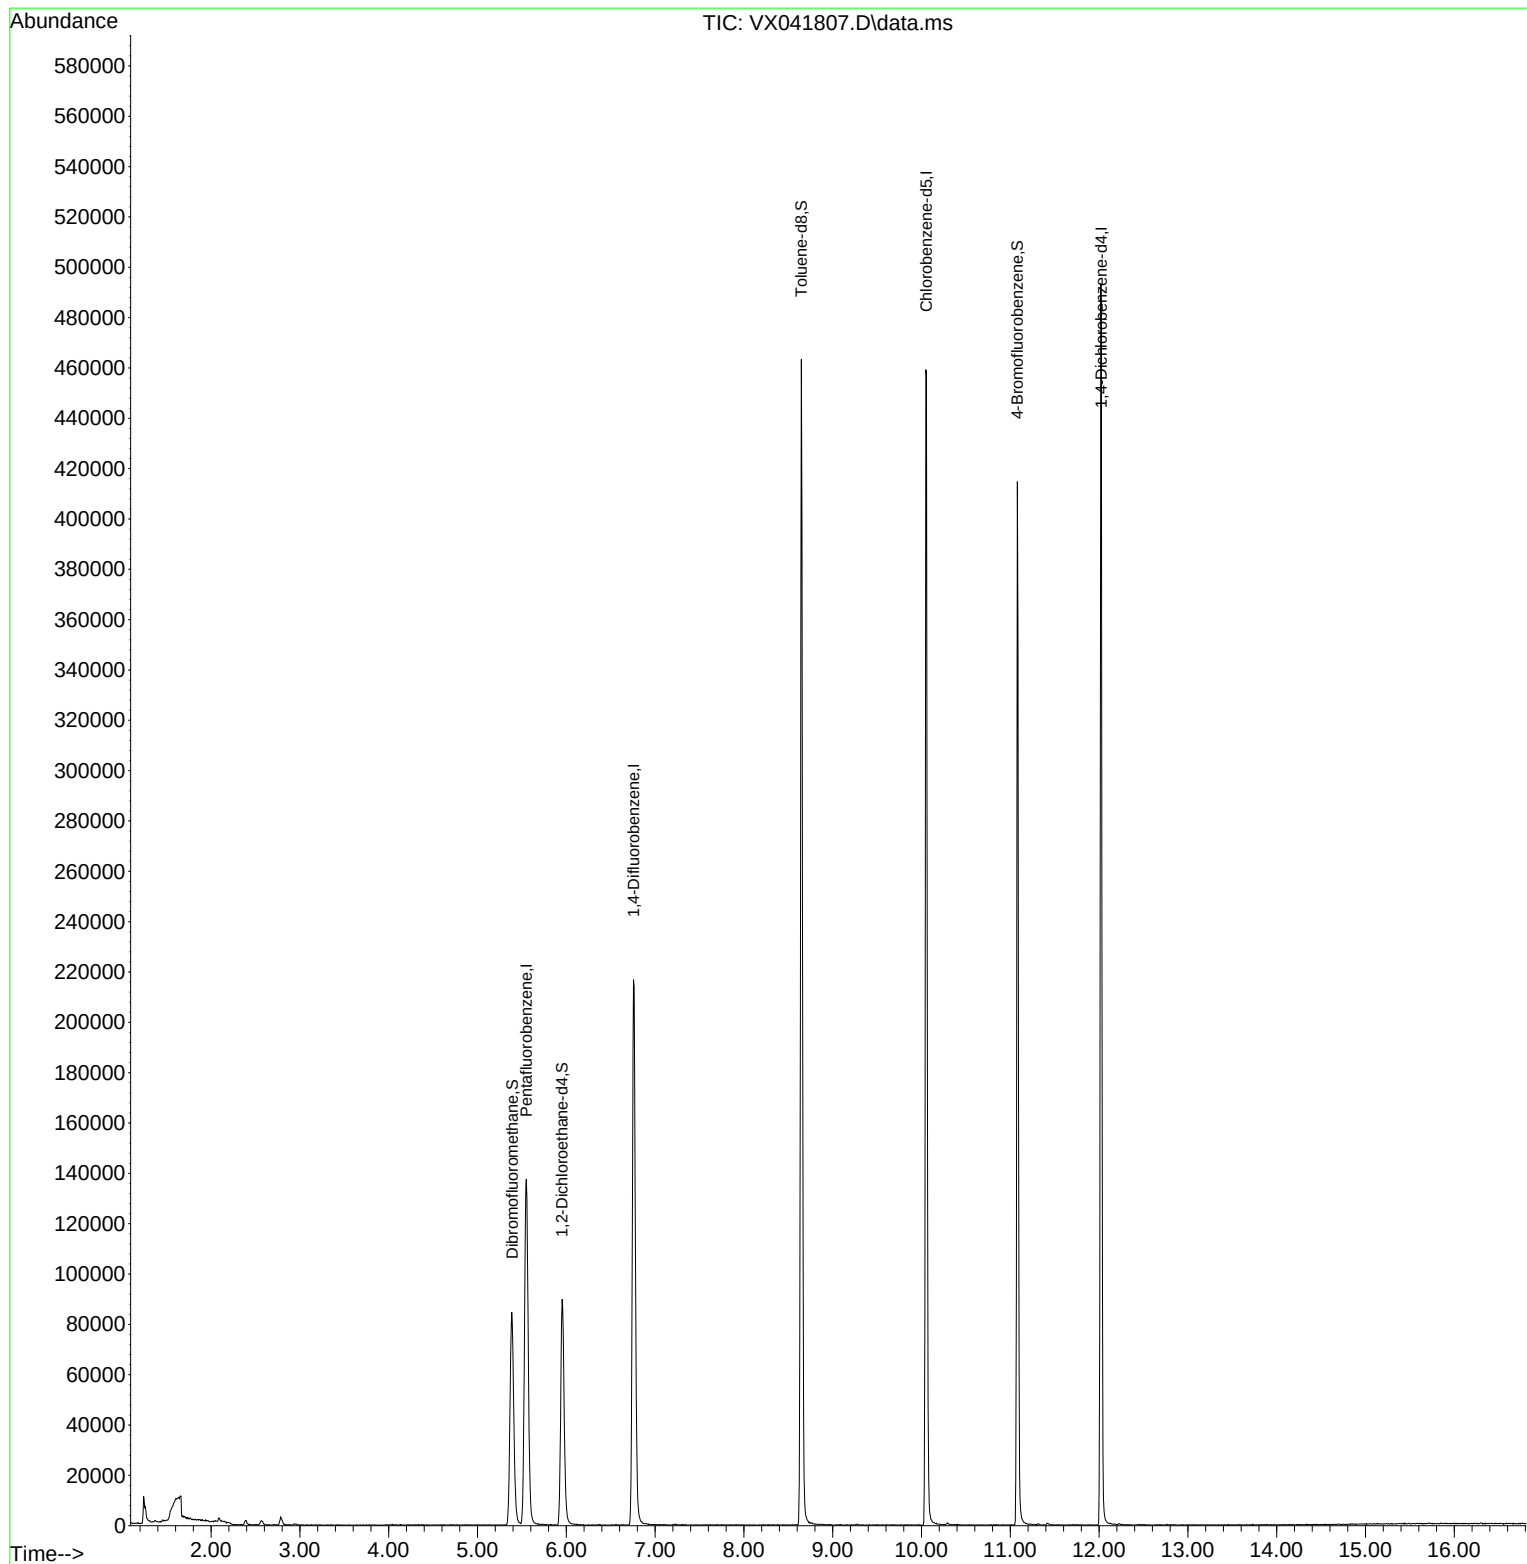


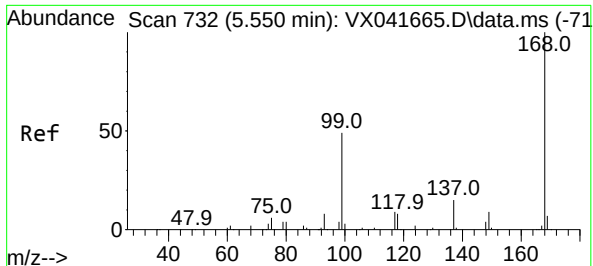

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041807.D
Acq: 10 Jun 2024 13:58




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tgt Ion:168 Resp: 146453
Ion Ratio Lower Upper
168 100
99 51.3 56.6 85.0#

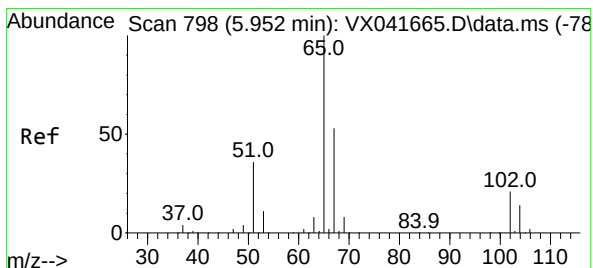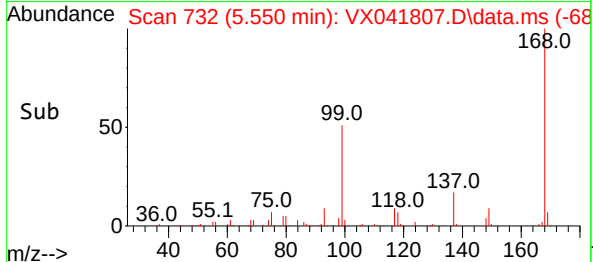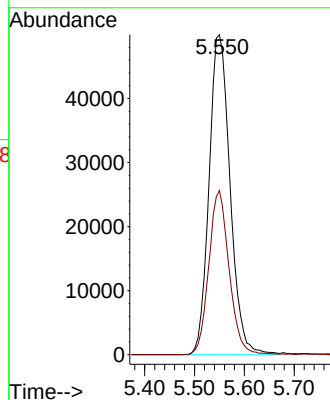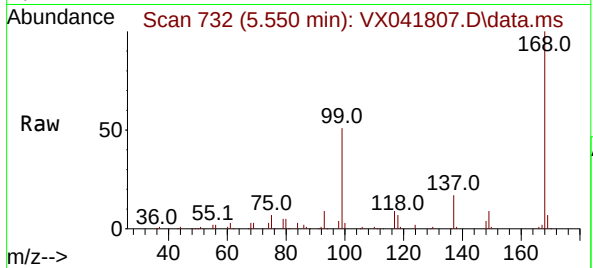

#33
1,2-Dichloroethane-d4
Concen: 49.731 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX041807.D
Acq: 10 Jun 2024 13:58

Tgt Ion: 65 Resp: 89327
Ion Ratio Lower Upper
65 100
67 51.2 0.0 100.2


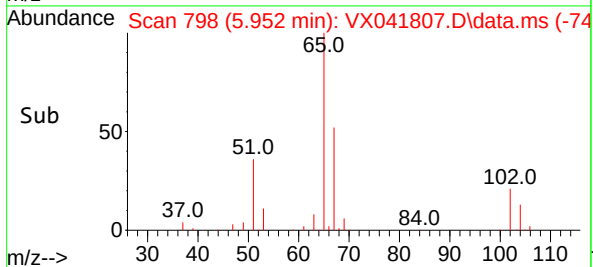
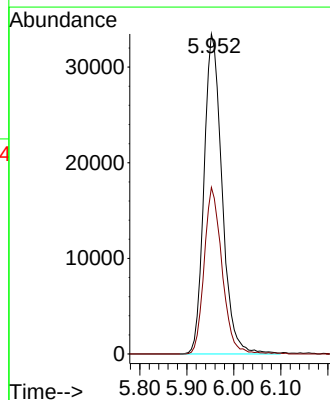
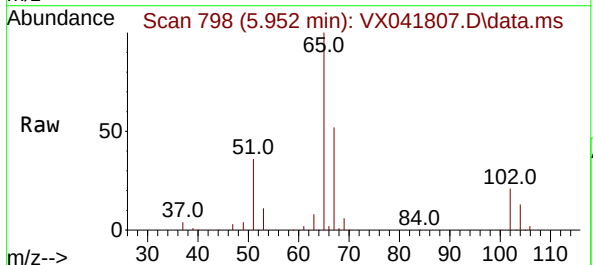


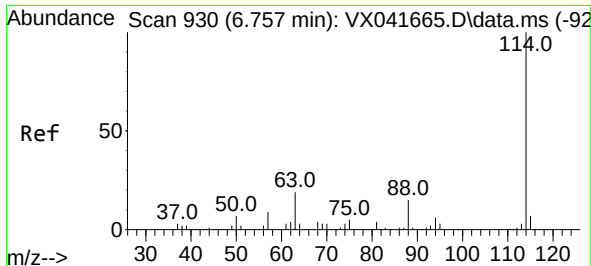

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX041807.D
Acq: 10 Jun 2024 13:58




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tgt Ion:114 Resp: 229360
Ion Ratio Lower Upper
114 100
63 20.0 0.0 45.0
88 15.5 0.0 36.6

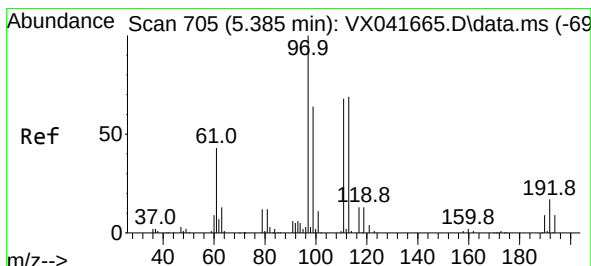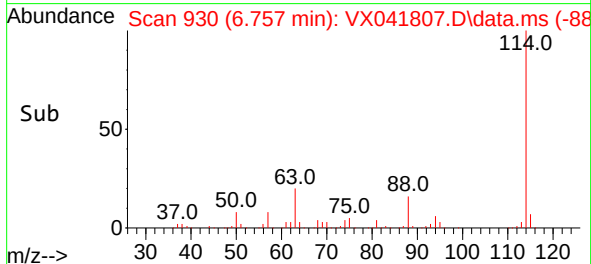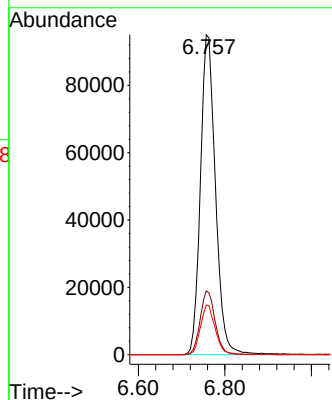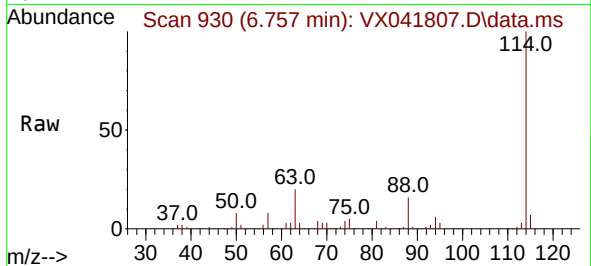

#35
Dibromofluoromethane
Concen: 46.100 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX041807.D
Acq: 10 Jun 2024 13:58

Tgt Ion:113 Resp: 73105
Ion Ratio Lower Upper
113 100
111 103.4 82.9 124.3
192 24.5 13.3 19.9#


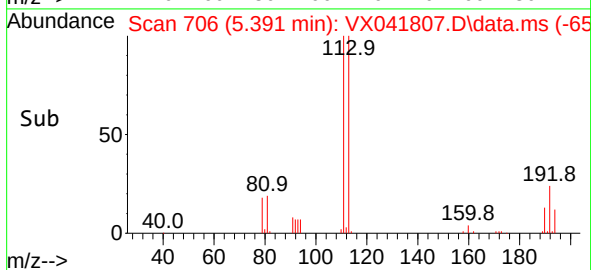
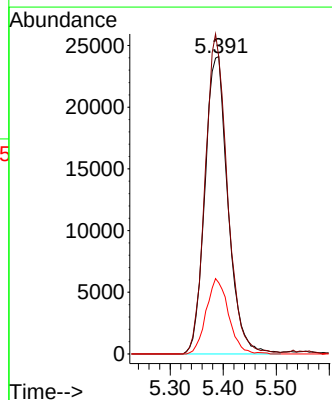
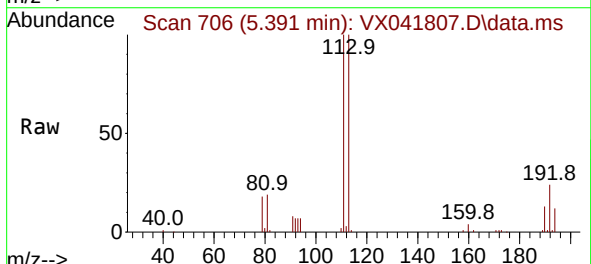


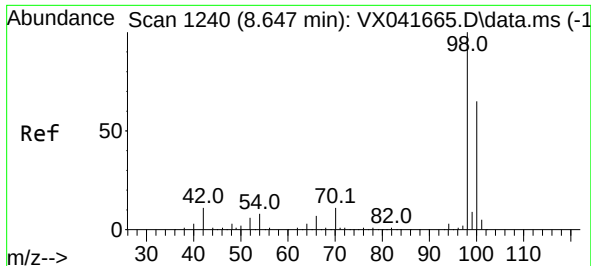

#50
Toluene-d8
Concen: 49.113 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX041807.D
Acq: 10 Jun 2024 13:58




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tgt Ion: 98 Resp: 272132
Ion Ratio Lower Upper
98 100
100 66.4 53.1 79.7

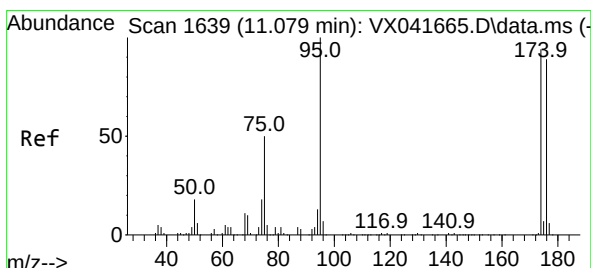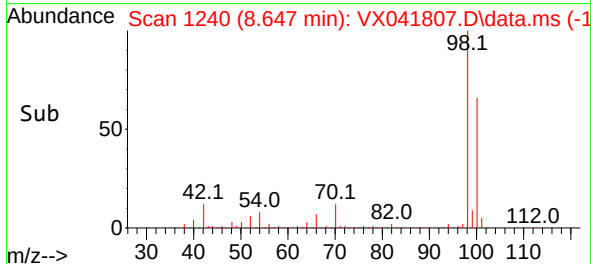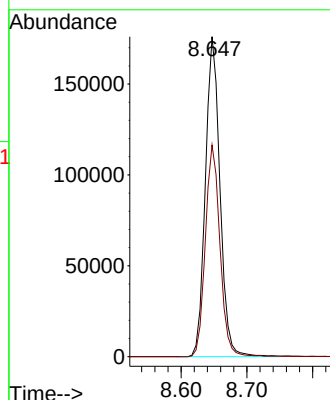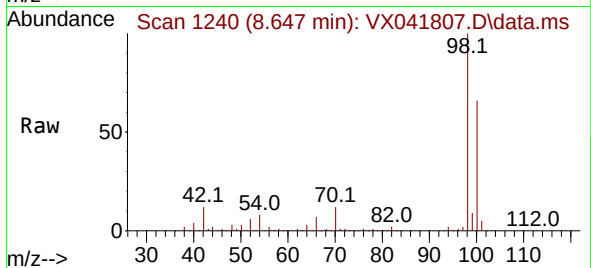

#62
4-Bromofluorobenzene
Concen: 49.753 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX041807.D
Acq: 10 Jun 2024 13:58

Tgt Ion: 95 Resp: 101747
Ion Ratio Lower Upper
95 100
174 95.4 0.0 135.6
176 91.9 0.0 131.0


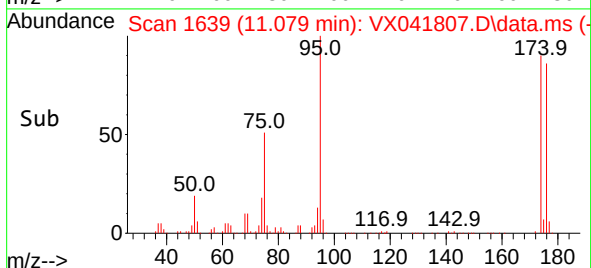
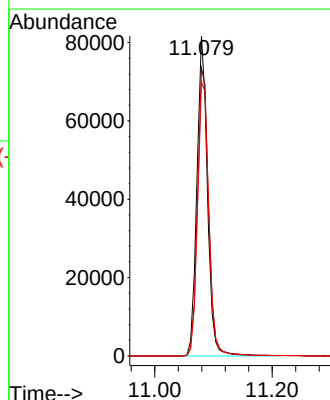
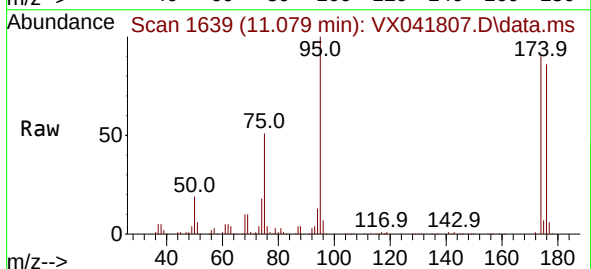


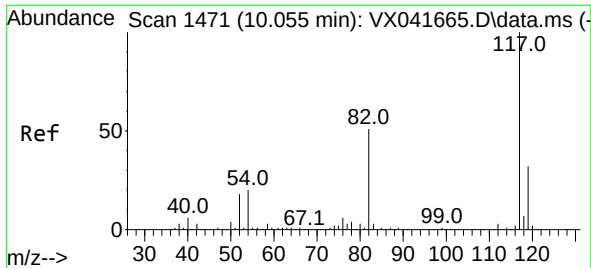

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX041807.D
Acq: 10 Jun 2024 13:58

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Tgt Ion:117 Resp: 225249
Ion Ratio Lower Upper
117 100
82 51.2 46.2 69.4
119 31.8 25.5 38.3

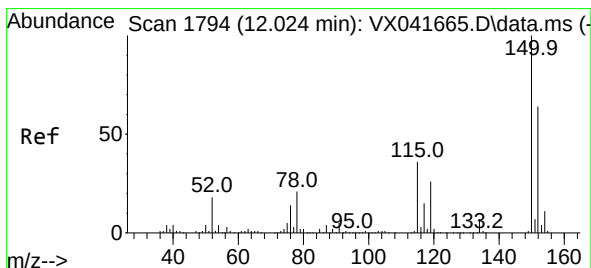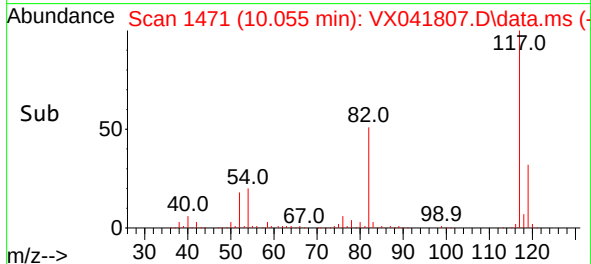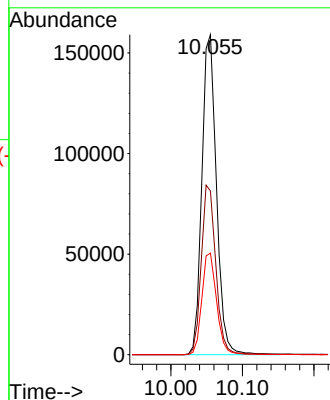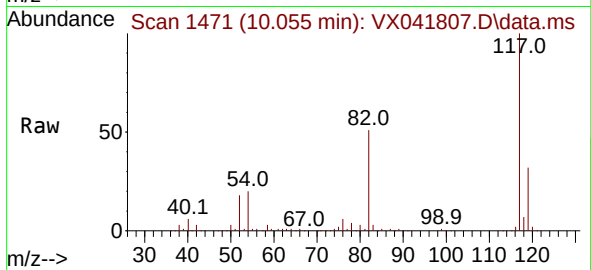

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX041807.D
Acq: 10 Jun 2024 13:58

Tgt Ion:152 Resp: 111856
Ion Ratio Lower Upper
152 100
115 54.5 43.3 129.9
150 157.3 0.0 345.0

