

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061024\
 Data File : VX041810.D
 Acq On : 10 Jun 2024 15:08
 Operator : JC/MD
 Sample : P2767-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-2A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
 Title : SW846 8260

Signal : TIC: VX041810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV2	9505	16839	2.54%	0.435%
2	1.612	69	86	87	rBV8	8673	33814	5.10%	0.873%
3	1.721	100	104	111	rVB	11531	15924	2.40%	0.411%
4	2.776	270	277	286	rBV4	5330	14536	2.19%	0.375%
5	3.093	320	329	337	rBV2	4905	11181	1.69%	0.289%
6	5.385	694	705	722	rBV2	78425	233205	35.16%	6.018%
7	5.550	722	732	749	rVB2	128021	367302	55.38%	9.479%
8	5.952	789	798	816	rBV	81751	222597	33.56%	5.744%
9	6.757	921	930	947	rBV	198244	481708	72.63%	12.431%
10	8.647	1234	1240	1255	rVB	431558	663233	100.00%	17.116%
11	10.055	1465	1471	1488	rBV	442379	619488	93.40%	15.987%
12	11.079	1634	1639	1656	rBV	377065	495018	74.64%	12.775%
13	11.890	1770	1772	1778	rVB2	7340	7865	1.19%	0.203%
14	12.024	1788	1794	1803	rBV	456956	601228	90.65%	15.515%
15	12.244	1823	1830	1838	rBV2	18227	24782	3.74%	0.640%
16	12.646	1893	1896	1900	rVB3	5582	7036	1.06%	0.182%
17	12.701	1900	1905	1912	rVB	16713	21326	3.22%	0.550%
18	13.030	1955	1959	1967	rVB	5816	7282	1.10%	0.188%
19	13.640	2052	2059	2060	rVV2	8623	13526	2.04%	0.349%
20	13.664	2060	2063	2069	rVB	13422	17137	2.58%	0.442%




Sum of corrected areas: 3875027

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061024\
Data File : VX041810.D
Acq On : 10 Jun 2024 15:08
Operator : JC/MD
Sample : P2767-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

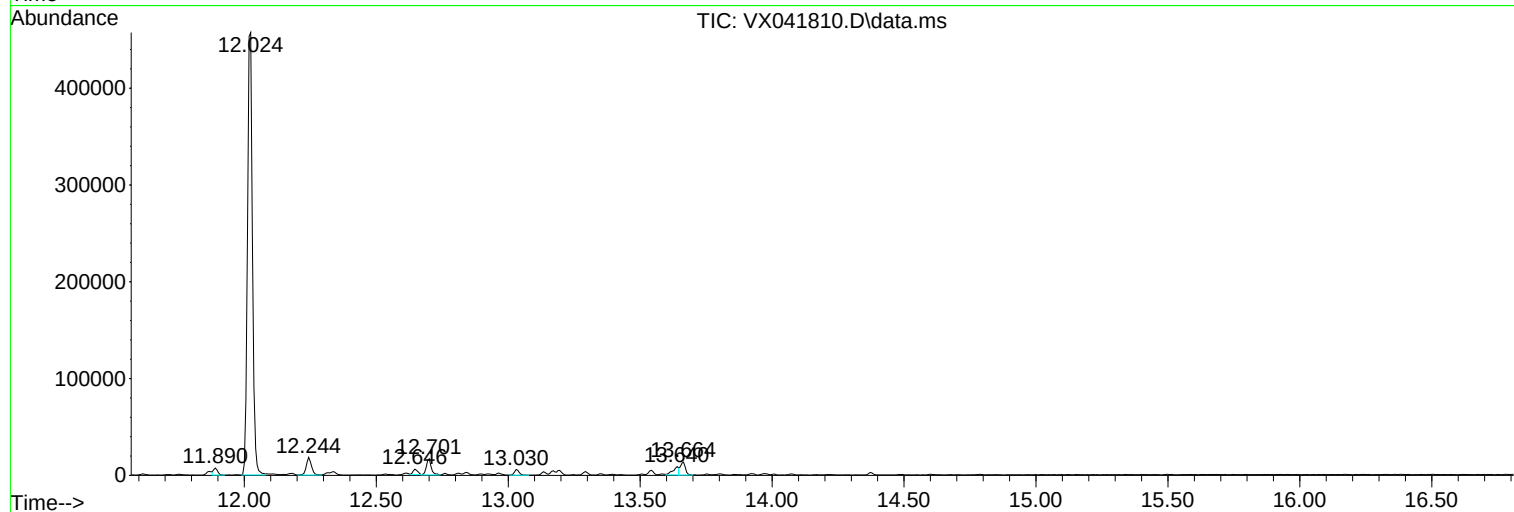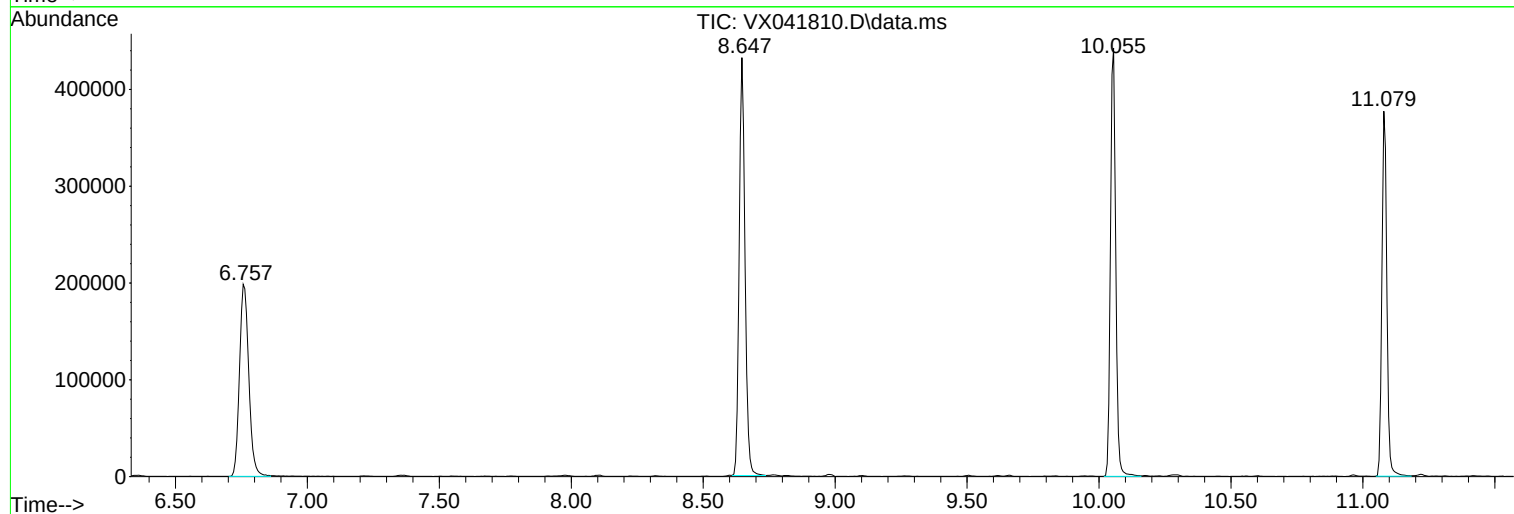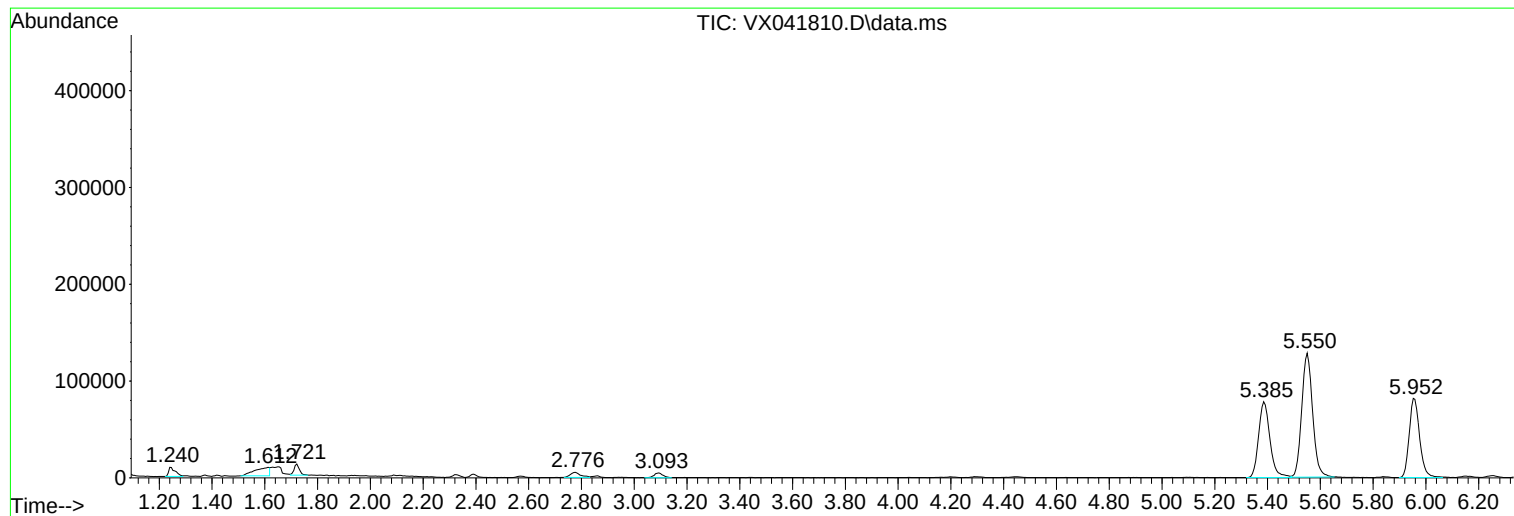

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061024\
Data File : VX041810.D
Acq On : 10 Jun 2024 15:08
Operator : JC/MD
Sample : P2767-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061024\
Data File : VX041810.D
Acq On : 10 Jun 2024 15:08
Operator : JC/MD
Sample : P2767-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------