

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046601.D
 Acq On : 10 Jun 2025 14:38
 Operator : JC/MD
 Sample : Q2230-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-MW901-060425

Quant Time: Jun 11 01:48:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	112231	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	225068	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	232456	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	116598	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	100300	50.233	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 100.460%			
35) Dibromofluoromethane	5.397	113	82652	49.936	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.880%			
50) Toluene-d8	8.653	98	296387	54.315	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 108.640%			
62) 4-Bromofluorobenzene	11.079	95	125497	55.586	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 111.180%			
Target Compounds						Qvalue
3) Chloromethane	1.307	50	454	0.320	ug/l #	86
16) Acetone	2.392	43	37286	51.274	ug/l	93
17) Carbon Disulfide	2.532	76	224	0.281	ug/l #	76
18) Methyl Acetate	2.538	43	1206	0.507	ug/l #	55
25) 2-Butanone	4.580	43	9330	8.394	ug/l	97
28) Bromochloromethane	5.105	49	636	0.464	ug/l #	17
30) Chloroform	5.111	83	8181	2.715	ug/l	100
31) Cyclohexane	5.489	56	1114	0.480	ug/l	91
36) 1,1-Dichloropropene	5.568	75	10698	4.525	ug/l #	52
38) Carbon Tetrachloride	5.568	117	13063	4.933	ug/l #	16
39) Methylcyclohexane	7.385	83	2176	0.780	ug/l #	82
40) Benzene	6.056	78	2130	0.320	ug/l	91
52) Toluene	8.720	92	6393	1.563	ug/l	98
55) 1,1,2-Trichloroethane	9.110	97	570	0.347	ug/l #	15
67) Ethyl Benzene	10.195	91	35673	3.738	ug/l	98
68) m/p-Xylenes	10.299	106	53415	15.428	ug/l	100
69) o-Xylene	10.640	106	64394	19.229	ug/l	99
70) Styrene	10.640	104	3388	0.591	ug/l #	1
73) Isopropylbenzene	10.963	105	11077	1.209	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	67801	27.453	ug/l #	36
78) n-propylbenzene	11.305	91	26062	2.349	ug/l	98
79) 2-Chlorotoluene	11.378	91	17550	2.623	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.451	105	52157	6.829	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	67801	79.192	ug/l #	1
82) 4-Chlorotoluene	11.451	91	6306	0.795	ug/l #	48
83) tert-Butylbenzene	11.750	119	21879	2.814	ug/l #	57
84) 1,2,4-Trimethylbenzene	11.750	105	191613	24.799	ug/l	99
85) sec-Butylbenzene	11.890	105	9000	0.901	ug/l	90
86) p-Isopropyltoluene	12.006	119	6219	0.747	ug/l	89
89) n-Butylbenzene	12.329	91	15319	1.873	ug/l #	35
90) Hexachloroethane	12.530	117	2816	1.902	ug/l #	19
92) 1,2-Dibromo-3-Chloropr...	12.957	75	328	0.499	ug/l #	10
95) Naphthalene	13.774	128	30304	3.513	ug/l #	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046601.D
Acq On : 10 Jun 2025 14:38
Operator : JC/MD
Sample : Q2230-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425

Quant Time: Jun 11 01:48:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration




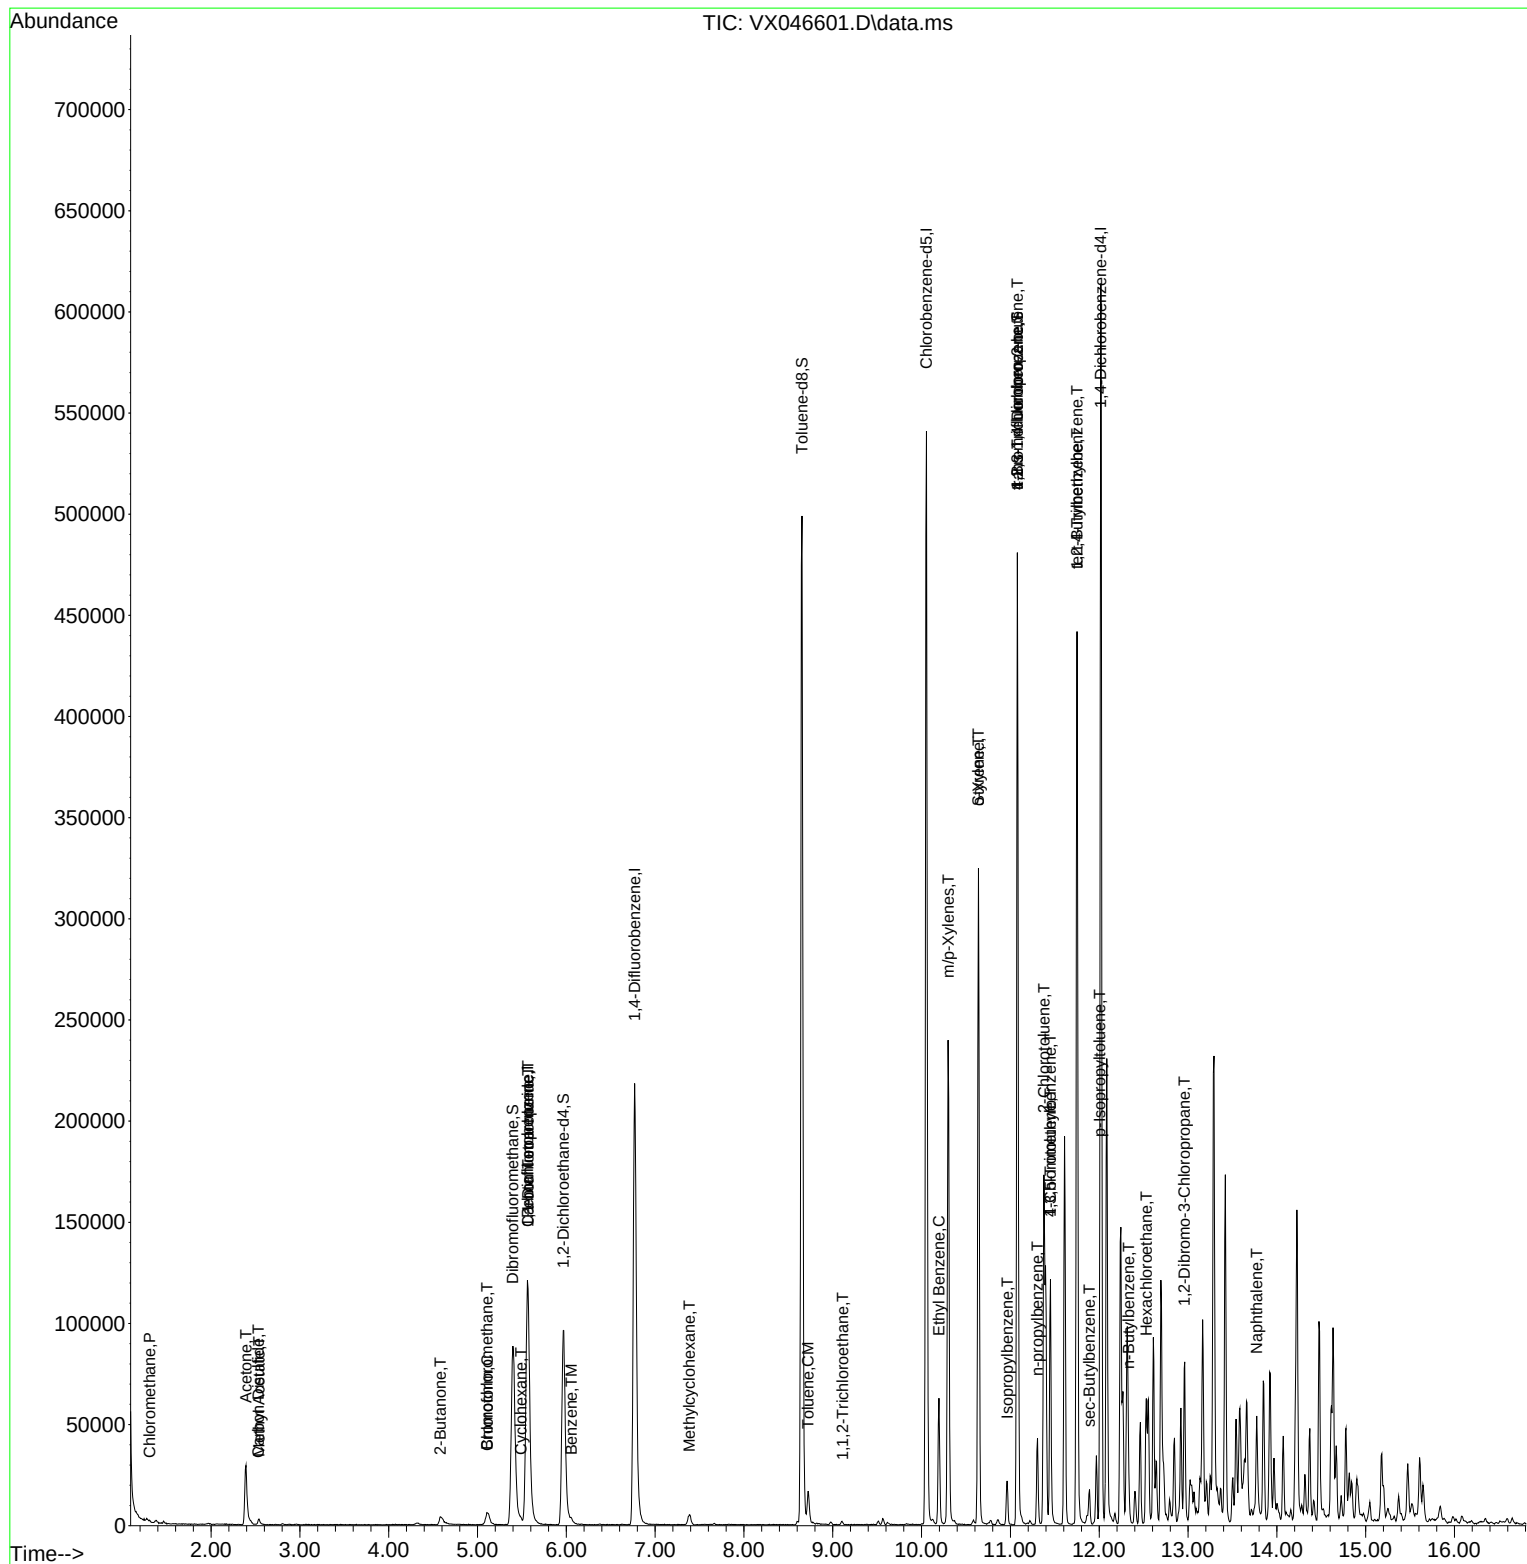




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion:168 Resp: 112231
Ion Ratio Lower Upper
168 100
99 70.1 54.9 82.3

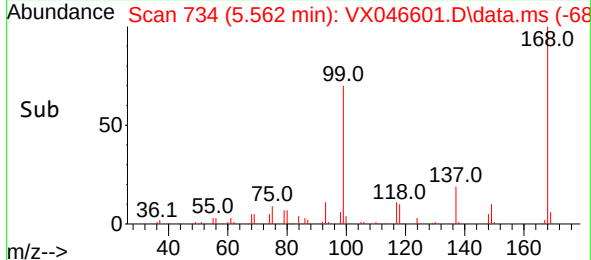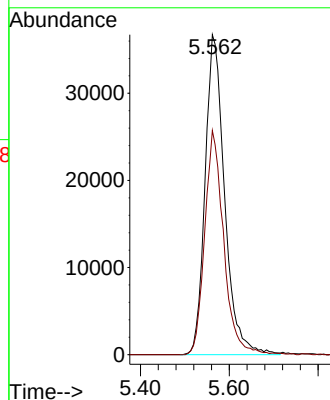

#3
Chloromethane
Concen: 0.320 ug/l
RT: 1.307 min Scan# 36
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 50 Resp: 454
Ion Ratio Lower Upper
50 100
52 23.9 25.4 38.2#


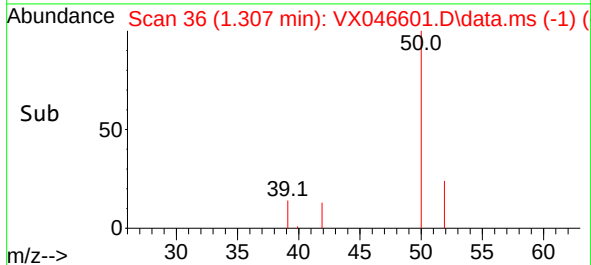
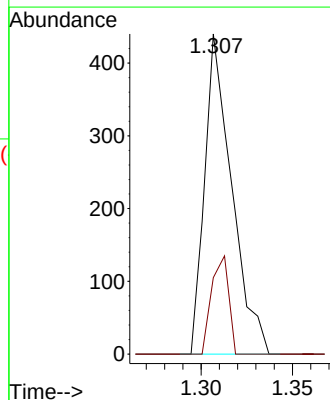





#16
Acetone
Concen: 51.274 ug/l
RT: 2.392 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion: 43 Resp: 37286
Ion Ratio Lower Upper
43 100
58 29.8 21.2 31.8

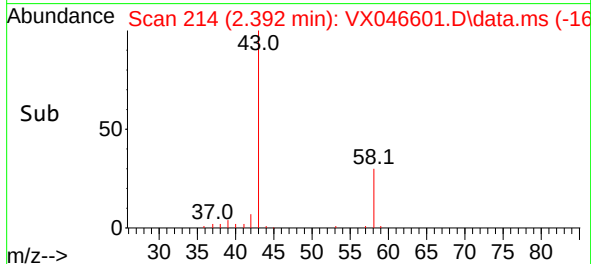

#17
Carbon Disulfide
Concen: 0.281 ug/l
RT: 2.532 min Scan# 237
Delta R.T. 0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 76 Resp: 224
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.4#




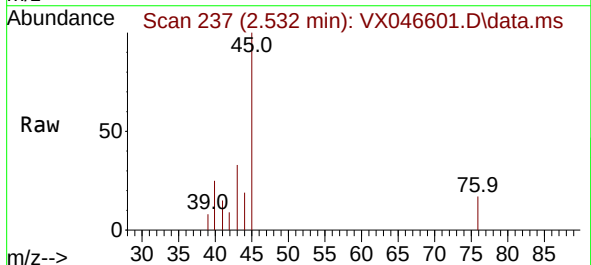




#18
Methyl Acetate
Concen: 0.507 ug/l
RT: 2.538 min Scan# 21
Delta R.T. -0.183 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion: 43 Resp: 1206
Ion Ratio Lower Upper
43 100
74 0.0 16.7 25.1#

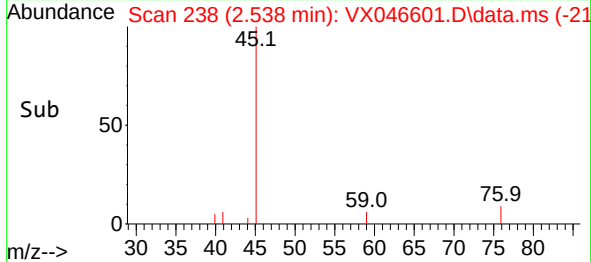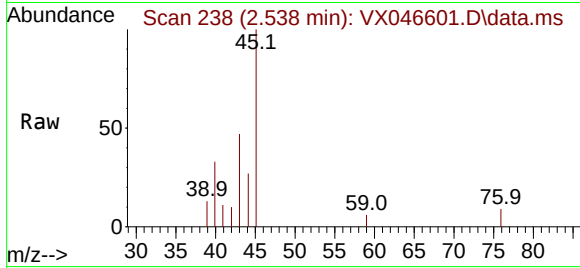

#25
2-Butanone
Concen: 8.394 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.006 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 43 Resp: 9330
Ion Ratio Lower Upper
43 100
72 21.5 18.4 27.6


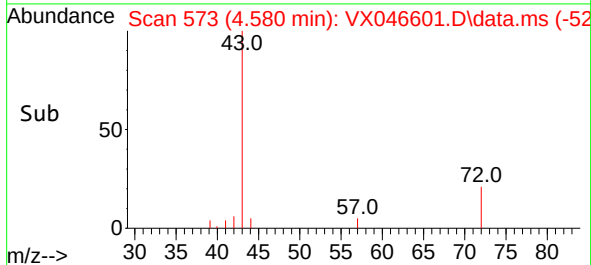

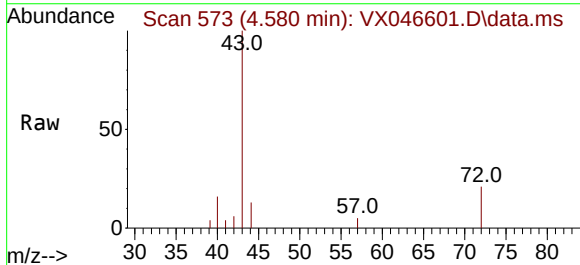


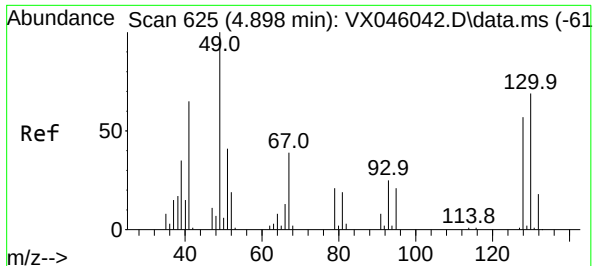

#28
Bromochloromethane
Concen: 0.464 ug/l
RT: 5.105 min Scan# 61
Delta R.T. 0.189 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion: 49 Resp: 636
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.0
130 0.0 56.2 84.2#

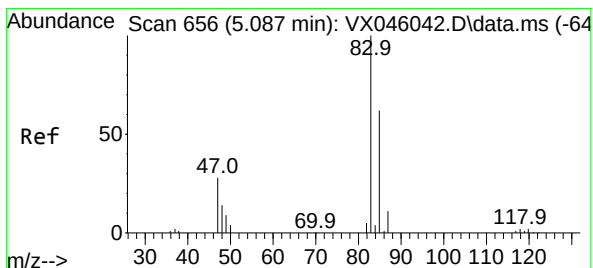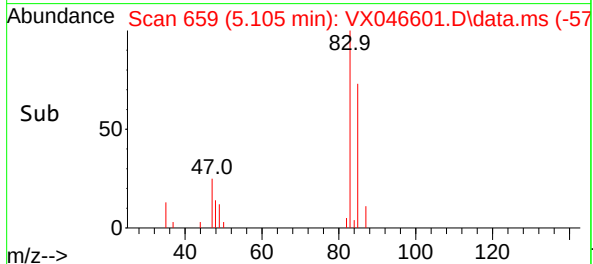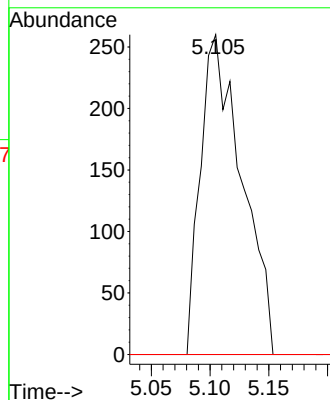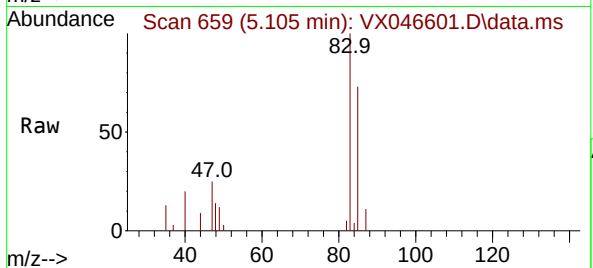

#30
Chloroform
Concen: 2.715 ug/l
RT: 5.111 min Scan# 660
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 83 Resp: 8181
Ion Ratio Lower Upper
83 100
85 61.2 49.3 73.9


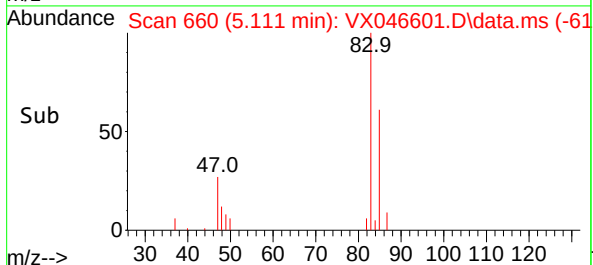
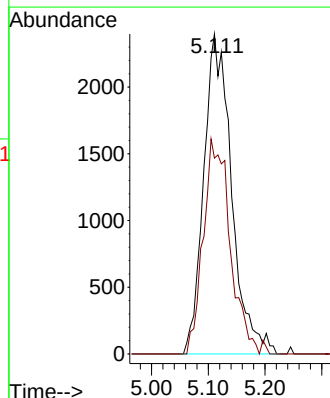
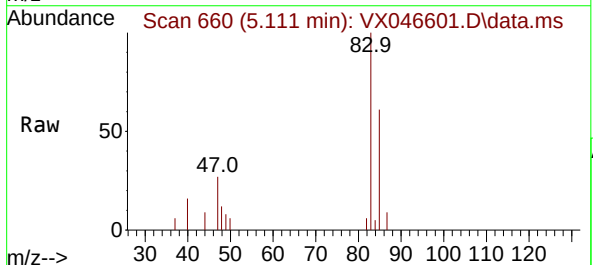




#31
Cyclohexane
Concen: 0.480 ug/l
RT: 5.489 min Scan# 718
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion: 56 Resp: 1114
Ion Ratio Lower Upper
56 100
69 27.6 24.4 36.6
84 73.7 66.9 100.3

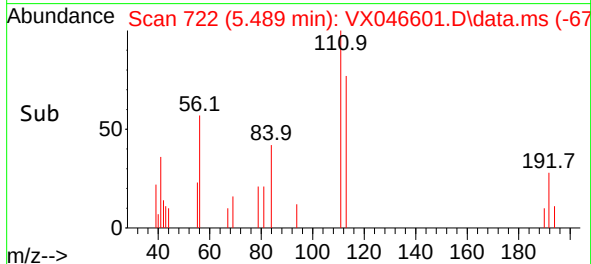

#33
1,2-Dichloroethane-d4
Concen: 50.233 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.006 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 65 Resp: 100300
Ion Ratio Lower Upper
65 100
67 50.7 0.0 99.0


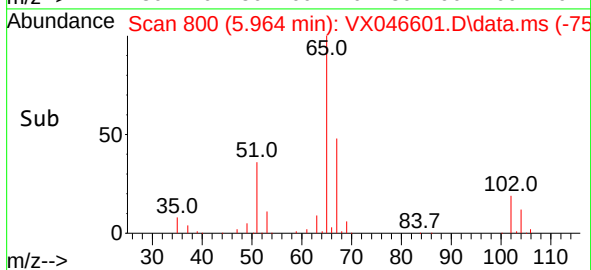






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion:114 Resp: 225068
Ion Ratio Lower Upper
114 100
63 22.9 0.0 49.2
88 17.2 0.0 33.6

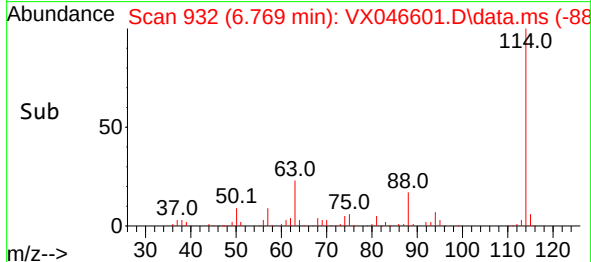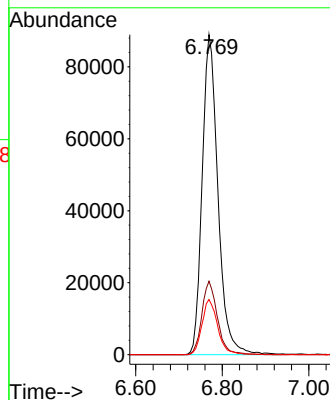

#35
Dibromofluoromethane
Concen: 49.936 ug/l
RT: 5.397 min Scan# 707
Delta R.T. -0.006 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion:113 Resp: 82652
Ion Ratio Lower Upper
113 100
111 103.8 83.1 124.7
192 17.3 13.3 19.9



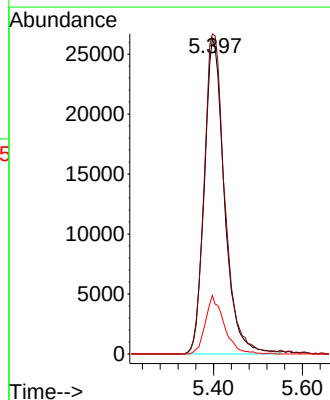
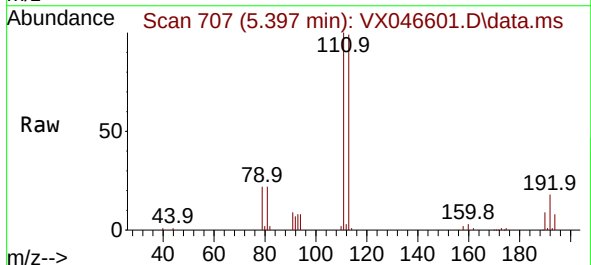




#36
1,1-Dichloropropene
Concen: 4.525 ug/l
RT: 5.568 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion: 75 Resp: 10698
Ion Ratio Lower Upper
75 100
110 9.2 16.3 48.9#
77 0.0 24.3 36.5#

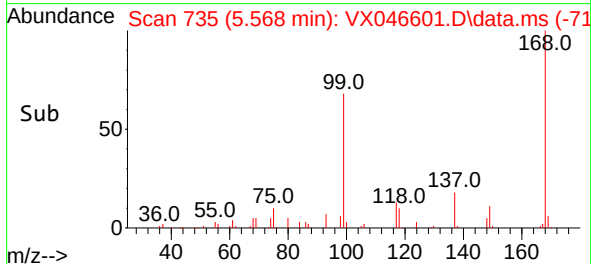

#38
Carbon Tetrachloride
Concen: 4.933 ug/l
RT: 5.568 min Scan# 735
Delta R.T. -0.128 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 117 Resp: 13063
Ion Ratio Lower Upper
117 100
119 3.8 75.2 112.8#
121 0.0 24.2 36.4#

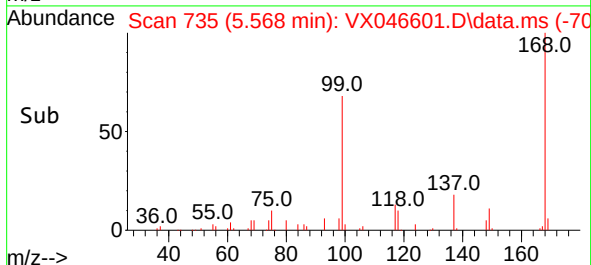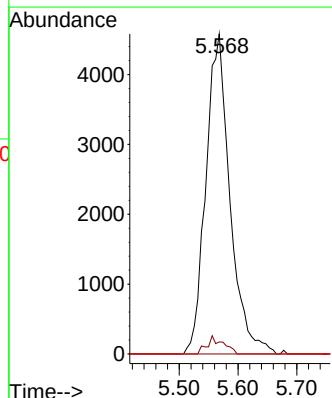

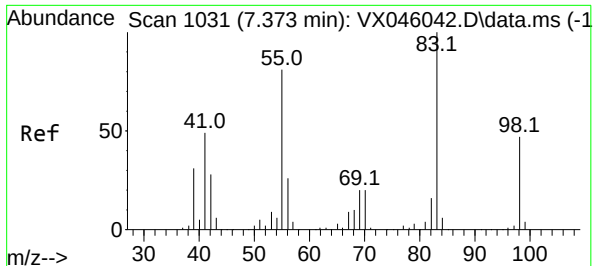

#39

Methylcyclohexane

Concen: 0.780 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. -0.006 min

Lab File: VX046601.D

Acq: 10 Jun 2025 14:38

Instrument :

MSVOA_X

ClientSampleId :

GW-MW901-060425





Tgt Ion: 83 Resp: 2176

Ion Ratio Lower Upper

83 100

55 56.5 64.7 97.1#

98 48.3 37.4 56.2

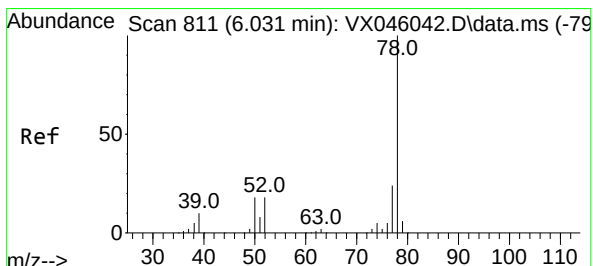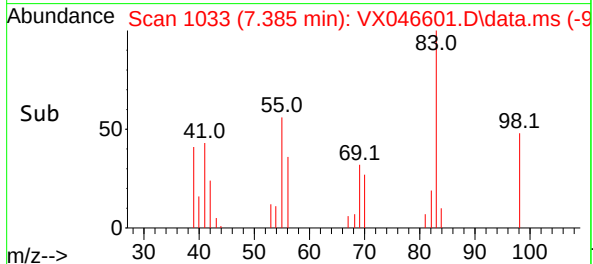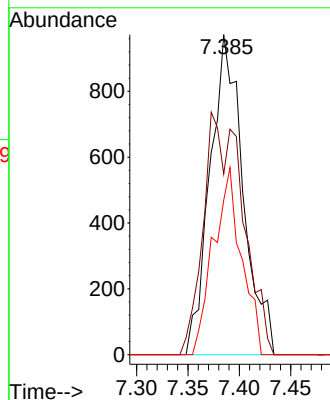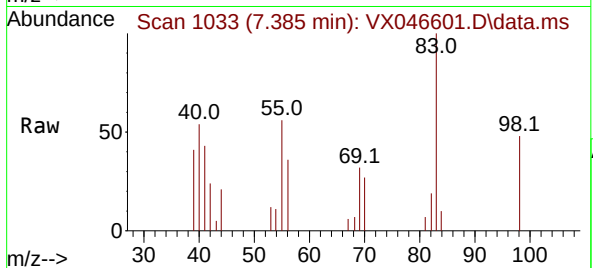

#40

Benzene

Concen: 0.320 ug/l

RT: 6.056 min Scan# 815

Delta R.T. -0.000 min

Lab File: VX046601.D




Acq: 10 Jun 2025 14:38


Tgt Ion: 78 Resp: 2130

Ion Ratio Lower Upper

78 100

77 19.1 19.0 28.4


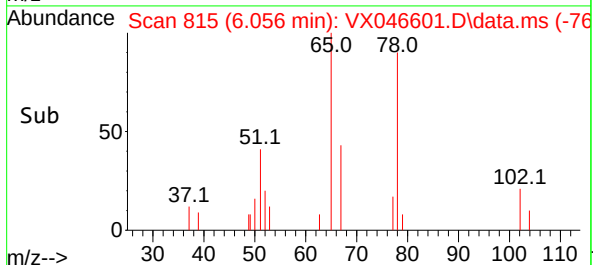
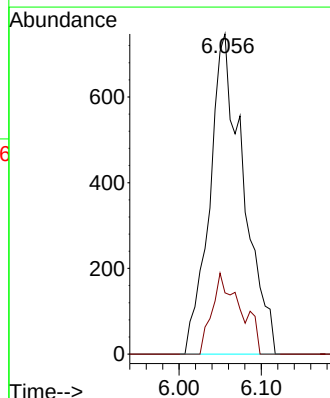
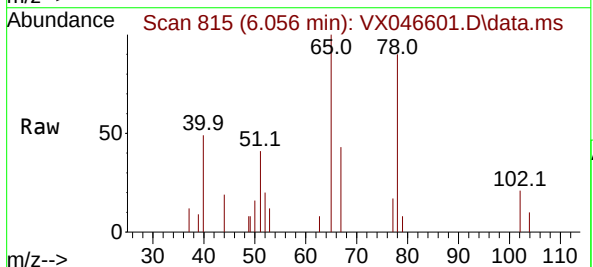




#50
Toluene-d8
Concen: 54.315 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion: 98 Resp: 296387
Ion Ratio Lower Upper
98 100
100 65.7 53.5 80.3

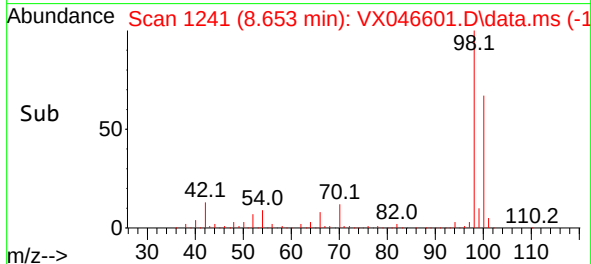

#52
Toluene
Concen: 1.563 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 92 Resp: 6393
Ion Ratio Lower Upper
92 100
91 173.9 136.6 205.0

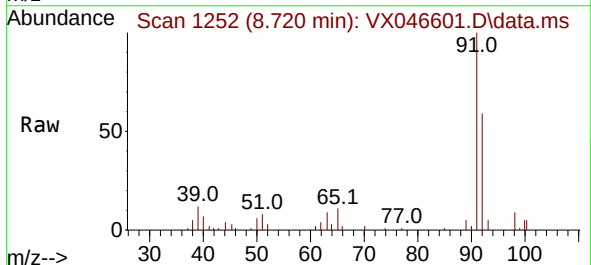



#55

1,1,2-Trichloroethane

Concen: 0.347 ug/l

RT: 9.110 min Scan# 1

Delta R.T. -0.043 min

Lab File: VX046601.D


Acq: 10 Jun 2025 14:38

Instrument :

MSVOA_X

ClientSampleId :

GW-MW901-060425



Tgt Ion: 97 Resp: 570




Ion Ratio Lower Upper

97 100

83 0.0 69.0 103.6#

85 0.0 44.3 66.5#

99 0.0 47.8 71.6#

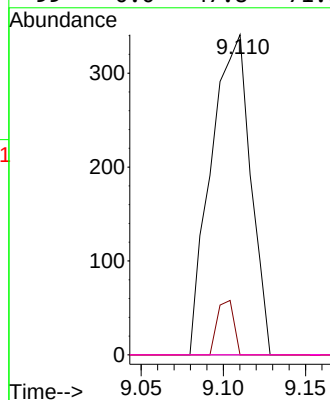

#62

4-Bromofluorobenzene

Concen: 55.586 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX046601.D

Acq: 10 Jun 2025 14:38




Tgt Ion: 95 Resp: 125497


Ion Ratio Lower Upper

95 100

174 68.6 0.0 135.8

176 65.8 0.0 131.4


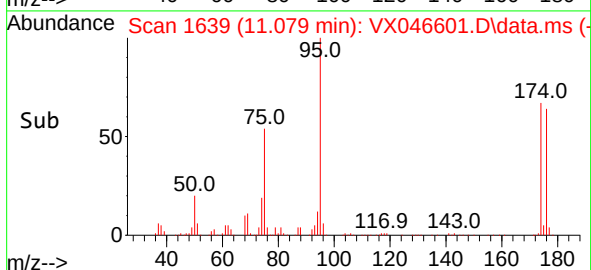

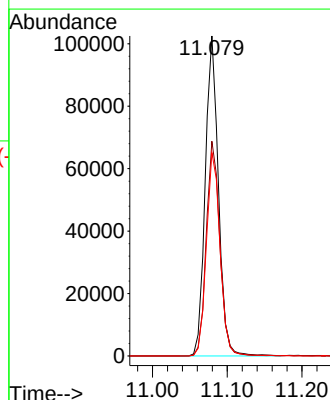




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion:117 Resp: 232456
Ion Ratio Lower Upper
117 100
82 57.1 50.6 76.0
119 31.4 25.8 38.6

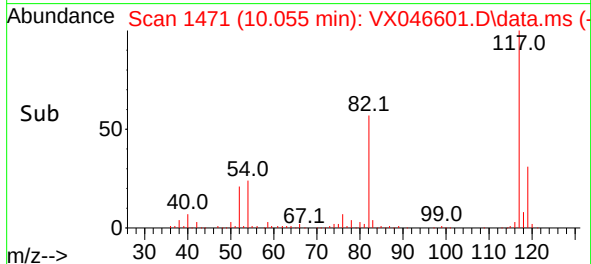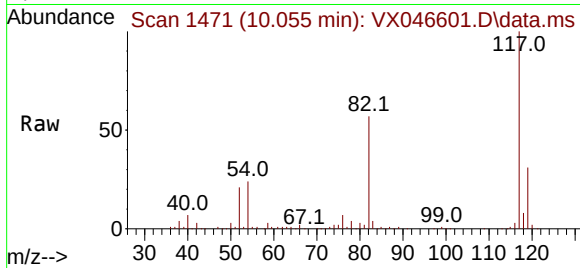

#67
Ethyl Benzene
Concen: 3.738 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 91 Resp: 35673
Ion Ratio Lower Upper
91 100
106 28.5 23.4 35.2



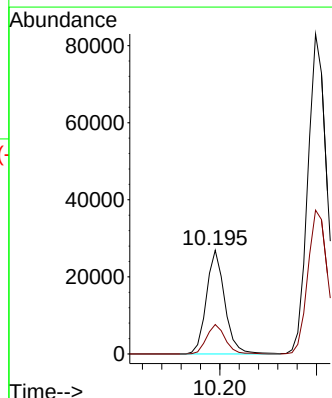
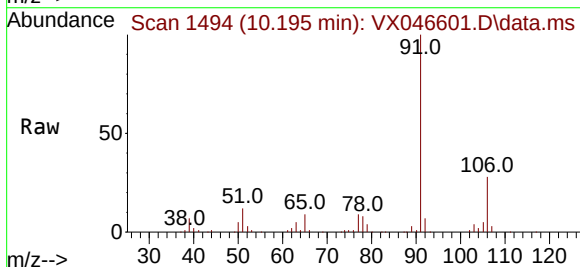




#68
m/p-Xylenes
Concen: 15.428 ug/l
RT: 10.299 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion:106 Resp: 53415
Ion Ratio Lower Upper
106 100
91 213.7 171.2 256.8

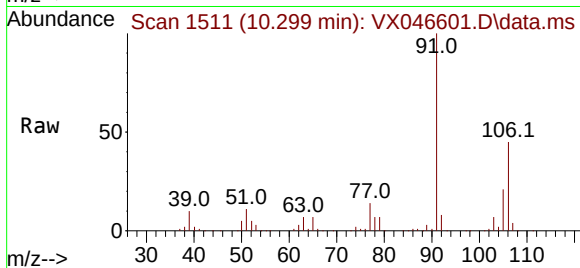

#69
o-Xylene
Concen: 19.229 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion:106 Resp: 64394
Ion Ratio Lower Upper
106 100
91 226.5 112.7 338.1


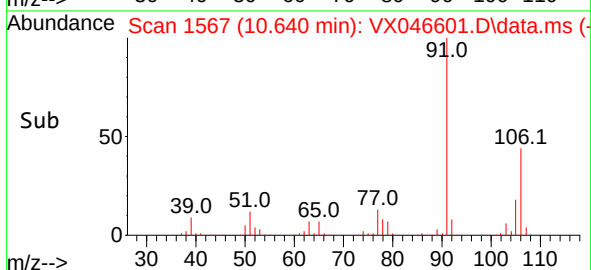

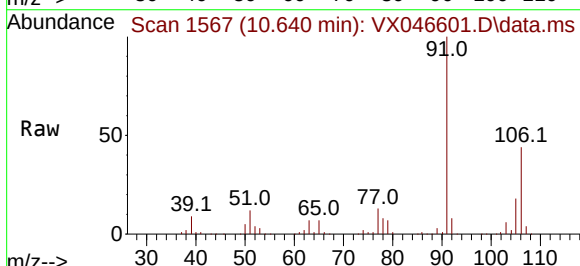




#70
Styrene
Concen: 0.591 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion:104 Resp: 3388
Ion Ratio Lower Upper
104 100
78 313.8 45.7 68.5#
103 259.1 43.7 65.5#

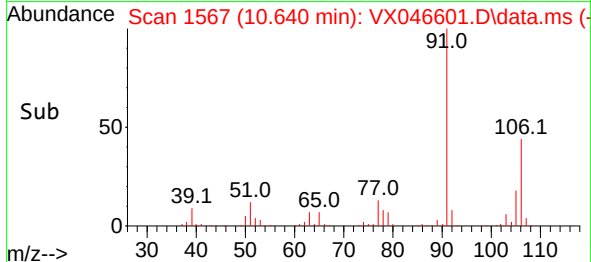

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion:152 Resp: 116598
Ion Ratio Lower Upper
152 100
115 62.9 46.9 140.7
150 155.3 0.0 351.0


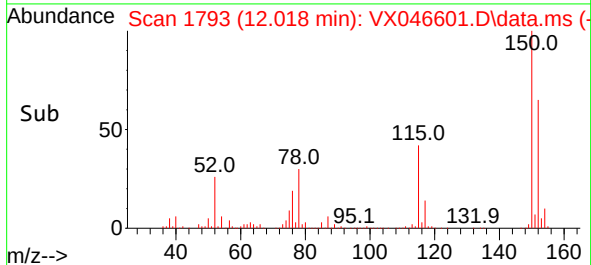






#73
Isopropylbenzene
Concen: 1.209 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion:105 Resp: 11077
Ion Ratio Lower Upper
105 100
120 25.2 12.8 38.4

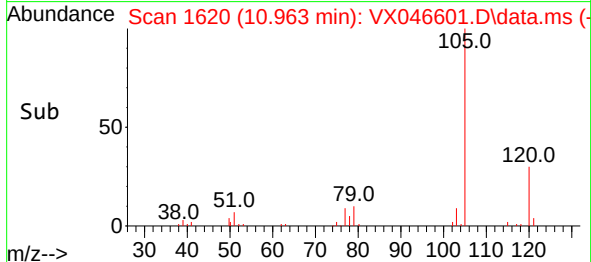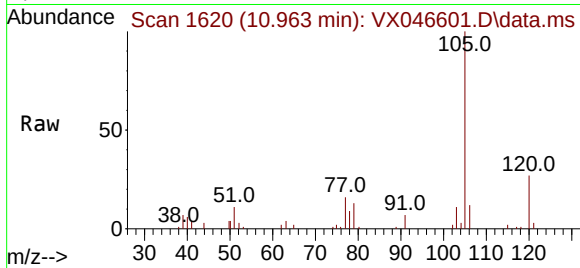

#76
1,2,3-Trichloropropane
Concen: 27.453 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 75 Resp: 67801
Ion Ratio Lower Upper
75 100
77 1.0 20.5 61.5#


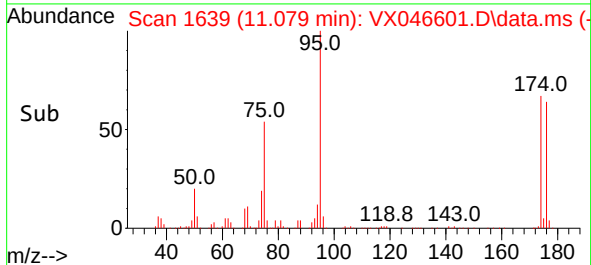

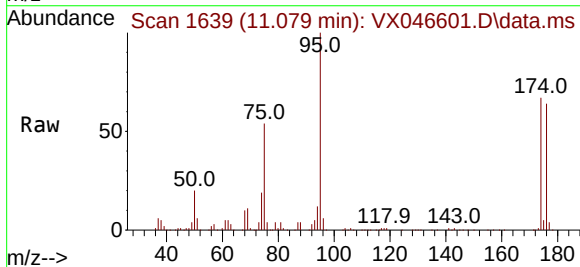




#78
n-propylbenzene
Concen: 2.349 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion: 91 Resp: 26062
Ion Ratio Lower Upper
91 100
120 20.7 10.8 32.4

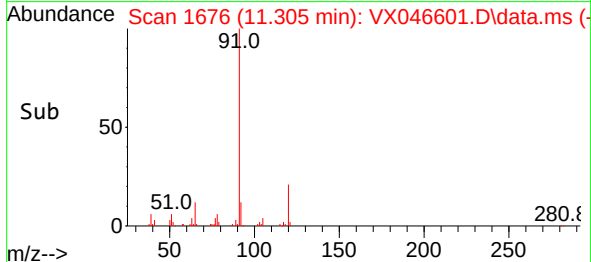

#79
2-Chlorotoluene
Concen: 2.623 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 91 Resp: 17550
Ion Ratio Lower Upper
91 100
126 0.0 15.6 46.7#


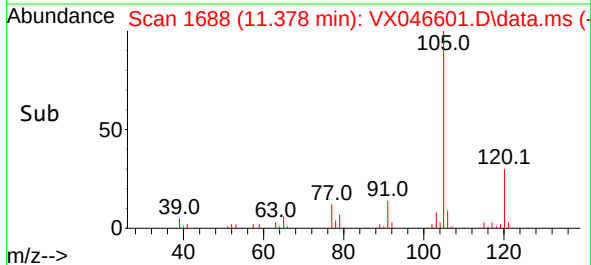






#80
 1,3,5-Trimethylbenzene
 Concen: 6.829 ug/l
 RT: 11.451 min Scan# 1700
 Delta R.T. 0.000 min
 Lab File: VX046601.D
 Acq: 10 Jun 2025 14:38




Instrument :
 MSVOA_X
 ClientSampleId :
 GW-MW901-060425


Tgt Ion:105 Resp: 52157
 Ion Ratio Lower Upper
 105 100
 120 46.0 23.1 69.2

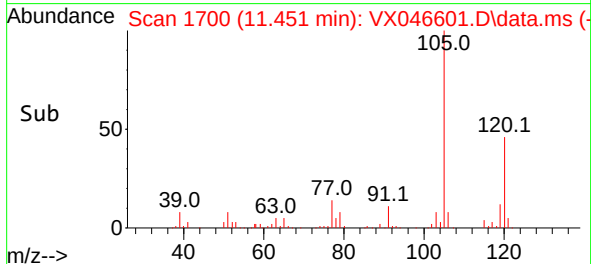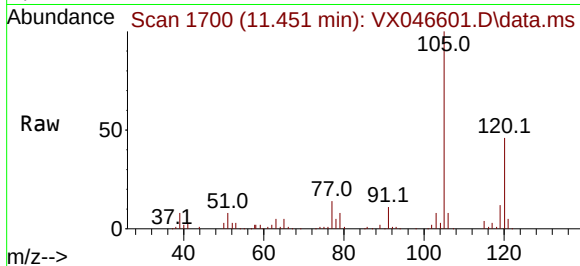

#81
 trans-1,4-Dichloro-2-butene
 Concen: 79.192 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. 0.061 min
 Lab File: VX046601.D
 Acq: 10 Jun 2025 14:38

Tgt Ion: 75 Resp: 67801
 Ion Ratio Lower Upper
 75 100
 53 0.0 100.5 150.7#
 89 0.0 37.0 55.6#




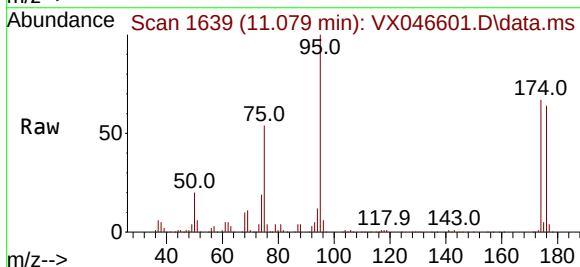




#82
4-Chlorotoluene
Concen: 0.795 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion: 91 Resp: 6306
Ion Ratio Lower Upper
91 100
126 0.0 13.3 39.8#

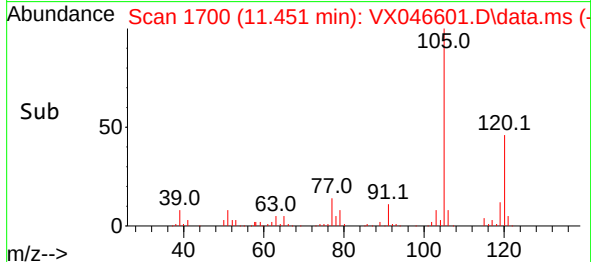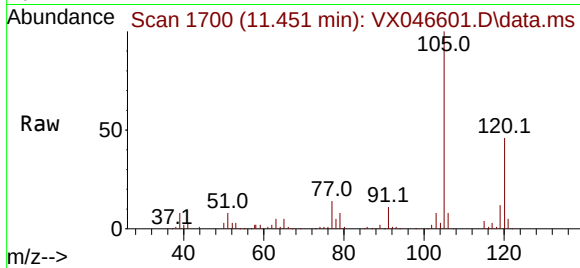

#83
tert-Butylbenzene
Concen: 2.814 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.037 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Tgt Ion: 119 Resp: 21879
Ion Ratio Lower Upper
119 100
91 98.8 32.9 98.7#
134 0.0 11.4 34.1#

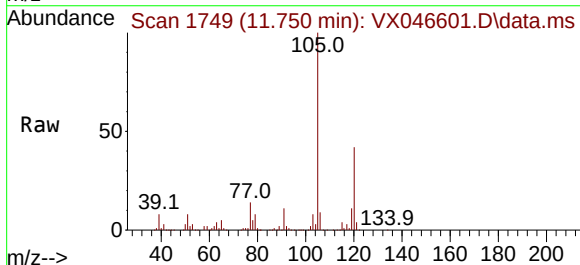



#84

1,2,4-Trimethylbenzene

Concen: 24.799 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX046601.D

Acq: 10 Jun 2025 14:38

Instrument :

MSVOA_X

ClientSampleId :





GW-MW901-060425

Tgt Ion:105 Resp: 191613

Ion Ratio Lower Upper

105 100

120 43.3 21.2 63.6

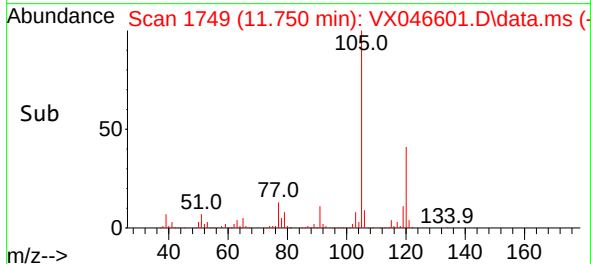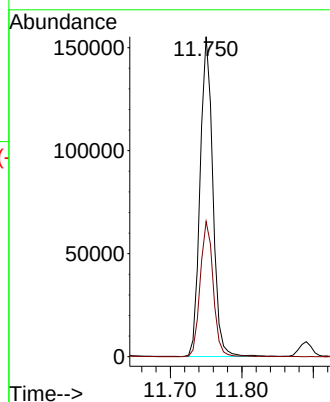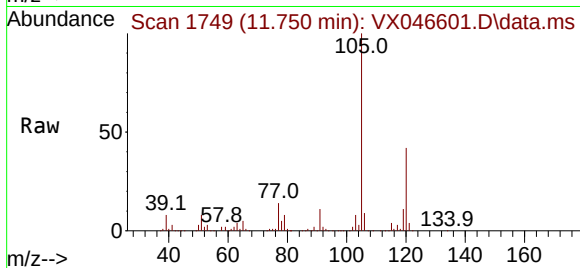

#85

sec-Butylbenzene

Concen: 0.901 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX046601.D




Acq: 10 Jun 2025 14:38


Tgt Ion:105 Resp: 9000

Ion Ratio Lower Upper

105 100

134 23.8 9.7 29.1

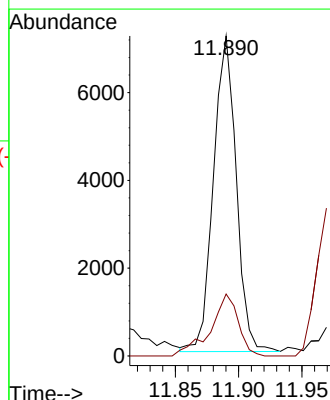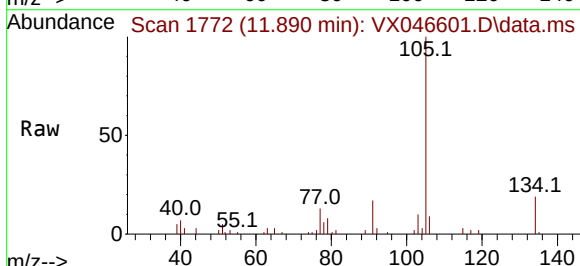

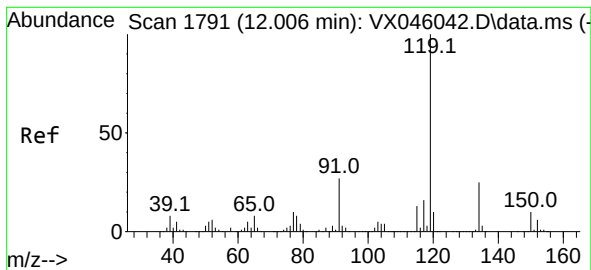

#86

p-Isopropyltoluene

Concen: 0.747 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX046601.D

Acq: 10 Jun 2025 14:38

Instrument :

MSVOA_X

ClientSampleId :

GW-MW901-060425





Tgt Ion:119 Resp: 6219

Ion Ratio Lower Upper

119 100

134 27.3 12.5 37.5

91 36.0 13.8 41.4

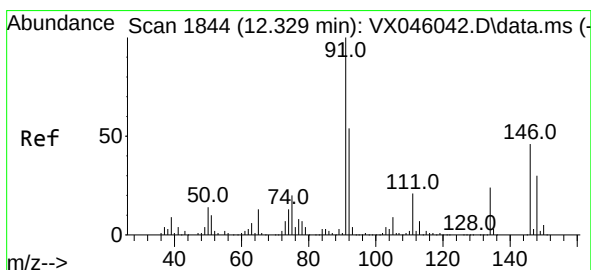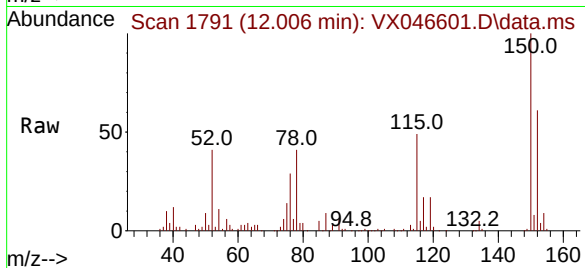

#89

n-Butylbenzene

Concen: 1.873 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX046601.D

Acq: 10 Jun 2025 14:38




Tgt Ion: 91 Resp: 15319


Ion Ratio Lower Upper

91 100

92 33.4 26.9 80.7

134 95.6 11.8 35.3#


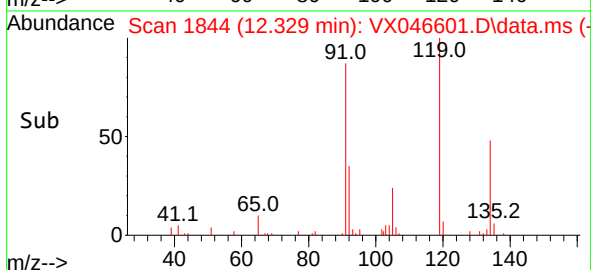

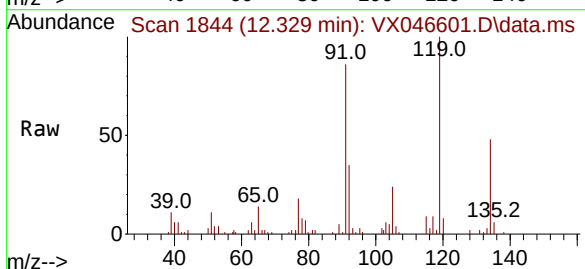




#90
Hexachloroethane
Concen: 1.902 ug/l
RT: 12.530 min Scan# 117
Delta R.T. -0.006 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38




Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425


Tgt Ion:117 Resp: 2816
Ion Ratio Lower Upper
117 100
201 0.0 31.6 94.7#

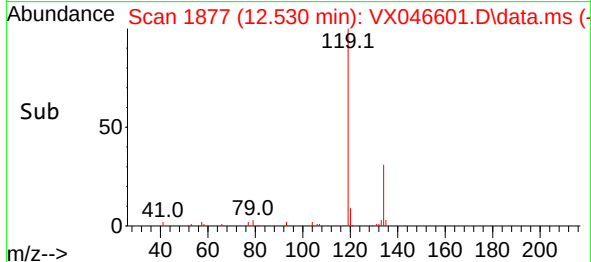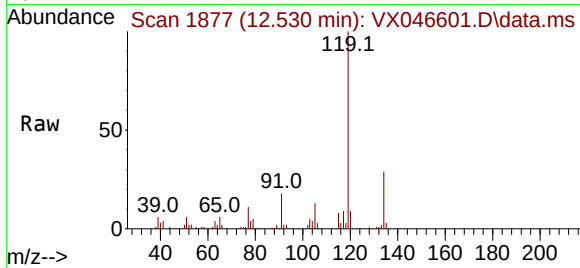

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.499 ug/l
RT: 12.957 min Scan# 1947
Delta R.T. 0.018 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38


Tgt Ion: 75 Resp: 328
Ion Ratio Lower Upper
75 100
155 0.0 34.9 104.8#
157 0.0 43.8 131.4#

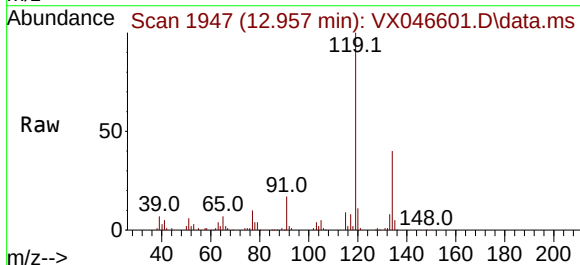



#95
Naphthalene
Concen: 3.513 ug/l
RT: 13.774 min Scan# 20
Delta R.T. -0.000 min
Lab File: VX046601.D
Acq: 10 Jun 2025 14:38

Instrument :
MSVOA_X
ClientSampleId :
GW-MW901-060425

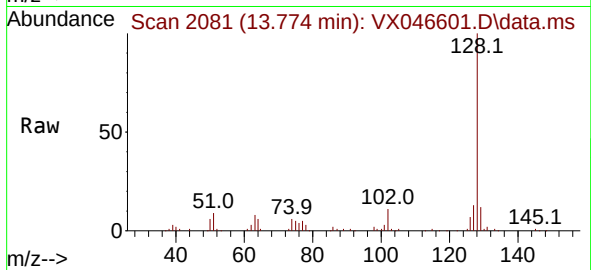

Tgt Ion:128 Resp: 30304
Ion Ratio Lower Upper
128 100
127 13.8 10.4 15.6
129 13.0 8.6 13.0#

