


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061119\
Data File : VX010217.D
Acq On : 11 Jun 2019 08:55
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Title : SW846 8260
Last Update : Sat Jun 08 02:12:13 2019

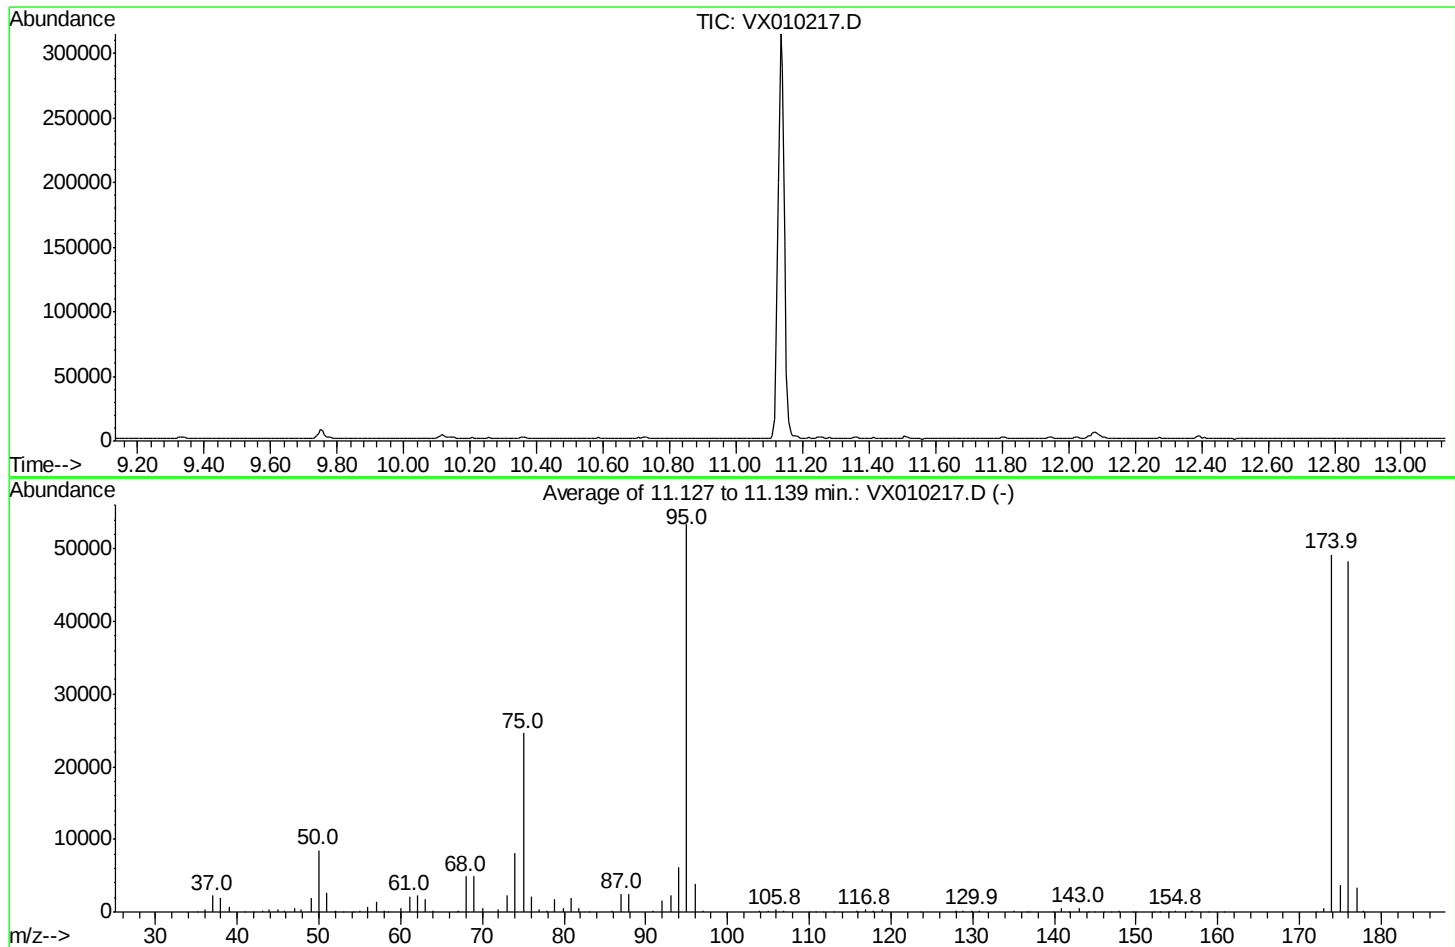

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	8518	PASS
75	95	30	60	46.2	24658	PASS
95	95	100	100	100.0	53376	PASS
96	95	5	9	7.4	3953	PASS
173	174	0.00	2	1.1	557	PASS
174	95	50	100	92.1	49173	PASS
175	174	5	9	7.6	3757	PASS
176	174	95	101	98.1	48256	PASS
177	176	5	9	6.8	3298	PASS