

Data File : VX016695.D
Acq On : 11 Jun 2020 11:47
Operator : JC/SP
Sample : L2963-13DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF012MW031-200608DL

Quant Time: Jun 12 06:54:05 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260
QLast Update : Wed May 27 16:31:05 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	228747	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	357632	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	357629	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	168164	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	132348	46.59	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.18%	
35) Dibromofluoromethane	5.47	113	111832	50.78	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.56%	
50) Toluene-d8	8.70	98	439148	51.24	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.48%	
62) 4-Bromofluorobenzene	11.12	95	166683	50.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.66%	


Target Compounds				Qvalue		
4) Vinyl Chloride	1.39	62	6947	2.415	ug/l	97
5) Bromomethane	1.65	94	595	0.425	ug/l #	77
10) Methyl Iodide	2.50	142	648	3.300	ug/l #	93
11) Tert butyl alcohol	3.01	59	150	0.206	ug/l #	72
12) 1,1-Dichloroethene	2.36	96	568	0.258	ug/l #	60
13) Acrolein	2.28	56	432	1.394	ug/l #	3
15) Acrylonitrile	3.12	53	460	0.308	ug/l #	29
16) Acetone	2.42	43	1139	0.915	ug/l #	82
17) Carbon Disulfide	2.55	76	1825	0.279	ug/l	97
21) trans-1,2-Dichloroethene	3.14	96	572	0.235	ug/l #	81
25) 2-Butanone	4.64	43	674	0.320	ug/l #	49
27) cis-1,2-Dichloroethene	4.56	96	140758	49.976	ug/l	87
31) Cyclohexane	5.63	56	4260	1.079	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	15510	4.580	ug/l #	52
38) Carbon Tetrachloride	5.63	117	22047	6.196	ug/l #	16
51) 4-Methyl-2-Pentanone	8.62	43	840	0.213	ug/l	93
65) Chlorobenzene	10.12	112	4422	0.606	ug/l	100
76) 1,2,3-Trichloropropane	11.12	75	80095	21.669	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.12	75	80095	53.302	ug/l #	14
89) n-Butylbenzene	12.37	91	2098	0.258	ug/l	94
91) 1,2-Dichlorobenzene	12.38	146	1724	0.336	ug/l	94
93) 1,2,4-Trichlorobenzene	13.63	180	1338	0.393	ug/l	92
94) Hexachlorobutadiene	13.76	225	1053	0.787	ug/l	76
95) Naphthalene	13.82	128	2755	0.236	ug/l	99
96) 1,2,3-Trichlorobenzene	14.00	180	1331	0.399	ug/l	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX016695.D
Acq On : 11 Jun 2020 11:47
Operator : JC/SP
Sample : L2963-13DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF012MW031-200608DL

Quant Time: Jun 12 06:54:05 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260
QLast Update : Wed May 27 16:31:05 2020
Response via : Initial Calibration

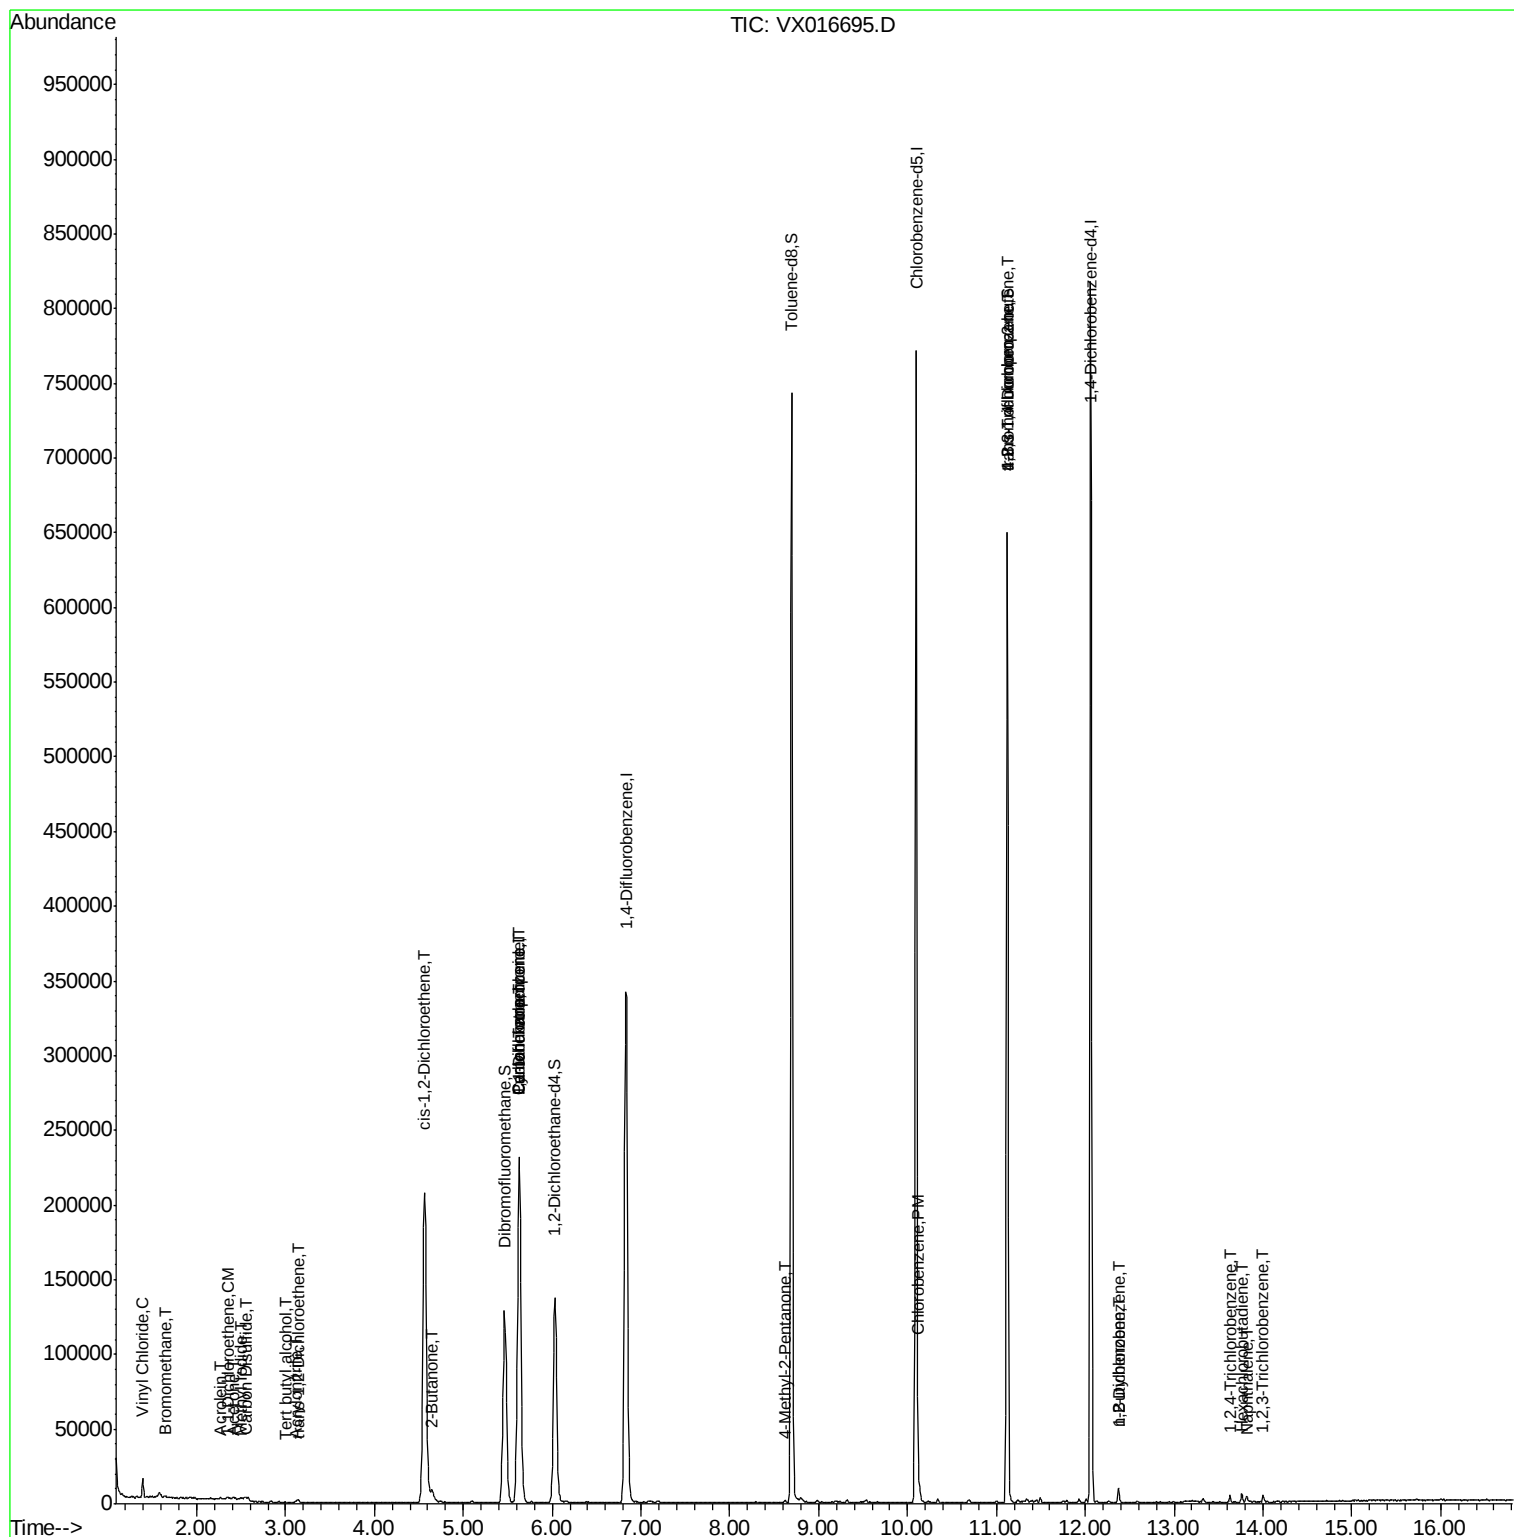



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :


LF012MW031-200608DL

Tgt Ion:168 Resp: 228747

Ion Ratio Lower Upper




168 100

99 53.3 45.2 67.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

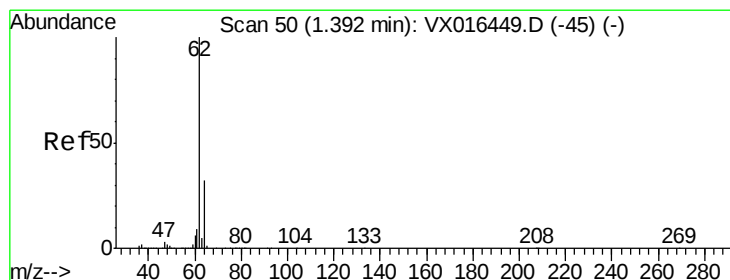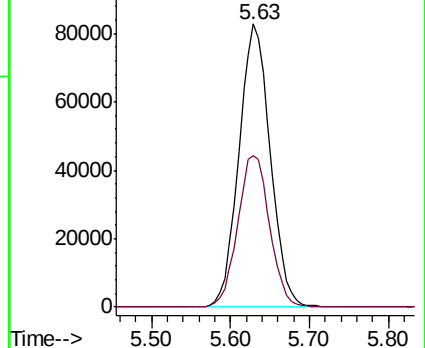

#4

Vinyl Chloride

Concen: 2.415 ug/l

RT: 1.39 min Scan# 50

Delta R.T. -0.00 min

Lab File: VX016695.D


Acq: 11 Jun 2020 11:47

Tgt Ion: 62 Resp: 6947

Ion Ratio Lower Upper



62 100


64 34.1 25.9 38.9



Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 63.90 (63.60 to 64.60): VX0

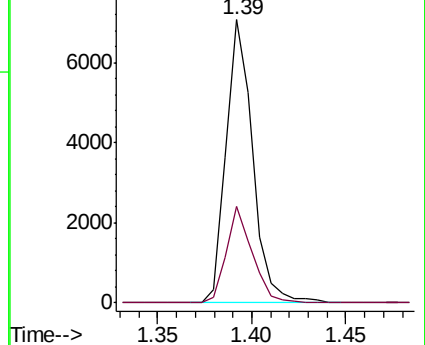

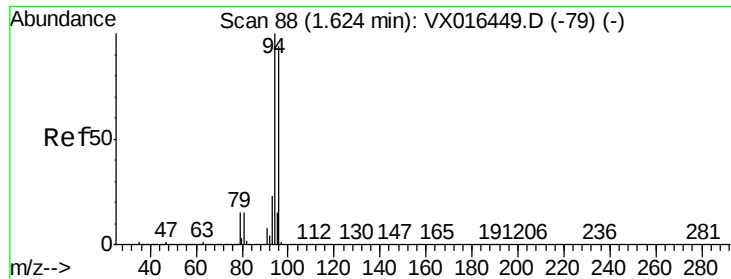

#5

Bromomethane

Concen: 0.425 ug/l

RT: 1.65 min Scan# 92

Delta R.T. 0.02 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :


LF012MW031-200608DL

Tgt Ion: 94 Resp: 595

Ion Ratio Lower Upper

94 100

96 72.1 75.1 112.7#

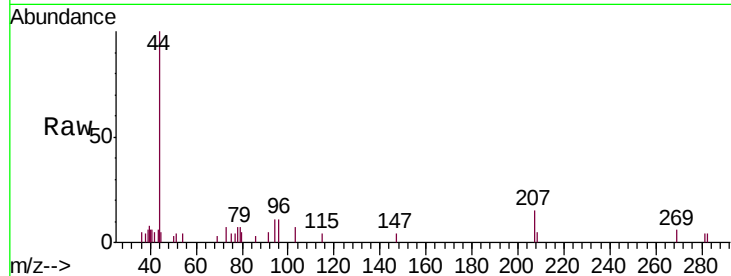

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.65

200

150



100

50

0

1.60 1.65 1.70

Time-->

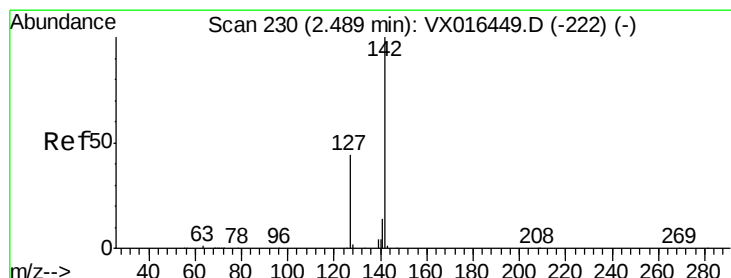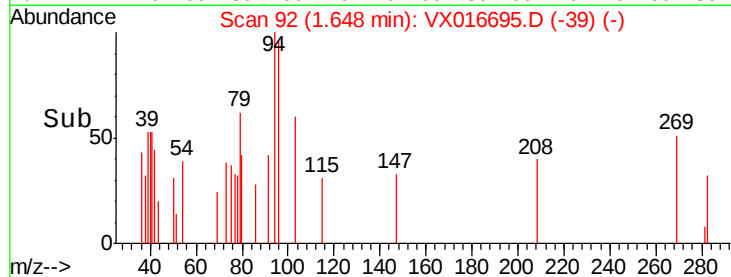

#10

Methyl Iodide

Concen: 3.300 ug/l

RT: 2.50 min Scan# 231

Delta R.T. 0.01 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47


Tgt Ion: 142 Resp: 648

Ion Ratio Lower Upper

142 100

127 42.4 35.3 52.9

141 6.5 11.4 17.2#

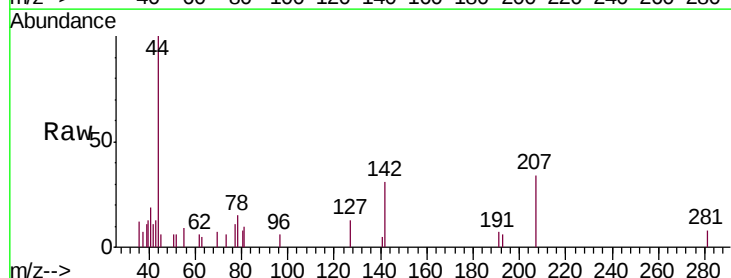

Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

400

300


200


100

0

2.45 2.50 2.55

Time-->

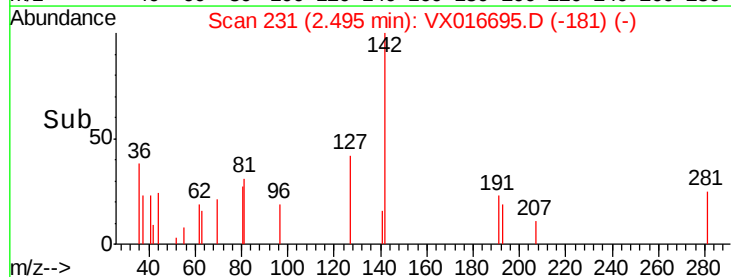




#11




Tert butyl alcohol
 Concen: 0.206 ug/l
 RT: 3.01 min Scan# 315
 Delta R.T. -0.01 min
 Lab File: VX016695.D
 Acq: 11 Jun 2020 11:47

Instrument :
 MSVOA_X
 ClientSampleId :
 LF012MW031-200608DL

Tgt Ion: 59 Resp: 150
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.2 12.4#

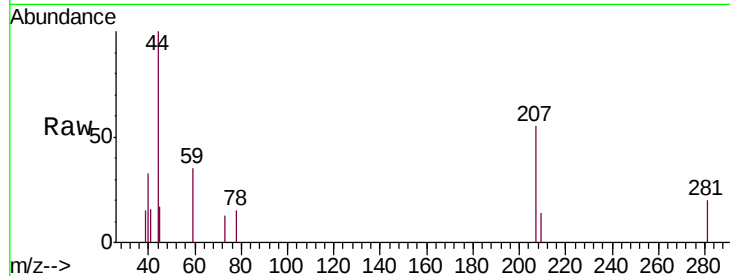


Abundance Ion 59.00 (58.70 to 59.70): VX0
 Ion 57.00 (56.70 to 57.70): VX0

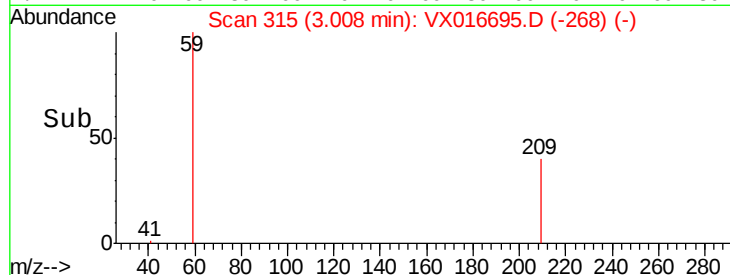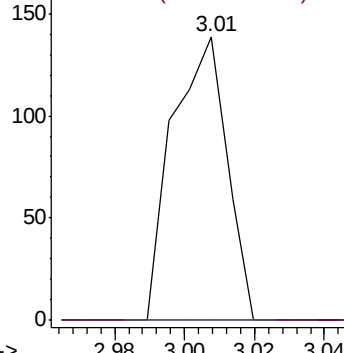



#12


1,1-Dichloroethene
 Concen: 0.258 ug/l
 RT: 2.36 min Scan# 208
 Delta R.T. -0.00 min
 Lab File: VX016695.D
 Acq: 11 Jun 2020 11:47

Tgt Ion: 96 Resp: 568
 Ion Ratio Lower Upper
 96 100
 61 101.7 126.6 189.8#
 98 37.7 51.3 76.9#

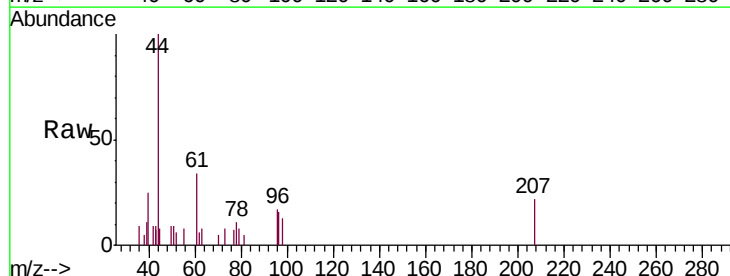

Abundance Ion 95.90 (95.60 to 96.60): VX0
 Ion 60.90 (60.60 to 61.60): VX0
 Ion 97.90 (97.60 to 98.60): VX0

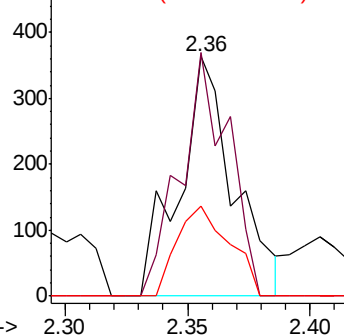



#13

Acrolein

Concen: 1.394 ug/l

RT: 2.28 min Scan# 195

Delta R.T. 0.01 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :





LF012MW031-200608DL

Tgt Ion: 56 Resp: 432

Ion Ratio Lower Upper

56 100

55 153.9 58.3 87.5#

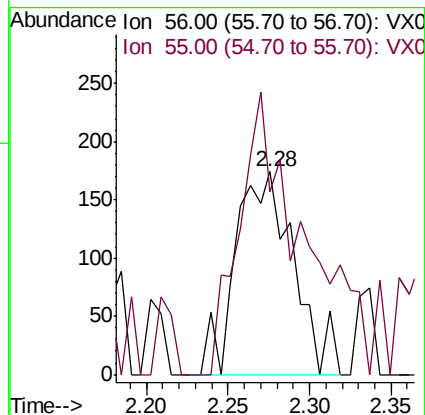

#15

Acrylonitrile

Concen: 0.308 ug/l

RT: 3.12 min Scan# 333

Delta R.T. -0.00 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47




Tgt Ion: 53 Resp: 460


Ion Ratio Lower Upper

53 100

52 0.0 66.7 100.1#

51 48.7 28.6 43.0#

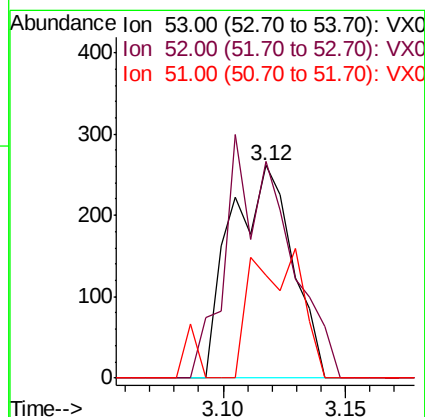



#16

Acetone

Concen: 0.915 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.00 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :


LF012MW031-200608DL

Tgt Ion: 43 Resp: 1139

Ion Ratio Lower Upper

43 100

58 22.5 26.1 39.1#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.42

600

400



200

0

Time--> 2.35

2.40

2.45



#17

Carbon Disulfide

Concen: 0.279 ug/l

RT: 2.55 min Scan# 240

Delta R.T. -0.00 min

Lab File: VX016695.D


Acq: 11 Jun 2020 11:47

Tgt Ion: 76 Resp: 1825

Ion Ratio Lower Upper

76 100

78 8.0 7.4 11.0



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

2.55

1200

1000

800

600

400


200


0

Time--> 2.50

2.55

2.60





#21

trans-1,2-Dichloroethene

Concen: 0.235 ug/l

RT: 3.14 min Scan# 337

Delta R.T. -0.00 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :

LF012MW031-200608DL


Tgt Ion: 96 Resp: 572

Ion Ratio Lower Upper

96 100

61 118.7 115.3 172.9




98 78.1 51.9 77.9#



Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

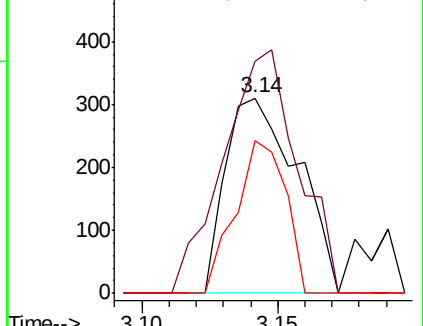

#25

2-Butanone

Concen: 0.320 ug/l

RT: 4.64 min Scan# 583

Delta R.T. 0.01 min

Lab File: VX016695.D


Acq: 11 Jun 2020 11:47

Tgt Ion: 43 Resp: 674

Ion Ratio Lower Upper



43 100


72 0.0 21.0 31.6#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

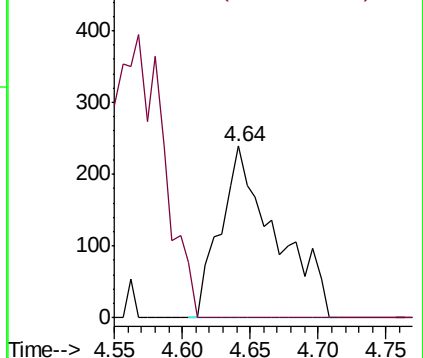







#27

cis-1,2-Dichloroethene
Concen: 49.976 ug/l
RT: 4.56 min Scan# 570
Delta R.T. -0.00 min
Lab File: VX016695.D
Acq: 11 Jun 2020 11:47

Instrument :
MSVOA_X
ClientSampleId :
LF012MW031-200608DL




Tgt Ion: 96 Resp: 140758
Ion Ratio Lower Upper
96 100
61 120.2 0.0 284.6
98 64.0 0.0 127.2

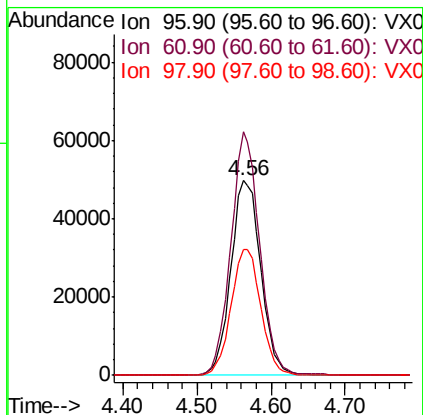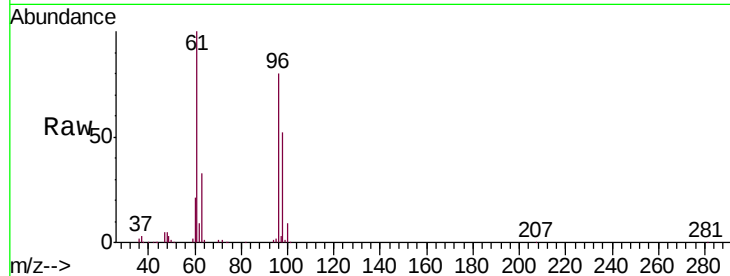


#31

Cyclohexane
Concen: 1.079 ug/l
RT: 5.63 min Scan# 745
Delta R.T. 0.08 min
Lab File: VX016695.D
Acq: 11 Jun 2020 11:47

Tgt Ion: 56 Resp: 4260
Ion Ratio Lower Upper
56 100
69 174.8 25.7 38.5#
84 153.7 70.0 105.0#

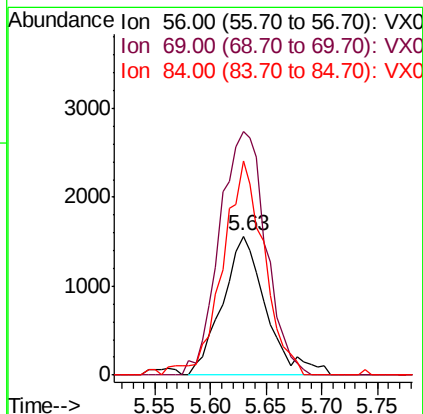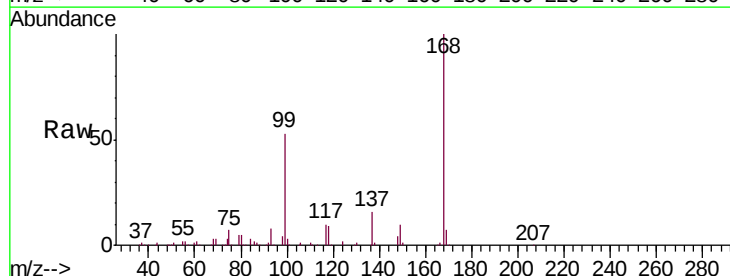



#33

1,2-Dichloroethane-d4

Concen: 46.589 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :


LF012MW031-200608DL

Tgt Ion: 65 Resp: 132348

Ion Ratio Lower Upper




65 100

67 52.0 0.0 104.8



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

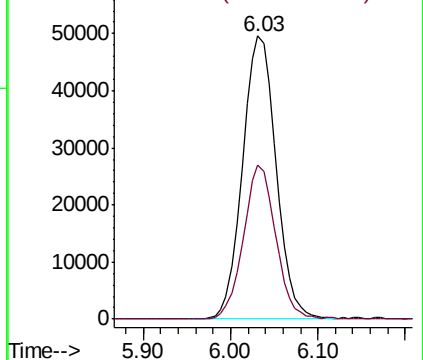

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 943

Delta R.T. 0.01 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47


Tgt Ion: 114 Resp: 357632

Ion Ratio Lower Upper

114 100

63 19.4 0.0 42.6



88 15.6 0.0 32.8




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

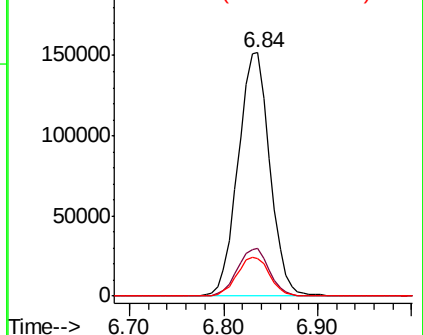



#35

Dibromofluoromethane

Concen: 50.784 ug/l

RT: 5.47 min Scan# 719

Delta R.T. 0.01 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :

LF012MW031-200608DL


Tgt Ion:113 Resp: 111832

Ion Ratio Lower Upper

113 100

111 103.2 83.0 124.6




192 22.7 17.7 26.5



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

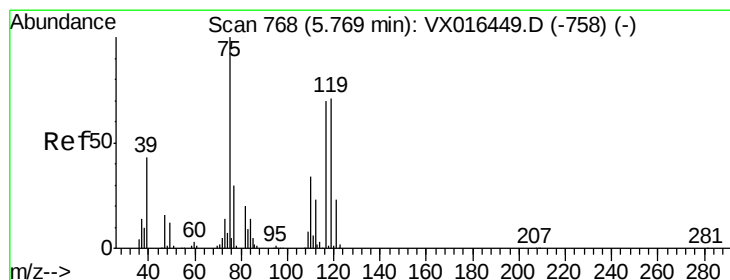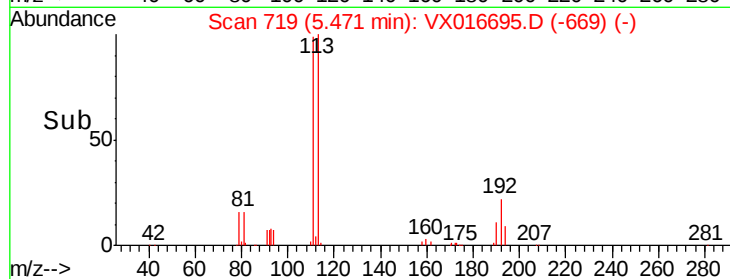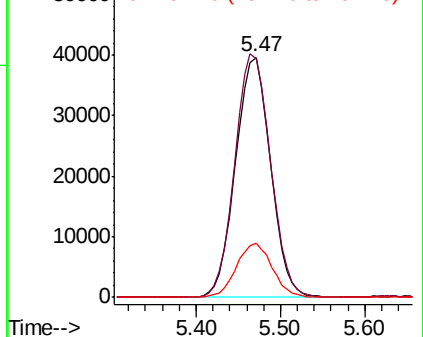

#36

1,1-Dichloropropene

Concen: 4.580 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.14 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47


Tgt Ion: 75 Resp: 15510

Ion Ratio Lower Upper

75 100

110 10.9 17.4 52.3#



77 0.1 24.2 36.4#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

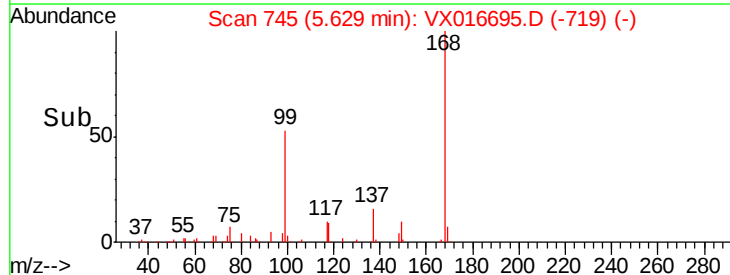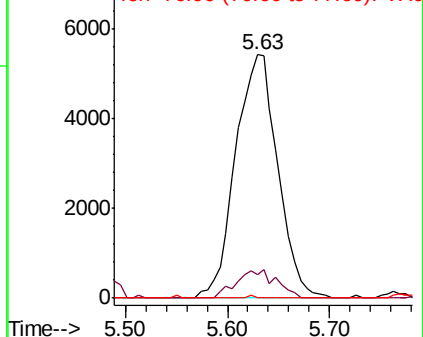

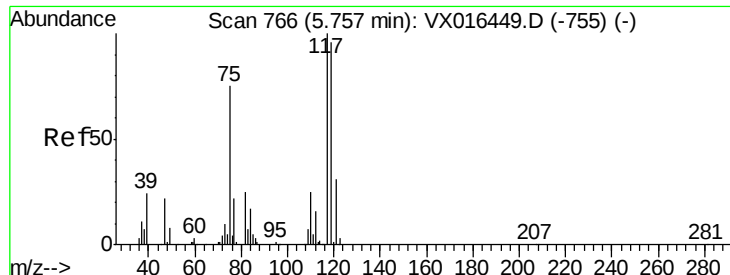

#38

Carbon Tetrachloride

Concen: 6.196 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.13 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :

LF012MW031-200608DL


Tgt Ion:117 Resp: 22047

Ion Ratio Lower Upper

117 100

119 4.9 76.3 114.5#




121 0.0 24.6 37.0#

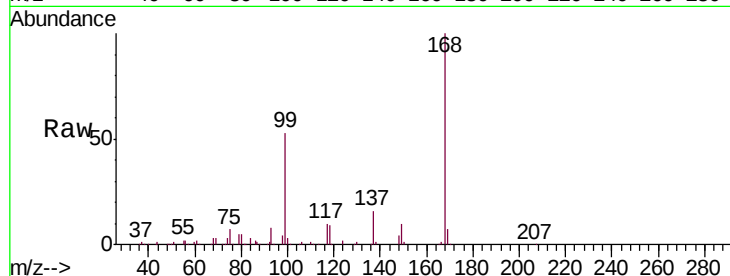

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

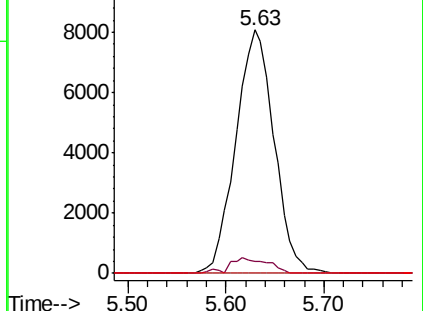

#50

Toluene-d8

Concen: 51.236 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX016695.D


Acq: 11 Jun 2020 11:47

Tgt Ion: 98 Resp: 439148

Ion Ratio Lower Upper



98 100


100 66.3 53.8 80.6



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V



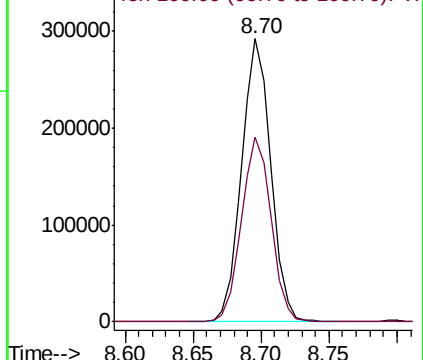





#51
 4-Methyl-2-Pentanone
 Concen: 0.213 ug/l
 RT: 8.62 min Scan# 1236
 Delta R.T. -0.00 min
 Lab File: VX016695.D
 Acq: 11 Jun 2020 11:47




Instrument :
 MSVOA_X
 ClientSampleID :
 LF012MW031-200608DL


Tgt Ion: 43 Resp: 840
 Ion Ratio Lower Upper
 43 100
 58 36.8 33.0 49.6

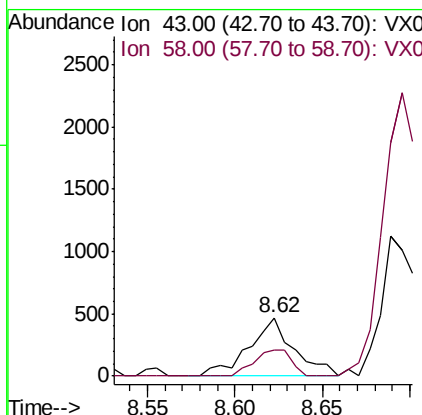

#62
 4-Bromofluorobenzene
 Concen: 50.329 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. -0.00 min
 Lab File: VX016695.D
 Acq: 11 Jun 2020 11:47

Tgt Ion: 95 Resp: 166683
 Ion Ratio Lower Upper
 95 100
 174 86.5 0.0 163.0
 176 84.3 0.0 156.8

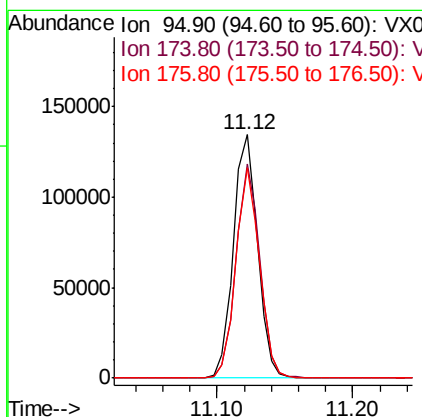







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX016695.D
Acq: 11 Jun 2020 11:47

Instrument :
MSVOA_X
ClientSampleId :
LF012MW031-200608DL

Tgt Ion:117 Resp: 357629
Ion Ratio Lower Upper
117 100
82 53.8 45.0 67.6
119 32.5 25.8 38.8

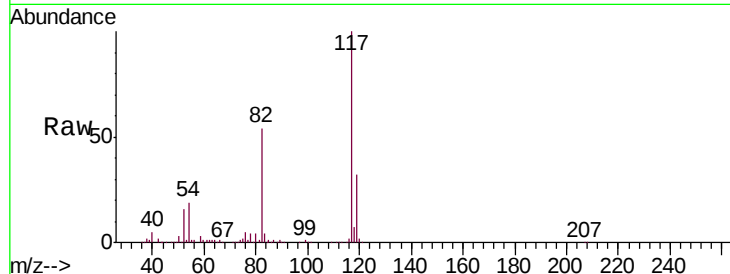


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V


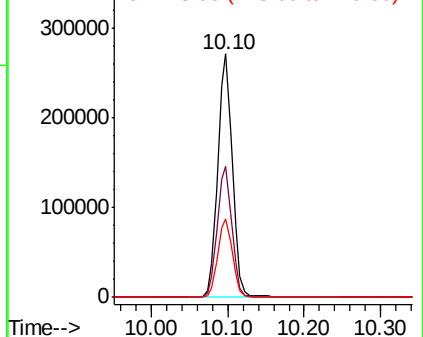



#65
Chlorobenzene
Concen: 0.606 ug/l
RT: 10.12 min Scan# 1482
Delta R.T. -0.00 min
Lab File: VX016695.D
Acq: 11 Jun 2020 11:47

Tgt Ion:112 Resp: 4422
Ion Ratio Lower Upper
112 100
114 32.8 26.0 39.0



Abundance Ion 111.90 (111.60 to 112.60): V
Ion 113.90 (113.60 to 114.60): V

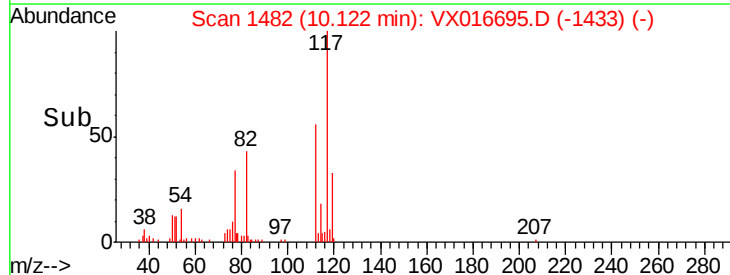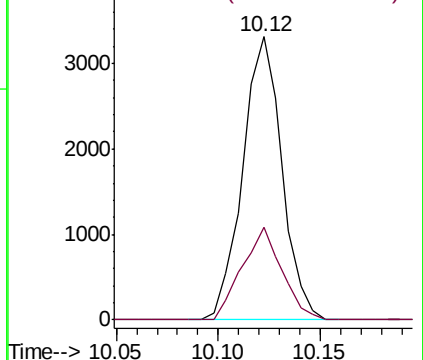

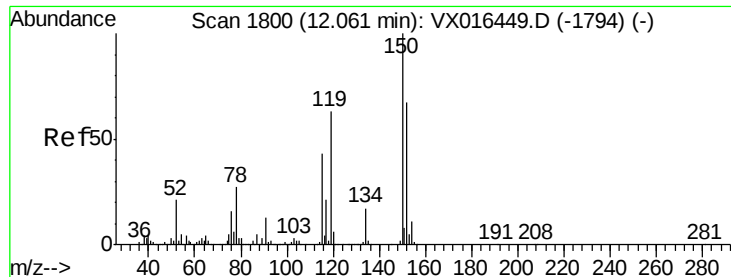

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :

LF012MW031-200608DL


Tgt Ion:152 Resp: 168164

Ion Ratio Lower Upper

152 100

115 58.6 39.9 119.6




150 156.2 0.0 341.0

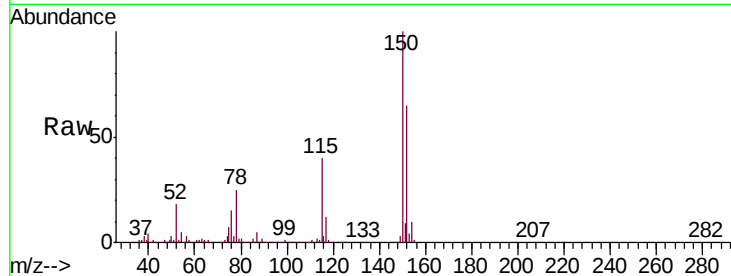

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

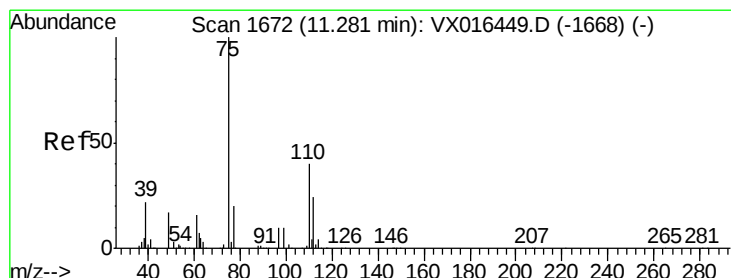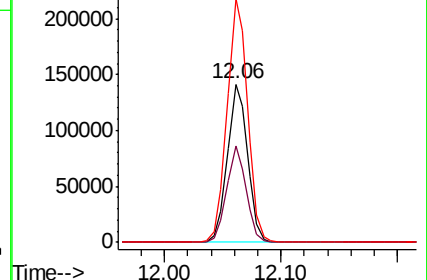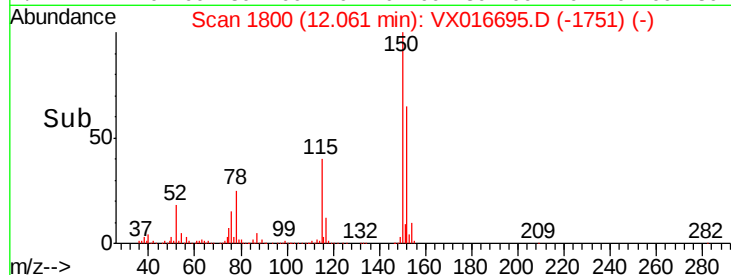

#76

1,2,3-Trichloropropane

Concen: 21.669 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX016695.D


Acq: 11 Jun 2020 11:47

Tgt Ion: 75 Resp: 80095

Ion Ratio Lower Upper



75 100


77 1.2 21.3 63.7#

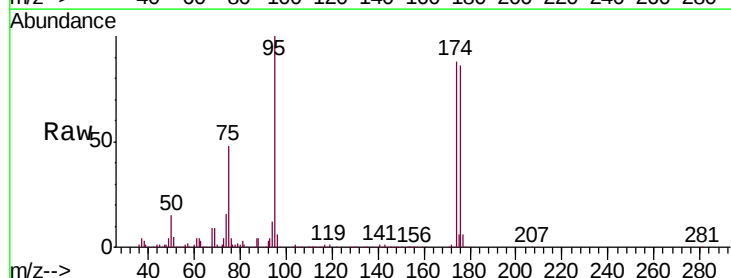

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

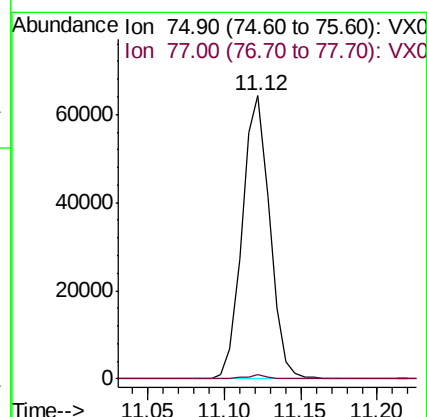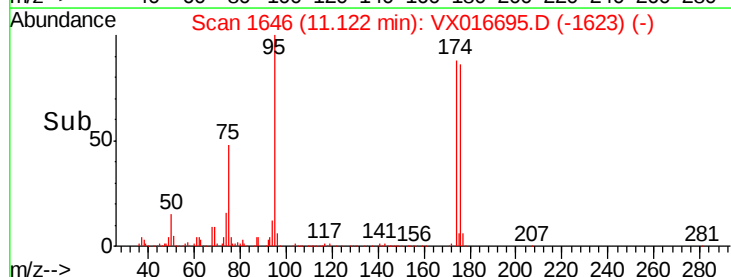



#81

trans-1,4-Dichloro-2-butene

Concen: 53.302 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :

LF012MW031-200608DL


Tgt Ion: 75 Resp: 80095

Ion Ratio Lower Upper

75 100

53 0.1 71.3 106.9#




89 0.0 36.6 55.0#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

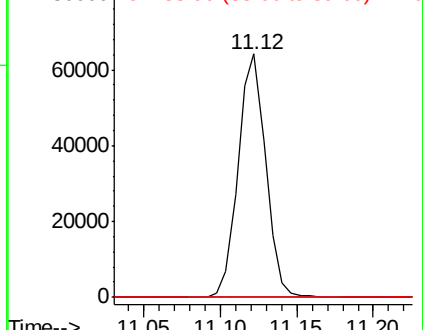

#89

n-Butylbenzene

Concen: 0.258 ug/l

RT: 12.37 min Scan# 1851

Delta R.T. -0.00 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47


Tgt Ion: 91 Resp: 2098

Ion Ratio Lower Upper

91 100

92 48.6 27.2 81.5



134 27.5 13.1 39.3




Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 92.00 (91.70 to 92.70): VX0

Ion 134.00 (133.70 to 134.70): V




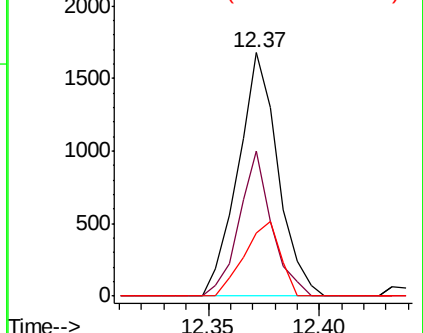




#91
 1,2-Dichlorobenzene
 Concen: 0.336 ug/l
 RT: 12.38 min Scan# 1852
 Delta R.T. -0.00 min
 Lab File: VX016695.D
 Acq: 11 Jun 2020 11:47




Instrument :
 MSVOA_X
 ClientSampleId :
 LF012MW031-200608DL


Tgt Ion:146 Resp: 1724
 Ion Ratio Lower Upper
 146 100
 111 42.0 21.4 64.3
 148 71.1 31.9 95.7

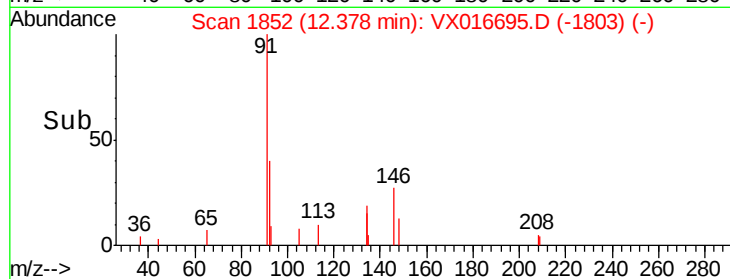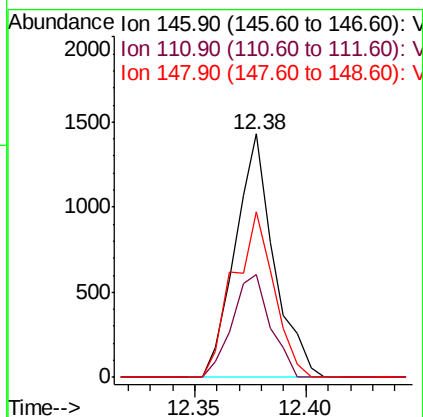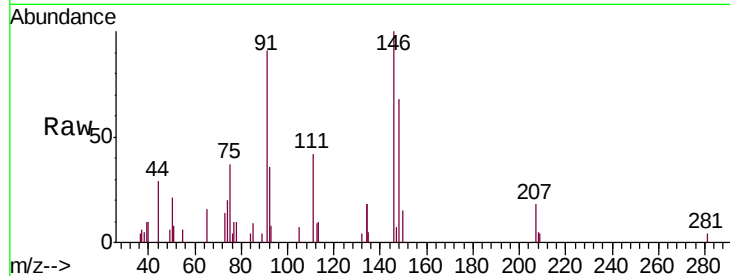

#93
 1,2,4-Trichlorobenzene
 Concen: 0.393 ug/l
 RT: 13.63 min Scan# 2057
 Delta R.T. -0.00 min
 Lab File: VX016695.D
 Acq: 11 Jun 2020 11:47

Tgt Ion:180 Resp: 1338
 Ion Ratio Lower Upper
 180 100
 182 87.4 48.3 144.8
 145 32.0 15.4 46.2

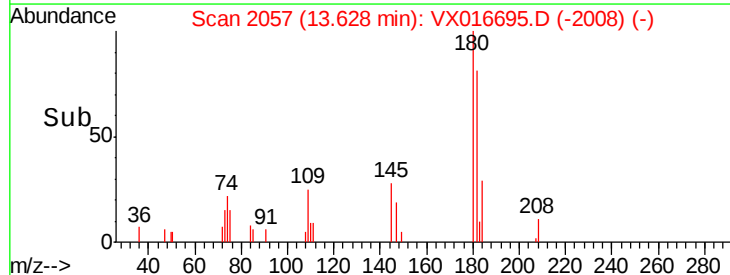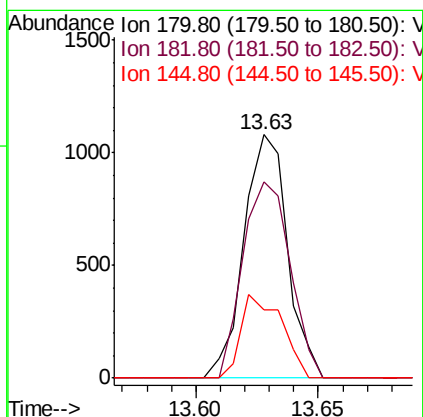



#94

Hexachlorobutadiene

Concen: 0.787 ug/l

RT: 13.76 min Scan# 2079

Delta R.T. -0.01 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47

Instrument :

MSVOA_X

ClientSampleId :

LF012MW031-200608DL


Tgt Ion: 225 Resp: 1053

Ion Ratio Lower Upper

225 100

223 46.0 32.3 96.8




227 44.1 31.6 94.7

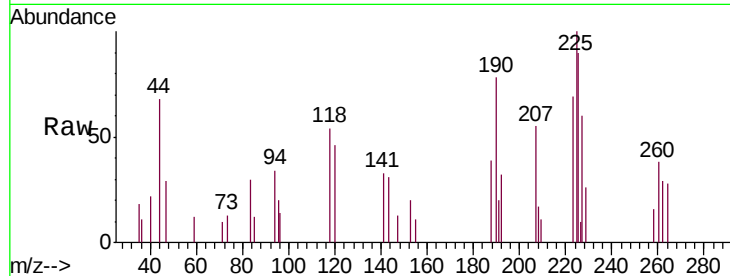

Abundance Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

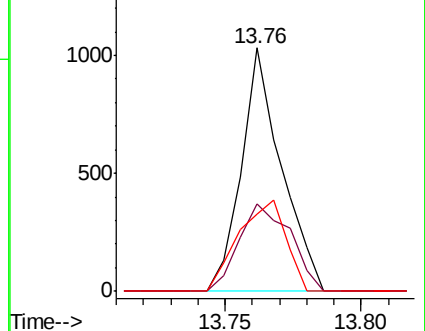

#95

Naphthalene

Concen: 0.236 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. -0.00 min

Lab File: VX016695.D

Acq: 11 Jun 2020 11:47


Tgt Ion: 128 Resp: 2755

Ion Ratio Lower Upper

128 100

127 12.7 10.6 15.8



129 10.6 8.6 13.0

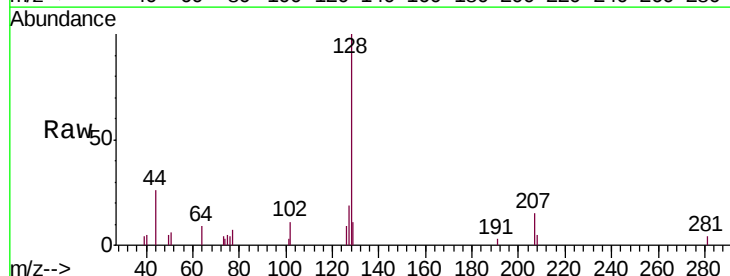


Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

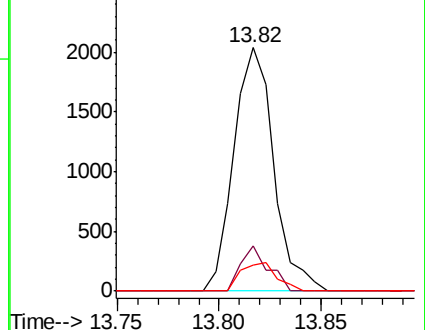


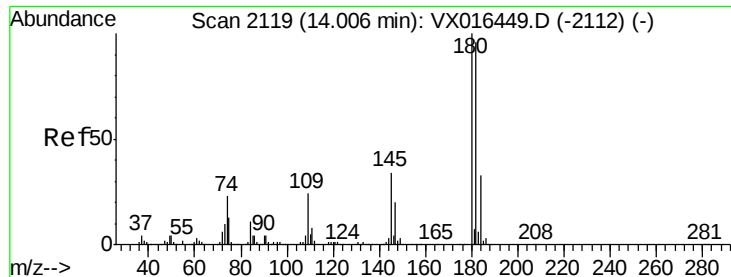

#96
 1,2,3-Trichlorobenzene
 Concen: 0.399 ug/l
 RT: 14.00 min Scan# 2118
 Delta R.T. -0.01 min
 Lab File: VX016695.D
 Acq: 11 Jun 2020 11:47

Instrument :
 MSVOA_X
 ClientSampleId :
 LF012MW031-200608DL

Tgt Ion	Ratio	Lower	Upper
180	100		
182	95.8	48.6	145.8
145	27.7	16.6	49.8

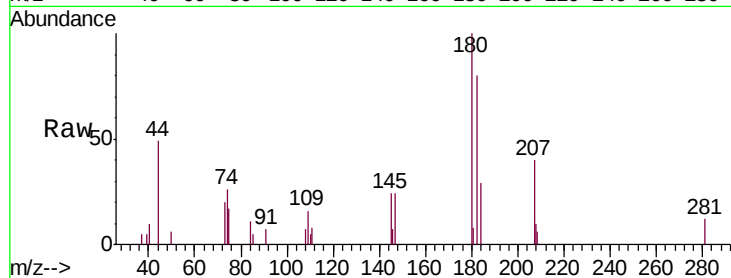

Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.90 (144.60 to 145.60): V

