

Data File : VX016704.D
Acq On : 11 Jun 2020 15:11
Operator : JC/SP
Sample : L2977-05 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-OC-2DL

Quant Time: Jun 12 06:56:06 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260
QLast Update : Wed May 27 16:31:05 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	205891	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	333602	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	346208	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	187718	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	126586	49.51	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.02%	
35) Dibromofluoromethane	5.46	113	106925	52.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.10%	
50) Toluene-d8	8.70	98	411280	51.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.88%	
62) 4-Bromofluorobenzene	11.12	95	174726	56.56	ug/l	0.00
Spiked Amount	50.000		Recovery	=	113.12%	


Target Compounds				Qvalue		
5) Bromomethane	1.62	94	607	0.482	ug/l #	39
10) Methyl Iodide	2.48	142	192	3.136	ug/l #	76
11) Tert butyl alcohol	3.00	59	221	0.337	ug/l #	72
13) Acrolein	2.27	56	116	0.416	ug/l #	1
16) Acetone	2.42	43	23878	21.315	ug/l	96
17) Carbon Disulfide	2.54	76	29572	5.027	ug/l	99
18) Methyl Acetate	2.75	43	609	0.212	ug/l #	57
20) Methylene Chloride	2.83	84	540	0.233	ug/l	91
25) 2-Butanone	4.65	43	5219	2.749	ug/l	98
26) 2,2-Dichloropropane	4.68	77	658	0.204	ug/l #	53
30) Chloroform	5.18	83	8448	2.122	ug/l	91
31) Cyclohexane	5.62	56	3576	1.006	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	14188	4.492	ug/l #	51
37) Ethyl Acetate	4.65	43	5219	1.376	ug/l #	71
38) Carbon Tetrachloride	5.63	117	19604	5.906	ug/l #	16
40) Benzene	6.11	78	7513	0.799	ug/l	97
41) Methacrylonitrile	5.13	41	418	0.201	ug/l #	30
52) Toluene	8.76	92	1962	0.331	ug/l	97
55) 1,1,2-Trichloroethane	9.06	97	902	0.382	ug/l #	14
68) m/p-Xylenes	10.34	106	2797	0.600	ug/l	90
69) o-Xylene	10.68	106	1303	0.289	ug/l	90
76) 1,2,3-Trichloropropane	11.12	75	84239	20.416	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.12	75	84239	50.220	ug/l #	14
95) Naphthalene	13.82	128	138457	10.621	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX016704.D
Acq On : 11 Jun 2020 15:11
Operator : JC/SP
Sample : L2977-05 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-OC-2DL

Quant Time: Jun 12 06:56:06 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260
QLast Update : Wed May 27 16:31:05 2020
Response via : Initial Calibration

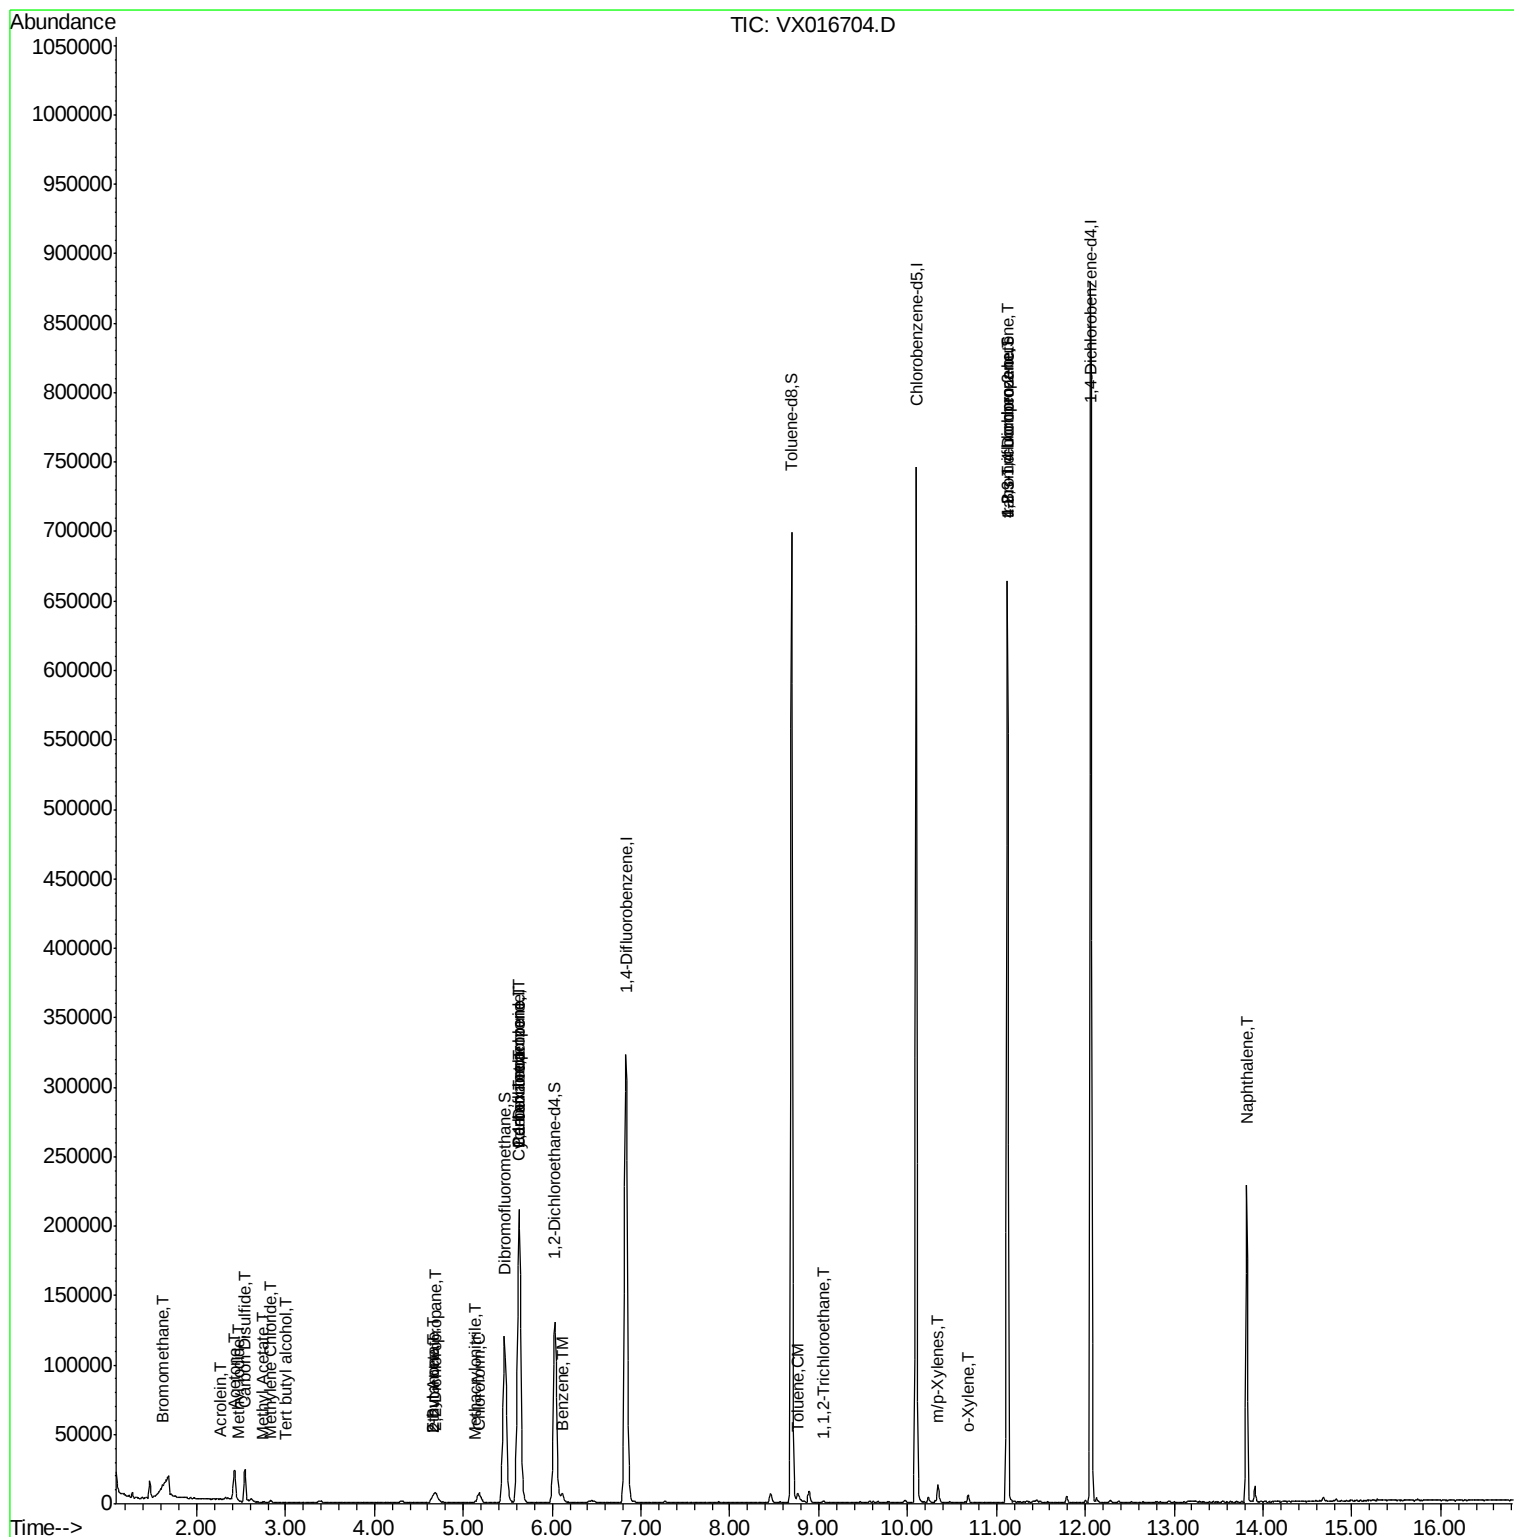



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Instrument :

MSVOA_X

ClientSampleId :


I-OC-2DL

Tgt Ion:168 Resp: 205891

Ion Ratio Lower Upper

168 100

99 54.5 45.2 67.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

80000

60000



40000

20000

0

5.50 5.60 5.70 5.80

Time-->



#5

Bromomethane

Concen: 0.482 ug/l

RT: 1.62 min Scan# 87

Delta R.T. -0.01 min

Lab File: VX016704.D


Acq: 11 Jun 2020 15:11

Tgt Ion: 94 Resp: 607

Ion Ratio Lower Upper

94 100

96 35.0 75.1 112.7#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

300


200


100

0

1.60 1.65

Time-->




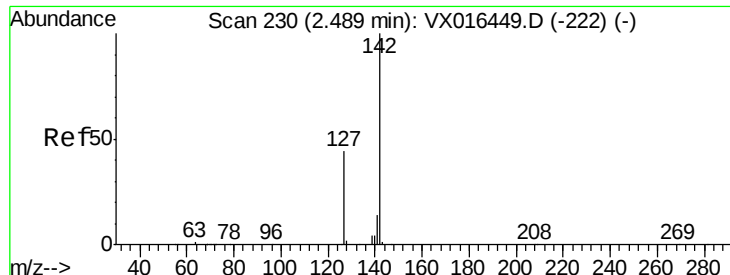




#10
Methyl Iodide
Concen: 3.136 ug/l
RT: 2.48 min Scan# 228
Delta R.T. -0.01 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Instrument :
MSVOA_X
ClientSampled :
I-OC-2DL

Tgt Ion: 142 Resp: 192
Ion Ratio Lower Upper
142 100
127 30.7 35.3 52.9#
141 0.0 11.4 17.2#




Abundance Ion 141.80 (141.50 to 142.50): V
Ion 126.80 (126.50 to 127.50): V
Ion 140.80 (140.50 to 141.50): V


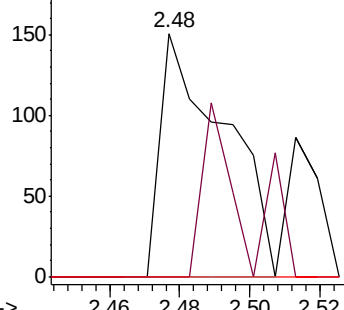



#11
Tert butyl alcohol
Concen: 0.337 ug/l
RT: 3.00 min Scan# 314
Delta R.T. -0.02 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Tgt Ion: 59 Resp: 221
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#



Abundance Ion 59.00 (58.70 to 59.70): VX0
Ion 57.00 (56.70 to 57.70): VX0




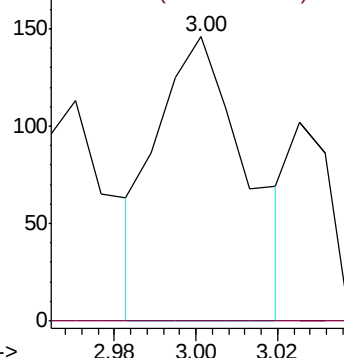


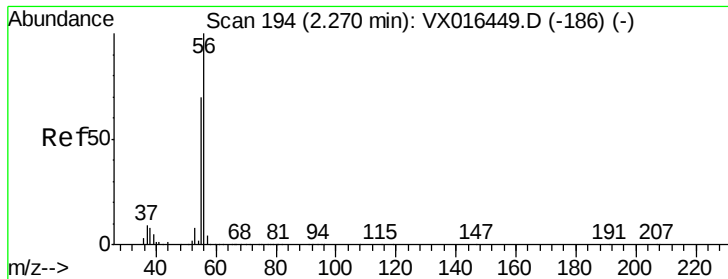

#13
Acrolein
Concen: 0.416 ug/l
RT: 2.27 min Scan# 194
Delta R.T. -0.00 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11




Instrument :
MSVOA_X
ClientSampleId :
I-OC-2DL


Tgt Ion: 56 Resp: 116
Ion Ratio Lower Upper
56 100
55 372.4 58.3 87.5#

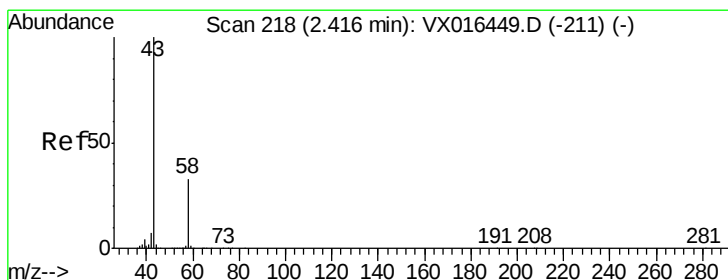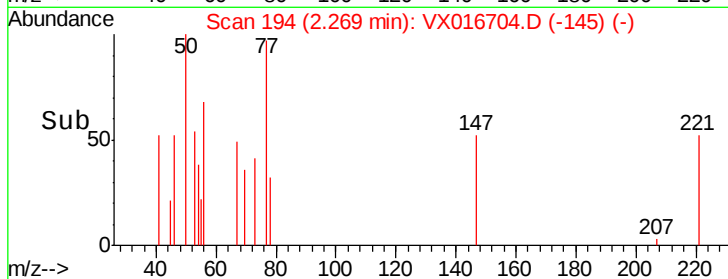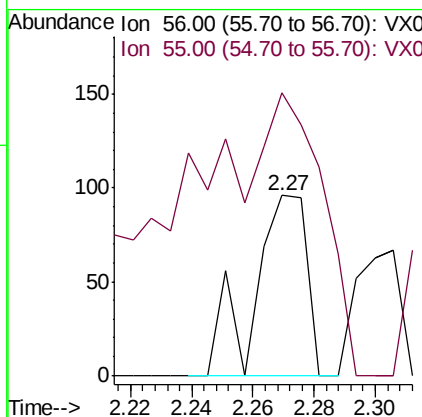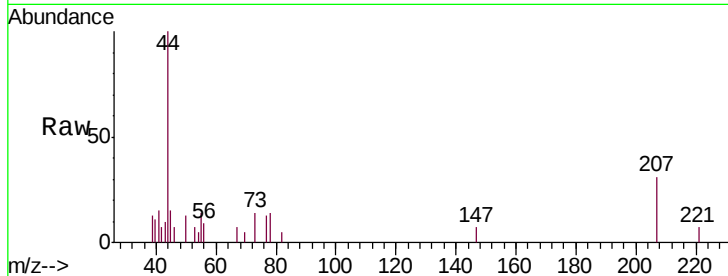

#16
Acetone
Concen: 21.315 ug/l
RT: 2.42 min Scan# 219
Delta R.T. 0.01 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Tgt Ion: 43 Resp: 23878
Ion Ratio Lower Upper
43 100
58 30.5 26.1 39.1


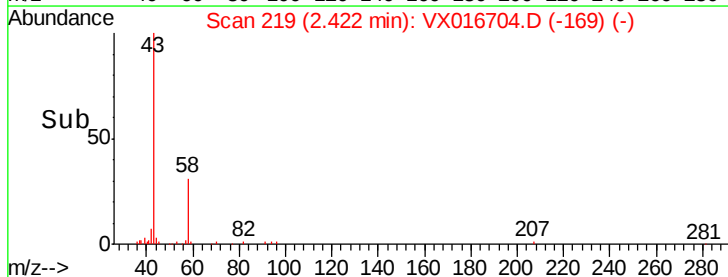
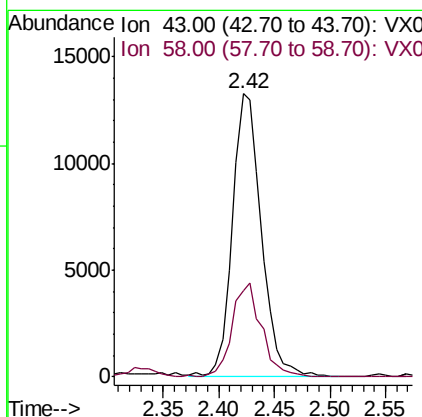
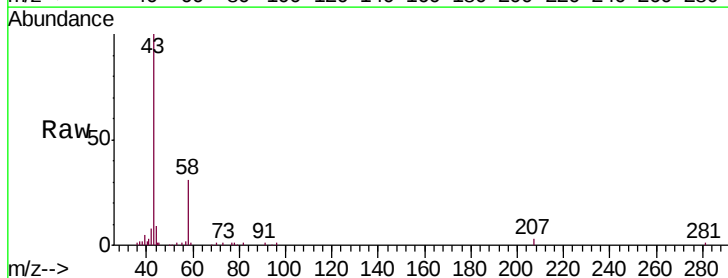




#17
Carbon Disulfide
Concen: 5.027 ug/l
RT: 2.54 min Scan# 239
Delta R.T. -0.01 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11




Instrument :
MSVOA_X
ClientSampleId :
I-OC-2DL


Tgt Ion: 76 Resp: 29572
Ion Ratio Lower Upper
76 100
78 8.7 7.4 11.0

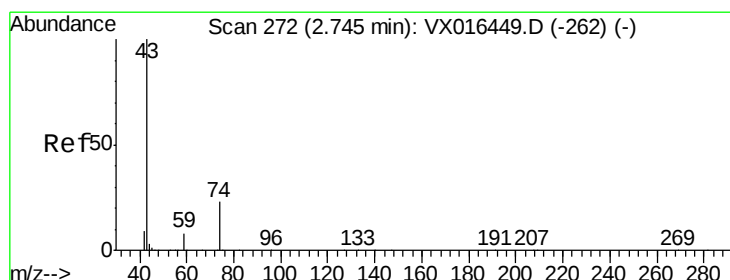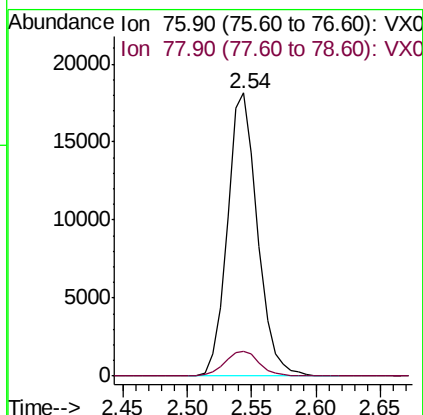

#18
Methyl Acetate
Concen: 0.212 ug/l
RT: 2.75 min Scan# 272
Delta R.T. -0.00 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Tgt Ion: 43 Resp: 609
Ion Ratio Lower Upper
43 100
74 3.3 19.7 29.5#

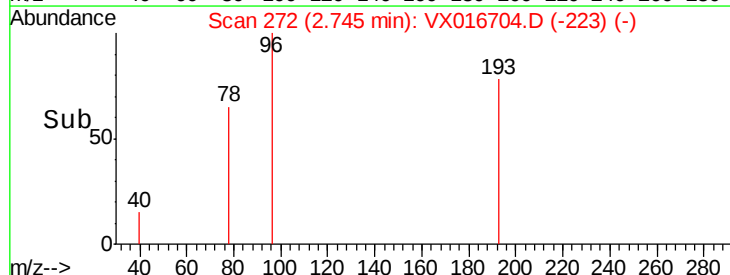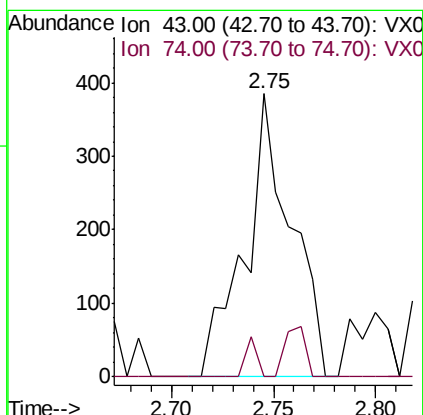







#20
Methylene Chloride
Concen: 0.233 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Instrument :
MSVOA_X
ClientSampleId :
I-OC-2DL

Tgt Ion:	84	Resp:	540
Ion	Ratio	Lower	Upper
84	100		
49	105.1	94.5	141.7
51	39.5	30.2	45.4
86	68.4	51.1	76.7




Abundance Ion 83.90 (83.60 to 84.60): VX0
Ion 48.90 (48.60 to 49.60): VX0
Ion 50.90 (50.60 to 51.60): VX0
Ion 85.90 (85.60 to 86.60): VX0


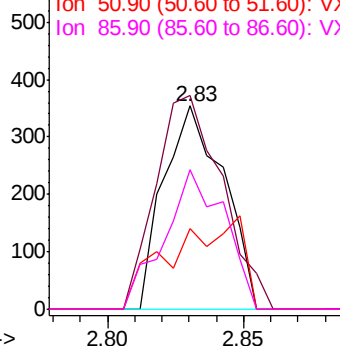



#25
2-Butanone
Concen: 2.749 ug/l
RT: 4.65 min Scan# 585
Delta R.T. 0.02 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Tgt Ion:	43	Resp:	5219
Ion	Ratio	Lower	Upper
43	100		
72	27.4	21.0	31.6



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 72.00 (71.70 to 72.70): VX0




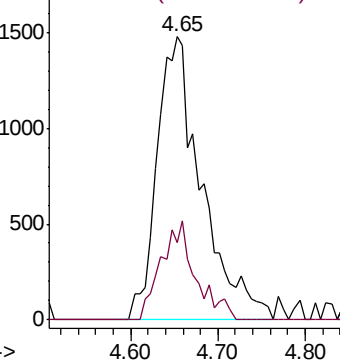


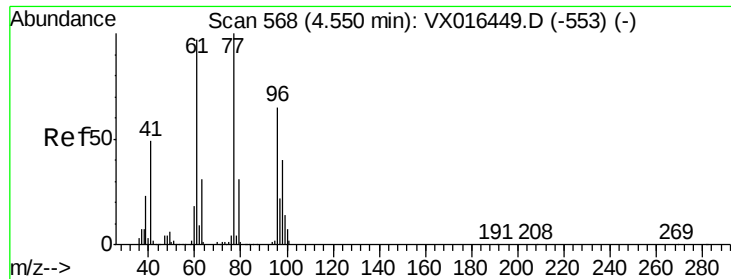

#26
 2,2-Dichloropropane
 Concen: 0.204 ug/l
 RT: 4.68 min Scan# 590
 Delta R.T. 0.13 min
 Lab File: VX016704.D
 Acq: 11 Jun 2020 15:11




Instrument :
 MSVOA_X
 ClientSampled :
 I-OC-2DL


Tgt Ion: 77 Resp: 658
 Ion Ratio Lower Upper
 77 100
 97 0.0 11.5 34.4#

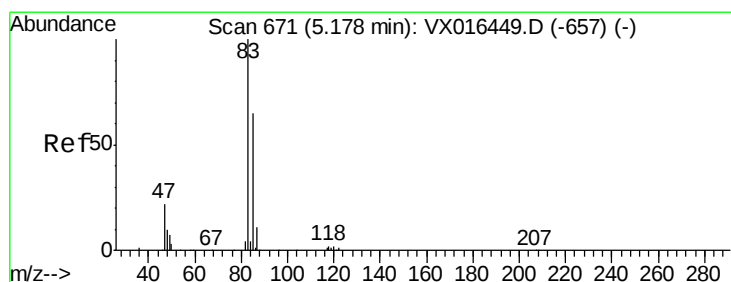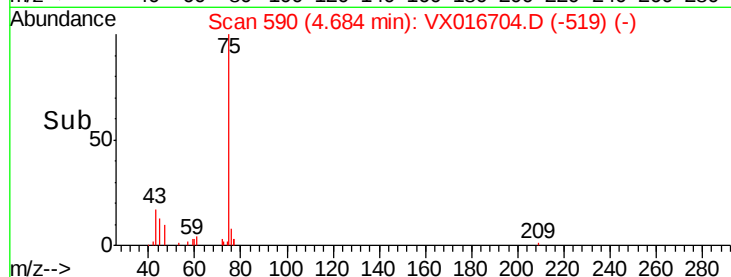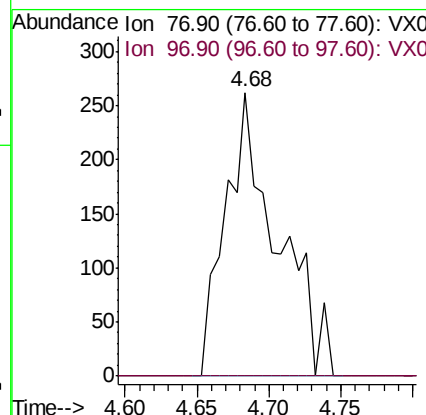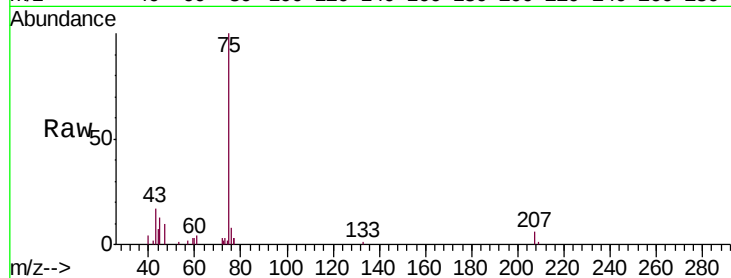

#30
 Chloroform
 Concen: 2.122 ug/l
 RT: 5.18 min Scan# 671
 Delta R.T. -0.00 min
 Lab File: VX016704.D
 Acq: 11 Jun 2020 15:11

Tgt Ion: 83 Resp: 8448
 Ion Ratio Lower Upper
 83 100
 85 71.7 52.0 78.0


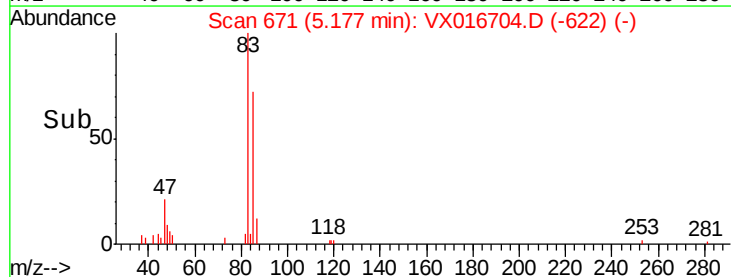
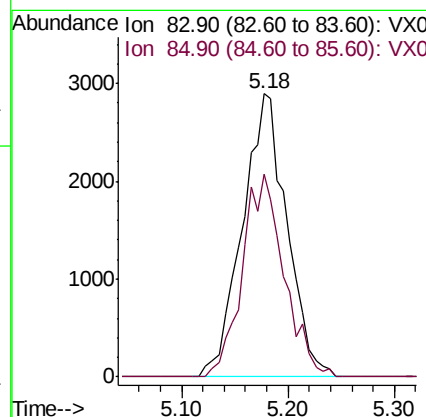
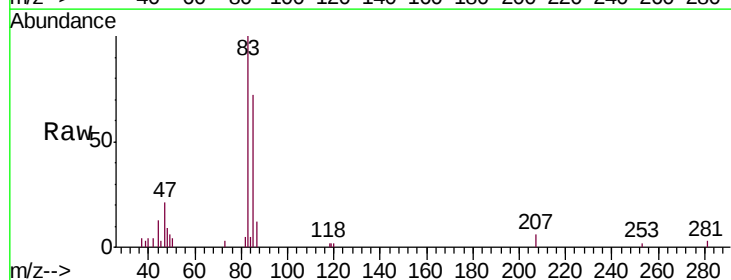


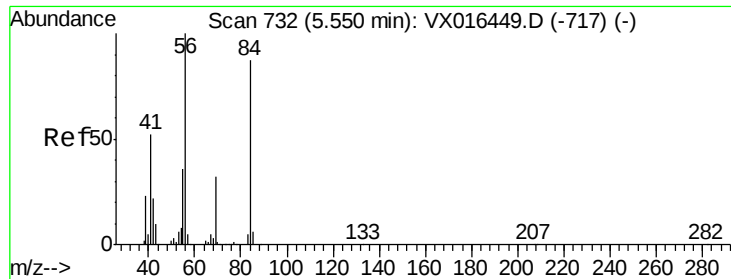

#31
Cyclohexane
Concen: 1.006 ug/l
RT: 5.62 min Scan# 743
Delta R.T. 0.07 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11




Instrument :
MSVOA_X
ClientSampleId :
I-OC-2DL


Tgt Ion: 56 Resp: 3576
Ion Ratio Lower Upper
56 100
69 179.8 25.7 38.5#
84 140.6 70.0 105.0#

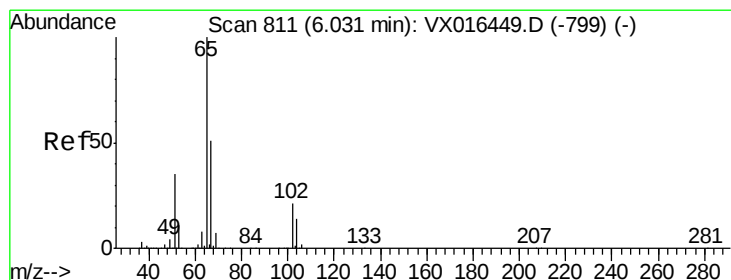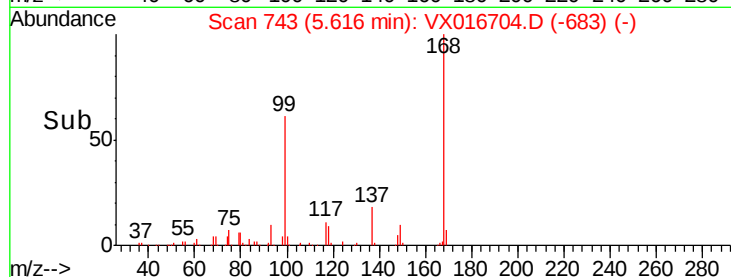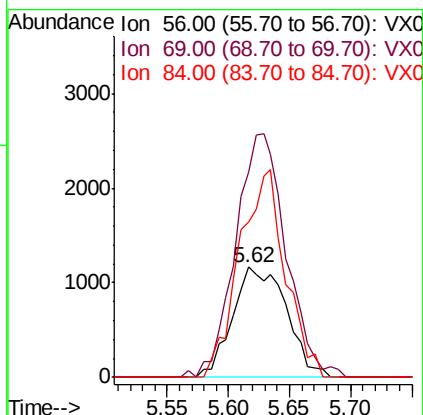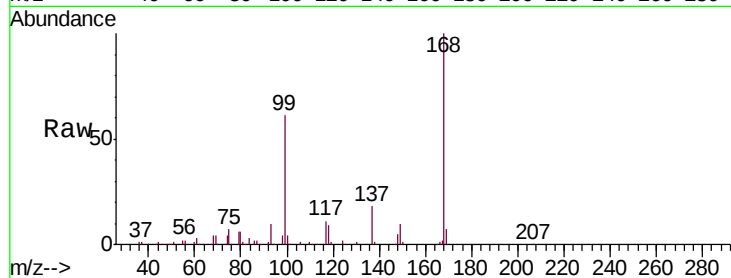

#33
1,2-Dichloroethane-d4
Concen: 49.508 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Tgt Ion: 65 Resp: 126586
Ion Ratio Lower Upper
65 100
67 52.7 0.0 104.8

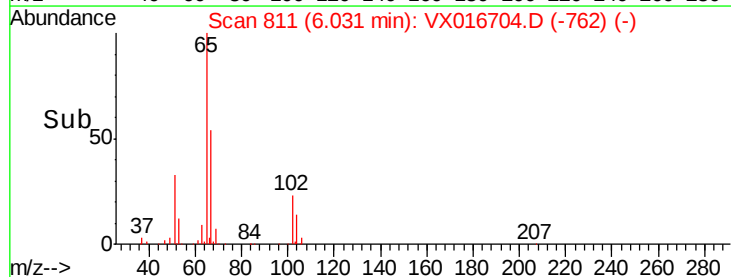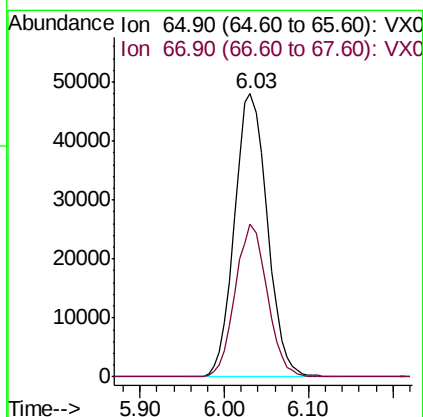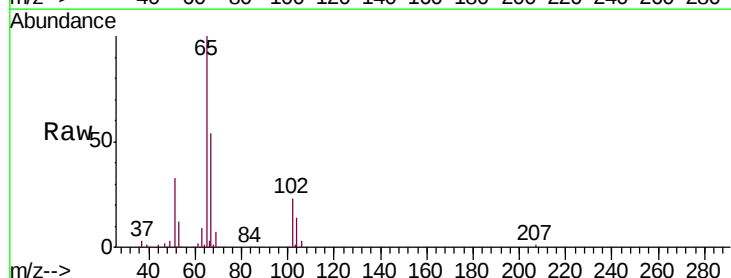



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Instrument :

MSVOA_X

ClientSampleId :

I-OC-2DL


Tgt Ion:114 Resp: 333602

Ion Ratio Lower Upper

114 100

63 18.9 0.0 42.6




88 16.7 0.0 32.8



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

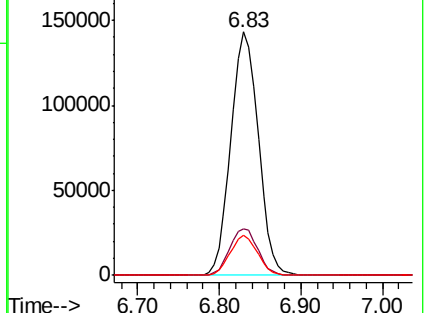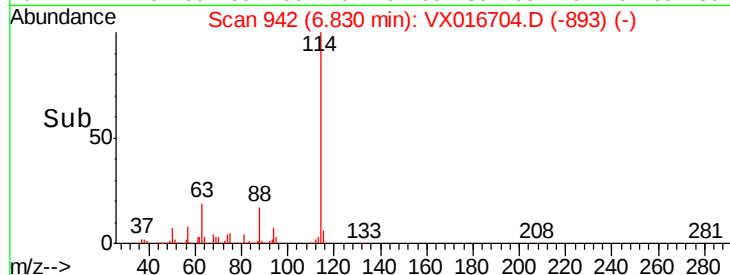

#35

Dibromofluoromethane

Concen: 52.053 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11


Tgt Ion:113 Resp: 106925

Ion Ratio Lower Upper

113 100

111 101.1 83.0 124.6



192 22.8 17.7 26.5




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

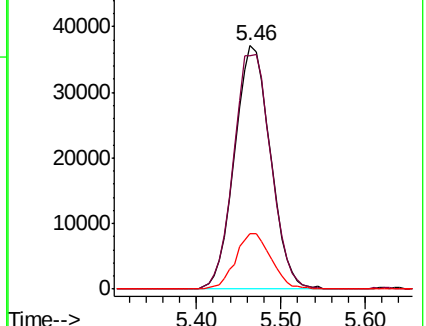



#36

1,1-Dichloropropene

Concen: 4.492 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.14 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Instrument :

MSVOA_X

ClientSampleId :

I-OC-2DL


Tgt Ion: 75 Resp: 14188

Ion Ratio Lower Upper

75 100

110 9.8 17.4 52.3#




77 0.0 24.2 36.4#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

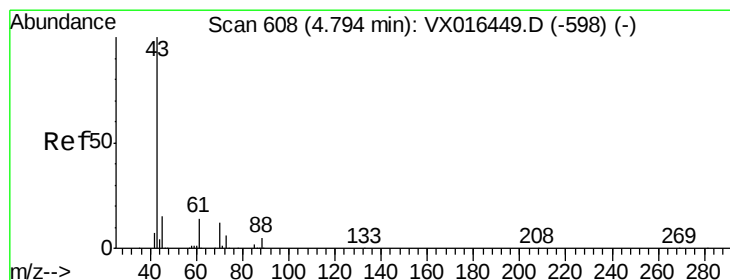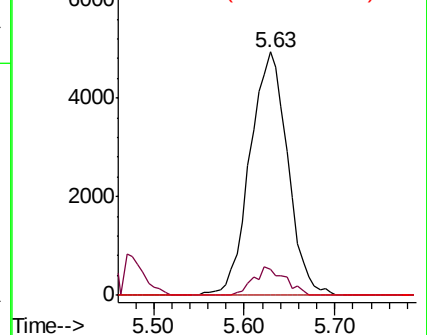

#37

Ethyl Acetate

Concen: 1.376 ug/l

RT: 4.65 min Scan# 585

Delta R.T. -0.14 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11


Tgt Ion: 43 Resp: 5219

Ion Ratio Lower Upper

43 100

61 3.0 11.3 16.9#



70 0.0 9.3 13.9#




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

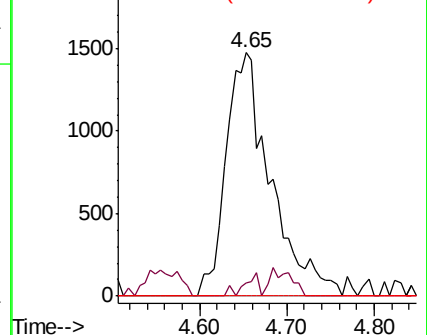



#38

Carbon Tetrachloride

Concen: 5.906 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.13 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Instrument :

MSVOA_X

ClientSampleId :

I-OC-2DL


Tgt Ion:117 Resp: 19604

Ion Ratio Lower Upper

117 100

119 4.5 76.3 114.5#




121 0.0 24.6 37.0#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

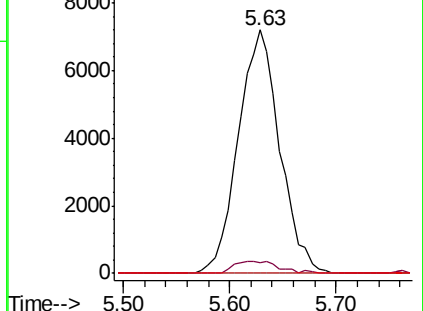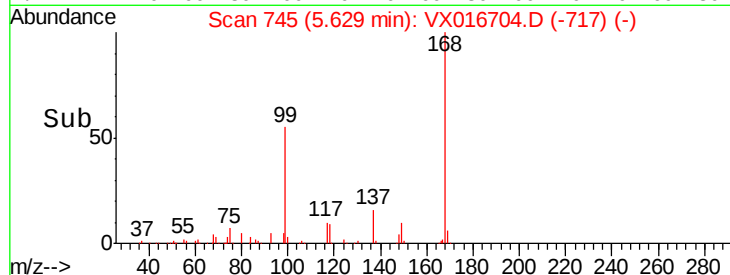

#40

Benzene

Concen: 0.799 ug/l

RT: 6.11 min Scan# 824

Delta R.T. -0.00 min

Lab File: VX016704.D


Acq: 11 Jun 2020 15:11

Tgt Ion: 78 Resp: 7513

Ion Ratio Lower Upper



78 100


77 24.9 18.9 28.3



Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

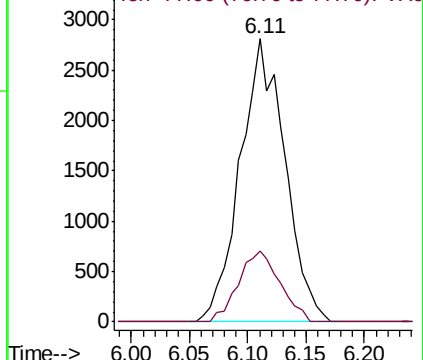


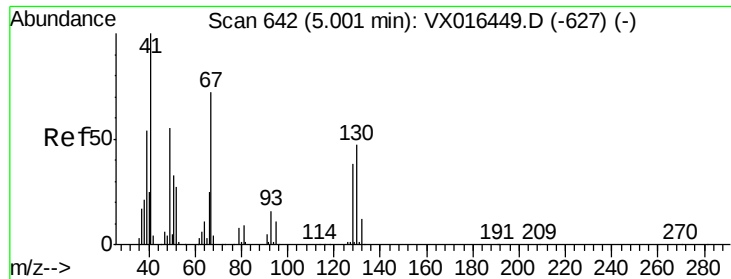




#41
Methacrylonitrile
Concen: 0.201 ug/l
RT: 5.13 min Scan# 663
Delta R.T. 0.13 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Instrument :
MSVOA_X
ClientSampleId :
I-OC-2DL

Tgt Ion: 41 Resp: 418
Ion Ratio Lower Upper
41 100
39 14.1 43.0 64.4#
67 0.0 58.9 88.3#
52 0.0 23.1 34.7#

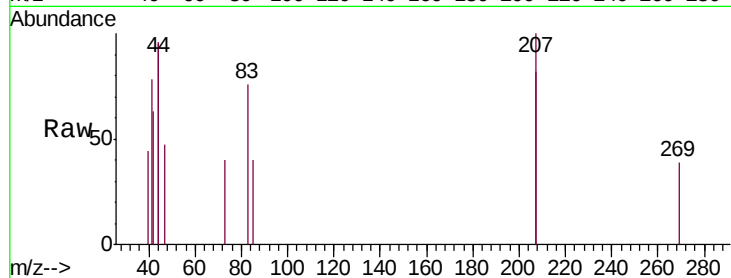


Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 39.00 (38.70 to 39.70): VX0
Ion 67.00 (66.70 to 67.70): VX0
Ion 52.00 (51.70 to 52.70): VX0

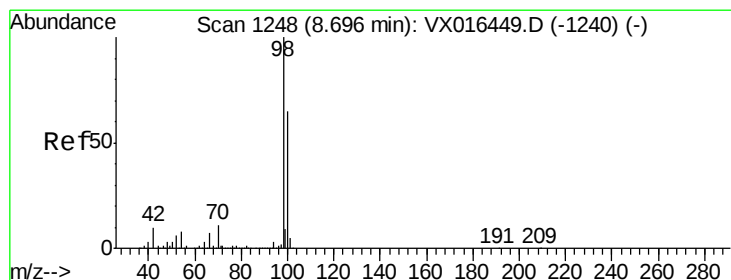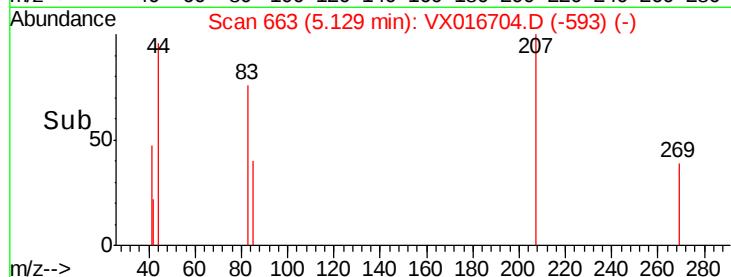
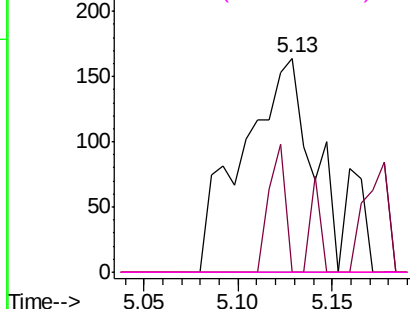



#50
Toluene-d8
Concen: 51.441 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Tgt Ion: 98 Resp: 411280
Ion Ratio Lower Upper
98 100
100 66.2 53.8 80.6

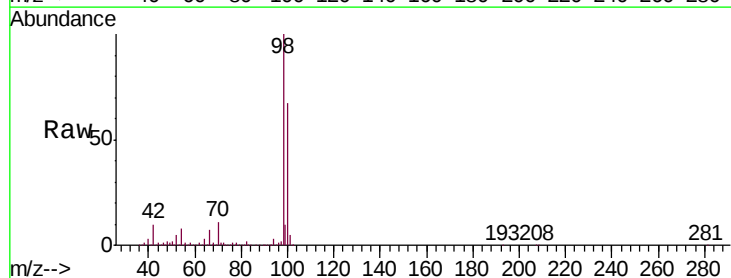

Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): V

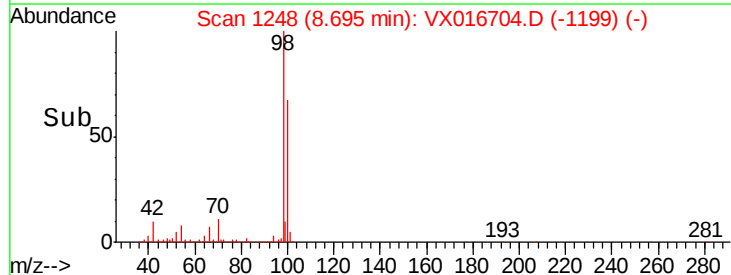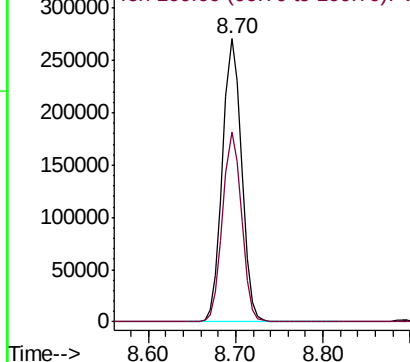

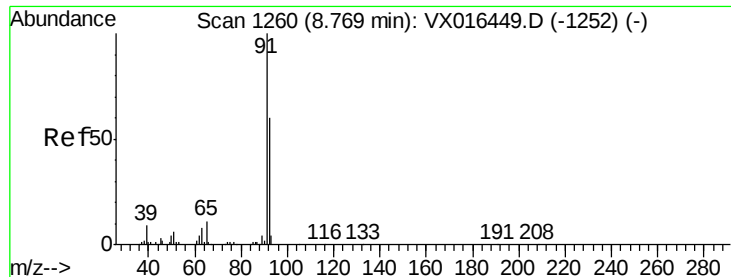

#52

Toluene

Concen: 0.331 ug/l

RT: 8.76 min Scan# 1259

Delta R.T. -0.01 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Instrument :

MSVOA_X

ClientSampleId :


I-OC-2DL

Tgt Ion: 92 Resp: 1962

Ion Ratio Lower Upper




92 100

91 173.0 135.0 202.4

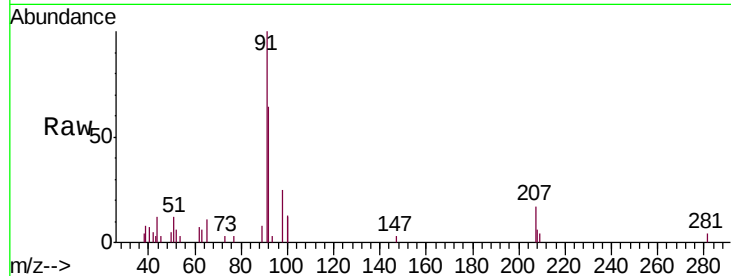

Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0

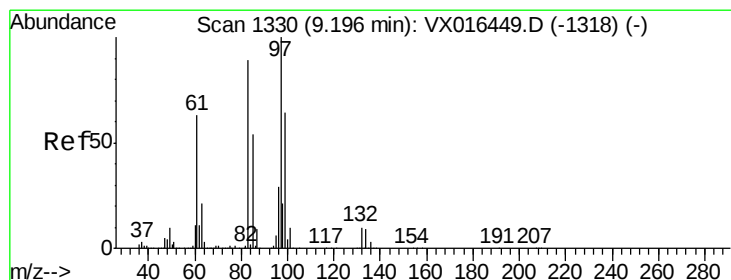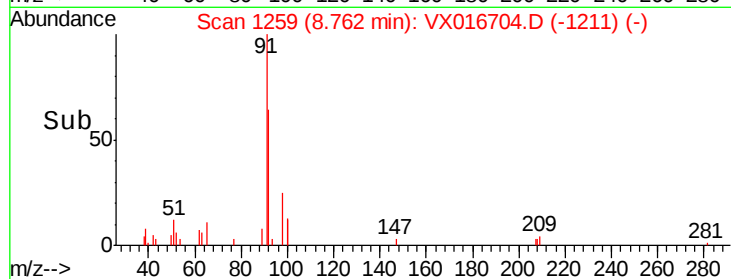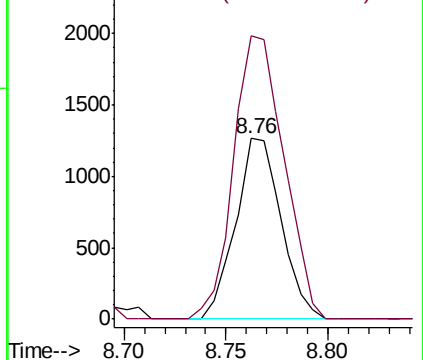

#55

1,1,2-Trichloroethane

Concen: 0.382 ug/l

RT: 9.06 min Scan# 1308

Delta R.T. -0.13 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Tgt Ion: 97 Resp: 902


Ion Ratio Lower Upper

97 100

83 0.0 70.9 106.3#

85 0.0 43.4 65.2#

99 0.0 51.0 76.6#


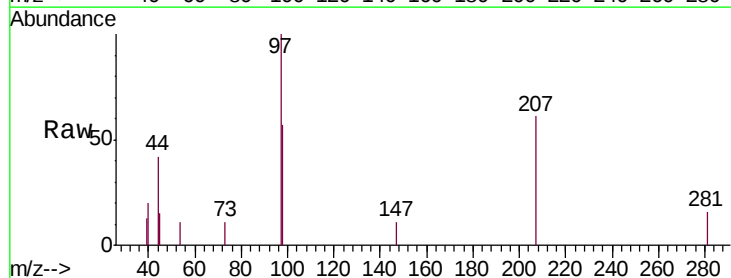



Abundance Ion 96.90 (96.60 to 97.60): VX0

Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

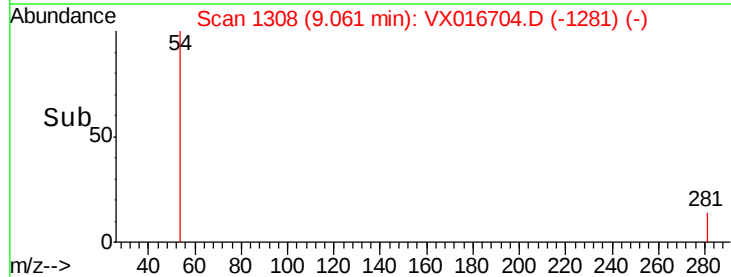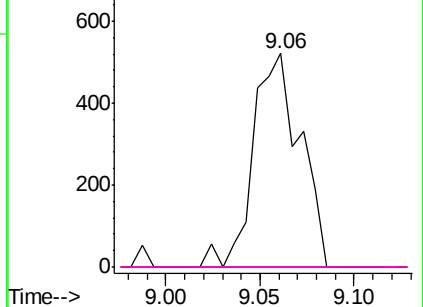



#62

4-Bromofluorobenzene

Concen: 56.558 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Instrument :

MSVOA_X

ClientSampleId :

I-OC-2DL


Tgt Ion: 95 Resp: 174726

Ion Ratio Lower Upper

95 100

174 86.5 0.0 163.0




176 82.1 0.0 156.8



Abundance Ion 94.90 (94.60 to 95.60): VX016704.D (-1597) (-)

Ion 173.80 (173.50 to 174.50): VX016704.D (-1597) (-)

Ion 175.80 (175.50 to 176.50): VX016704.D (-1597) (-)

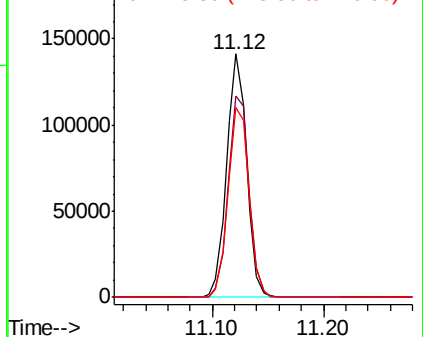

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11


Tgt Ion: 117 Resp: 346208

Ion Ratio Lower Upper

117 100

82 52.7 45.0 67.6



119 31.2 25.8 38.8




Abundance Ion 116.90 (116.60 to 117.60): VX016704.D (-1429) (-)

Ion 82.00 (81.70 to 82.70): VX016704.D (-1429) (-)

Ion 118.90 (118.60 to 119.60): VX016704.D (-1429) (-)

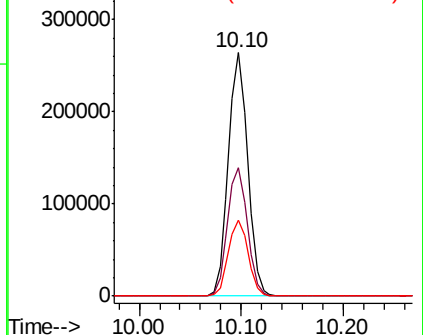







#68
m/p-Xylenes
Concen: 0.600 ug/l
RT: 10.34 min Scan# 1518
Delta R.T. -0.00 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Instrument :
MSVOA_X
ClientSampleId :
I-OC-2DL

Tgt Ion:106 Resp: 2797
Ion Ratio Lower Upper
106 100
91 188.7 163.8 245.8




Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0

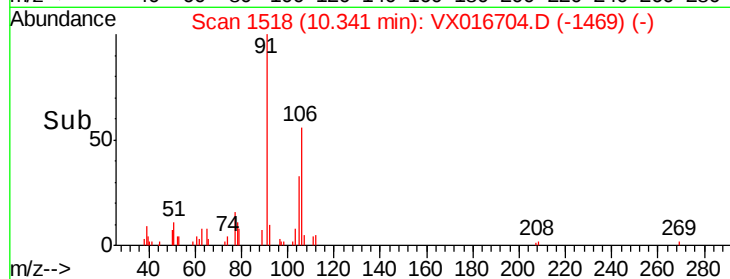
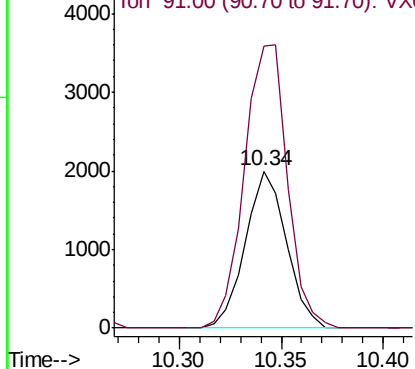



#69
o-Xylene
Concen: 0.289 ug/l
RT: 10.68 min Scan# 1574
Delta R.T. -0.00 min
Lab File: VX016704.D
Acq: 11 Jun 2020 15:11

Tgt Ion:106 Resp: 1303
Ion Ratio Lower Upper
106 100
91 203.5 109.6 328.8



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0

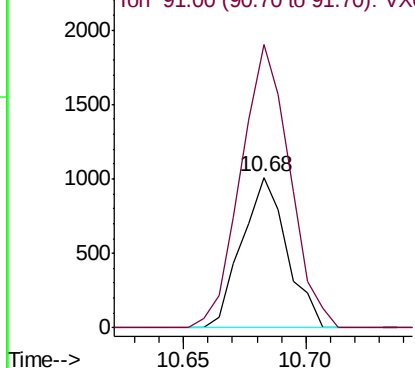



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Instrument :

MSVOA_X

ClientSampled :

I-OC-2DL


Tgt Ion: 152 Resp: 187718

Ion Ratio Lower Upper

152 100

115 57.9 39.9 119.6




150 157.2 0.0 341.0



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

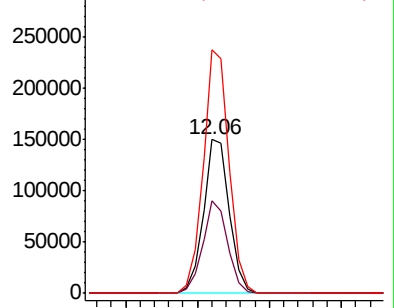

#76

1,2,3-Trichloropropane

Concen: 20.416 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX016704.D


Acq: 11 Jun 2020 15:11

Tgt Ion: 75 Resp: 84239

Ion Ratio Lower Upper



75 100


77 1.3 21.3 63.7#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

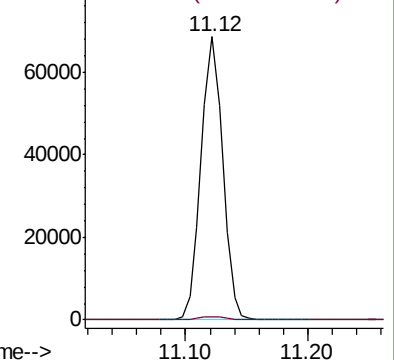



#81

trans-1,4-Dichloro-2-butene

Concen: 50.220 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Instrument :

MSVOA_X

ClientSampleId :

I-OC-2DL





Tgt Ion: 75 Resp: 84239

Ion Ratio Lower Upper

75 100

53 0.2 71.3 106.9#

89 0.0 36.6 55.0#

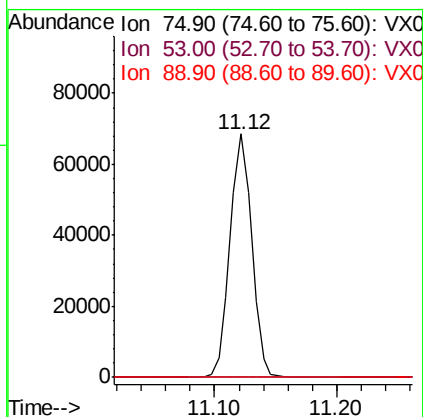

#95

Naphthalene

Concen: 10.621 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. -0.00 min

Lab File: VX016704.D

Acq: 11 Jun 2020 15:11

Tgt Ion: 128 Resp: 138457

Ion Ratio Lower Upper

128 100

127 12.7 10.6 15.8

129 11.1 8.6 13.0

