


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061120\
Data File : VX016691.D
Acq On : 11 Jun 2020 09:11
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Title : SW846 8260
Last Update : Wed May 27 16:31:05 2020

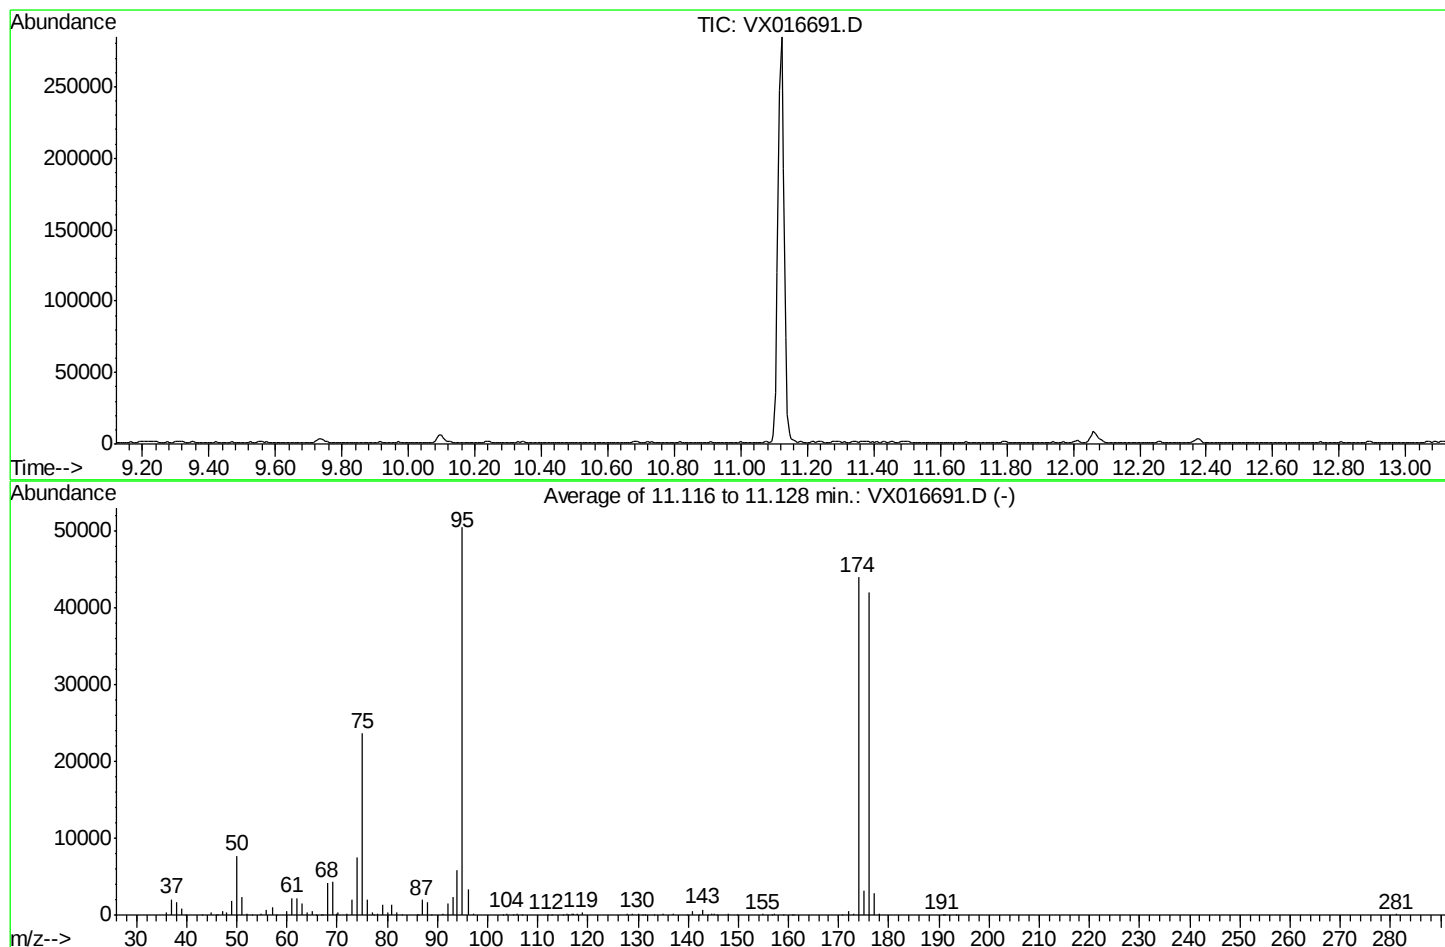

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	7743	PASS
75	95	30	60	46.8	23602	PASS
95	95	100	100	100.0	50408	PASS
96	95	5	9	6.6	3311	PASS
173	174	0.00	2	0.4	167	PASS
174	95	50	100	87.2	43941	PASS
175	174	5	9	7.4	3230	PASS
176	174	95	101	95.4	41904	PASS
177	176	5	9	6.8	2856	PASS