

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061121\
 Data File : VX022669.D
 Acq On : 11 Jun 2021 15:56
 Operator : JC/MD
 Sample : M2688-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1

Quant Time: Jun 12 02:29:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 10 12:20:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	58667	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	117674	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	103724	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	41093	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	49705	47.109	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	94.220%		
35) Dibromofluoromethane	5.397	113	34610	46.098	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.200%		
50) Toluene-d8	8.653	98	144067	48.677	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.360%		
62) 4-Bromofluorobenzene	11.085	95	50609	45.213	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.420%		
Target Compounds						
						Qvalue
6) Chloroethane	1.672	64	101	0.204	ug/l	# 43
11) Tert butyl alcohol	2.971	59	980	4.011	ug/l	# 73
13) Acrolein	2.251	56	59	0.576	ug/l	# 14
14) Allyl chloride	2.788	41	671	0.487	ug/l	# 76
16) Acetone	2.386	43	6828	14.452	ug/l	92
17) Carbon Disulfide	2.526	76	425	0.265	ug/l	# 75
23) Vinyl Acetate	3.446	43	587	0.234	ug/l	# 8
25) 2-Butanone	4.580	43	3626	4.732	ug/l	# 75
31) Cyclohexane	5.489	56	3224	2.533	ug/l	# 78
36) 1,1-Dichloropropene	5.562	75	6048	5.158	ug/l	# 48
37) Ethyl Acetate	4.580	43	3626	2.433	ug/l	# 64
38) Carbon Tetrachloride	5.562	117	7005	6.984	ug/l	# 15
39) Methylcyclohexane	7.391	83	1727	1.412	ug/l	90
40) Benzene	6.037	78	1632	0.468	ug/l	95
48) Methyl methacrylate	7.677	41	385	0.341	ug/l	# 10
51) 4-Methyl-2-Pentanone	8.580	43	887	0.594	ug/l	# 82
52) Toluene	8.726	92	22383	10.310	ug/l	97
53) t-1,3-Dichloropropene	8.726	75	245	3.416	ug/l	# 1
55) 1,1,2-Trichloroethane	9.110	97	187	0.211	ug/l	# 15
56) Ethyl methacrylate	9.073	69	19	2.304	ug/l	# 29
67) Ethyl Benzene	10.195	91	16354	4.109	ug/l	99
68) m/p-Xylenes	10.305	106	24647	17.098	ug/l	99
69) o-Xylene	10.646	106	10724	7.678	ug/l	97
70) Styrene	10.646	104	631	1.692	ug/l	# 1
73) Isopropylbenzene	10.963	105	2966	0.879	ug/l	94
76) 1,2,3-Trichloropropane	11.085	75	27922	25.627	ug/l	# 39
78) n-propylbenzene	11.305	91	4593	1.127	ug/l	99
79) 2-Chlorotoluene	11.384	91	2573	1.043	ug/l	# 41
80) 1,3,5-Trimethylbenzene	11.457	105	5101	1.815	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.085	75	27922	64.376	ug/l	# 12
82) 4-Chlorotoluene	11.451	91	737	0.261	ug/l	# 45
83) tert-Butylbenzene	11.756	119	2401	0.910	ug/l	# 51
84) 1,2,4-Trimethylbenzene	11.756	105	20112	7.055	ug/l	95
85) sec-Butylbenzene	11.896	105	2247	0.652	ug/l	89
89) n-Butylbenzene	12.329	91	1355	0.497	ug/l	# 3
90) Hexachloroethane	12.530	117	322	4.303	ug/l	# 9

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061121\
Data File : VX022669.D
Acq On : 11 Jun 2021 15:56
Operator : JC/MD
Sample : M2688-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Time: Jun 12 02:29:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 12:20:00 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
92) 1,2-Dibromo-3-Chloropr...	13.170	75	30	4.037	ug/l #	1
95) Naphthalene	13.780	128	5526	3.010	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061121\
Data File : VX022669.D
Acq On : 11 Jun 2021 15:56
Operator : JC/MD
Sample : M2688-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Time: Jun 12 02:29:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 12:20:00 2021
Response via : Initial Calibration




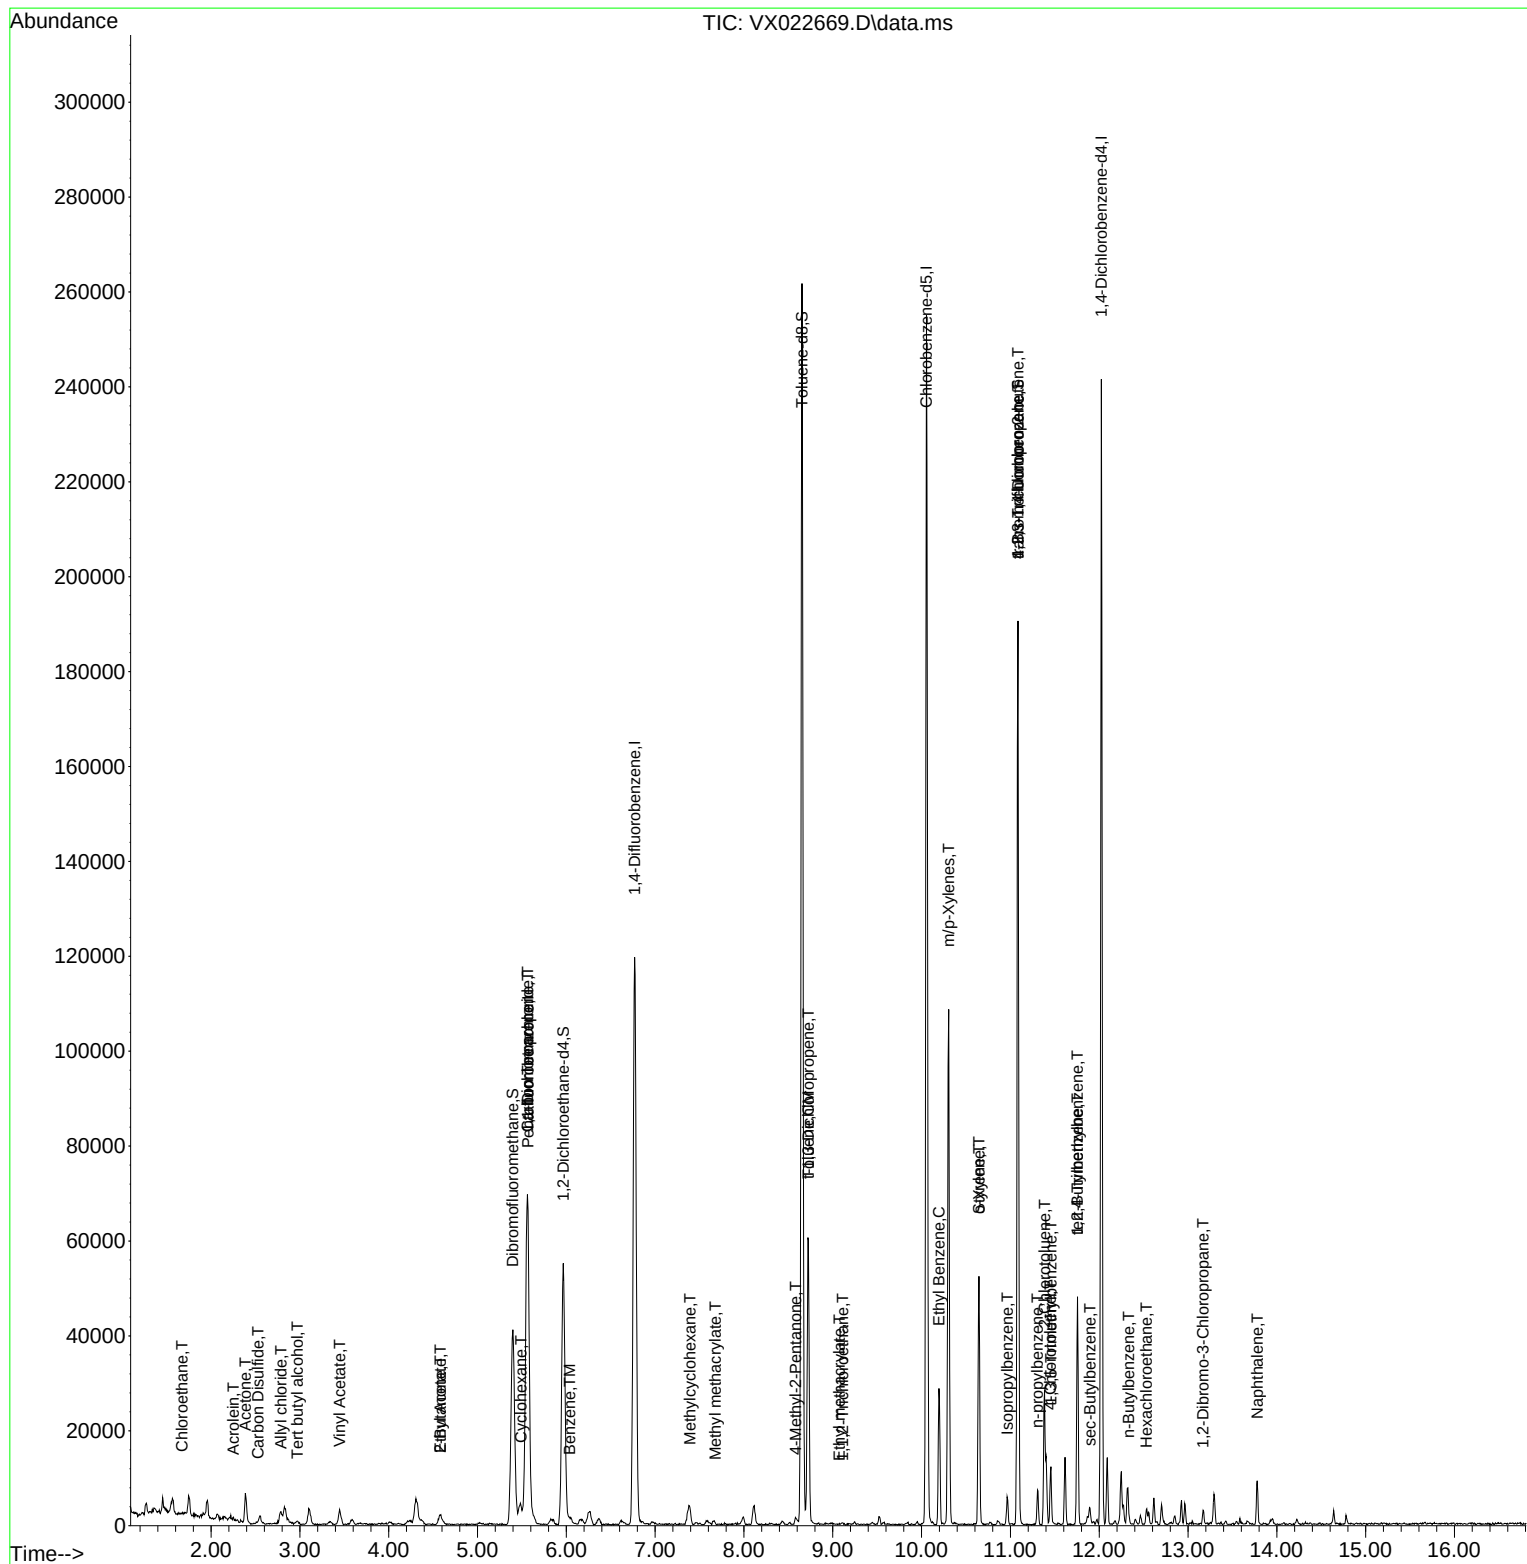




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.006 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion:168 Resp: 58667
Ion Ratio Lower Upper
168 100
99 70.8 45.8 68.6#

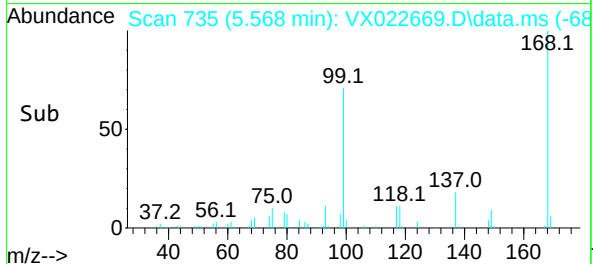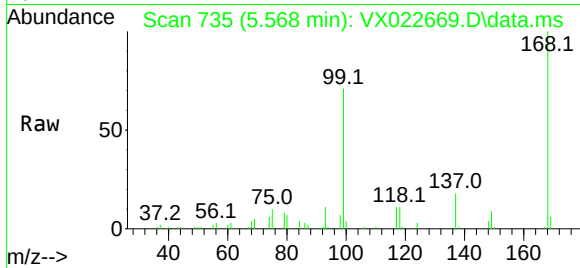

#6
Chloroethane
Concen: 0.204 ug/l
RT: 1.672 min Scan# 96
Delta R.T. -0.007 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 64 Resp: 101
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

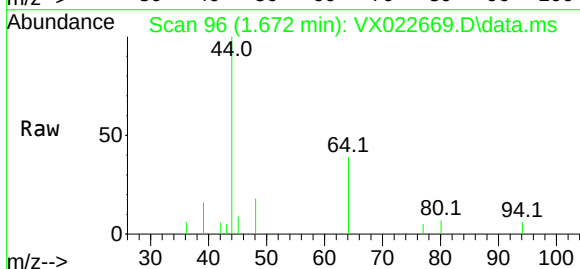







#11

Tert butyl alcohol
Concen: 4.011 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Instrument :
MSVOA_X
ClientSampled :
MW-1




Tgt Ion: 59 Resp: 980
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

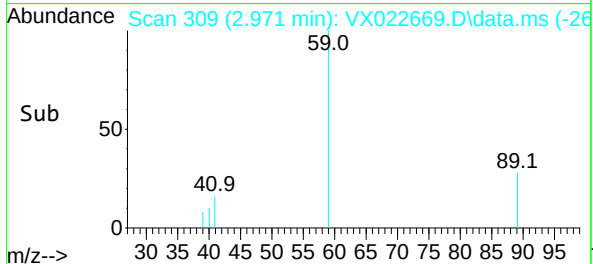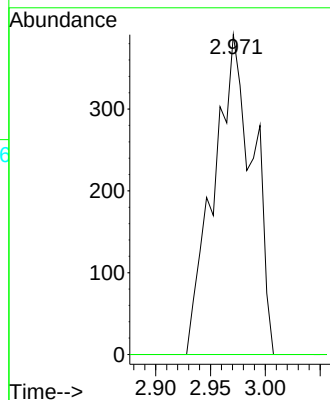


#13

Acrolein
Concen: 0.576 ug/l
RT: 2.251 min Scan# 191
Delta R.T. 0.012 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 56 Resp: 59
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#



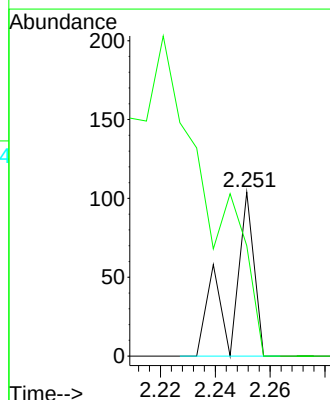
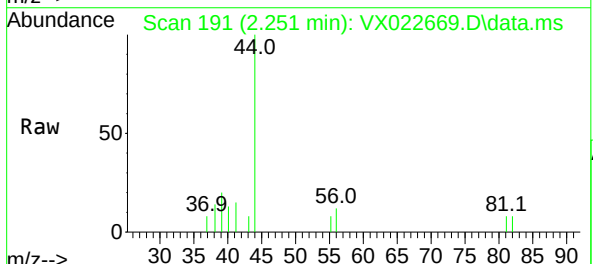


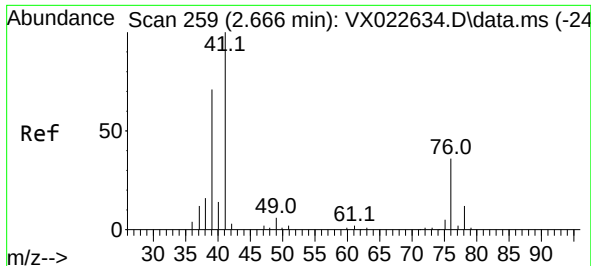

#14
Allyl chloride
Concen: 0.487 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.122 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 41 Resp: 671
Ion Ratio Lower Upper
41 100
39 64.2 51.6 77.4
76 0.0 30.5 45.7#

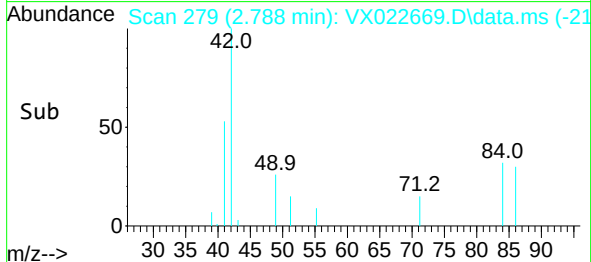

#16
Acetone
Concen: 14.452 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 43 Resp: 6828
Ion Ratio Lower Upper
43 100
58 30.3 27.8 41.8


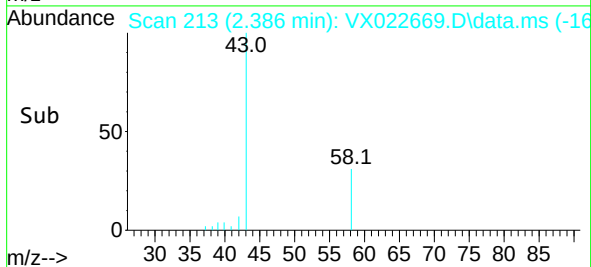

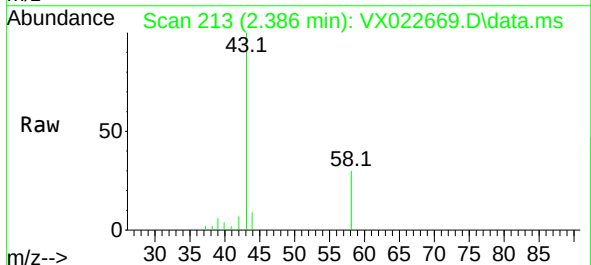




#17
Carbon Disulfide
Concen: 0.265 ug/l
RT: 2.526 min Scan# 236
Delta R.T. 0.012 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion: 76 Resp: 425
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

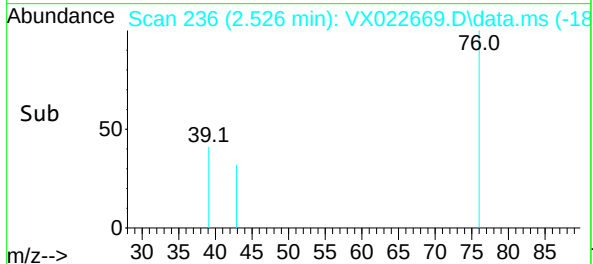

#23
Vinyl Acetate
Concen: 0.234 ug/l
RT: 3.446 min Scan# 387
Delta R.T. -0.281 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 43 Resp: 587
Ion Ratio Lower Upper
43 100
86 48.6 9.9 14.9#


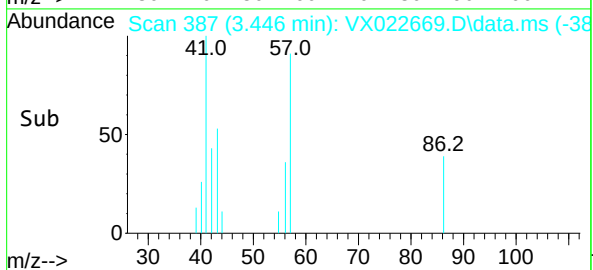

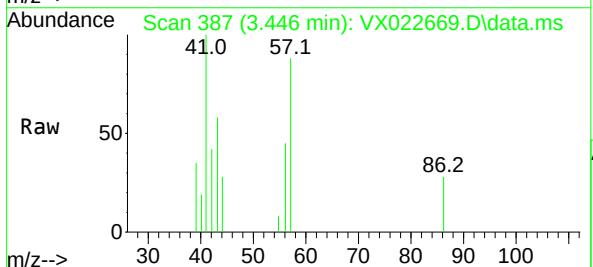




#25
2-Butanone
Concen: 4.732 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.012 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion: 43 Resp: 3626
Ion Ratio Lower Upper
43 100
72 16.2 23.7 35.5#

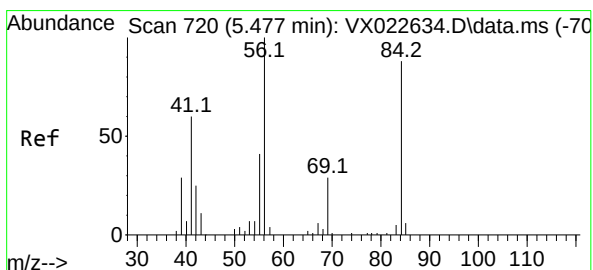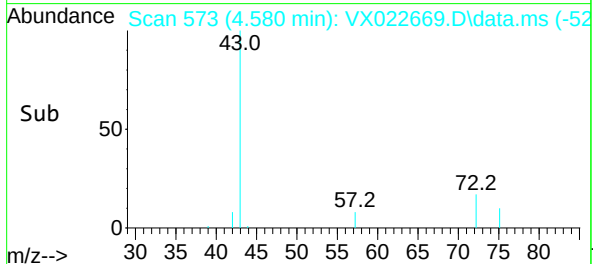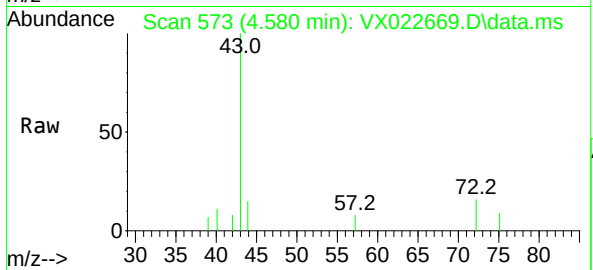

#31
Cyclohexane
Concen: 2.533 ug/l
RT: 5.489 min Scan# 722
Delta R.T. 0.012 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 56 Resp: 3224
Ion Ratio Lower Upper
56 100
69 24.8 25.3 37.9#
84 65.5 71.4 107.0#

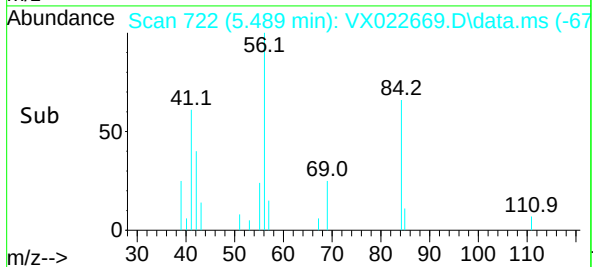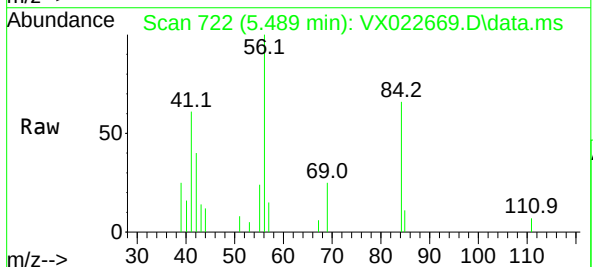







#33

1,2-Dichloroethane-d4
Concen: 47.109 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Instrument :
MSVOA_X
ClientSampled :
MW-1




Tgt Ion: 65 Resp: 49705
Ion Ratio Lower Upper
65 100
67 53.4 0.0 105.4




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 114 Resp: 117674
Ion Ratio Lower Upper
114 100
63 21.6 0.0 40.8
88 16.9 0.0 32.8

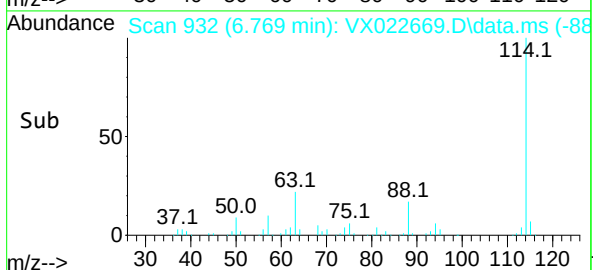



#35

Dibromofluoromethane

Concen: 46.098 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.006 min

Lab File: VX022669.D

Acq: 11 Jun 2021 15:56





Tgt Ion:113 Resp: 34610

Ion Ratio Lower Upper

113 100

111 106.7 81.9 122.9

192 16.5 16.7 25.1#

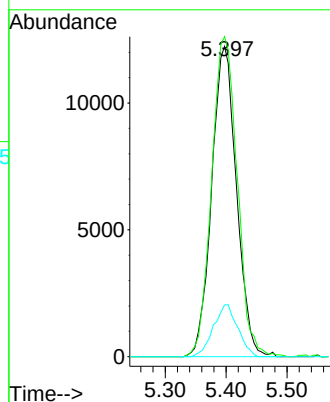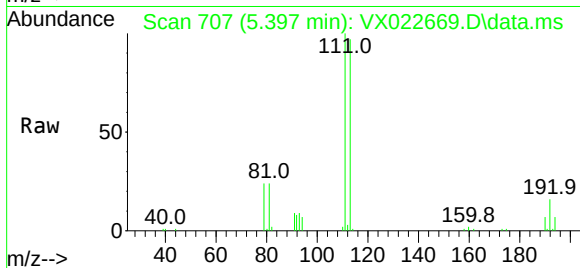

#36

1,1-Dichloropropene

Concen: 5.158 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.140 min

Lab File: VX022669.D

Acq: 11 Jun 2021 15:56




Tgt Ion: 75 Resp: 6048


Ion Ratio Lower Upper

75 100

110 7.9 18.1 54.4#

77 0.0 25.3 37.9#

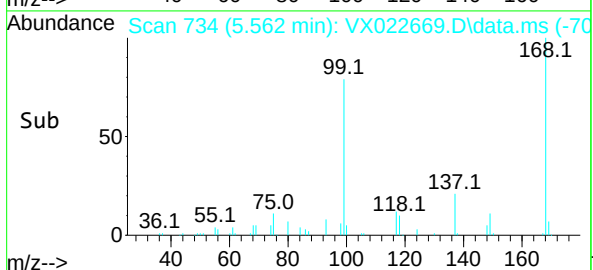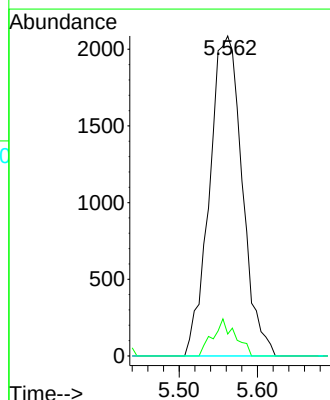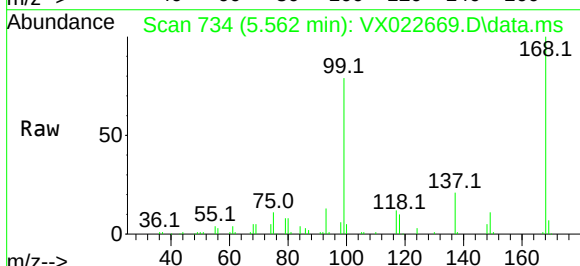

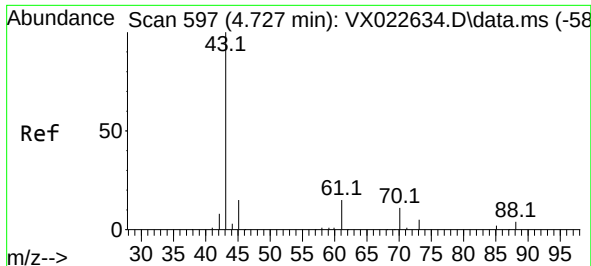

#37

Ethyl Acetate

Concen: 2.433 ug/l

RT: 4.580 min Scan# 573





Delta R.T. -0.147 min

Lab File: VX022669.D

Acq: 11 Jun 2021 15:56

Tgt Ion:	43	Resp:	3626
Ion	Ratio	Lower	Upper
43	100		
61	0.0	12.8	19.2#
70	0.0	10.5	15.7#

Instrument :
MSVOA_X
ClientSampleId :
MW-1

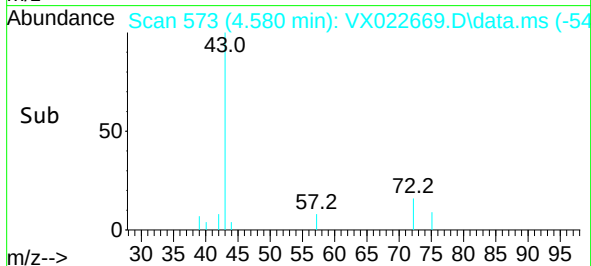

#38

Carbon Tetrachloride

Concen: 6.984 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.116 min

Lab File: VX022669.D

Acq: 11 Jun 2021 15:56

Tgt Ion:	117	Resp:	7005
Ion	Ratio	Lower	Upper
117	100		
119	3.2	76.2	114.2#
121	0.0	24.8	37.2#

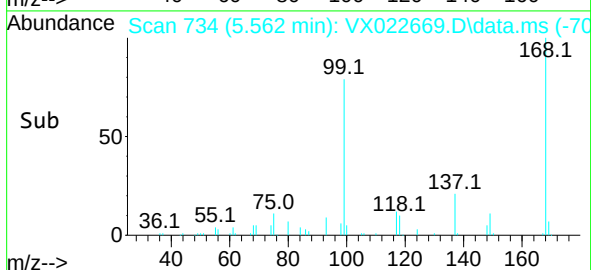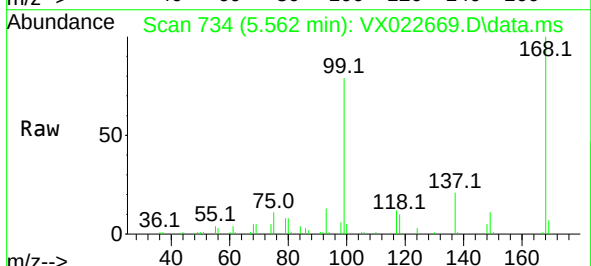



#39

Methylcyclohexane

Concen: 1.412 ug/l

RT: 7.391 min Scan# 1034

Delta R.T. 0.006 min

Lab File: VX022669.D

Acq: 11 Jun 2021 15:56

Tgt Ion: 83 Resp: 1727





Ion	Ratio	Lower	Upper
83	100		
55	80.0	58.9	88.3
98	56.6	38.1	57.1

Instrument :

MSVOA_X

ClientSampled :

MW-1

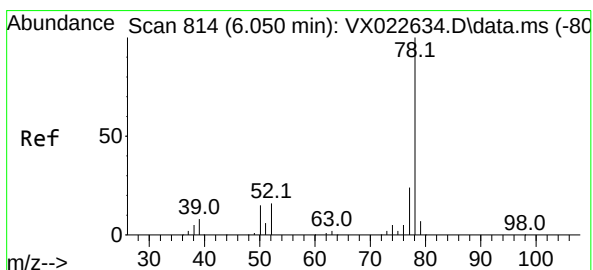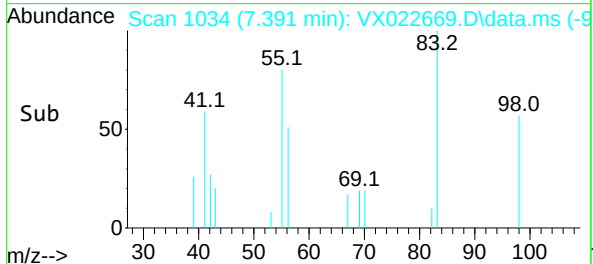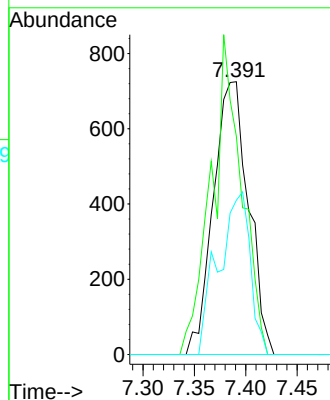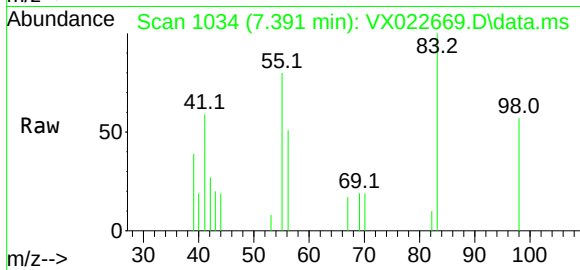

#40

Benzene

Concen: 0.468 ug/l

RT: 6.037 min Scan# 812




Delta R.T. -0.013 min


Lab File: VX022669.D

Acq: 11 Jun 2021 15:56

Tgt Ion: 78 Resp: 1632

Ion	Ratio	Lower	Upper
78	100		
77	21.3	18.9	28.3



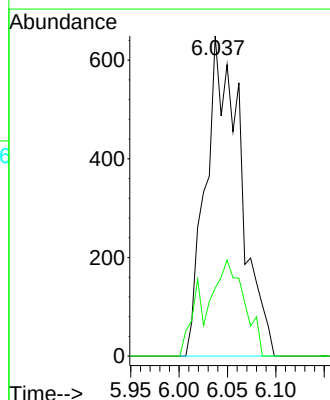
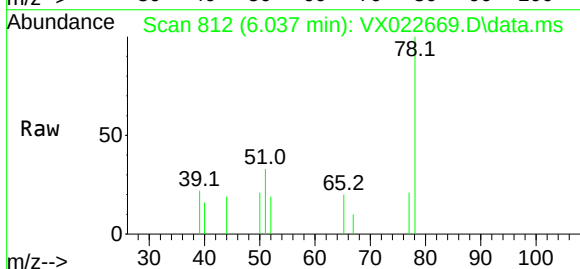




#48
Methyl methacrylate
Concen: 0.341 ug/l
RT: 7.677 min Scan# 1081
Delta R.T. -0.019 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion: 41 Resp: 385
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 0.0 44.6 67.0#

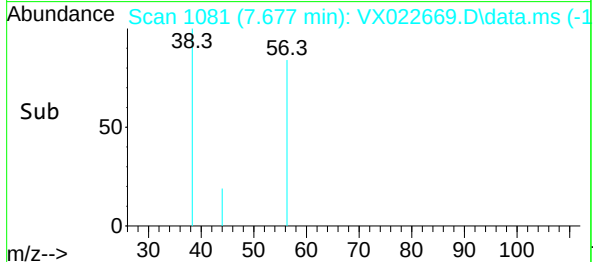

#50
Toluene-d8
Concen: 48.677 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 98 Resp: 144067
Ion Ratio Lower Upper
98 100
100 66.5 51.9 77.9


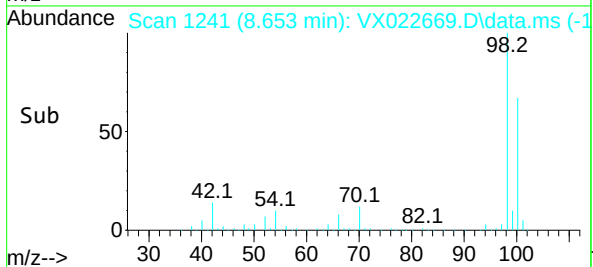

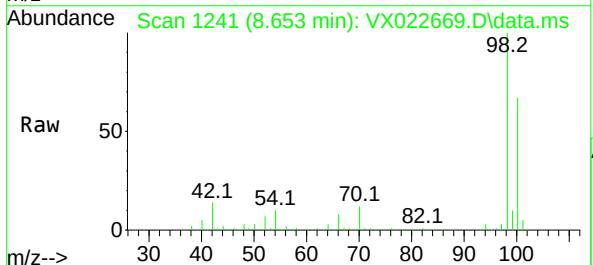




#51
4-Methyl-2-Pentanone
Concen: 0.594 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. -0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 43 Resp: 887
Ion Ratio Lower Upper
43 100
58 32.6 35.4 53.0#

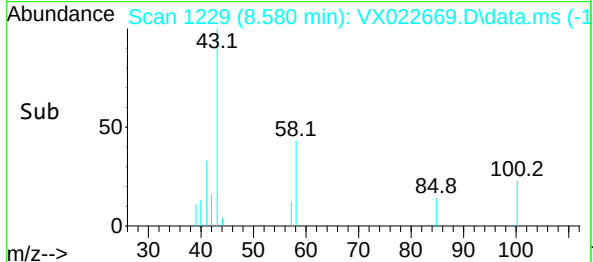

#52
Toluene
Concen: 10.310 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 92 Resp: 22383
Ion Ratio Lower Upper
92 100
91 167.3 137.1 205.7


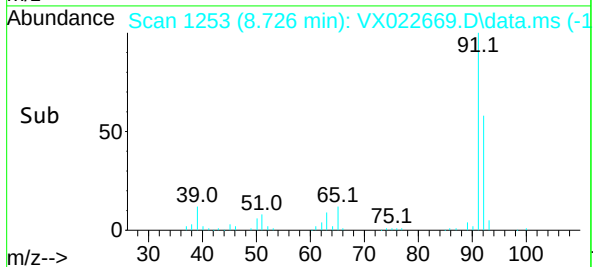

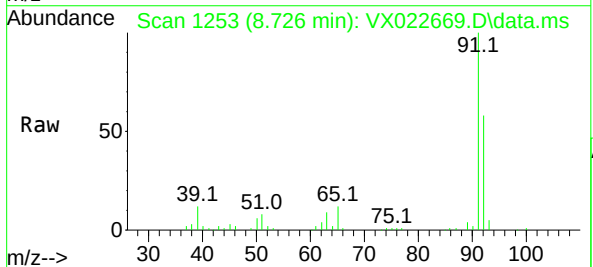




#53
t-1,3-Dichloropropene
Concen: 3.416 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. -0.256 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion: 75 Resp: 245
Ion Ratio Lower Upper
75 100
77 158.7 24.9 37.3#

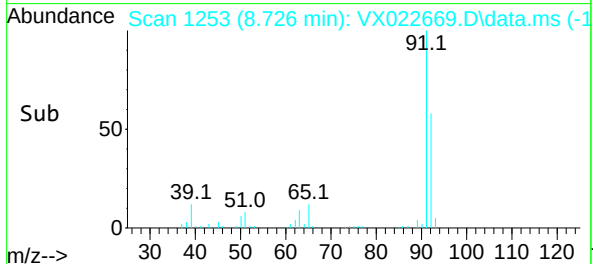

#55
1,1,2-Trichloroethane
Concen: 0.211 ug/l
RT: 9.110 min Scan# 1316
Delta R.T. -0.049 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 97 Resp: 187
Ion Ratio Lower Upper
97 100
83 0.0 69.3 103.9#
85 0.0 44.3 66.5#
99 0.0 50.3 75.5#


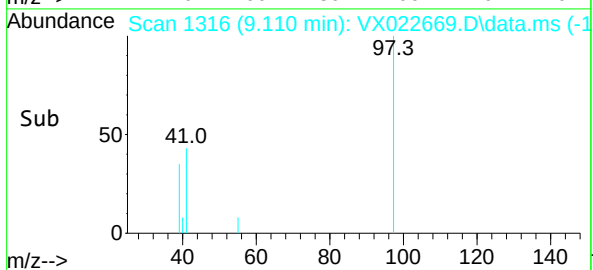

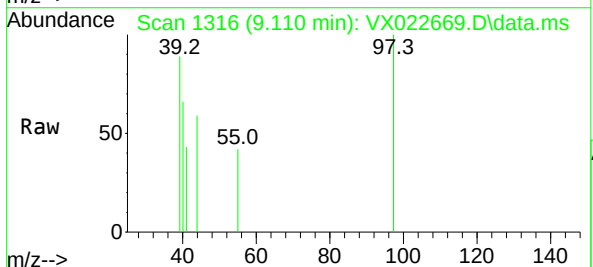




#56
Ethyl methacrylate
Concen: 2.304 ug/l
RT: 9.073 min Scan# 1310
Delta R.T. -0.049 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion:	69	Resp:	19
Ion	Ratio	Lower	Upper
69	100		
41	0.0	46.8	70.2#
39	0.0	24.7	37.1#

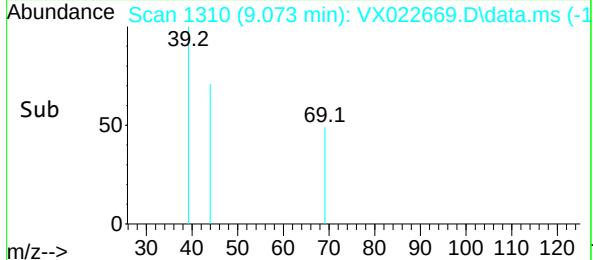

#62
4-Bromofluorobenzene
Concen: 45.213 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion:	95	Resp:	50609
Ion	Ratio	Lower	Upper
95	100		
174	63.7	0.0	154.6
176	60.5	0.0	155.8


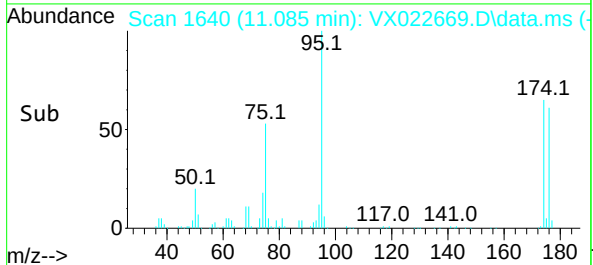

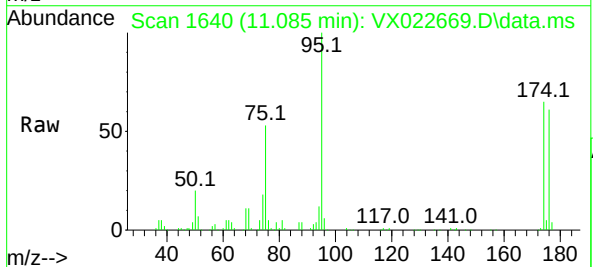




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion:117 Resp: 103724
Ion Ratio Lower Upper
117 100
82 60.8 47.4 71.2
119 31.1 26.6 39.8

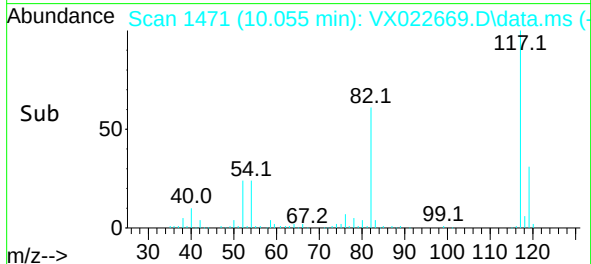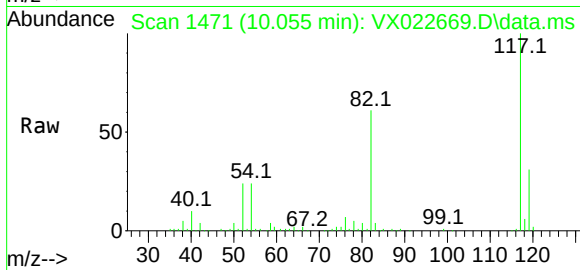

#67
Ethyl Benzene
Concen: 4.109 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 91 Resp: 16354
Ion Ratio Lower Upper
91 100
106 30.2 24.6 37.0




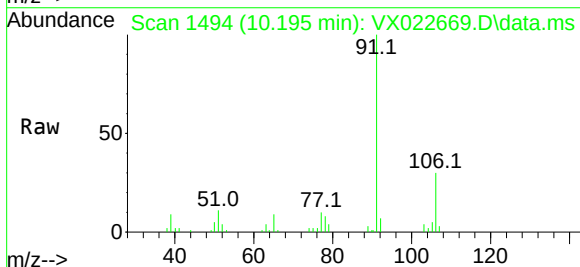


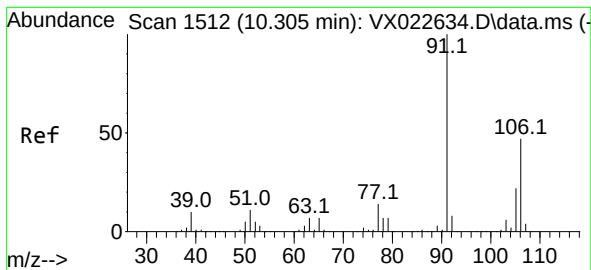

#68
m/p-Xylenes
Concen: 17.098 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion:106 Resp: 24647
Ion Ratio Lower Upper
106 100
91 202.6 162.8 244.2

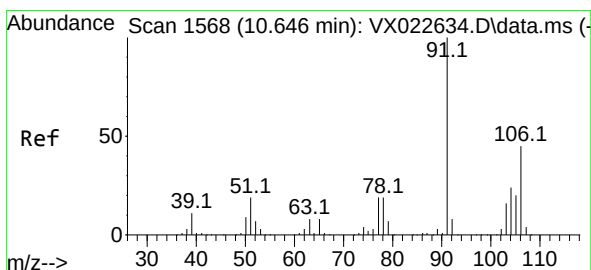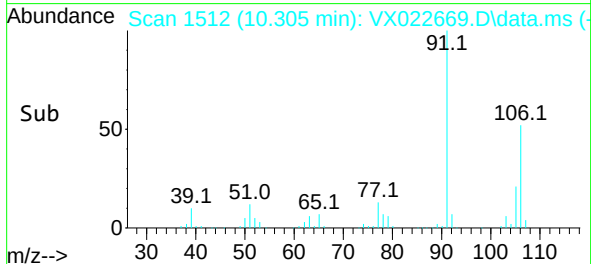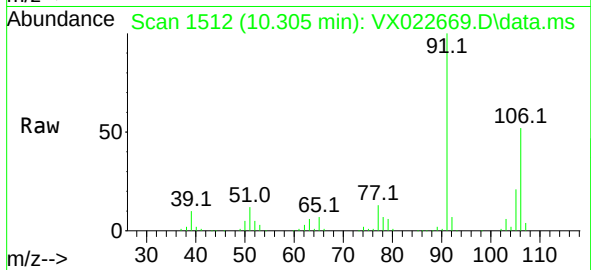

#69
o-Xylene
Concen: 7.678 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion:106 Resp: 10724
Ion Ratio Lower Upper
106 100
91 221.5 108.1 324.2




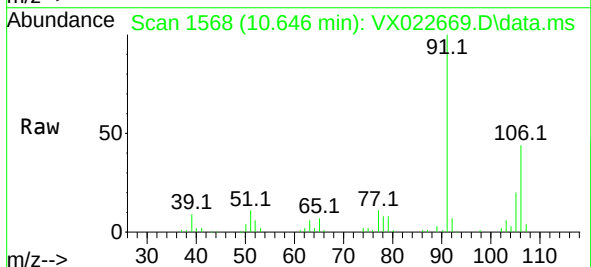




#70
Styrene
Concen: 1.692 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion:104 Resp: 631
Ion Ratio Lower Upper
104 100
78 273.4 40.0 60.0#
103 234.4 43.4 65.0#

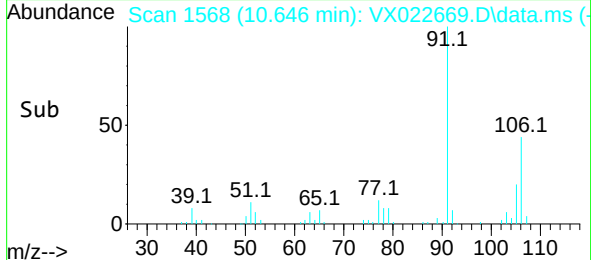

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion:152 Resp: 41093
Ion Ratio Lower Upper
152 100
115 67.8 41.1 123.3
150 164.0 0.0 349.0

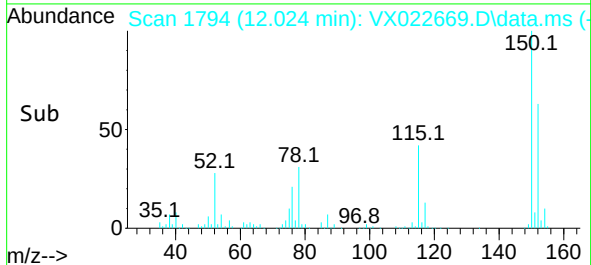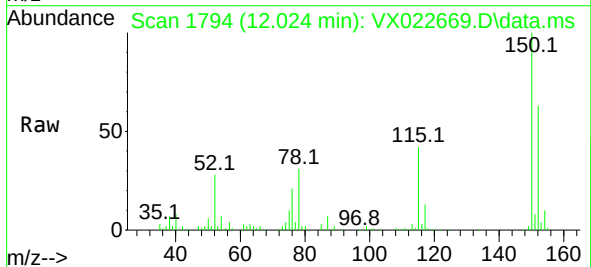

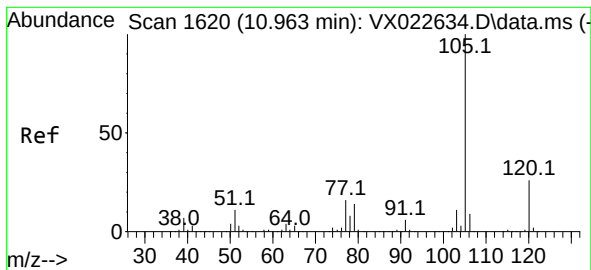

#73

Isopropylbenzene

Concen: 0.879 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX022669.D





Acq: 11 Jun 2021 15:56

Tgt Ion:105 Resp: 2966

Ion Ratio Lower Upper

105 100

120 23.3 13.2 39.6

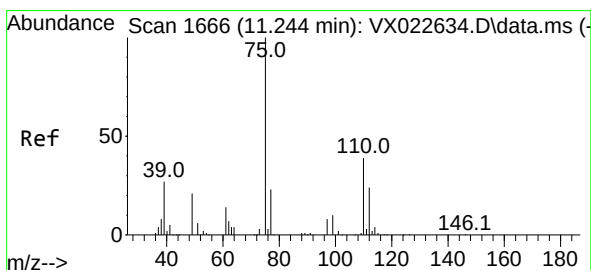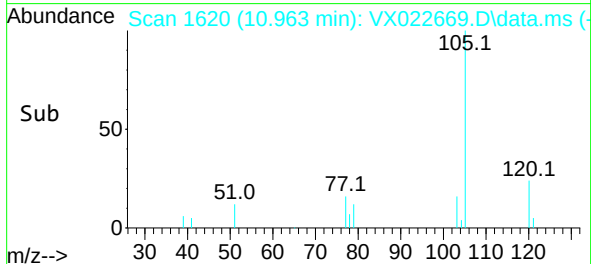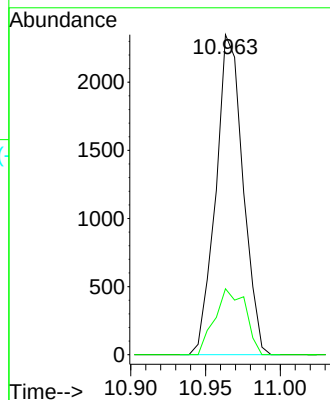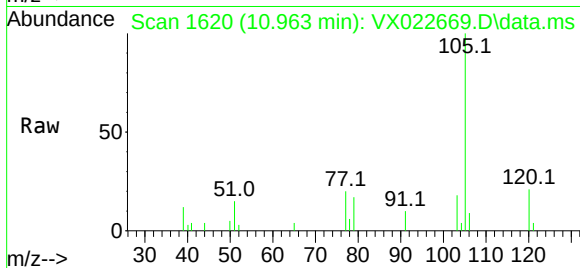

#76

1,2,3-Trichloropropane

Concen: 25.627 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.159 min

Lab File: VX022669.D




Acq: 11 Jun 2021 15:56


Tgt Ion: 75 Resp: 27922

Ion Ratio Lower Upper

75 100

77 1.1 19.1 57.5#

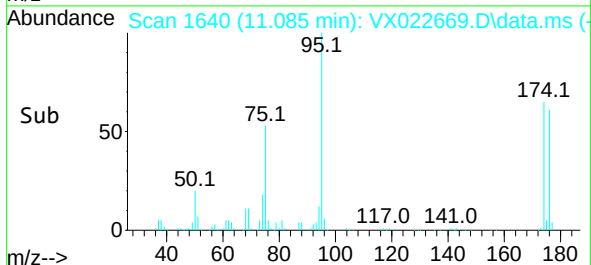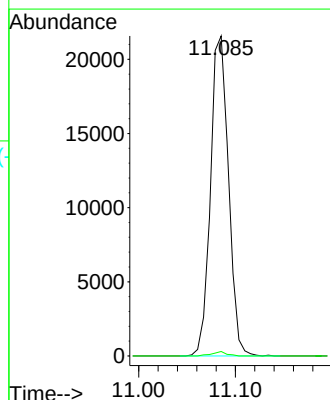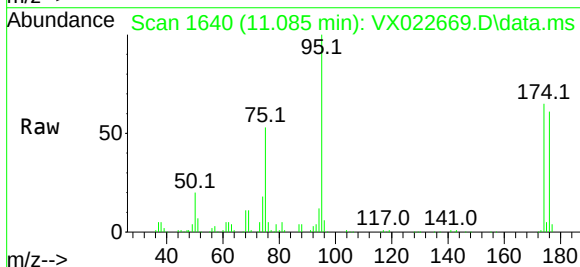



#78

n-propylbenzene

Concen: 1.127 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX022669.D





Acq: 11 Jun 2021 15:56

Tgt Ion: 91 Resp: 4593

Ion Ratio Lower Upper

91 100

120 23.5 11.5 34.5

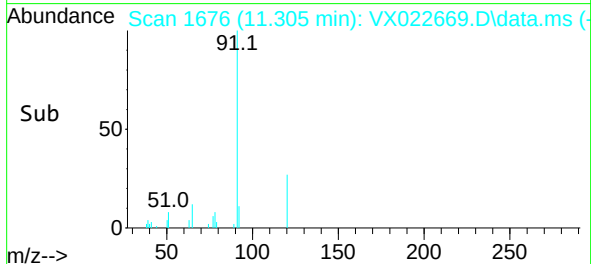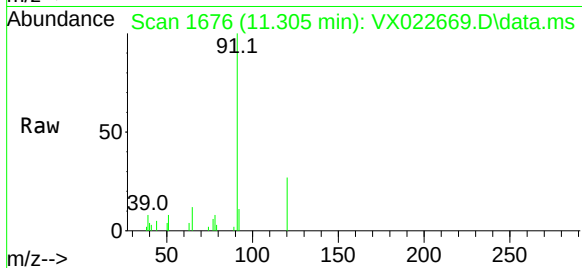

#79

2-Chlorotoluene

Concen: 1.043 ug/l

RT: 11.384 min Scan# 1689

Delta R.T. 0.018 min

Lab File: VX022669.D




Acq: 11 Jun 2021 15:56


Tgt Ion: 91 Resp: 2573

Ion Ratio Lower Upper

91 100

126 0.0 16.6 49.8#


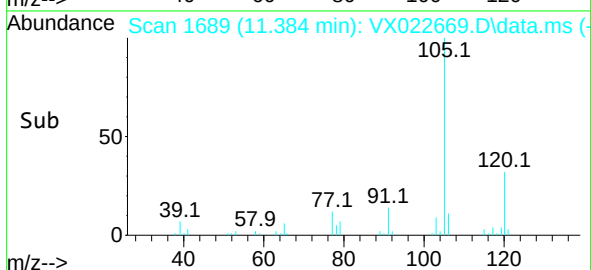

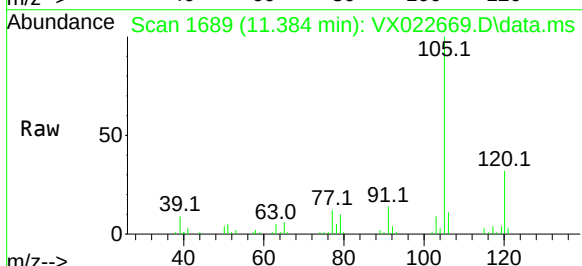


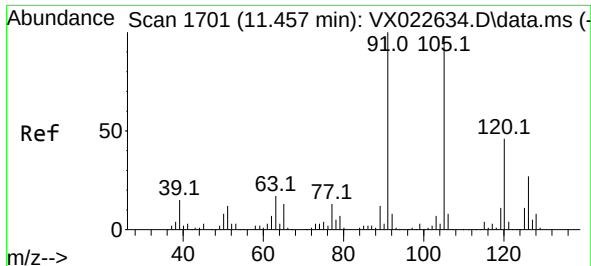

#80
1,3,5-Trimethylbenzene
Concen: 1.815 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion:105 Resp: 5101
Ion Ratio Lower Upper
105 100
120 46.7 23.8 71.5

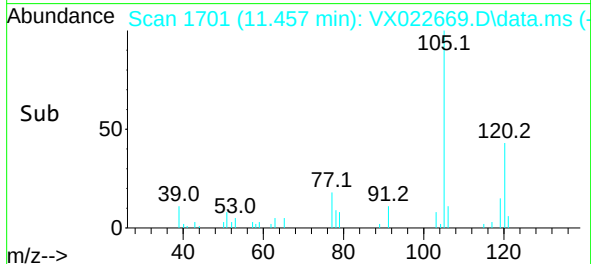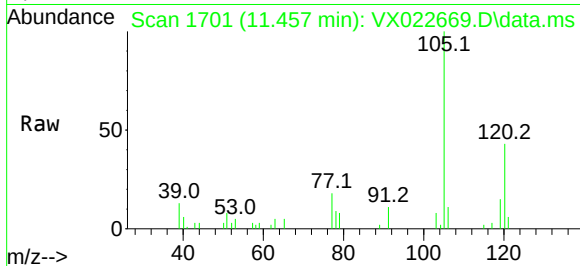

#81
trans-1,4-Dichloro-2-butene
Concen: 64.376 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 75 Resp: 27922
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


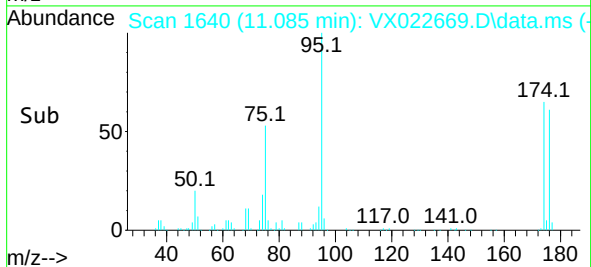

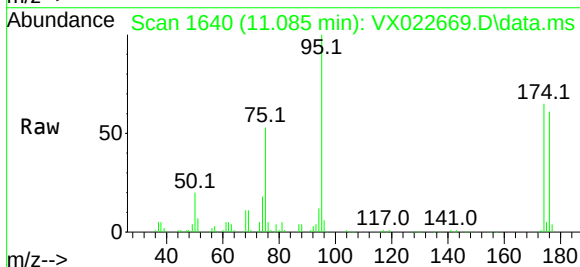


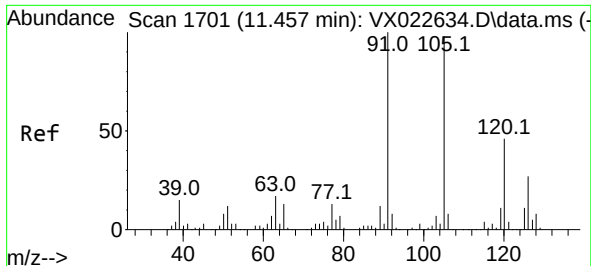

#82
4-Chlorotoluene
Concen: 0.261 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion: 91 Resp: 737
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

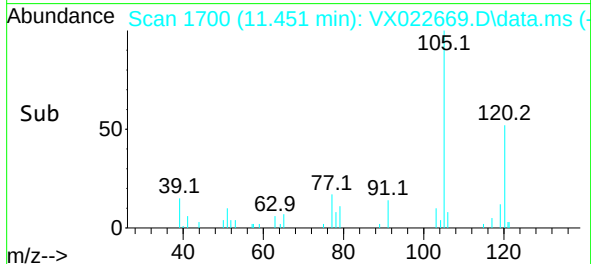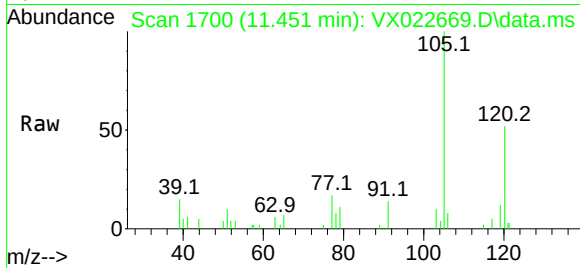

#83
tert-Butylbenzene
Concen: 0.910 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 119 Resp: 2401
Ion Ratio Lower Upper
119 100
91 91.6 27.9 83.7#
134 0.0 11.3 33.9#


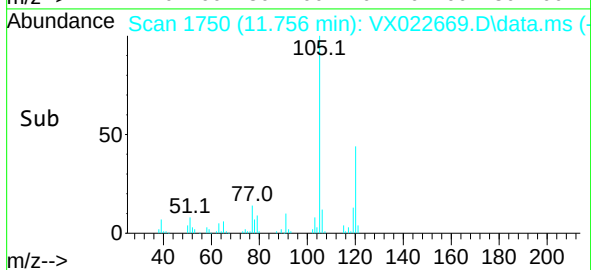

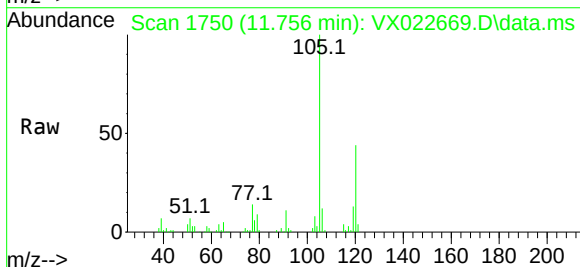




#84
1,2,4-Trimethylbenzene
Concen: 7.055 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion:105 Resp: 20112
Ion Ratio Lower Upper
105 100
120 41.5 22.4 67.3

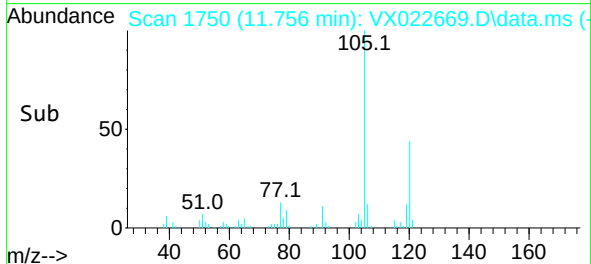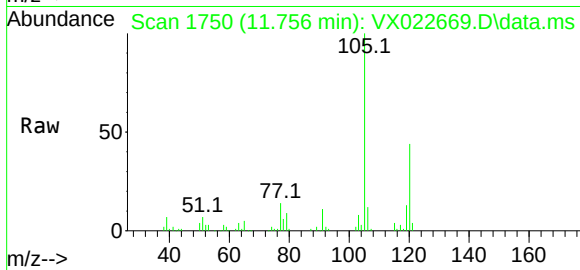

#85
sec-Butylbenzene
Concen: 0.652 ug/l
RT: 11.896 min Scan# 1773
Delta R.T. 0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion:105 Resp: 2247
Ion Ratio Lower Upper
105 100
134 24.8 10.0 29.8


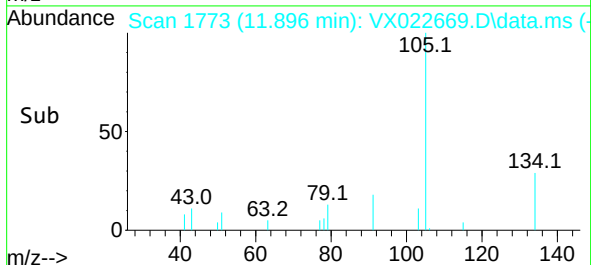

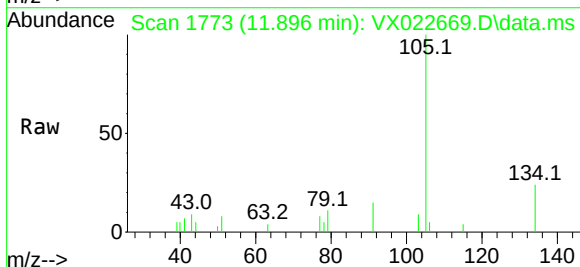




#89
n-Butylbenzene
Concen: 0.497 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 91 Resp: 1355
Ion Ratio Lower Upper
91 100
92 0.0 27.4 82.0#
134 97.8 13.2 39.5#

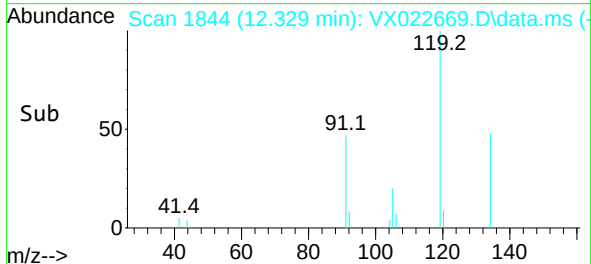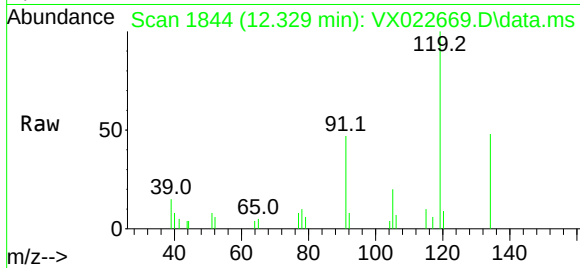

#90
Hexachloroethane
Concen: 4.303 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.012 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 117 Resp: 322
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#


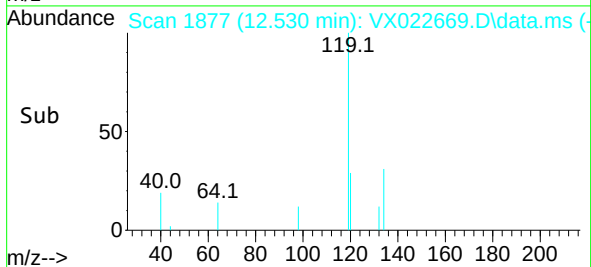

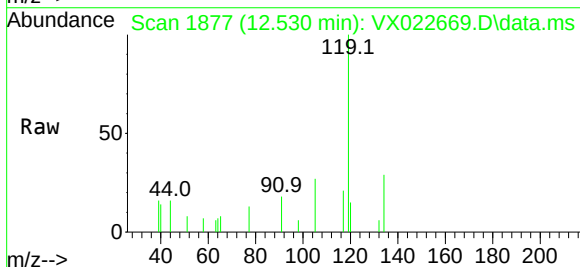




#92
1,2-Dibromo-3-Chloropropane
Concen: 4.037 ug/l
RT: 13.170 min Scan# 1982
Delta R.T. 0.225 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Instrument :
MSVOA_X
ClientSampled :
MW-1

Tgt Ion: 75 Resp: 30
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

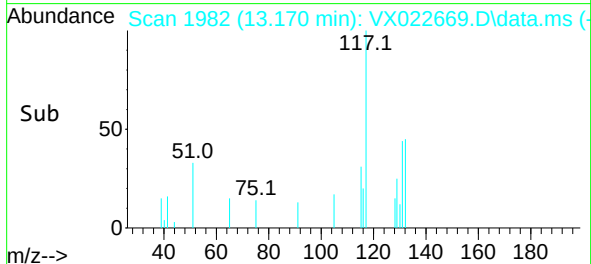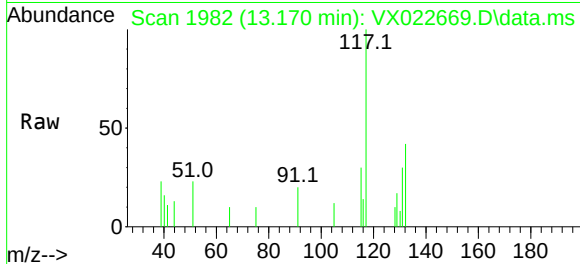

#95
Naphthalene
Concen: 3.010 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022669.D
Acq: 11 Jun 2021 15:56

Tgt Ion: 128 Resp: 5526
Ion Ratio Lower Upper
128 100
127 14.4 10.3 15.5
129 12.8 8.8 13.2

