
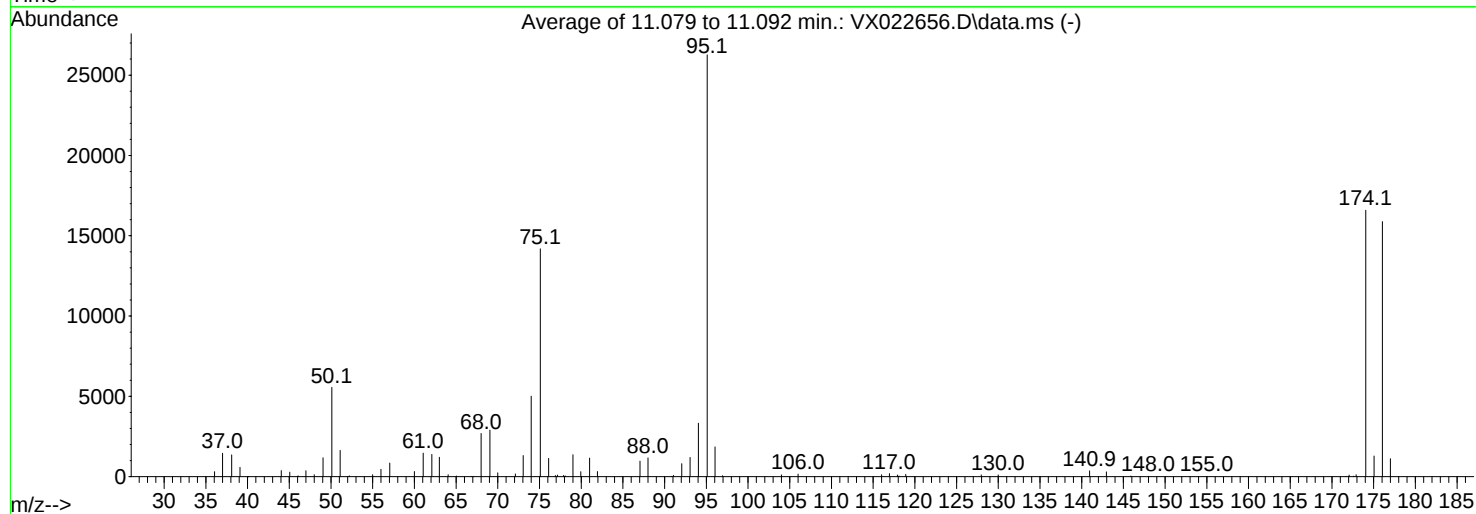


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061121\
Data File : VX022656.D
Acq On : 11 Jun 2021 09:21
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Title : SW846 8260
Last Update : Thu Jun 10 12:20:00 2021

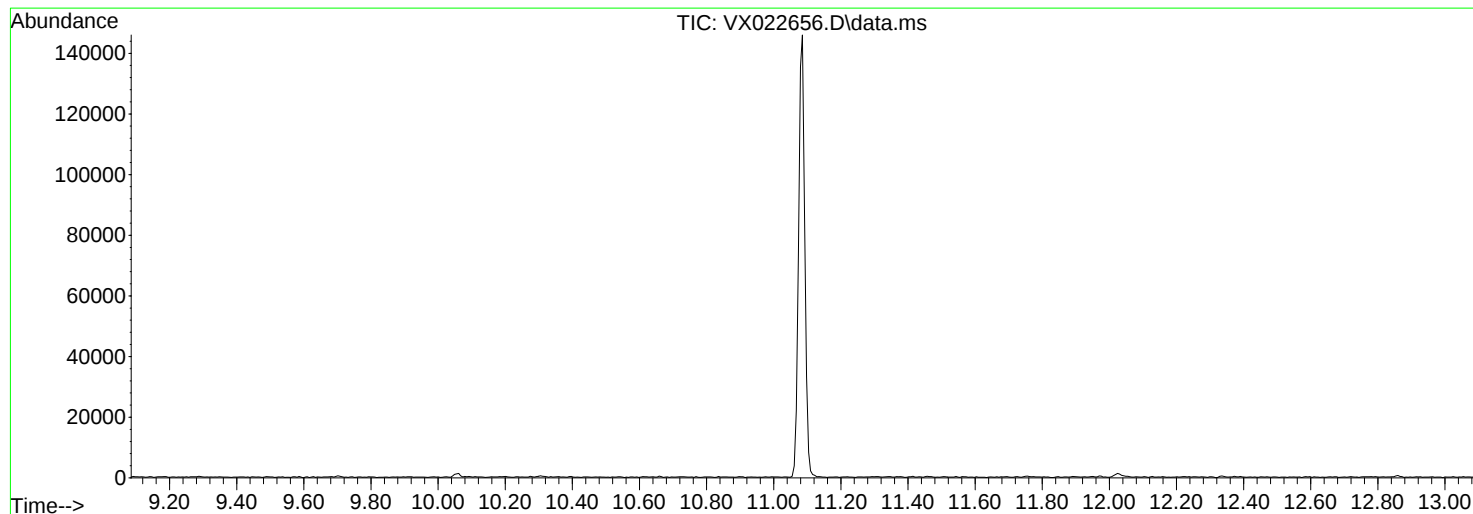

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	5555	PASS
75	95	30	60	54.0	14188	PASS
95	95	100	100	100.0	26264	PASS
96	95	5	9	7.1	1853	PASS
173	174	0.00	2	0.7	124	PASS
174	95	50	100	63.2	16587	PASS
175	174	5	9	7.7	1285	PASS
176	174	95	101	95.7	15879	PASS
177	176	5	9	7.1	1121	PASS