

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX061220\
 Data File : VX016727.D
 Acq On : 12 Jun 2020 14:47
 Operator : JC/SP
 Sample : L3001-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PAD-RINSE

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.471	60	63	68	rBV	10879	14130	1.27%	0.209%
2	2.087	157	164	170	rBV	10659	16901	1.52%	0.250%
3	2.416	213	218	226	rVB	9360	17520	1.58%	0.259%
4	5.184	659	672	682	rVB2	25582	77643	6.99%	1.146%
5	5.470	707	719	735	rBV	124365	362663	32.67%	5.354%
6	5.629	735	745	761	rVB	220229	623869	56.20%	9.211%
7	6.031	801	811	827	rBV	134259	360294	32.45%	5.319%
8	6.434	867	877	886	rVB6	3731	11748	1.06%	0.173%
9	6.830	932	942	956	rBV	332011	800576	72.11%	11.820%
10	7.879	1106	1114	1122	rBV	69955	131987	11.89%	1.949%
11	8.695	1241	1248	1258	rBV	719897	1110167	100.00%	16.391%
12	8.805	1260	1266	1272	rVB3	8077	15409	1.39%	0.228%
13	9.567	1385	1391	1397	rBV	143417	214400	19.31%	3.165%
14	10.098	1472	1478	1484	rBV	750372	1008037	90.80%	14.883%
15	10.841	1592	1600	1605	rBV	74378	102579	9.24%	1.514%
16	10.896	1605	1609	1614	rVB2	10556	14381	1.30%	0.212%
17	11.122	1640	1646	1656	rBV	659191	830965	74.85%	12.269%
18	12.061	1795	1800	1808	rVB	861517	1059889	95.47%	15.648%


Sum of corrected areas: 6773158

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061220\
Data File : VX016727.D
Acq On : 12 Jun 2020 14:47
Operator : JC/SP
Sample : L3001-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PAD-RINSE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

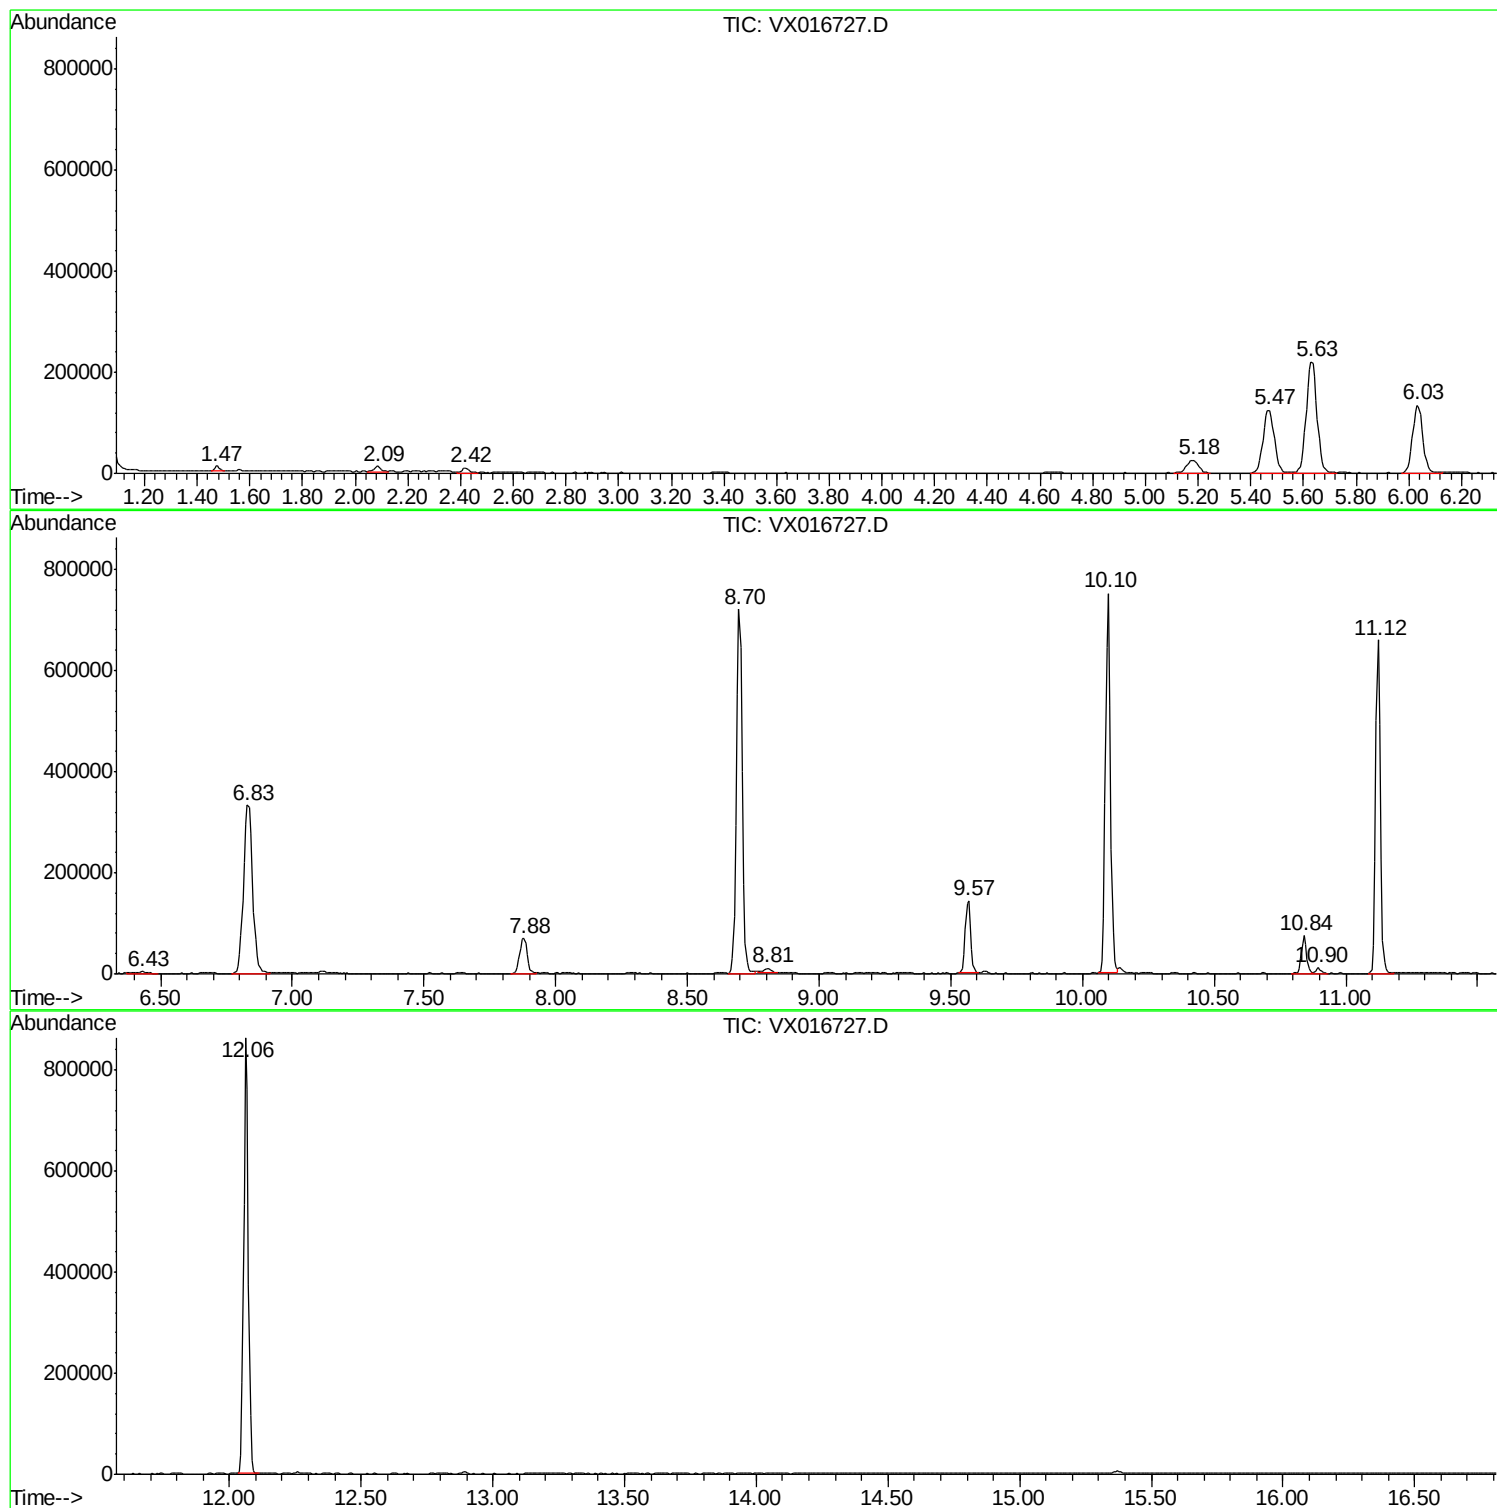

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061220\
Data File : VX016727.D
Acq On : 12 Jun 2020 14:47
Operator : JC/SP
Sample : L3001-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PAD-RINSE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061220\
Data File : VX016727.D
Acq On : 12 Jun 2020 14:47
Operator : JC/SP
Sample : L3001-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PAD-RINSE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc