

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX061220\
Data File : VX016731.D
Acq On : 12 Jun 2020 16:18
Operator : JC/SP
Sample : L3004-02 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF015MW045-200611

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	46	50	61	rVB	445808	421249	34.01%	4.900%
2	4.568	557	571	582	rBV	372757	1032611	83.37%	12.012%
3	5.465	707	718	733	rBV	130181	373784	30.18%	4.348%
4	5.629	734	745	758	rVV2	223033	629405	50.82%	7.322%
5	6.032	797	811	822	rBV	138098	360992	29.15%	4.199%
6	6.830	931	942	955	rBV	338521	804542	64.96%	9.359%
7	8.696	1240	1248	1256	rBV	729221	1124272	90.77%	13.078%
8	8.769	1256	1260	1272	rVB2	14554	29530	2.38%	0.344%
9	10.098	1469	1478	1493	rBV2	785101	1238555	100.00%	14.408%
10	11.122	1640	1646	1659	rBV	677404	837203	67.60%	9.739%
11	12.012	1787	1792	1795	rBV	13522	17450	1.41%	0.203%
12	12.061	1795	1800	1809	rVV	872721	1198978	96.80%	13.947%
13	12.372	1844	1851	1858	rBV	401003	528024	42.63%	6.142%


Sum of corrected areas: 8596595

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061220\
Data File : VX016731.D
Acq On : 12 Jun 2020 16:18
Operator : JC/SP
Sample : L3004-02 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF015MW045-200611

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

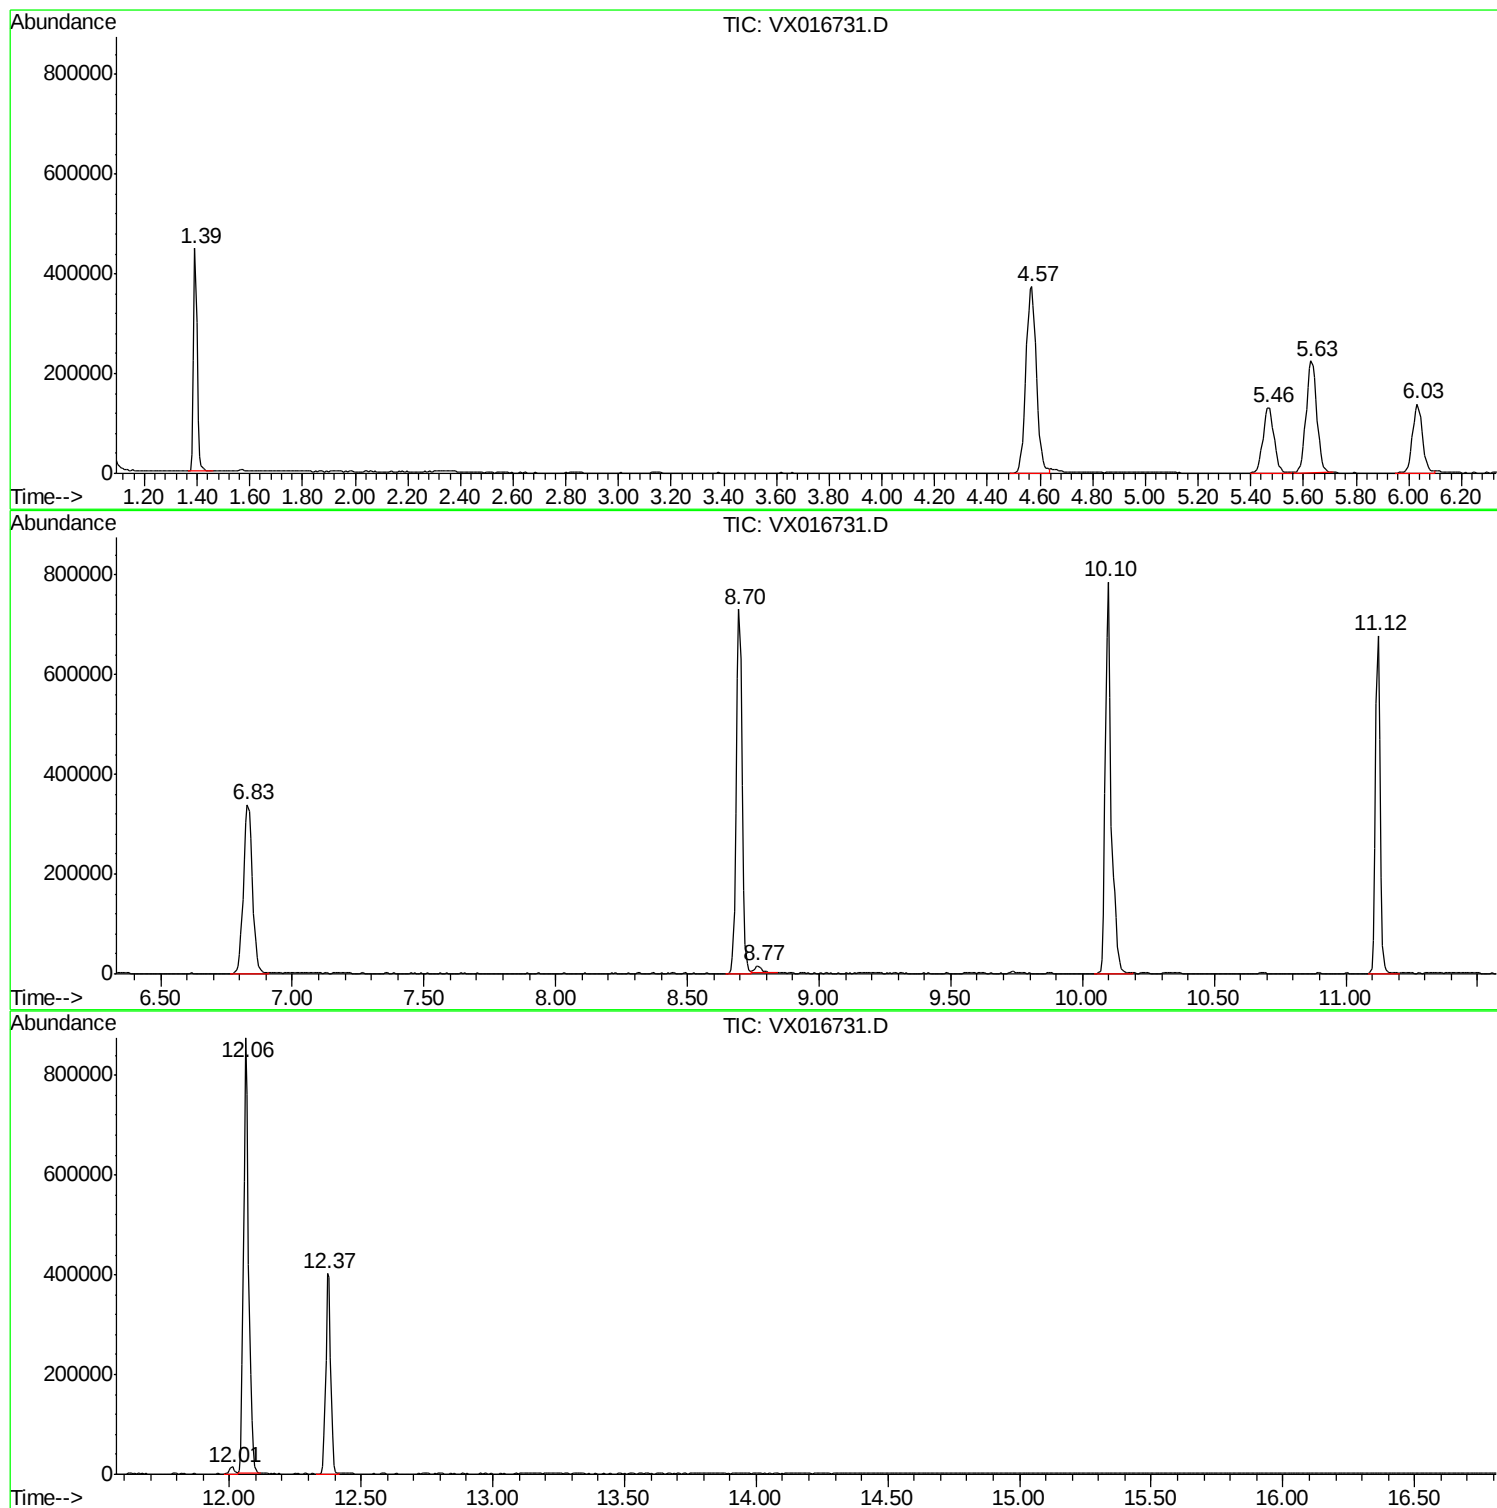

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061220\
Data File : VX016731.D
Acq On : 12 Jun 2020 16:18
Operator : JC/SP
Sample : L3004-02 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF015MW045-200611

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061220\
Data File : VX016731.D
Acq On : 12 Jun 2020 16:18
Operator : JC/SP
Sample : L3004-02 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF015MW045-200611

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc