



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061223\
Data File : VX036115.D
Acq On : 12 Jun 2023 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Title : SW846 8260
Last Update : Wed May 31 12:50:30 2023

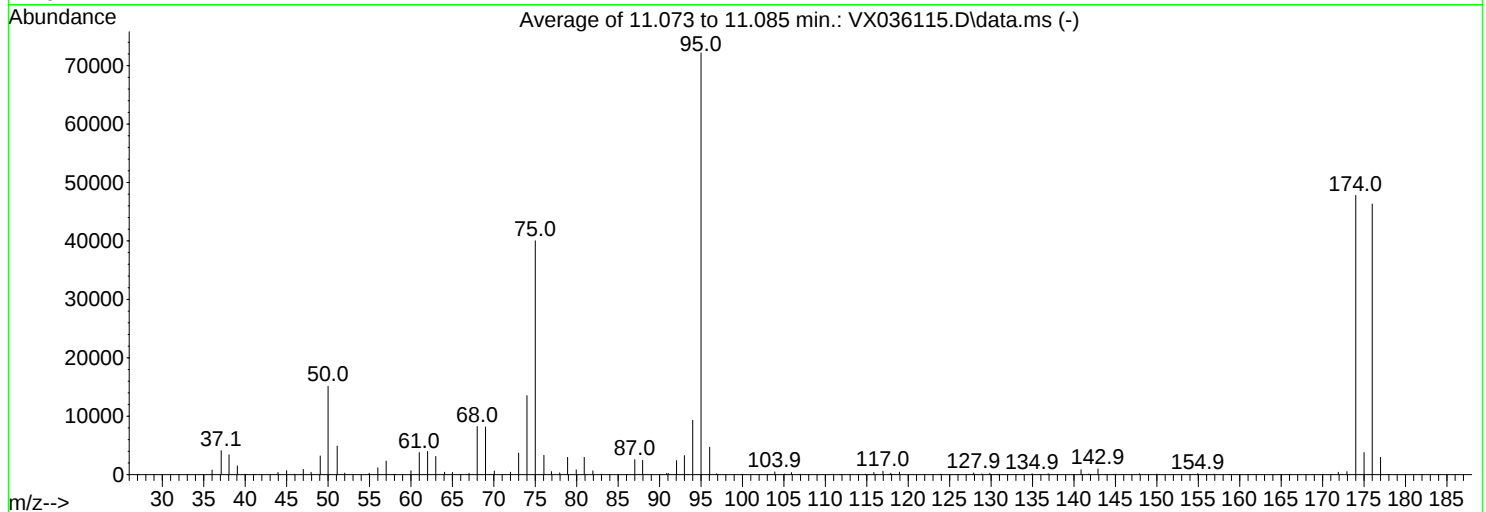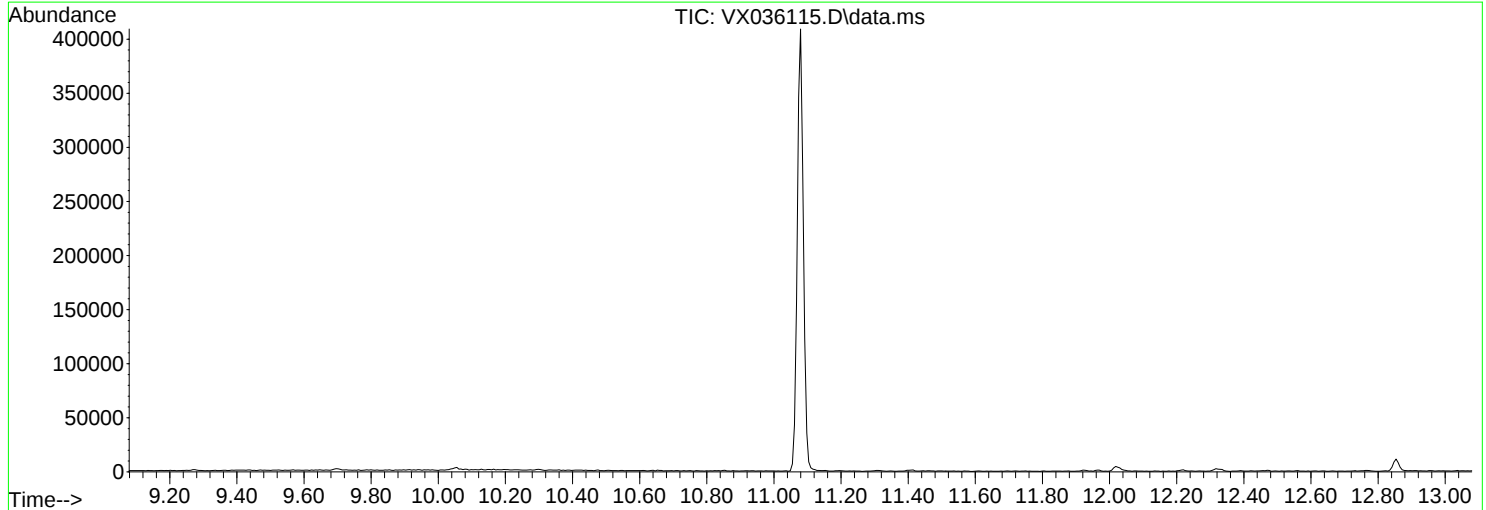

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	15143	PASS
75	95	30	60	55.4	40029	PASS
95	95	100	100	100.0	72197	PASS
96	95	5	9	6.5	4696	PASS
173	174	0.00	2	1.1	532	PASS
174	95	50	100	66.2	47779	PASS
175	174	5	9	7.9	3790	PASS
176	174	95	101	96.9	46304	PASS
177	176	5	9	6.4	2970	PASS

Scan 1631 (11.031 min): VX036115.D\data.ms
BFB

m/z	Abundance
36.00	208.0
38.10	204.0
40.00	136.0
40.80	53.0
43.90	281.0

Instrument :
MSVOA_X
ClientSampleId :
BFB

m/z	Abundance
36.00	1200.0
37.10	4720.0
38.00	3905.0
39.10	1718.0
40.00	223.0
41.20	59.0
43.00	76.0
44.00	800.0
45.00	726.0
46.00	88.0
47.00	1260.0
48.00	555.0
49.00	3903.0
50.00	17312.0
51.10	5405.0
52.00	393.0
54.90	199.0
56.00	1296.0
57.00	2761.0
57.90	162.0
60.00	637.0
61.00	3909.0
62.00	4101.0
63.00	3402.0
64.00	399.0
65.00	531.0
67.10	243.0
68.00	8834.0
69.00	8722.0
70.10	819.0
72.00	350.0
73.00	3996.0
74.00	14349.0
75.00	42008.0
76.00	3568.0
76.90	464.0
77.90	373.0
78.90	3443.0
80.00	878.0
80.90	2833.0
81.90	637.0
82.90	104.0
87.00	2634.0
88.00	2418.0
90.90	287.0
92.10	2177.0
93.00	3043.0
94.00	9568.0
95.00	73544.0
96.10	4991.0
97.00	145.0
103.00	67.0
104.00	406.0
105.10	120.0
105.90	372.0
107.00	52.0
111.00	81.0
111.80	71.0
113.00	55.0
114.80	94.0
115.80	475.0
116.90	558.0
117.70	276.0
118.90	497.0
123.80	81.0
127.90	265.0
129.00	90.0
129.90	205.0
130.80	82.0
135.00	90.0
136.80	124.0
140.90	714.0
141.70	137.0
142.90	891.0
143.80	52.0
144.80	78.0
145.00	78.0
145.80	97.0
147.90	139.0
150.00	88.0
155.00	154.0
156.90	100.0
158.70	113.0
161.00	60.0
171.10	89.0
171.90	529.0
173.00	464.0
174.00	41544.0
175.00	3432.0
176.00	40456.0
177.00	2844.0

Instrument :
MSVOA_X
ClientSampleId :
BFB

m/z	Abundance
36.10	1091.0
37.10	4640.0
38.10	4264.0
39.00	1847.0
40.00	203.0
41.20	64.0
43.00	69.0
44.00	772.0
45.00	862.0
45.90	131.0
47.00	868.0
47.90	472.0
49.10	3621.0
50.00	17400.0
51.10	5983.0
52.10	247.0
55.00	408.0
56.00	1410.0
57.00	2545.0
58.10	107.0
60.00	869.0
61.00	4569.0
62.00	4659.0
63.00	3797.0
64.10	499.0
65.00	414.0
66.90	378.0
68.00	9967.0
69.00	9320.0
70.00	739.0
72.00	602.0
73.00	4352.0
74.00	15735.0
75.00	48192.0
76.10	3837.0
77.00	639.0
78.00	255.0
78.90	3176.0
79.90	929.0
80.90	3746.0
81.90	825.0
83.00	71.0
86.10	66.0
87.00	3133.0
87.90	3019.0
90.80	330.0
91.10	320.0
92.00	2874.0
93.00	3974.0
94.00	11288.0
95.00	86056.0
96.00	5458.0
96.90	265.0
103.80	637.0
105.00	117.0
105.80	426.0
107.00	132.0
111.00	81.0
113.00	191.0
114.80	66.0
115.90	416.0
117.00	714.0
117.90	425.0
119.00	546.0
123.90	104.0
127.80	355.0
128.90	208.0
129.80	243.0
131.00	155.0
134.90	182.0
136.90	225.0
140.90	1008.0
141.80	127.0
142.90	1120.0
143.80	61.0
145.00	203.0
146.00	62.0
147.90	252.0
150.00	122.0
154.90	230.0
156.90	132.0
158.80	85.0
159.00	87.0
171.90	418.0
173.00	599.0
174.00	56016.0
175.00	4474.0
176.00	54592.0
177.00	3175.0
177.80	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB

m/z	Abundance
36.10	761.0
37.00	2969.0
38.00	2603.0
39.10	987.0
39.90	226.0
41.10	65.0
44.00	448.0
45.00	488.0
45.90	59.0
47.00	599.0
47.90	234.0
49.00	2117.0
50.00	10717.0
51.10	3273.0
51.90	165.0
53.10	54.0
54.90	143.0
56.00	803.0
57.00	1723.0
58.10	77.0
60.00	514.0
61.00	2847.0
62.00	3145.0
63.00	2181.0
64.00	325.0
64.90	231.0
67.00	148.0
68.00	5952.0
69.00	6422.0
70.00	382.0
72.00	254.0
73.00	2733.0
74.00	10481.0
75.00	29888.0
76.00	2589.0
77.00	420.0
77.90	302.0
78.90	2293.0
79.90	697.0
80.90	2282.0
82.00	509.0
83.00	74.0
87.00	1986.0
87.90	1979.0
91.00	382.0
92.00	2200.0
93.00	2767.0
94.00	7099.0
95.00	56992.0
96.10	3640.0
96.80	84.0
103.80	326.0
105.00	64.0
106.00	299.0
106.80	84.0
111.00	70.0
114.80	82.0
115.80	225.0
116.20	171.0
117.00	469.0
117.90	329.0
118.90	274.0
123.90	66.0
128.00	275.0
128.80	139.0
129.90	293.0
130.90	103.0
134.90	198.0
137.00	108.0
140.80	810.0
141.90	75.0
142.90	957.0
143.70	61.0
144.80	108.0
146.00	52.0
147.80	114.0
150.00	126.0
154.90	178.0
156.90	80.0
159.00	84.0
171.90	332.0
172.90	534.0
174.00	45776.0
175.00	3464.0
176.00	43864.0
177.00	2892.0
178.00	78.0

Instrument :
MSVOA_X
ClientSampleId :
BFB