


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061319\
Data File : VX010266.D
Acq On : 13 Jun 2019 09:22
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Title : SW846 8260
Last Update : Sat Jun 08 02:12:13 2019

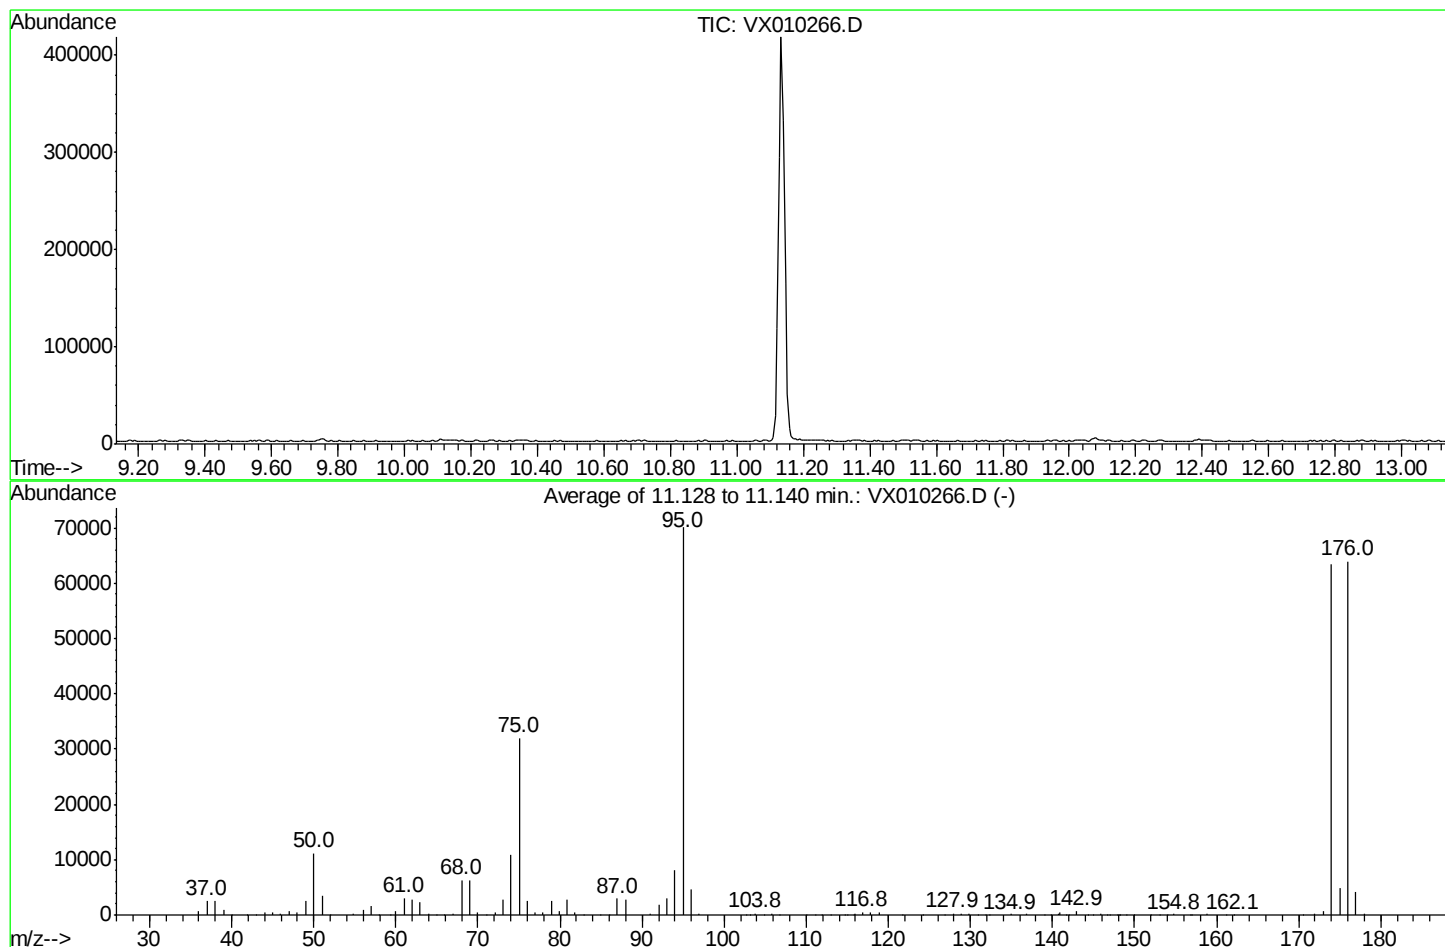

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	11204	PASS
75	95	30	60	45.7	32018	PASS
95	95	100	100	100.0	70104	PASS
96	95	5	9	6.8	4747	PASS
173	174	0.00	2	1.1	695	PASS
174	95	50	100	90.5	63416	PASS
175	174	5	9	7.6	4825	PASS
176	174	95	101	100.8	63928	PASS
177	176	5	9	6.5	4178	PASS