

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029434.D
 Acq On : 13 Jun 2022 23:58
 Operator : JC/MD
 Sample : VX0613WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK659

Quant Time: Jun 14 06:27:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 14 06:26:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	386515	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	348721	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	168673	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	138759	46.367	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.740%
7) Chloroethane-d5	1.666	69	98652	53.045	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.080%
11) 1,1-Dichloroethene-d2	2.306	63	192079	35.624	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.240%
21) 2-Butanone-d5	4.464	46	236438	104.204	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.200%
24) Chloroform-d	5.062	84	267949	46.895	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	5.958	65	175089	47.396	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.800%
32) Benzene-d6	5.982	84	541467	49.710	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.420%
36) 1,2-Dichloropropane-d6	7.311	67	160766	50.391	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.780%
41) Toluene-d8	8.652	98	486770	47.401	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.800%
43) trans-1,3-Dichloroprop...	8.951	79	65016	41.328	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.660%
47) 2-Hexanone-d5	9.390	63	181920	105.425	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.420%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	233260	49.863	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.720%
66) 1,2-Dichlorobenzene-d4	12.323	152	176574	50.352	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.700%
Target Compounds						
39) cis-1,3-Dichloropropene	8.329	75	4875	1.097	ug/L	Qvalue # 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029434.D
Acq On : 13 Jun 2022 23:58
Operator : JC/MD
Sample : VX0613WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK659

Quant Time: Jun 14 06:27:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 14 06:26:43 2022
Response via : Initial Calibration

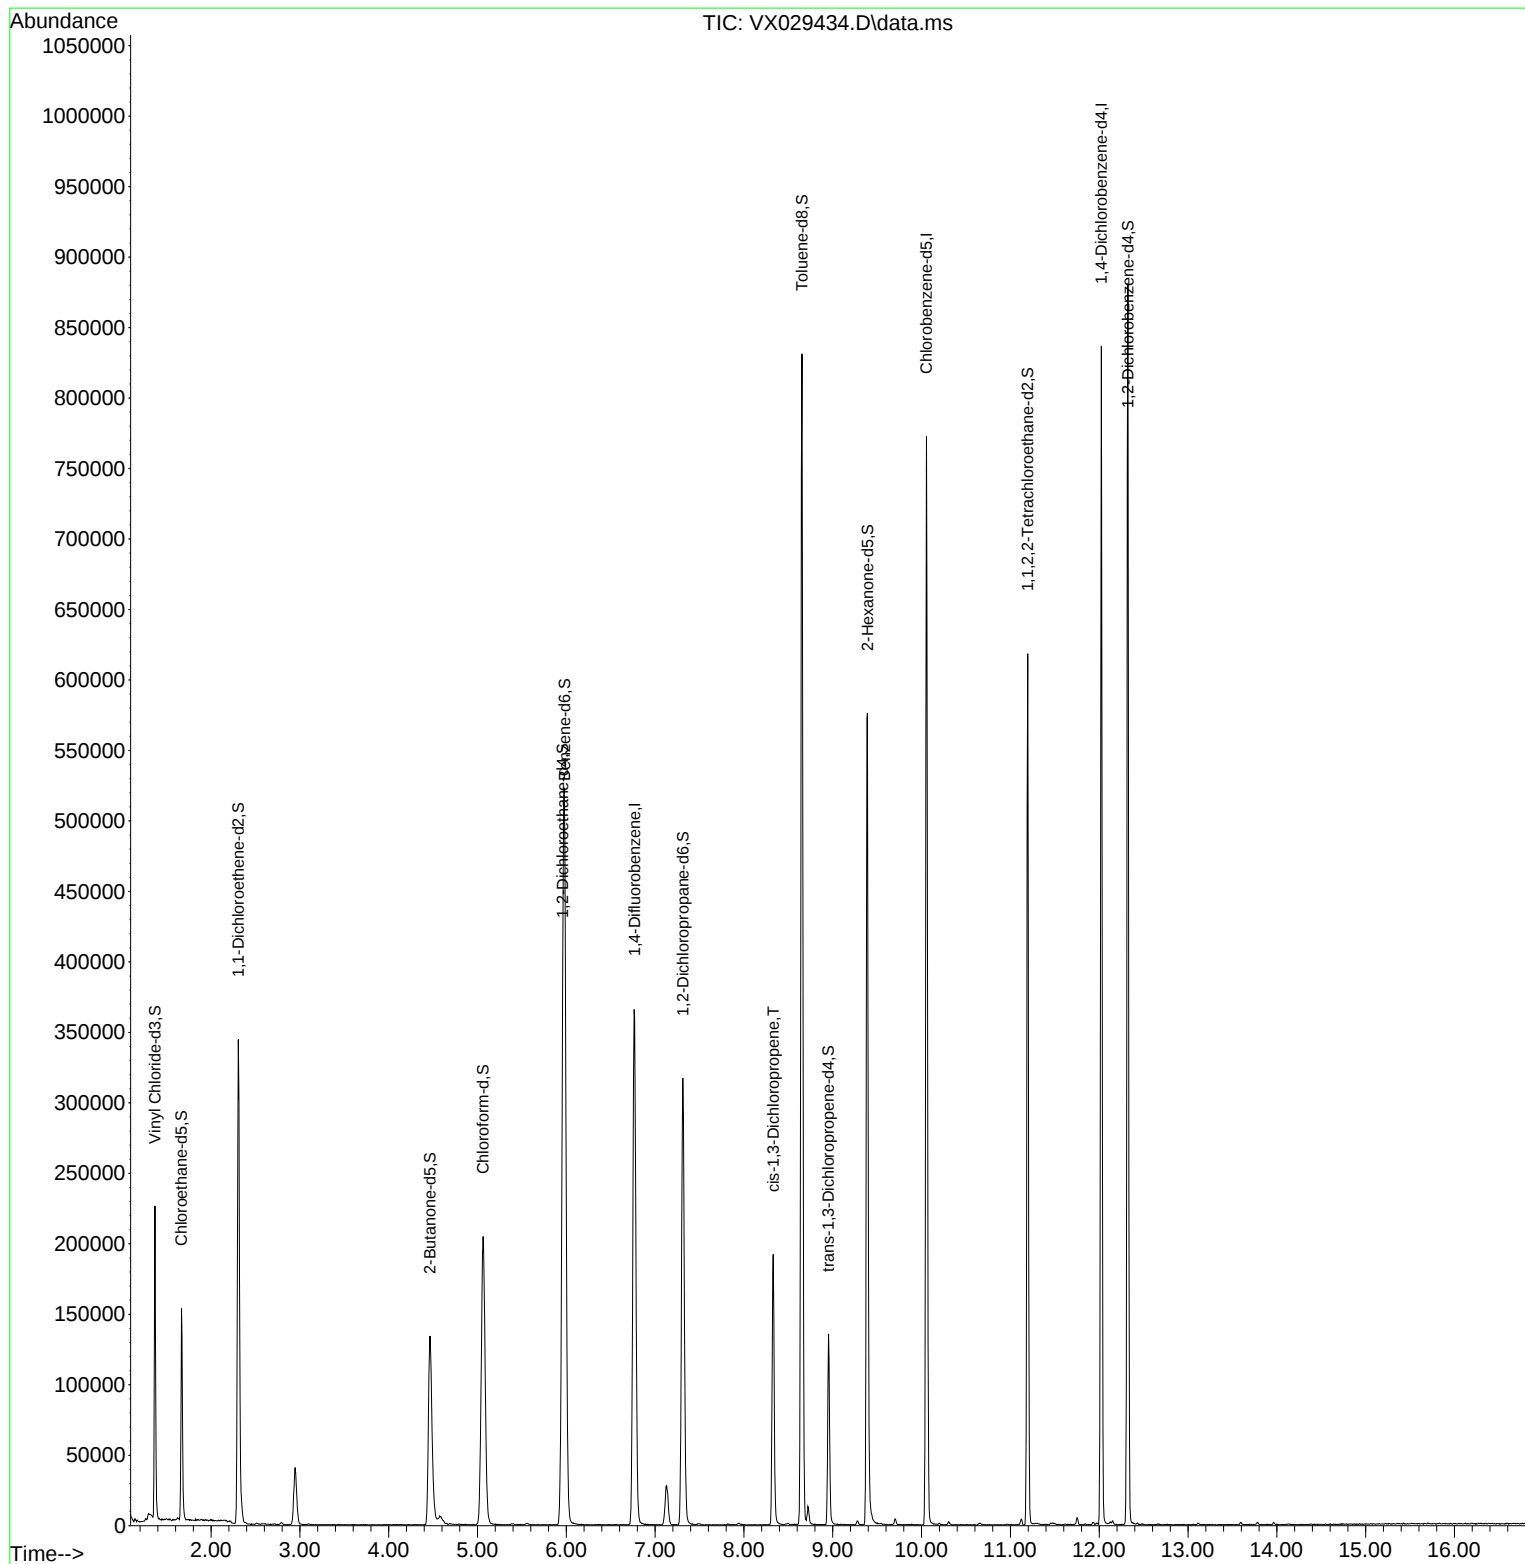

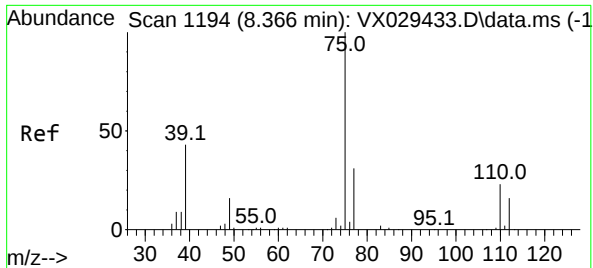

#39
 cis-1,3-Dichloropropene
 Concen: 1.097 ug/L
 RT: 8.329 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VX029434.D
 Acq: 13 Jun 2022 23:58

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK659

Tgt Ion: 75 Resp: 4875
 Ion Ratio Lower Upper
 75 100
 77 45.9 21.1 39.1#

