

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029410.D
 Acq On : 13 Jun 2022 13:52
 Operator : JC/MD
 Sample : VX0613MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK657

Quant Time: Jun 14 04:23:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 14 04:22:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	364185	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	327596	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	154923	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	139937	49.628	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	99.260%
7) Chloroethane-d5	1.666	69	110594	63.112	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	126.220%
11) 1,1-Dichloroethene-d2	2.306	63	192878	37.965	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.940%
21) 2-Butanone-d5	4.459	46	229070	107.147	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.150%
24) Chloroform-d	5.062	84	263615	48.965	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.940%
26) 1,2-Dichloroethane-d4	5.958	65	177073	50.872	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.740%
32) Benzene-d6	5.977	84	543487	53.113	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.220%
36) 1,2-Dichloropropane-d6	7.312	67	160732	53.629	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.260%
41) Toluene-d8	8.653	98	491471	50.945	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.880%
43) trans-1,3-Dichloroprop...	8.952	79	73753	49.905	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.820%
47) 2-Hexanone-d5	9.384	63	177750	109.651	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.650%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	231524	52.683	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.360%
66) 1,2-Dichlorobenzene-d4	12.323	152	172317	53.500	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.000%
Target Compounds						
					Qvalue	
34) Trichloroethene	7.135	95	15877	4.205	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029410.D
Acq On : 13 Jun 2022 13:52
Operator : JC/MD
Sample : VX0613MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK657


Quant Time: Jun 14 04:23:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 14 04:22:00 2022
Response via : Initial Calibration

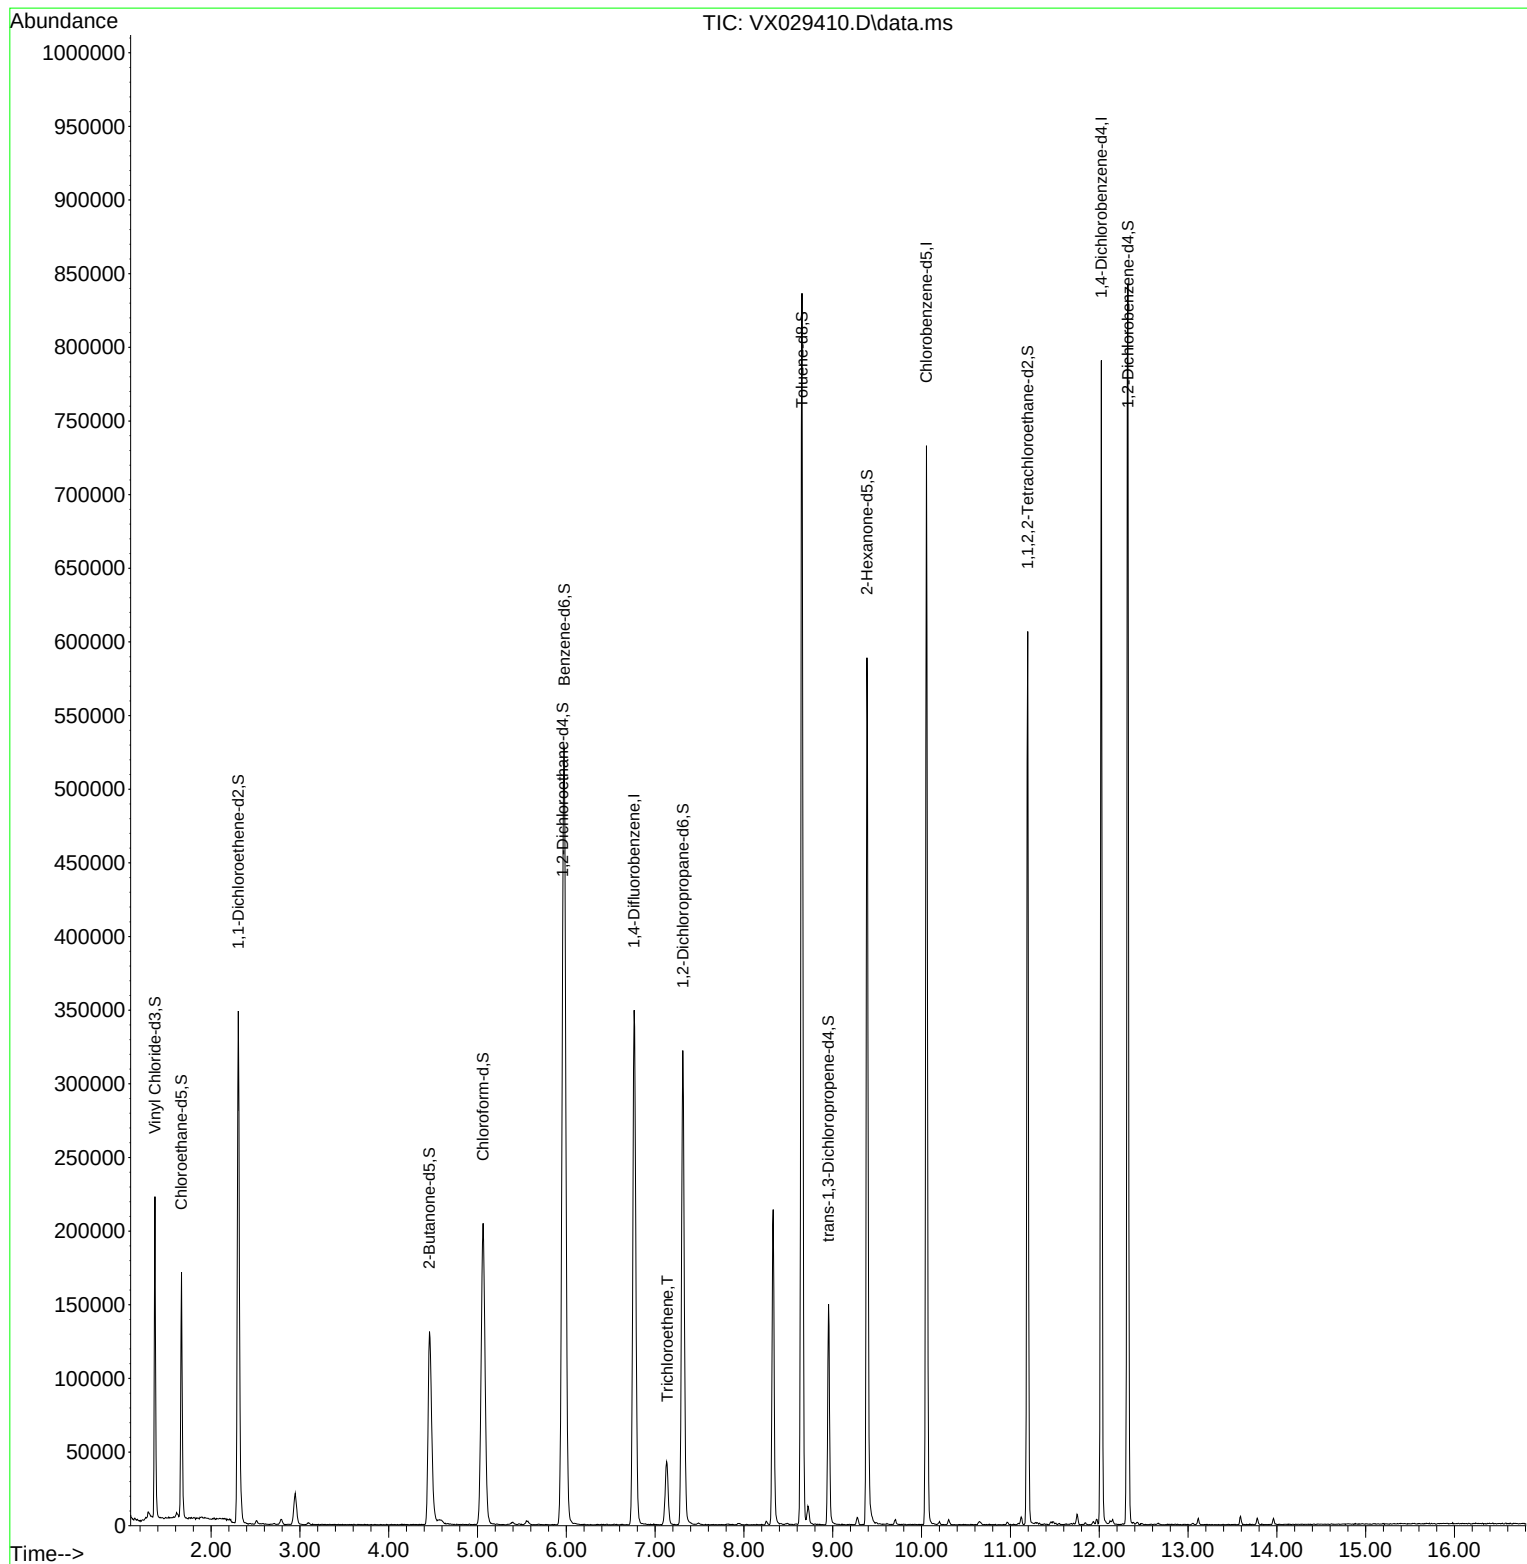

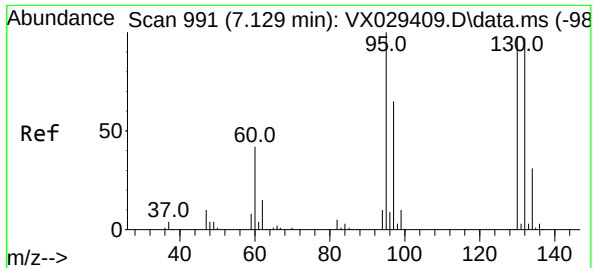

#34
 Trichloroethene
 Concen: 4.205 ug/L
 RT: 7.135 min Scan# 991
 Delta R.T. 0.006 min
 Lab File: VX029410.D
 Acq: 13 Jun 2022 13:52

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK657

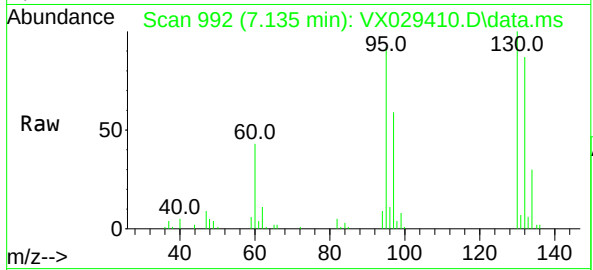

Tgt Ion: 95 Resp: 15877

Ion	Ratio	Lower	Upper
95	100		
97	64.5	45.5	84.5
132	94.5	69.9	129.7
130	108.8	70.8	131.6

