

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029412.D
 Acq On : 13 Jun 2022 15:03
 Operator : JC/MD
 Sample : N3249-05 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYT1

Quant Time: Jun 14 04:23:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 14 04:22:00 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	313104	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	277687	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	137790	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	126471	52.169	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	104.340%	
7) Chloroethane-d5	1.660	69	100362	66.617	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	133.240%#	
11) 1,1-Dichloroethene-d2	2.306	63	175269	40.128	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	80.260%	
21) 2-Butanone-d5	4.452	46	208334	113.346	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	113.350%	
24) Chloroform-d	5.056	84	245469	53.033	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.060%	
26) 1,2-Dichloroethane-d4	5.952	65	160993	53.798	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	107.600%	
32) Benzene-d6	5.970	84	492297	56.757	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	113.520%	
36) 1,2-Dichloropropane-d6	7.305	67	148462	58.438	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	116.880%	
41) Toluene-d8	8.647	98	449690	54.992	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	109.980%	
43) trans-1,3-Dichloroprop...	8.952	79	67659	54.010	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	108.020%	
47) 2-Hexanone-d5	9.384	63	162270	118.093	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	118.090%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	211085	56.665	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	113.320%	
66) 1,2-Dichlorobenzene-d4	12.323	152	161702	56.446	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	112.900%	
Target Compounds						
34) Trichloroethene	7.129	95	10411	3.253	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029412.D
Acq On : 13 Jun 2022 15:03
Operator : JC/MD
Sample : N3249-05 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYT1

Quant Time: Jun 14 04:23:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 14 04:22:00 2022
Response via : Initial Calibration

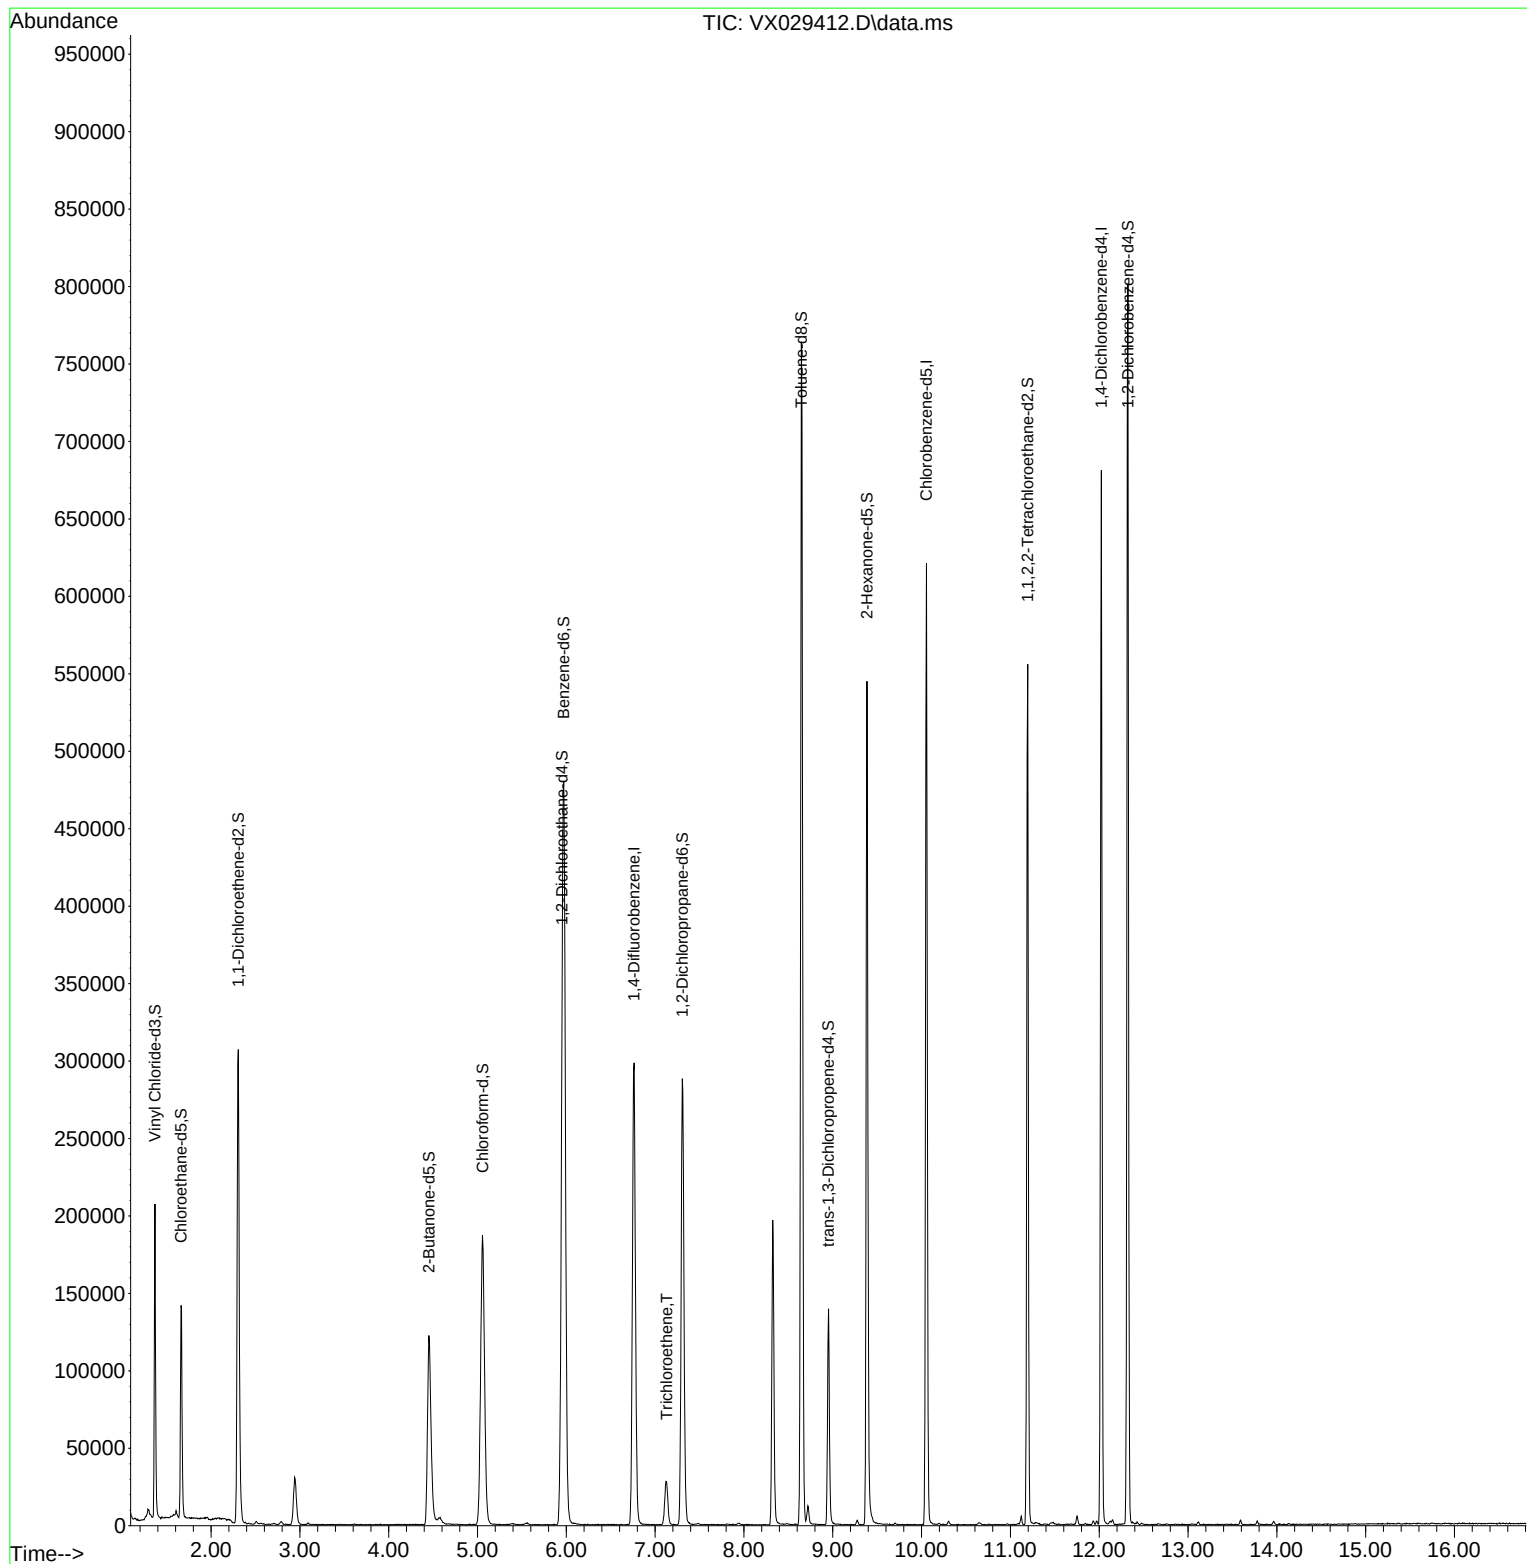

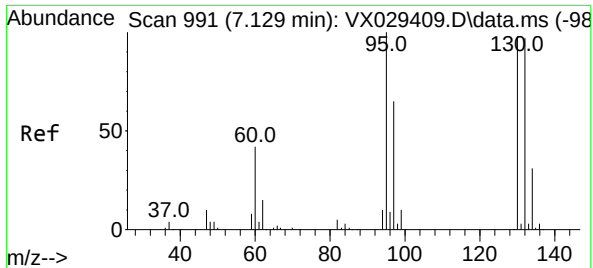

#34
 Trichloroethene
 Concen: 3.253 ug/L
 RT: 7.129 min Scan# 991
 Delta R.T. 0.000 min
 Lab File: VX029412.D
 Acq: 13 Jun 2022 15:03

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYT1

Tgt Ion: 95 Resp: 10411

Ion	Ratio	Lower	Upper
95	100		
97	58.6	45.5	84.5
132	87.2	69.9	129.7
130	105.7	70.8	131.6

