

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029414.D
 Acq On : 13 Jun 2022 15:49
 Operator : JC/MD
 Sample : N3291-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX1

Quant Time: Jun 14 04:24:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 14 04:22:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	380046	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	335482	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	159894	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	117343	39.878	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.760%
7) Chloroethane-d5	1.666	69	94091	51.453	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.900%
11) 1,1-Dichloroethene-d2	2.306	63	164555	31.039	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.080%
21) 2-Butanone-d5	4.458	46	208215	93.327	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.330%
24) Chloroform-d	5.062	84	233325	41.530	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.060%
26) 1,2-Dichloroethane-d4	5.964	65	154167	42.443	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.880%
32) Benzene-d6	5.976	84	465232	44.396	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.800%
36) 1,2-Dichloropropane-d6	7.311	67	139342	45.399	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.800%
41) Toluene-d8	8.653	98	416562	42.165	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.320%
43) trans-1,3-Dichloroprop...	8.951	79	63711	42.097	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.200%
47) 2-Hexanone-d5	9.384	63	158866	95.698	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.700%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	205248	45.606	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.220%
66) 1,2-Dichlorobenzene-d4	12.323	152	148518	44.677	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.360%
Target Compounds						
					Qvalue	
34) Trichloroethene	7.129	95	16231	4.198	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029414.D
Acq On : 13 Jun 2022 15:49
Operator : JC/MD
Sample : N3291-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX1


Quant Time: Jun 14 04:24:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 14 04:22:00 2022
Response via : Initial Calibration

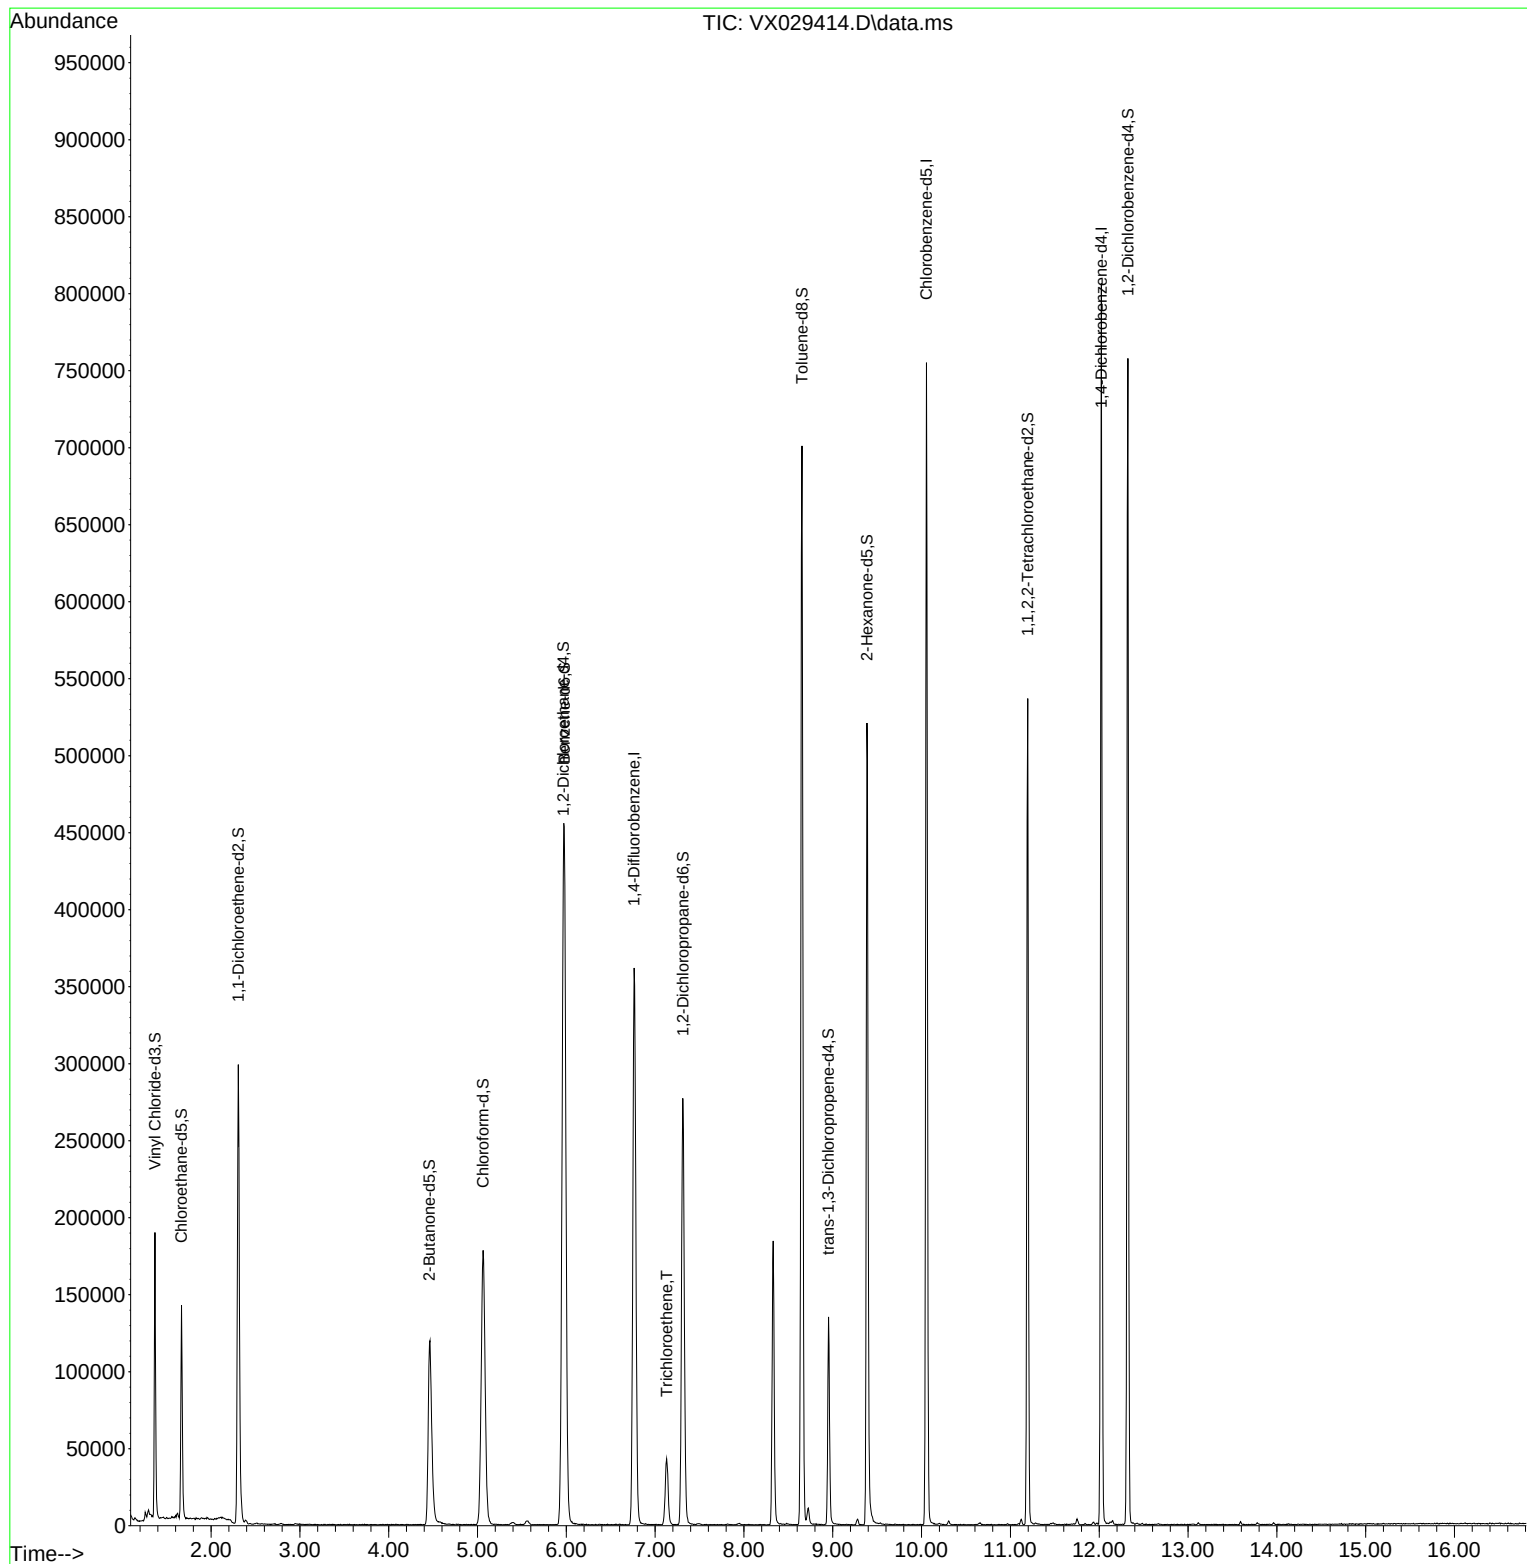

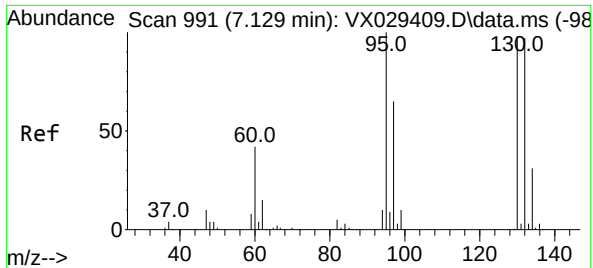

#34
 Trichloroethene
 Concen: 4.198 ug/L
 RT: 7.129 min Scan# 991
 Delta R.T. -0.000 min
 Lab File: VX029414.D
 Acq: 13 Jun 2022 15:49

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX1

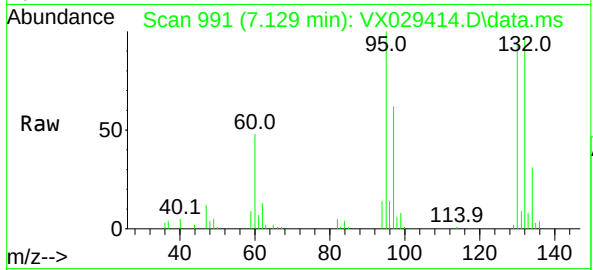

Tgt Ion: 95 Resp: 16231

Ion	Ratio	Lower	Upper
95	100		
97	62.2	45.5	84.5
132	96.1	69.9	129.7
130	92.6	70.8	131.6

