

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029425.D
 Acq On : 13 Jun 2022 20:06
 Operator : JC/MD
 Sample : N3291-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY8

Quant Time: Jun 14 04:26:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 14 04:22:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	368755	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	329930	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	154484	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	117464	41.141	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.280%
7) Chloroethane-d5	1.666	69	92456	52.107	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.220%
11) 1,1-Dichloroethene-d2	2.306	63	163498	31.783	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.560%
21) 2-Butanone-d5	4.465	46	210246	97.123	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.120%
24) Chloroform-d	5.068	84	232274	42.609	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.220%
26) 1,2-Dichloroethane-d4	5.964	65	153973	43.687	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.380%
32) Benzene-d6	5.976	84	462921	44.919	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.840%
36) 1,2-Dichloropropane-d6	7.312	67	140545	46.562	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.120%
41) Toluene-d8	8.653	98	417790	43.001	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.000%
43) trans-1,3-Dichloroprop...	8.952	79	60540	40.675	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.340%
47) 2-Hexanone-d5	9.384	63	160396	98.245	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.250%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	205987	46.540	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.080%
66) 1,2-Dichlorobenzene-d4	12.323	152	148764	46.318	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.640%
Target Compounds						
					Qvalue	
34) Trichloroethene	7.135	95	13478	3.545	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029425.D
Acq On : 13 Jun 2022 20:06
Operator : JC/MD
Sample : N3291-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY8


Quant Time: Jun 14 04:26:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 14 04:22:00 2022
Response via : Initial Calibration

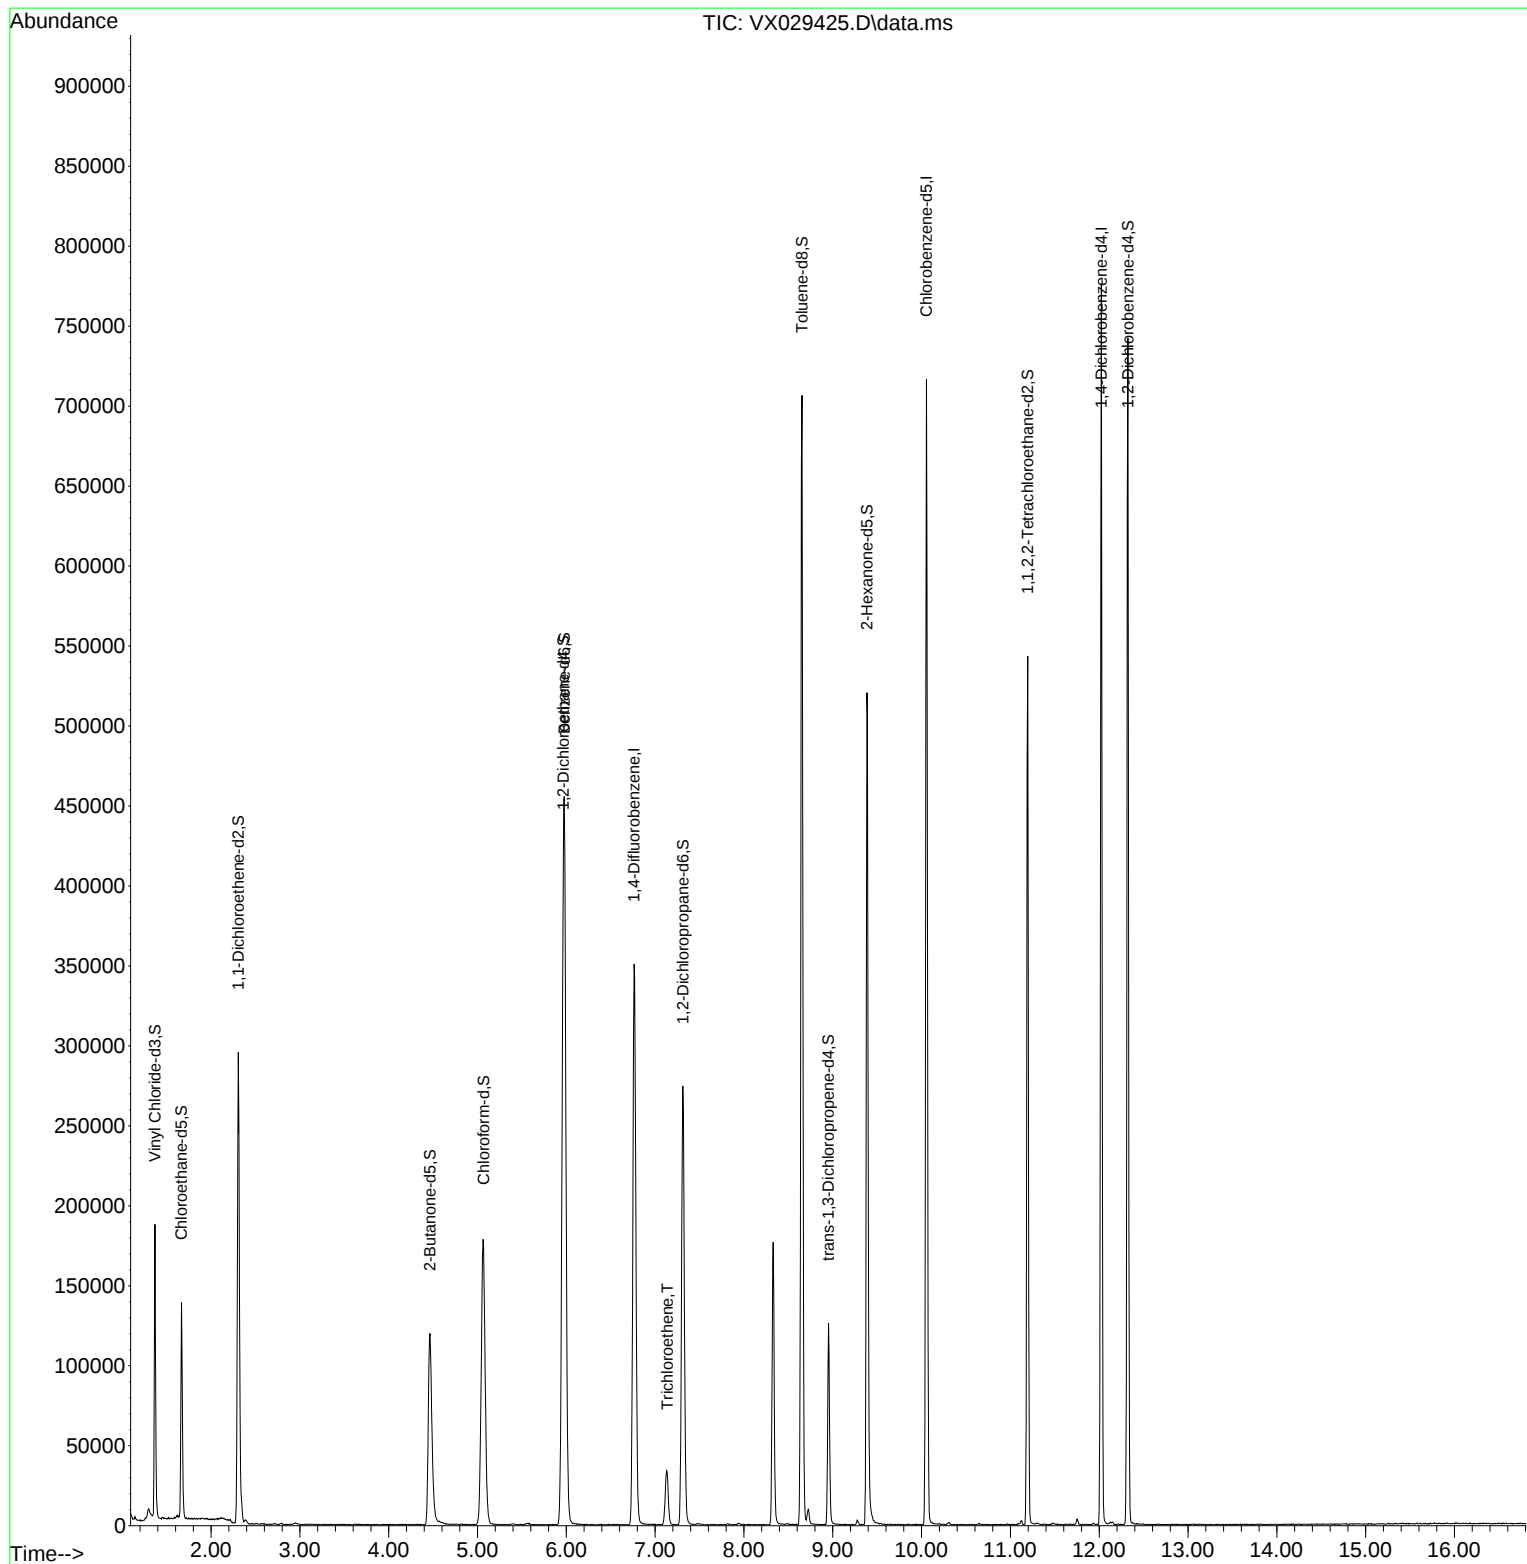

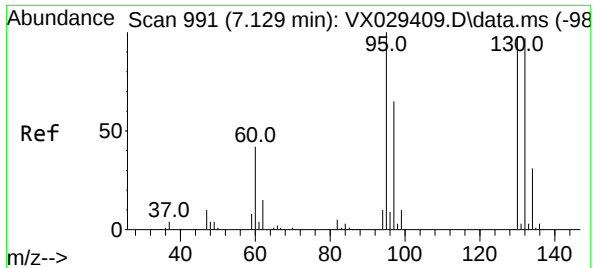

#34
 Trichloroethene
 Concen: 3.545 ug/L
 RT: 7.135 min Scan# 991
 Delta R.T. 0.006 min
 Lab File: VX029425.D
 Acq: 13 Jun 2022 20:06

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY8

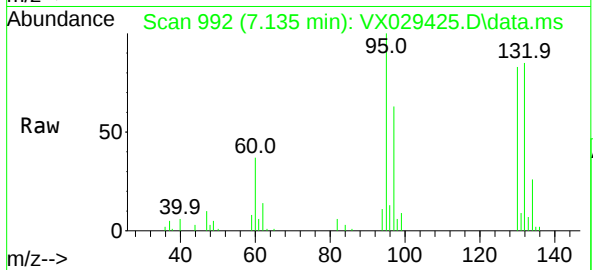

Tgt Ion: 95 Resp: 13478

Ion	Ratio	Lower	Upper
95	100		
97	63.2	45.5	84.5
132	84.7	69.9	129.7
130	83.5	70.8	131.6

