

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029407.D
 Acq On : 13 Jun 2022 12:13
 Operator : JC/MD
 Sample : VIBLK642
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	11	13	19	rVB2	4938	4786	0.30%	0.038%
2	1.294	31	34	37	rBV2	4992	7001	0.44%	0.056%
3	1.368	42	46	54	rVB	223984	228481	14.45%	1.816%
4	1.666	91	95	105	rVB	168734	199755	12.64%	1.588%
5	2.306	194	200	211	rBV	357765	578021	36.57%	4.594%
6	2.514	228	234	240	rBV	13428	22176	1.40%	0.176%
7	2.715	262	267	271	rBV4	1466	2800	0.18%	0.022%
8	2.794	275	280	288	rVB4	4352	7955	0.50%	0.063%
9	2.947	297	305	315	rBV	16590	38912	2.46%	0.309%
10	3.099	324	330	339	rVB4	8191	19403	1.23%	0.154%
11	3.343	368	370	374	rBV3	468	605	0.04%	0.005%
12	3.416	380	382	385	rVB2	292	328	0.02%	0.003%
13	3.459	388	389	392	rBV3	392	310	0.02%	0.002%
14	3.605	411	413	415	rBV2	890	769	0.05%	0.006%
15	3.940	465	468	470	rBV2	243	314	0.02%	0.002%
16	4.215	508	513	514	rBV3	271	386	0.02%	0.003%
17	4.233	514	516	521	rVB2	436	517	0.03%	0.004%
18	4.465	544	554	569	rBV	130647	382743	24.21%	3.042%
19	4.714	593	595	598	rBV2	360	339	0.02%	0.003%
20	4.903	620	626	634	rVB7	1847	4932	0.31%	0.039%
21	5.062	639	652	667	rBV	205304	631158	39.93%	5.016%
22	5.263	681	685	689	rVB4	526	757	0.05%	0.006%
23	5.391	698	706	712	rBV6	2844	8040	0.51%	0.064%
24	5.550	728	732	739	rVB5	2465	5929	0.38%	0.047%
25	5.647	745	748	749	rBV3	722	760	0.05%	0.006%
26	5.678	749	753	761	rVB5	1896	4951	0.31%	0.039%
27	5.800	769	773	776	rBV2	358	561	0.04%	0.004%
28	5.879	784	786	789	rBV	267	409	0.03%	0.003%
29	5.970	789	801	819	rBV2	530752	1580797	100.00%	12.563%
30	6.178	833	835	837	rBV2	367	346	0.02%	0.003%
31	6.232	842	844	846	rBV3	320	319	0.02%	0.003%
32	6.543	892	895	901	rVV4	492	888	0.06%	0.007%
33	6.763	922	931	948	rVV	367605	865945	54.78%	6.882%
34	7.129	982	991	1001	rBV3	50791	118920	7.52%	0.945%
35	7.312	1011	1021	1030	rBV	313481	690583	43.69%	5.488%
36	7.787	1097	1099	1101	rBV2	491	353	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029407.D
 Acq On : 13 Jun 2022 12:13
 Operator : JC/MD
 Sample : VIBLK642
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.830	1101	1106	1112	rVB5	2130	4490	0.28%	0.036%
38	7.933	1120	1123	1124	rBV2	809	707	0.04%	0.006%
39	8.250	1172	1175	1177	rBV3	309	346	0.02%	0.003%
40	8.330	1181	1188	1200	rBV	217790	368952	23.34%	2.932%
41	8.488	1210	1214	1217	rBV5	873	1188	0.08%	0.009%
42	8.580	1224	1229	1234	rBV2	3377	5638	0.36%	0.045%
43	8.653	1234	1241	1248	rBV	845723	1312699	83.04%	10.433%
44	8.720	1248	1252	1260	rVB	20804	33924	2.15%	0.270%
45	8.854	1271	1274	1276	rBV2	313	384	0.02%	0.003%
46	8.952	1284	1290	1306	rVV	158460	238122	15.06%	1.892%
47	9.061	1306	1308	1311	rVV2	674	762	0.05%	0.006%
48	9.092	1311	1313	1315	rVV2	386	464	0.03%	0.004%
49	9.159	1319	1324	1331	rVB4	3028	5279	0.33%	0.042%
50	9.275	1338	1343	1349	rBV2	13728	20010	1.27%	0.159%
51	9.384	1355	1361	1381	rBV	586008	848004	53.64%	6.739%
52	9.525	1381	1384	1390	rVB6	2683	4087	0.26%	0.032%
53	9.610	1395	1398	1404	rVB2	2045	2855	0.18%	0.023%
54	9.701	1410	1413	1419	rVB4	1440	2324	0.15%	0.018%
55	9.817	1430	1432	1434	rBV2	383	337	0.02%	0.003%
56	10.055	1465	1471	1483	rBV	765512	1020145	64.53%	8.108%
57	10.195	1489	1494	1501	rVB	13862	19325	1.22%	0.154%
58	10.305	1507	1512	1518	rBV	15099	21378	1.35%	0.170%
59	10.652	1563	1569	1578	rVB2	17691	33850	2.14%	0.269%
60	10.750	1583	1585	1590	rBV4	432	789	0.05%	0.006%
61	10.805	1590	1594	1597	rBV3	1575	2145	0.14%	0.017%
62	10.963	1616	1620	1627	rVB	16009	21511	1.36%	0.171%
63	11.018	1627	1629	1630	rBV2	387	335	0.02%	0.003%
64	11.085	1637	1640	1642	rBV4	1792	2244	0.14%	0.018%
65	11.122	1643	1646	1650	rVB	5857	7191	0.45%	0.057%
66	11.195	1652	1658	1664	rBV	606300	776283	49.11%	6.169%
67	11.378	1683	1688	1689	rBV2	699	661	0.04%	0.005%
68	11.451	1696	1700	1708	rBV	19248	26078	1.65%	0.207%
69	11.683	1733	1738	1739	rBV4	641	933	0.06%	0.007%
70	11.756	1745	1750	1756	rVB2	23473	31108	1.97%	0.247%
71	11.841	1760	1764	1768	rVB3	1258	1671	0.11%	0.013%
72	11.896	1770	1773	1776	rBV	453	307	0.02%	0.002%
73	11.933	1776	1779	1782	rBV3	2577	3881	0.25%	0.031%
74	11.969	1782	1785	1789	rVB	20428	23363	1.48%	0.186%
75	12.024	1789	1794	1805	rVB	811301	1018264	64.41%	8.093%
76	12.128	1807	1811	1813	rBV4	2113	3263	0.21%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029407.D
 Acq On : 13 Jun 2022 12:13
 Operator : JC/MD
 Sample : VIBLK642
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.219	1825	1826	1829	rBV3	448	435	0.03%	0.003%
78	12.268	1831	1834	1835	rBV2	437	441	0.03%	0.004%
79	12.323	1837	1843	1850	rVV	867204	1126549	71.26%	8.953%
80	12.427	1857	1860	1864	rVB4	1956	2463	0.16%	0.020%
81	12.609	1886	1890	1892	rVB3	311	390	0.02%	0.003%
82	12.652	1895	1897	1898	rBV2	471	454	0.03%	0.004%
83	12.865	1928	1932	1933	rBV3	432	382	0.02%	0.003%
84	12.951	1942	1946	1948	rVB3	1584	2092	0.13%	0.017%
85	12.975	1948	1950	1953	rVB2	318	383	0.02%	0.003%
86	13.012	1953	1956	1959	rVB3	377	415	0.03%	0.003%
87	13.061	1959	1964	1967	rBV5	583	940	0.06%	0.007%
88	13.115	1967	1973	1978	rBV	28137	35516	2.25%	0.282%
89	13.201	1985	1987	1989	rBV2	283	315	0.02%	0.003%
90	13.286	1997	2001	2004	rVB2	324	387	0.02%	0.003%
91	13.591	2045	2051	2062	rVB	35039	45597	2.88%	0.362%
92	13.670	2062	2064	2068	rBV2	344	338	0.02%	0.003%
93	13.780	2077	2082	2089	rVB	32421	43503	2.75%	0.346%
94	13.835	2089	2091	2093	rVB2	517	504	0.03%	0.004%
95	13.859	2093	2095	2097	rBV2	470	412	0.03%	0.003%
96	13.963	2106	2112	2122	rVB	32577	42131	2.67%	0.335%
97	14.201	2148	2151	2152	rBV2	508	364	0.02%	0.003%
98	15.005	2279	2283	2286	rBV4	568	781	0.05%	0.006%
99	15.280	2326	2328	2331	rBV3	572	684	0.04%	0.005%
100	15.335	2335	2337	2341	rBV5	472	705	0.04%	0.006%




Sum of corrected areas: 12582727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029407.D
Acq On : 13 Jun 2022 12:13
Operator : JC/MD
Sample : VIBLK642
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

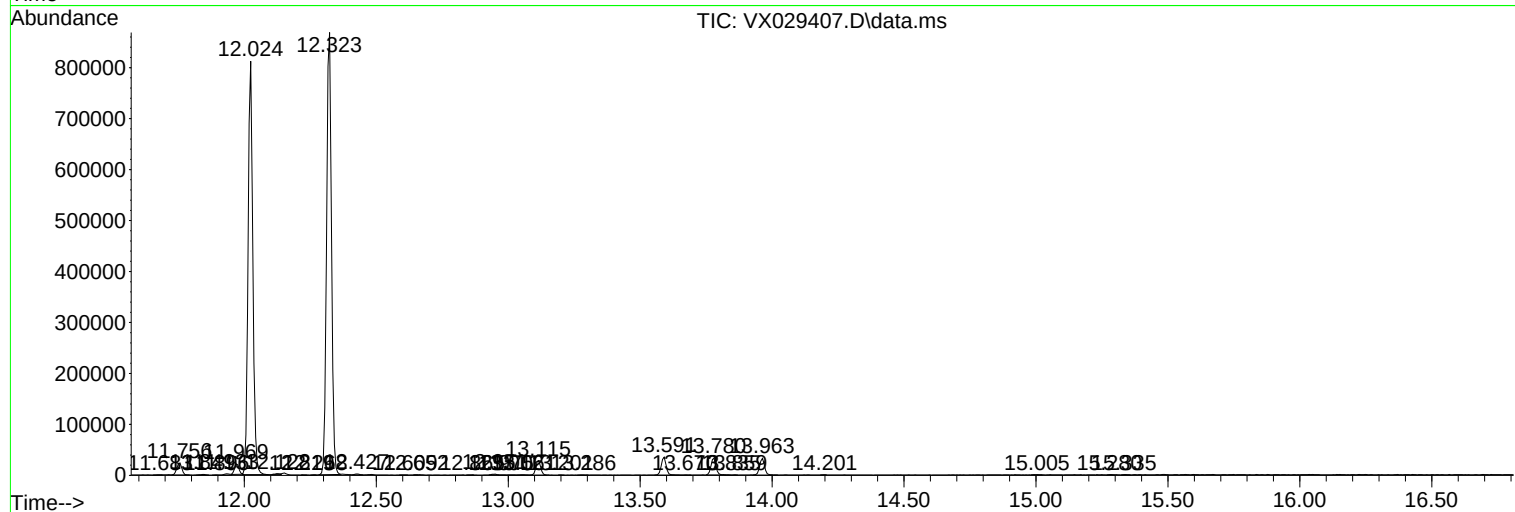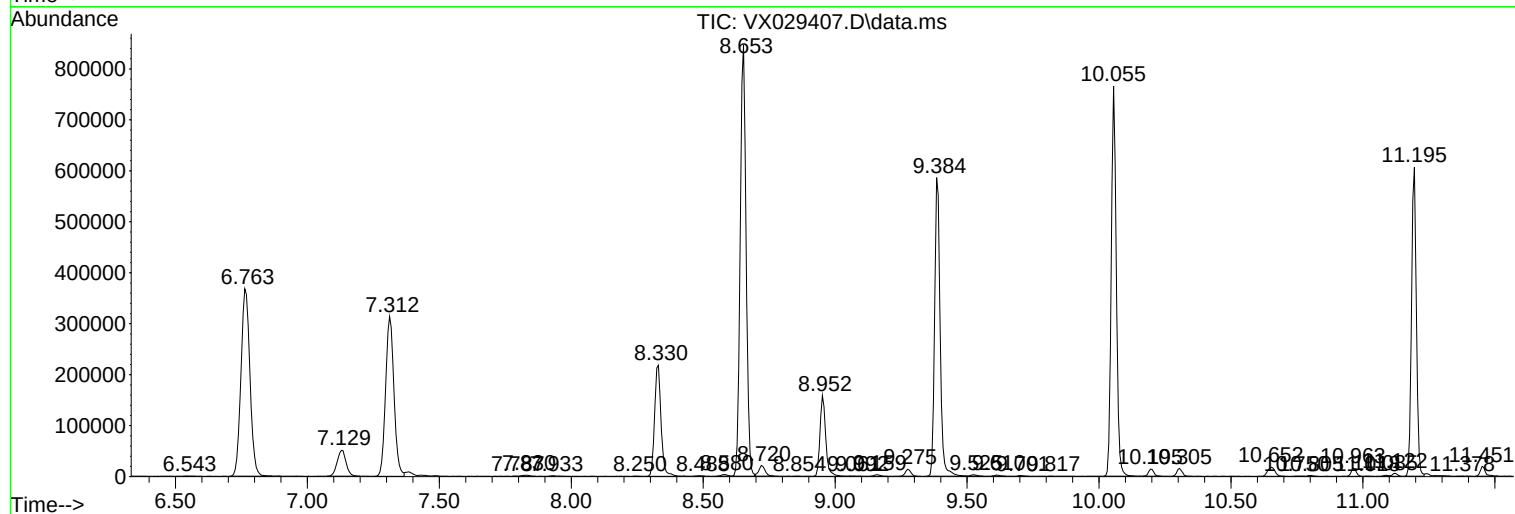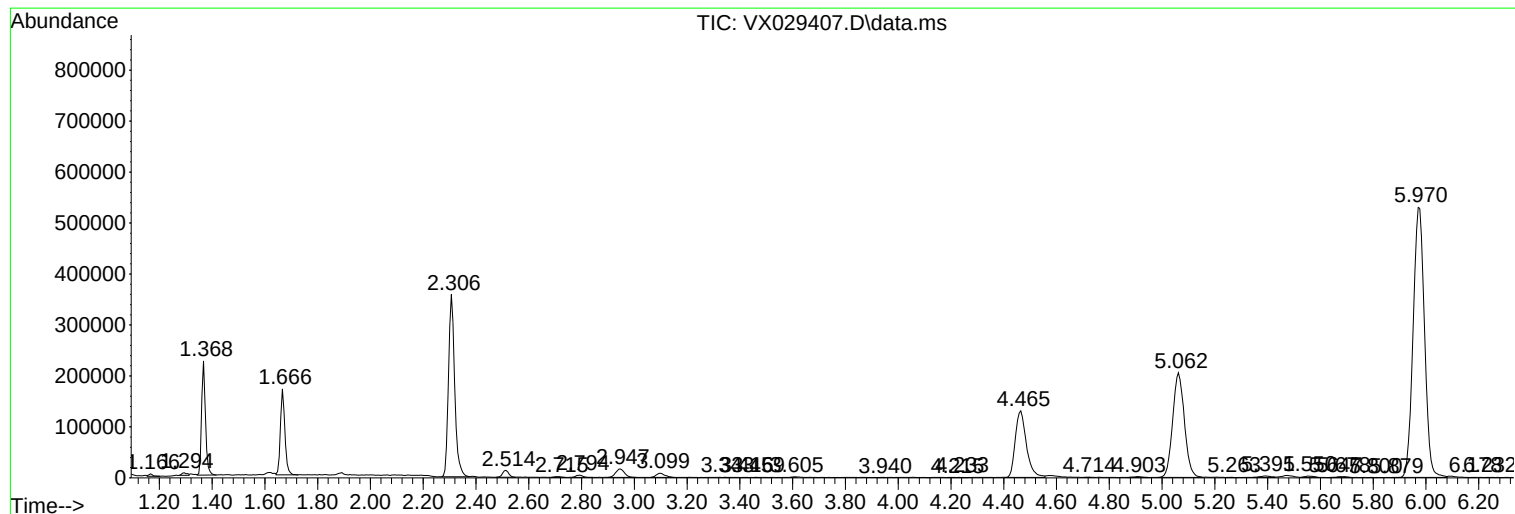

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029407.D
Acq On : 13 Jun 2022 12:13
Operator : JC/MD
Sample : VIBLK642
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029407.D
Acq On : 13 Jun 2022 12:13
Operator : JC/MD
Sample : VIBLK642
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------