

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029411.D
 Acq On : 13 Jun 2022 14:15
 Operator : JC/MD
 Sample : VX0613WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK658

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	218853	220248	13.96%	1.839%
2	1.666	91	95	105	rVB	165232	195068	12.36%	1.629%
3	2.306	194	200	212	rVB	349685	555549	35.21%	4.640%
4	2.508	230	233	239	rVB2	1703	2636	0.17%	0.022%
5	2.788	273	279	289	rBV	7772	13595	0.86%	0.114%
6	2.947	296	305	314	rBV	22118	51224	3.25%	0.428%
7	3.178	341	343	345	rBV	293	263	0.02%	0.002%
8	3.227	350	351	354	rVB	502	346	0.02%	0.003%
9	3.910	460	463	465	rBV3	336	389	0.02%	0.003%
10	4.117	496	497	500	rBV2	248	273	0.02%	0.002%
11	4.465	544	554	567	rBV	130833	373391	23.67%	3.118%
12	4.769	602	604	605	rBV2	480	310	0.02%	0.003%
13	5.062	638	652	670	rBV	207220	633772	40.17%	5.293%
14	5.275	685	687	690	rVB2	398	403	0.03%	0.003%
15	5.336	696	697	699	rVB	366	246	0.02%	0.002%
16	5.385	699	705	713	rBV5	1504	4416	0.28%	0.037%
17	5.477	716	720	721	rVV3	496	596	0.04%	0.005%
18	5.562	724	734	743	rBV5	2619	7392	0.47%	0.062%
19	5.672	750	752	754	rBV3	262	333	0.02%	0.003%
20	5.970	788	801	820	rBV2	535893	1577747	100.00%	13.177%
21	6.245	845	846	849	rVB2	330	294	0.02%	0.002%
22	6.294	849	854	855	rBV3	330	417	0.03%	0.003%
23	6.361	864	865	866	rVV	624	267	0.02%	0.002%
24	6.550	892	896	899	rBV3	297	425	0.03%	0.004%
25	6.763	922	931	949	rBV	354885	852828	54.05%	7.123%
26	7.129	980	991	1002	rBV2	41797	98046	6.21%	0.819%
27	7.312	1012	1021	1037	rBV	319417	698557	44.28%	5.834%
28	7.476	1046	1048	1050	rBV3	772	834	0.05%	0.007%
29	7.568	1061	1063	1066	rVB3	278	251	0.02%	0.002%
30	7.604	1066	1069	1073	rVB2	381	432	0.03%	0.004%
31	7.647	1073	1076	1080	rBV2	348	603	0.04%	0.005%
32	7.818	1101	1104	1107	rBV3	691	748	0.05%	0.006%
33	7.866	1110	1112	1115	rBV2	251	376	0.02%	0.003%
34	7.933	1120	1123	1128	rBV3	974	1693	0.11%	0.014%
35	8.208	1167	1168	1172	rBV3	248	345	0.02%	0.003%
36	8.330	1181	1188	1199	rBV	216655	354757	22.49%	2.963%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029411.D
 Acq On : 13 Jun 2022 14:15
 Operator : JC/MD
 Sample : VX0613WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK658

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.488	1211	1214	1221	rVB4	777	1591	0.10%	0.013%
38	8.653	1234	1241	1249	rBV	836602	1301139	82.47%	10.867%
39	8.720	1249	1252	1260	rVB	12973	20065	1.27%	0.168%
40	8.830	1269	1270	1276	rVB3	405	439	0.03%	0.004%
41	8.885	1278	1279	1281	rVB2	459	256	0.02%	0.002%
42	8.903	1281	1282	1285	rBV	434	339	0.02%	0.003%
43	8.952	1285	1290	1303	rBV	149632	222268	14.09%	1.856%
44	9.275	1338	1343	1350	rVB3	4737	7144	0.45%	0.060%
45	9.384	1356	1361	1376	rBV	581242	846031	53.62%	7.066%
46	9.610	1394	1398	1405	rVB4	638	1172	0.07%	0.010%
47	9.695	1410	1412	1417	rVB3	1421	1824	0.12%	0.015%
48	9.878	1441	1442	1444	rBV2	320	272	0.02%	0.002%
49	9.958	1454	1455	1458	rVB	579	346	0.02%	0.003%
50	9.994	1458	1461	1463	rBV2	622	631	0.04%	0.005%
51	10.055	1465	1471	1489	rVV	740911	993531	62.97%	8.298%
52	10.195	1491	1494	1501	rVB3	1822	2792	0.18%	0.023%
53	10.268	1504	1506	1508	rBV2	290	308	0.02%	0.003%
54	10.305	1508	1512	1520	rVB3	3119	4987	0.32%	0.042%
55	10.366	1520	1522	1523	rBV	418	300	0.02%	0.003%
56	10.427	1530	1532	1533	rBV2	367	255	0.02%	0.002%
57	10.457	1535	1537	1539	rVB	458	295	0.02%	0.002%
58	10.622	1562	1564	1565	rBV	359	277	0.02%	0.002%
59	10.659	1565	1570	1578	rVV6	1781	3506	0.22%	0.029%
60	10.720	1578	1580	1581	rVB	468	249	0.02%	0.002%
61	10.750	1581	1585	1586	rBV2	548	553	0.04%	0.005%
62	10.854	1601	1602	1606	rBV2	375	455	0.03%	0.004%
63	10.896	1608	1609	1610	rVV	568	261	0.02%	0.002%
64	10.921	1611	1613	1617	rVV2	456	531	0.03%	0.004%
65	10.963	1617	1620	1624	rVV4	1304	1591	0.10%	0.013%
66	11.030	1627	1631	1633	rVV	382	427	0.03%	0.004%
67	11.122	1638	1646	1652	rVB2	5217	7428	0.47%	0.062%
68	11.195	1652	1658	1668	rBV	612000	779934	49.43%	6.514%
69	11.451	1696	1700	1702	rBV5	1340	1940	0.12%	0.016%
70	11.543	1712	1715	1718	rBV3	778	1173	0.07%	0.010%
71	11.628	1725	1729	1732	rBV4	609	1036	0.07%	0.009%
72	11.665	1733	1735	1737	rVV2	678	722	0.05%	0.006%
73	11.707	1740	1742	1745	rVV2	696	836	0.05%	0.007%
74	11.750	1745	1749	1755	rVB3	5604	8323	0.53%	0.070%
75	11.841	1760	1764	1769	rVB3	1237	1809	0.11%	0.015%
76	11.933	1774	1779	1783	rBV3	2630	3889	0.25%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029411.D
 Acq On : 13 Jun 2022 14:15
 Operator : JC/MD
 Sample : VX0613WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK658

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.975	1783	1786	1789	rVB3	2021	2018	0.13%	0.017%
78	12.024	1789	1794	1806	rVB	805848	974257	61.75%	8.137%
79	12.122	1806	1810	1812	rBV4	2073	2916	0.18%	0.024%
80	12.323	1835	1843	1851	rBV	856917	1100075	69.72%	9.188%
81	12.427	1856	1860	1865	rBV5	1771	2409	0.15%	0.020%
82	12.579	1881	1885	1888	rBV2	366	478	0.03%	0.004%
83	12.628	1891	1893	1896	rBV2	470	621	0.04%	0.005%
84	12.817	1923	1924	1927	rVB	497	313	0.02%	0.003%
85	13.055	1960	1963	1966	rVV3	656	785	0.05%	0.007%
86	13.115	1970	1973	1980	rBV4	2931	3398	0.22%	0.028%
87	13.164	1980	1981	1985	rBV3	286	386	0.02%	0.003%
88	13.231	1990	1992	1993	rBV	405	328	0.02%	0.003%
89	13.396	2017	2019	2023	rBV3	263	490	0.03%	0.004%
90	13.591	2047	2051	2056	rVB3	3878	5244	0.33%	0.044%
91	13.780	2079	2082	2088	rVB	2384	3083	0.20%	0.026%
92	13.963	2108	2112	2118	rBV3	2898	4071	0.26%	0.034%
93	14.359	2174	2177	2178	rBV2	375	311	0.02%	0.003%
94	14.414	2184	2186	2187	rBV	412	313	0.02%	0.003%
95	14.749	2239	2241	2243	rBV3	396	327	0.02%	0.003%
96	14.865	2259	2260	2261	rBV	644	249	0.02%	0.002%
97	14.883	2261	2263	2266	rVB2	473	463	0.03%	0.004%
98	15.194	2313	2314	2315	rBV	466	277	0.02%	0.002%
99	15.286	2327	2329	2330	rBV	545	292	0.02%	0.002%
100	15.353	2338	2340	2342	rBV2	438	346	0.02%	0.003%




Sum of corrected areas: 11973445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029411.D
Acq On : 13 Jun 2022 14:15
Operator : JC/MD
Sample : VX0613WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK658

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

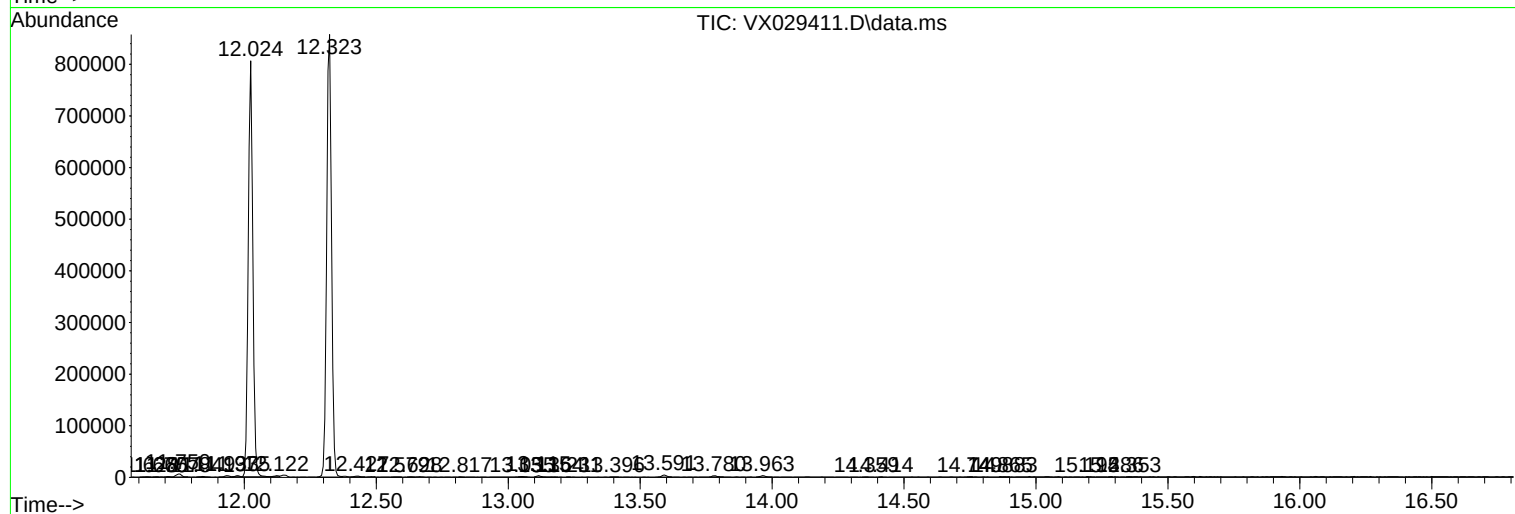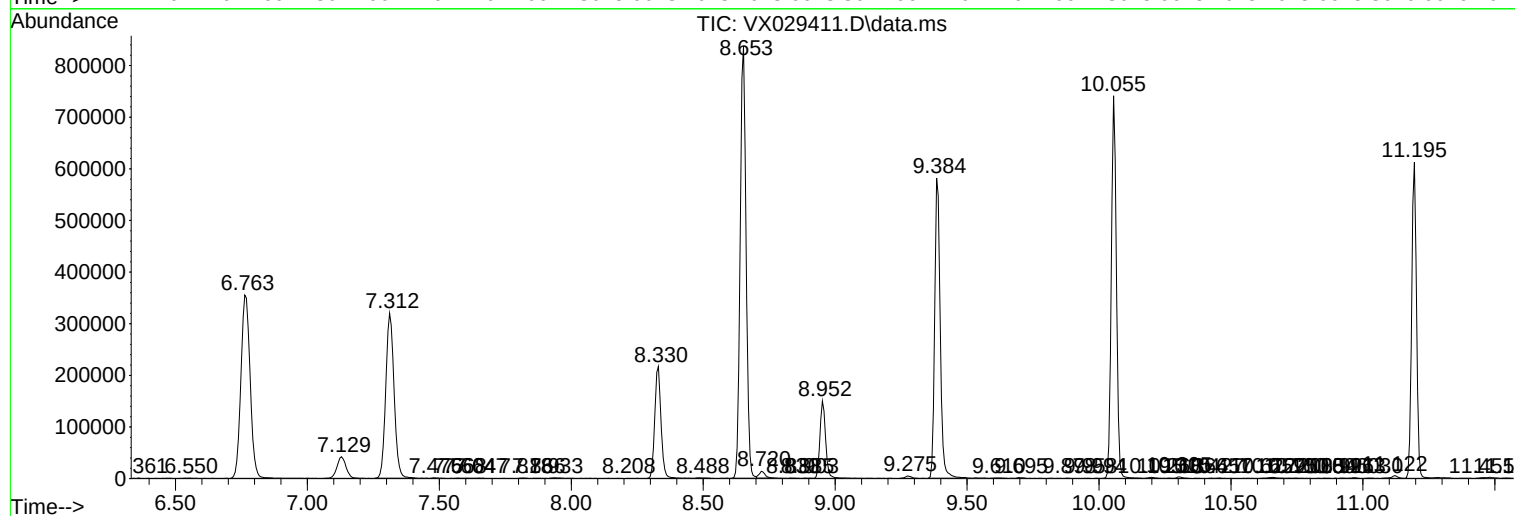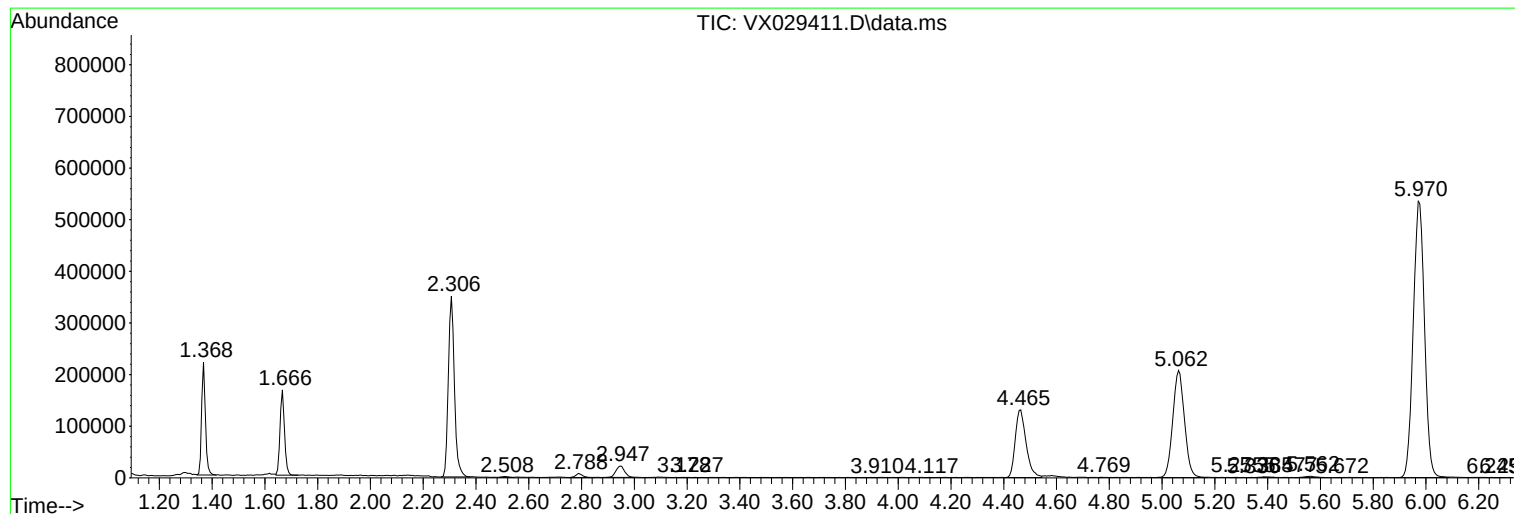

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029411.D
Acq On : 13 Jun 2022 14:15
Operator : JC/MD
Sample : VX0613WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK658

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029411.D
Acq On : 13 Jun 2022 14:15
Operator : JC/MD
Sample : VX0613WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK658

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------