

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029413.D
 Acq On : 13 Jun 2022 15:26
 Operator : JC/MD
 Sample : N3291-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	25	28	30	rBV	7180	7210	0.50%	0.065%
2	1.368	42	46	55	rVB	206237	202223	13.95%	1.817%
3	1.666	90	95	103	rVB	147085	180009	12.41%	1.617%
4	2.307	194	200	210	rBV	311915	494235	34.08%	4.440%
5	2.441	220	222	223	rBV	739	554	0.04%	0.005%
6	2.782	275	278	280	rBV3	595	869	0.06%	0.008%
7	2.947	299	305	308	rBV2	878	1383	0.10%	0.012%
8	3.477	390	392	394	rBV2	307	311	0.02%	0.003%
9	3.617	413	415	418	rBV2	513	402	0.03%	0.004%
10	3.776	438	441	443	rBV2	302	461	0.03%	0.004%
11	3.873	455	457	461	rVB3	248	361	0.02%	0.003%
12	3.910	461	463	466	rBV	234	317	0.02%	0.003%
13	4.044	483	485	489	rVB	340	372	0.03%	0.003%
14	4.459	543	553	568	rBV	120494	345017	23.79%	3.099%
15	4.782	605	606	608	rBV2	532	361	0.02%	0.003%
16	5.062	639	652	670	rBV	192170	604323	41.67%	5.429%
17	5.379	698	704	705	rBV3	2200	2429	0.17%	0.022%
18	5.458	715	717	720	rBV3	401	375	0.03%	0.003%
19	5.489	720	722	725	rVB	326	311	0.02%	0.003%
20	5.562	725	734	743	rBV4	4213	10951	0.76%	0.098%
21	5.678	750	753	757	rBV2	390	651	0.04%	0.006%
22	5.775	767	769	774	rVB3	291	327	0.02%	0.003%
23	5.971	788	801	819	rBV2	490589	1450111	100.00%	13.027%
24	6.428	874	876	878	rVB	409	303	0.02%	0.003%
25	6.458	878	881	884	rBV3	376	699	0.05%	0.006%
26	6.580	900	901	904	rBV	296	290	0.02%	0.003%
27	6.635	907	910	912	rVV3	319	357	0.02%	0.003%
28	6.763	922	931	945	rVV	360592	846453	58.37%	7.604%
29	6.976	965	966	969	rBV2	345	338	0.02%	0.003%
30	7.129	982	991	1001	rBV4	37726	92477	6.38%	0.831%
31	7.312	1012	1021	1037	rBV	290267	635824	43.85%	5.712%
32	7.464	1044	1046	1047	rBV	428	370	0.03%	0.003%
33	7.482	1047	1049	1054	rVB4	1053	1368	0.09%	0.012%
34	7.574	1062	1064	1067	rVB3	259	315	0.02%	0.003%
35	7.940	1117	1124	1129	rVV4	1183	2763	0.19%	0.025%
36	8.202	1165	1167	1170	rVB2	263	311	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029413.D
 Acq On : 13 Jun 2022 15:26
 Operator : JC/MD
 Sample : N3291-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.330	1181	1188	1199	rBV	191443	322036	22.21%	2.893%
38	8.494	1209	1215	1219	rVB3	601	1282	0.09%	0.012%
39	8.653	1233	1241	1248	rBV	756335	1185188	81.73%	10.647%
40	8.720	1249	1252	1258	rVV	11616	19770	1.36%	0.178%
41	8.787	1261	1263	1264	rVB2	547	313	0.02%	0.003%
42	8.903	1281	1282	1285	rBV2	465	507	0.03%	0.005%
43	8.952	1285	1290	1303	rVV	136960	202837	13.99%	1.822%
44	9.275	1339	1343	1349	rVB2	4150	6021	0.42%	0.054%
45	9.385	1356	1361	1378	rBV	550688	780461	53.82%	7.011%
46	9.580	1391	1393	1398	rBV2	343	545	0.04%	0.005%
47	9.647	1401	1404	1406	rBV3	391	392	0.03%	0.004%
48	9.775	1423	1425	1427	rBV	300	298	0.02%	0.003%
49	10.006	1461	1463	1465	rVB2	340	334	0.02%	0.003%
50	10.055	1465	1471	1485	rBV	733846	978536	67.48%	8.790%
51	10.201	1491	1495	1498	rVB2	1481	1846	0.13%	0.017%
52	10.305	1505	1512	1518	rBV4	2882	4354	0.30%	0.039%
53	10.488	1540	1542	1545	rBV2	313	320	0.02%	0.003%
54	10.543	1549	1551	1555	rVB2	245	325	0.02%	0.003%
55	10.647	1565	1568	1569	rBV3	1008	958	0.07%	0.009%
56	10.811	1591	1595	1596	rBV2	227	294	0.02%	0.003%
57	10.927	1608	1614	1615	rBV2	288	435	0.03%	0.004%
58	10.970	1617	1621	1624	rBV	1060	1328	0.09%	0.012%
59	11.085	1636	1640	1643	rBV3	1823	2915	0.20%	0.026%
60	11.122	1643	1646	1651	rVB	4116	5113	0.35%	0.046%
61	11.195	1652	1658	1666	rBV	559881	721441	49.75%	6.481%
62	11.457	1698	1701	1702	rBV2	1132	1322	0.09%	0.012%
63	11.616	1725	1727	1730	rBV3	339	465	0.03%	0.004%
64	11.677	1735	1737	1739	rBV2	738	831	0.06%	0.007%
65	11.750	1746	1749	1753	rBV3	4261	6064	0.42%	0.054%
66	11.841	1762	1764	1767	rBV2	689	649	0.04%	0.006%
67	11.933	1775	1779	1783	rBV4	2019	2848	0.20%	0.026%
68	11.969	1783	1785	1788	rBV3	996	1377	0.09%	0.012%
69	12.024	1788	1794	1801	rBV	776990	962894	66.40%	8.650%
70	12.128	1808	1811	1813	rBV4	1098	1644	0.11%	0.015%
71	12.152	1813	1815	1821	rVV3	3194	3170	0.22%	0.028%
72	12.262	1831	1833	1836	rBV2	473	398	0.03%	0.004%
73	12.323	1837	1843	1851	rVV	795475	1006410	69.40%	9.041%
74	12.482	1867	1869	1871	rVB2	458	343	0.02%	0.003%
75	12.585	1885	1886	1890	rVB	423	338	0.02%	0.003%
76	12.658	1896	1898	1901	rBV3	705	774	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029413.D
 Acq On : 13 Jun 2022 15:26
 Operator : JC/MD
 Sample : N3291-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.683	1901	1902	1905	rBV3	345	293	0.02%	0.003%
78	12.866	1930	1932	1935	rBV2	483	387	0.03%	0.003%
79	12.902	1937	1938	1942	rVB2	410	304	0.02%	0.003%
80	12.975	1949	1950	1953	rBV2	365	362	0.02%	0.003%
81	13.000	1953	1954	1958	rVV2	295	338	0.02%	0.003%
82	13.049	1960	1962	1968	rVV3	887	1124	0.08%	0.010%
83	13.116	1970	1973	1977	rVV4	1437	1970	0.14%	0.018%
84	13.164	1979	1981	1983	rBV2	323	320	0.02%	0.003%
85	13.591	2047	2051	2055	rVB3	1929	2627	0.18%	0.024%
86	13.780	2079	2082	2089	rVB2	1806	2675	0.18%	0.024%
87	13.835	2089	2091	2092	rBV	376	304	0.02%	0.003%
88	13.963	2109	2112	2116	rVB4	1536	1721	0.12%	0.015%
89	14.134	2136	2140	2142	rVB2	868	988	0.07%	0.009%
90	14.250	2157	2159	2161	rVB	425	362	0.02%	0.003%
91	14.274	2161	2163	2165	rBV2	507	443	0.03%	0.004%
92	14.585	2212	2214	2216	rBV2	407	330	0.02%	0.003%
93	14.676	2227	2229	2230	rBV2	453	369	0.03%	0.003%
94	14.725	2233	2237	2244	rVB5	488	1072	0.07%	0.010%
95	14.798	2247	2249	2252	rBV2	509	504	0.03%	0.005%
96	14.829	2252	2254	2256	rVB3	444	310	0.02%	0.003%
97	15.024	2284	2286	2288	rBV2	587	422	0.03%	0.004%
98	15.231	2318	2320	2321	rVB	663	342	0.02%	0.003%
99	15.585	2377	2378	2381	rBV2	532	490	0.03%	0.004%
100	16.402	2510	2512	2517	rBV3	937	881	0.06%	0.008%


Sum of corrected areas: 11131745

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029413.D
Acq On : 13 Jun 2022 15:26
Operator : JC/MD
Sample : N3291-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

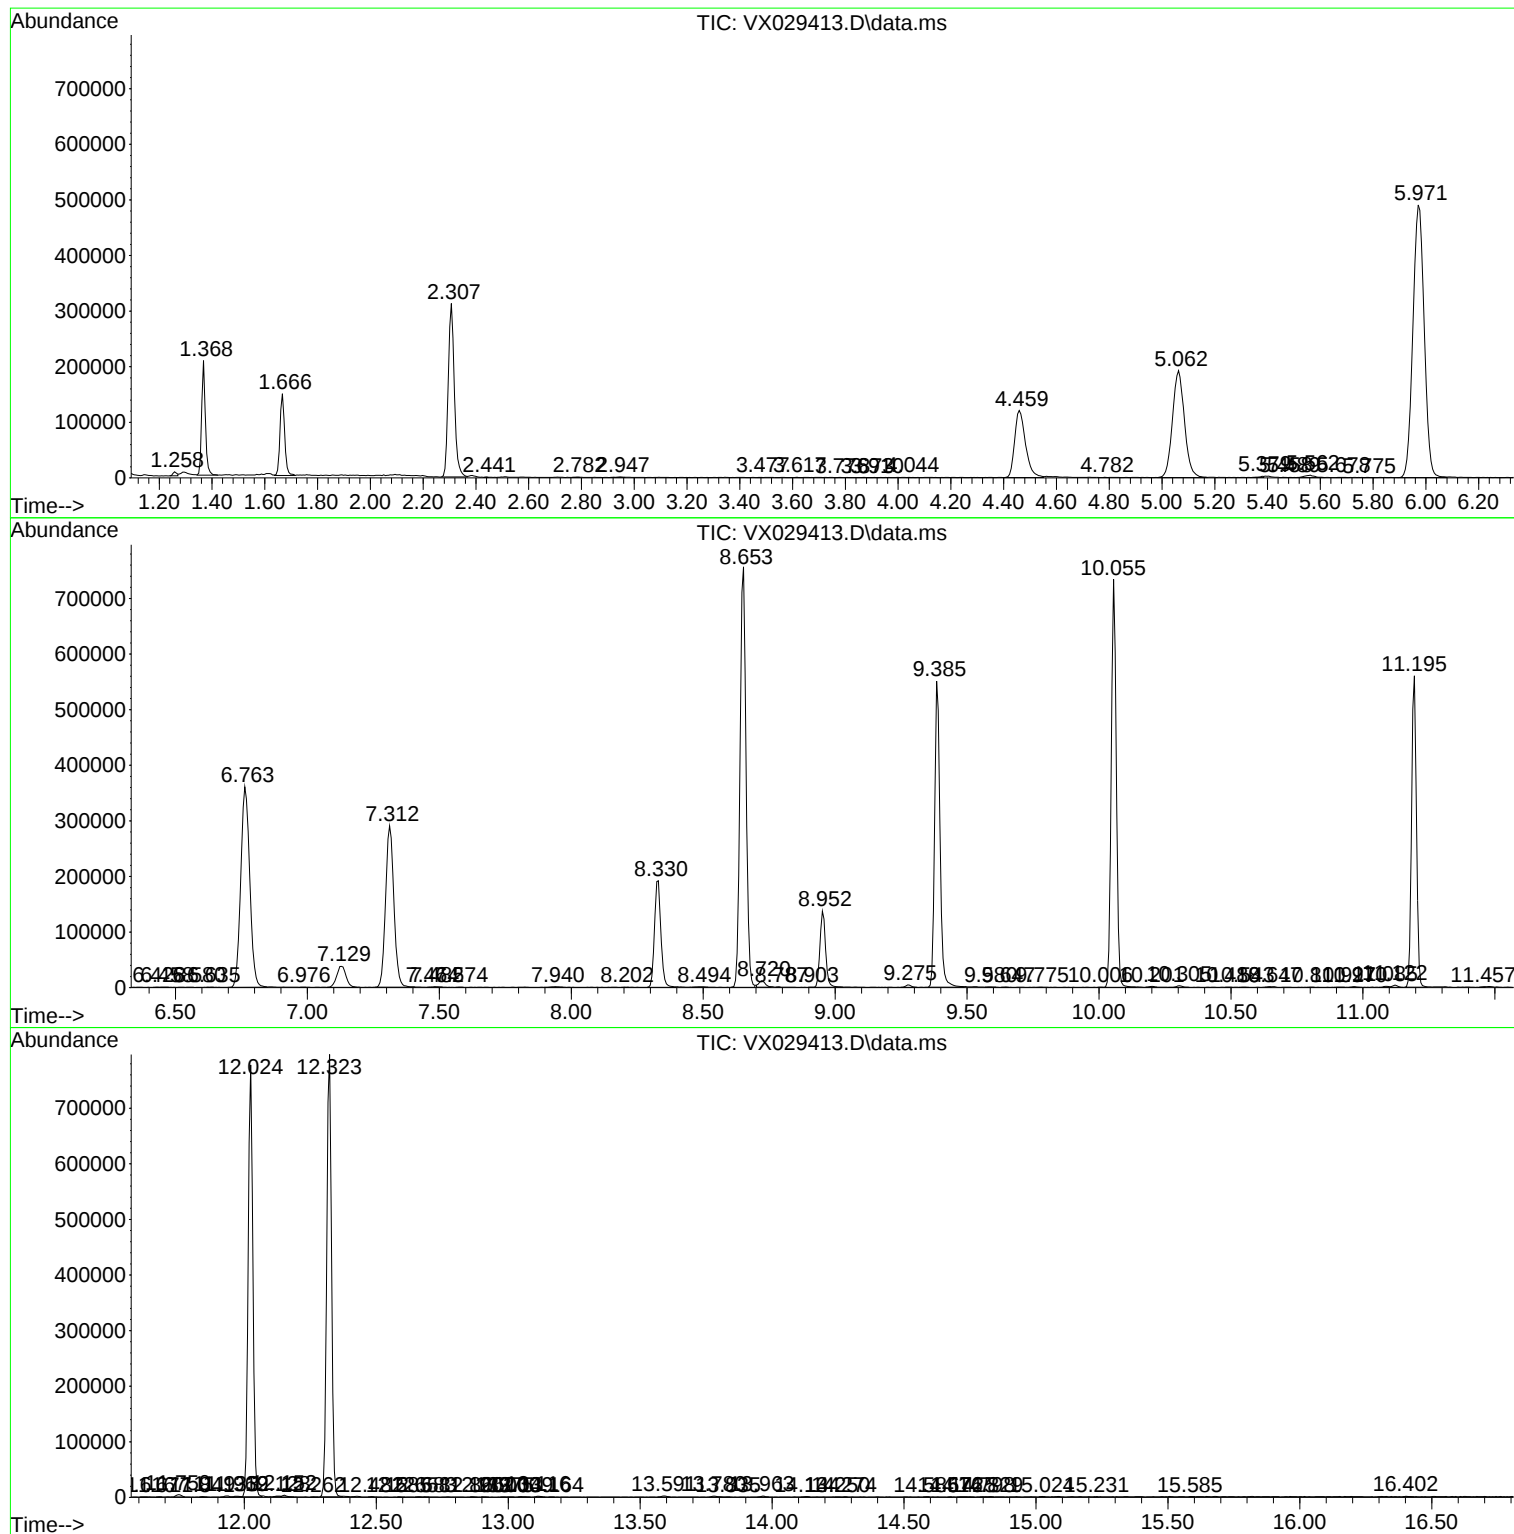

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029413.D
Acq On : 13 Jun 2022 15:26
Operator : JC/MD
Sample : N3291-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029413.D
Acq On : 13 Jun 2022 15:26
Operator : JC/MD
Sample : N3291-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc