

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029414.D
 Acq On : 13 Jun 2022 15:49
 Operator : JC/MD
 Sample : N3291-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	26	28	31	rBV2	4833	5134	0.38%	0.048%
2	1.367	42	46	54	rVB	185628	186859	13.80%	1.752%
3	1.666	91	95	103	rVB	138573	164586	12.15%	1.543%
4	2.306	194	200	211	rBV	297492	466128	34.42%	4.369%
5	2.709	260	266	267	rBV4	635	1193	0.09%	0.011%
6	2.788	273	279	285	rBV6	821	1744	0.13%	0.016%
7	2.946	302	305	309	rBV3	625	1066	0.08%	0.010%
8	3.178	341	343	345	rBV	344	264	0.02%	0.002%
9	3.434	381	385	387	rBV	246	283	0.02%	0.003%
10	3.556	403	405	408	rVB	497	382	0.03%	0.004%
11	3.934	465	467	470	rVB2	344	327	0.02%	0.003%
12	4.032	482	483	485	rBV2	390	370	0.03%	0.003%
13	4.080	489	491	494	rVV2	305	267	0.02%	0.003%
14	4.135	497	500	502	rBV	288	278	0.02%	0.003%
15	4.202	507	511	512	rBV2	407	447	0.03%	0.004%
16	4.464	544	554	569	rBV	119637	339855	25.10%	3.186%
17	5.062	639	652	672	rBV	178216	553968	40.91%	5.193%
18	5.391	699	706	707	rBV2	1483	2630	0.19%	0.025%
19	5.556	726	733	742	rVB6	2626	7528	0.56%	0.071%
20	5.970	790	801	820	rBV2	455221	1354111	100.00%	12.693%
21	6.184	835	836	842	rBV4	368	493	0.04%	0.005%
22	6.226	842	843	846	rVB	483	249	0.02%	0.002%
23	6.366	863	866	870	rBV3	436	698	0.05%	0.007%
24	6.543	892	895	896	rBV2	286	333	0.02%	0.003%
25	6.598	901	904	908	rVB2	407	480	0.04%	0.004%
26	6.763	921	931	950	rBV	361587	861370	63.61%	8.074%
27	6.891	950	952	956	rVV3	538	477	0.04%	0.004%
28	7.013	970	972	975	rBV3	277	311	0.02%	0.003%
29	7.129	981	991	1004	rBV2	42837	100034	7.39%	0.938%
30	7.311	1012	1021	1035	rBV	276820	600168	44.32%	5.626%
31	7.488	1046	1050	1057	rVB5	781	2116	0.16%	0.020%
32	7.574	1062	1064	1067	rVB2	376	406	0.03%	0.004%
33	7.726	1086	1089	1092	rBV2	173	296	0.02%	0.003%
34	7.811	1101	1103	1109	rVB	513	664	0.05%	0.006%
35	7.939	1118	1124	1125	rBV3	696	1063	0.08%	0.010%
36	8.183	1162	1164	1167	rBV2	310	384	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029414.D
 Acq On : 13 Jun 2022 15:49
 Operator : JC/MD
 Sample : N3291-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.330	1181	1188	1199	rBV	184133	301821	22.29%	2.829%
38	8.482	1211	1213	1215	rBV2	614	346	0.03%	0.003%
39	8.653	1234	1241	1248	rBV	700393	1097746	81.07%	10.290%
40	8.726	1249	1253	1261	rVV	10745	18828	1.39%	0.176%
41	8.787	1261	1263	1265	rVV2	532	461	0.03%	0.004%
42	8.811	1265	1267	1268	rVB	615	320	0.02%	0.003%
43	8.951	1281	1290	1302	rBV	135028	192975	14.25%	1.809%
44	9.177	1326	1327	1331	rVB	271	297	0.02%	0.003%
45	9.214	1331	1333	1336	rVB2	400	343	0.03%	0.003%
46	9.281	1339	1344	1348	rVB3	3711	5360	0.40%	0.050%
47	9.384	1356	1361	1378	rBV	520442	756470	55.86%	7.091%
48	9.598	1394	1396	1397	rBV2	448	340	0.03%	0.003%
49	9.695	1411	1412	1416	rBV	404	463	0.03%	0.004%
50	9.902	1445	1446	1449	rVB3	384	319	0.02%	0.003%
51	9.988	1459	1460	1463	rVB3	338	274	0.02%	0.003%
52	10.055	1466	1471	1485	rVB	754195	989929	73.11%	9.280%
53	10.305	1506	1512	1520	rBV3	2538	3709	0.27%	0.035%
54	10.567	1553	1555	1558	rBV3	302	398	0.03%	0.004%
55	10.658	1565	1570	1573	rVV4	1174	1691	0.12%	0.016%
56	10.786	1588	1591	1593	rBV2	324	330	0.02%	0.003%
57	10.969	1618	1621	1624	rVV2	767	798	0.06%	0.007%
58	11.097	1637	1642	1643	rBV4	770	1051	0.08%	0.010%
59	11.122	1643	1646	1651	rVB2	3508	4418	0.33%	0.041%
60	11.195	1652	1658	1670	rBV	536430	685044	50.59%	6.422%
61	11.280	1670	1672	1676	rBV2	712	796	0.06%	0.007%
62	11.384	1687	1689	1690	rBV2	328	259	0.02%	0.002%
63	11.427	1694	1696	1697	rBV	314	251	0.02%	0.002%
64	11.457	1697	1701	1702	rBV	901	902	0.07%	0.008%
65	11.548	1714	1716	1718	rVB	364	300	0.02%	0.003%
66	11.609	1724	1726	1729	rVB3	491	521	0.04%	0.005%
67	11.634	1729	1730	1733	rBV2	546	524	0.04%	0.005%
68	11.750	1745	1749	1757	rVB3	3881	5449	0.40%	0.051%
69	11.841	1761	1764	1768	rBV3	801	889	0.07%	0.008%
70	11.884	1768	1771	1774	rVB3	280	372	0.03%	0.003%
71	11.933	1776	1779	1783	rBV4	1468	1994	0.15%	0.019%
72	11.975	1783	1786	1789	rBV3	1005	1049	0.08%	0.010%
73	12.024	1789	1794	1803	rBV	805689	973254	71.87%	9.123%
74	12.213	1824	1825	1828	rBV2	355	448	0.03%	0.004%
75	12.323	1835	1843	1851	rBV	757365	941381	69.52%	8.824%
76	12.426	1856	1860	1864	rVV5	975	1782	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029414.D
 Acq On : 13 Jun 2022 15:49
 Operator : JC/MD
 Sample : N3291-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.487	1867	1870	1873	rVV3	874	971	0.07%	0.009%
78	12.628	1891	1893	1895	rBV2	289	330	0.02%	0.003%
79	12.768	1913	1916	1918	rVB2	222	264	0.02%	0.002%
80	12.841	1927	1928	1932	rBV2	242	264	0.02%	0.002%
81	12.963	1946	1948	1952	rVB2	438	286	0.02%	0.003%
82	13.115	1967	1973	1976	rBV4	1431	1993	0.15%	0.019%
83	13.268	1996	1998	2001	rBV	347	259	0.02%	0.002%
84	13.591	2048	2051	2056	rBV4	2196	2910	0.21%	0.027%
85	13.780	2079	2082	2088	rVB2	1279	1603	0.12%	0.015%
86	13.896	2098	2101	2103	rBV	298	349	0.03%	0.003%
87	13.963	2109	2112	2115	rVB3	1191	1296	0.10%	0.012%
88	14.127	2137	2139	2141	rBV2	589	480	0.04%	0.004%
89	14.243	2155	2158	2160	rBV3	325	401	0.03%	0.004%
90	14.371	2177	2179	2183	rBV2	346	361	0.03%	0.003%
91	14.426	2186	2188	2191	rVB2	310	279	0.02%	0.003%
92	14.621	2218	2220	2224	rBV3	314	485	0.04%	0.005%
93	14.755	2240	2242	2245	rVB3	458	515	0.04%	0.005%
94	14.786	2245	2247	2249	rBV2	357	394	0.03%	0.004%
95	14.889	2263	2264	2269	rBV2	516	698	0.05%	0.007%
96	14.944	2271	2273	2274	rBV	423	250	0.02%	0.002%
97	15.017	2283	2285	2286	rBV2	553	373	0.03%	0.003%
98	15.950	2436	2438	2440	rBV3	725	717	0.05%	0.007%
99	16.395	2509	2511	2515	rBV3	651	773	0.06%	0.007%
100	16.730	2564	2566	2570	rBV3	608	707	0.05%	0.007%

Sum of corrected areas: 10667822




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029414.D
Acq On : 13 Jun 2022 15:49
Operator : JC/MD
Sample : N3291-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

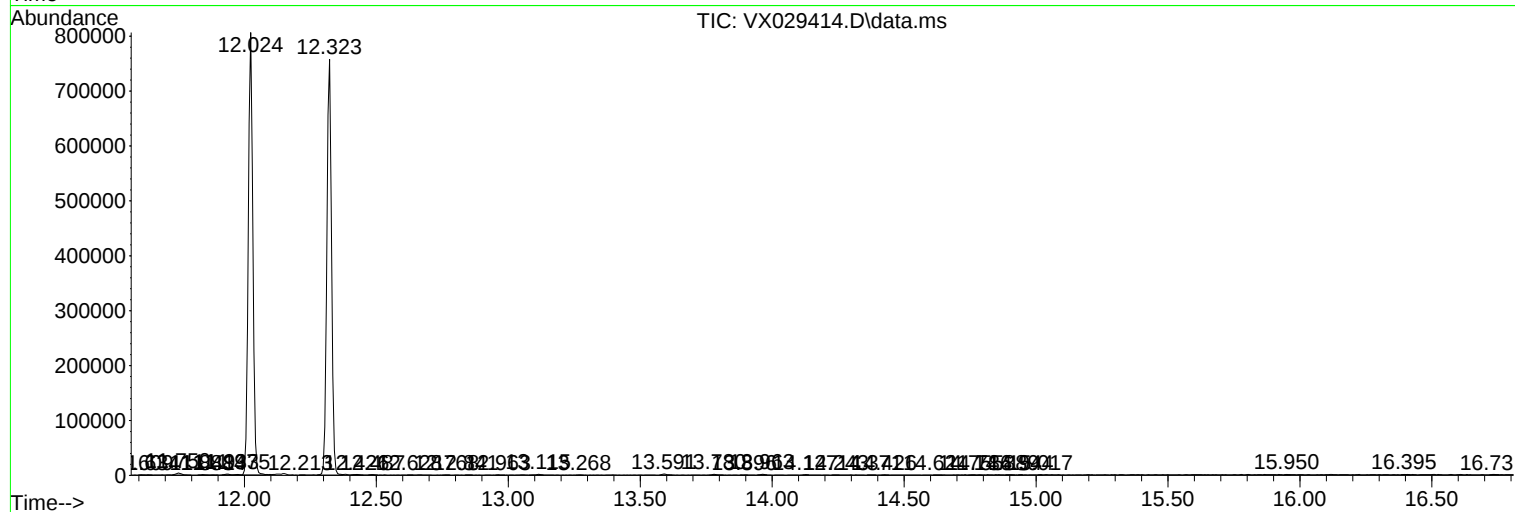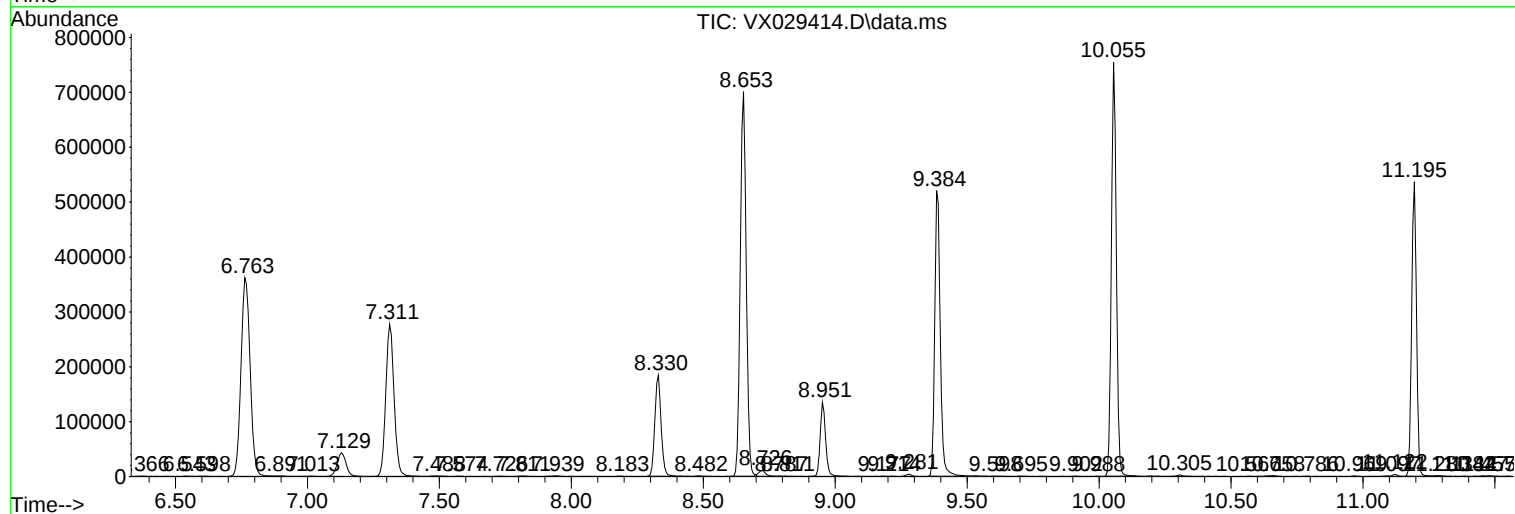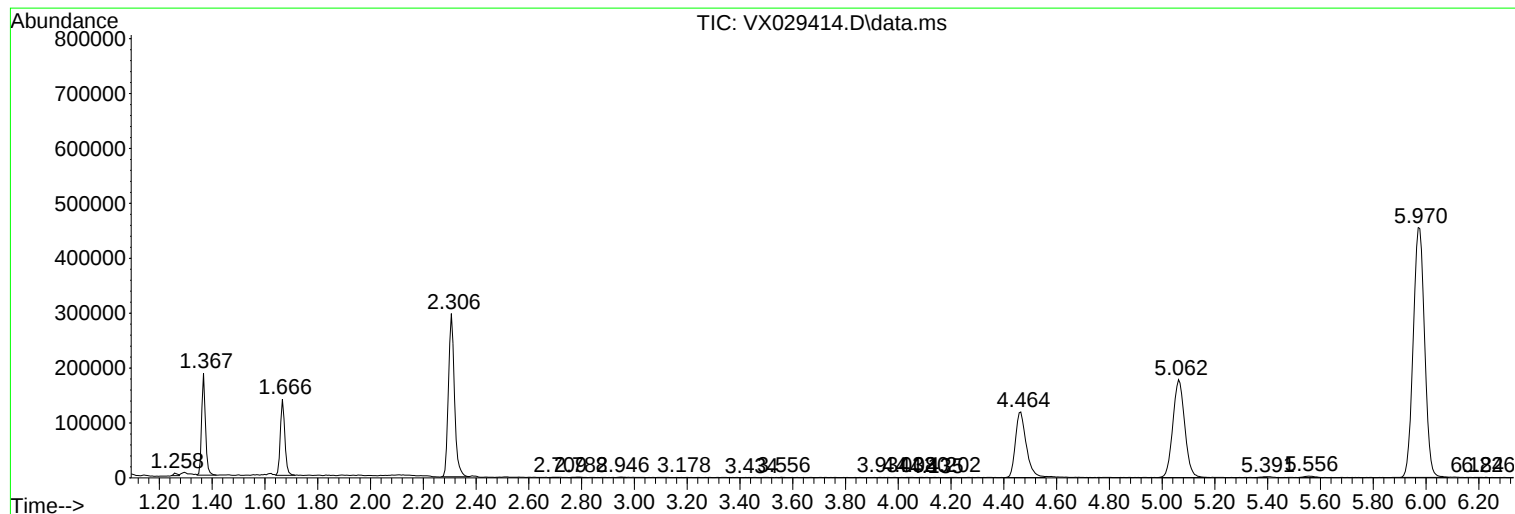

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029414.D
Acq On : 13 Jun 2022 15:49
Operator : JC/MD
Sample : N3291-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029414.D
Acq On : 13 Jun 2022 15:49
Operator : JC/MD
Sample : N3291-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc